
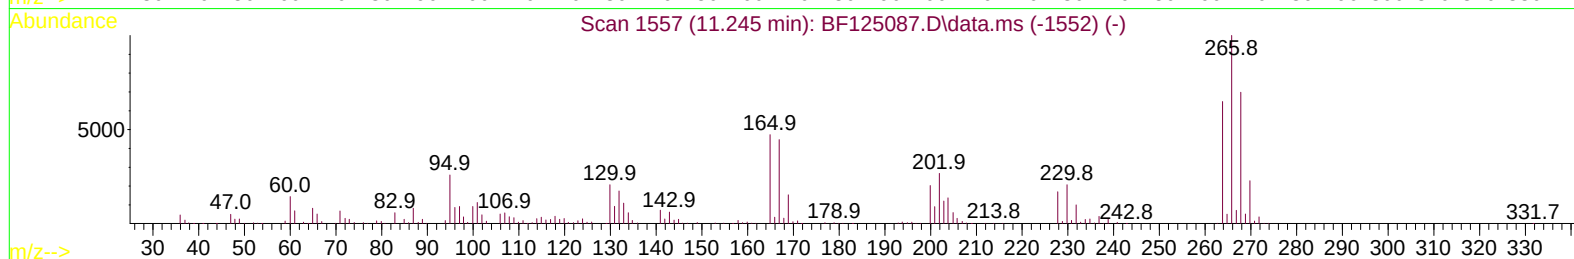
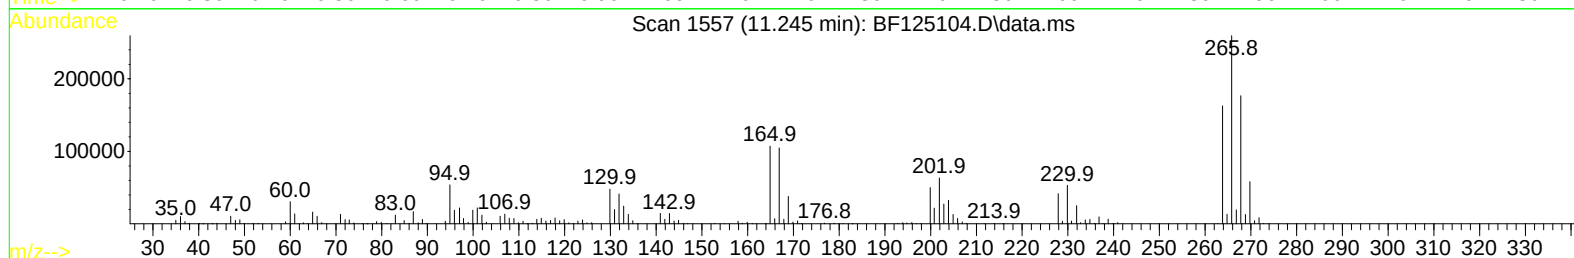


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081921\
 Data File : BF125104.D
 Acq On : 19 Aug 2021 9:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 12:24:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 18 17:03:50 2021
 Response via : Initial Calibration

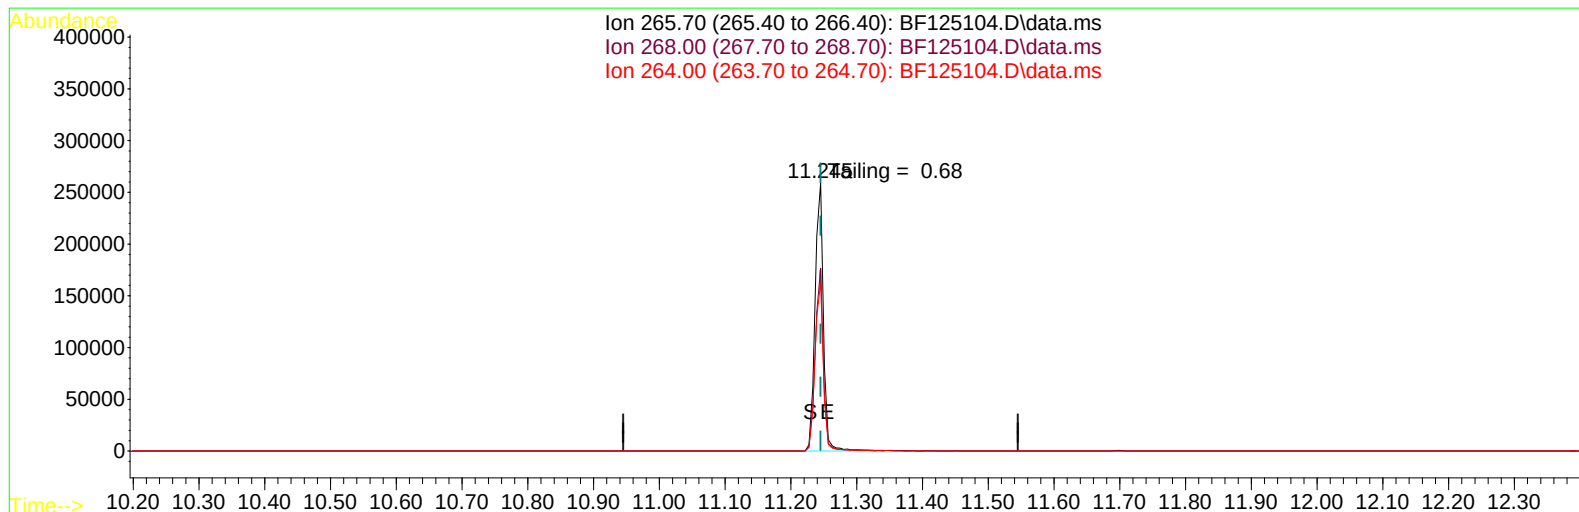

TIC: BF125104.D\data.ms

(70) Pentachlorophenol (C)




11.245min (-0.000) 37157.17 ng

response 229690

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.12
264.00	69.90	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081921\
 Data File : BF125104.D
 Acq On : 19 Aug 2021 9:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 12:24:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 18 17:03:50 2021
 Response via : Initial Calibration

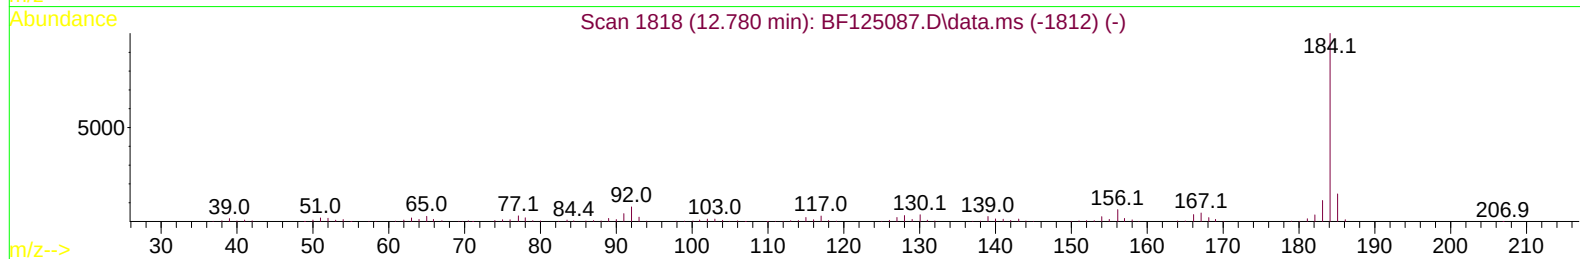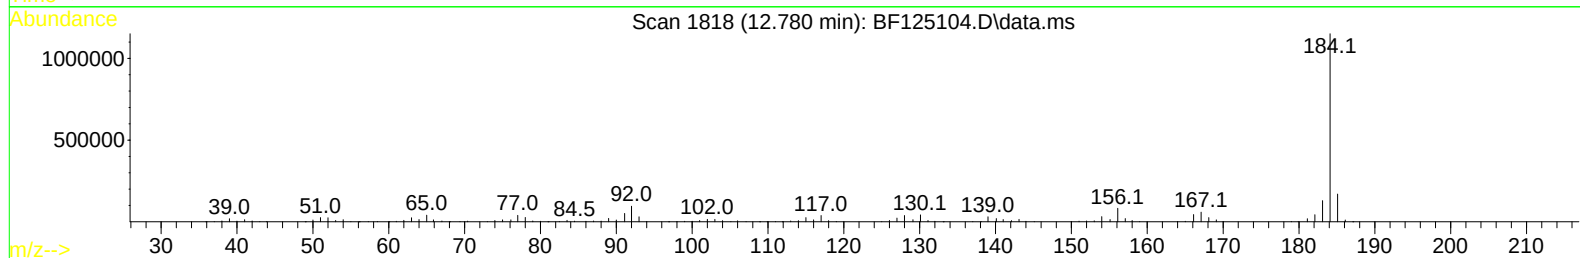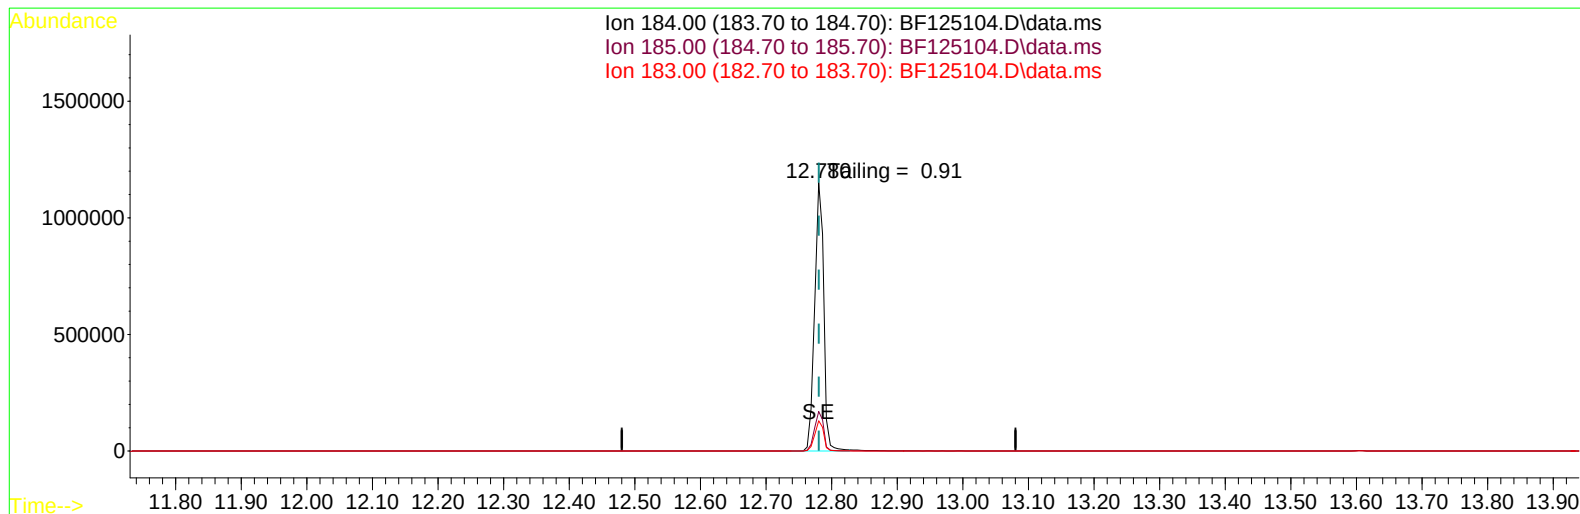

TIC: BF125104.D\data.ms

(77) Benzidine

12.780min (-0.000) 0.00 ng

response 1116179

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.77
183.00	10.10	11.28
0.00	0.00	0.00