
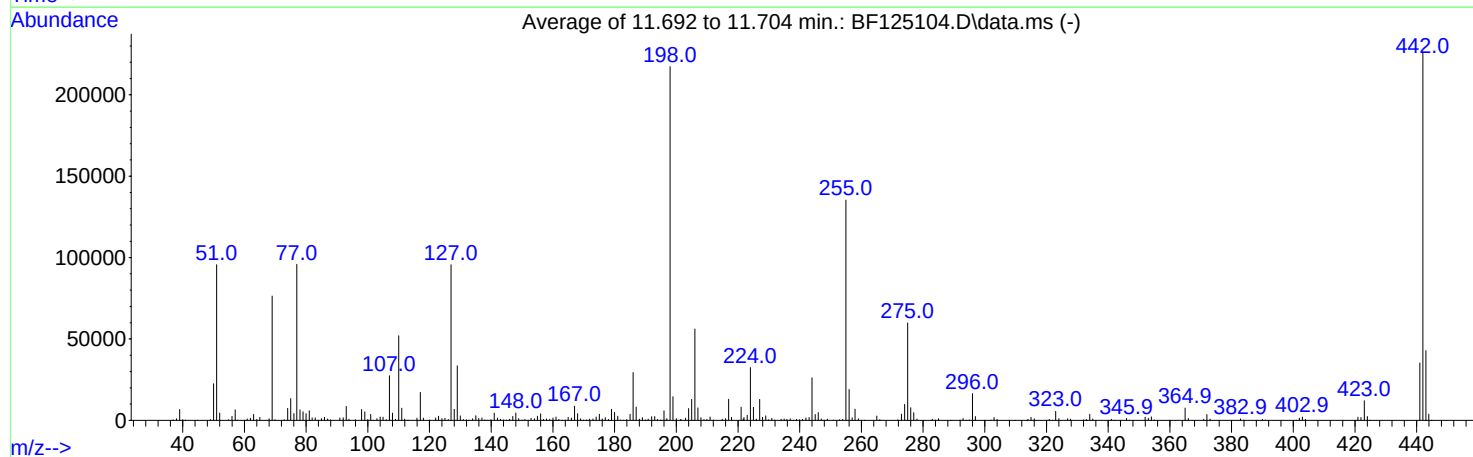


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081921\
 Data File : BF125104.D
 Acq On : 19 Aug 2021 9:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 18 17:03:50 2021

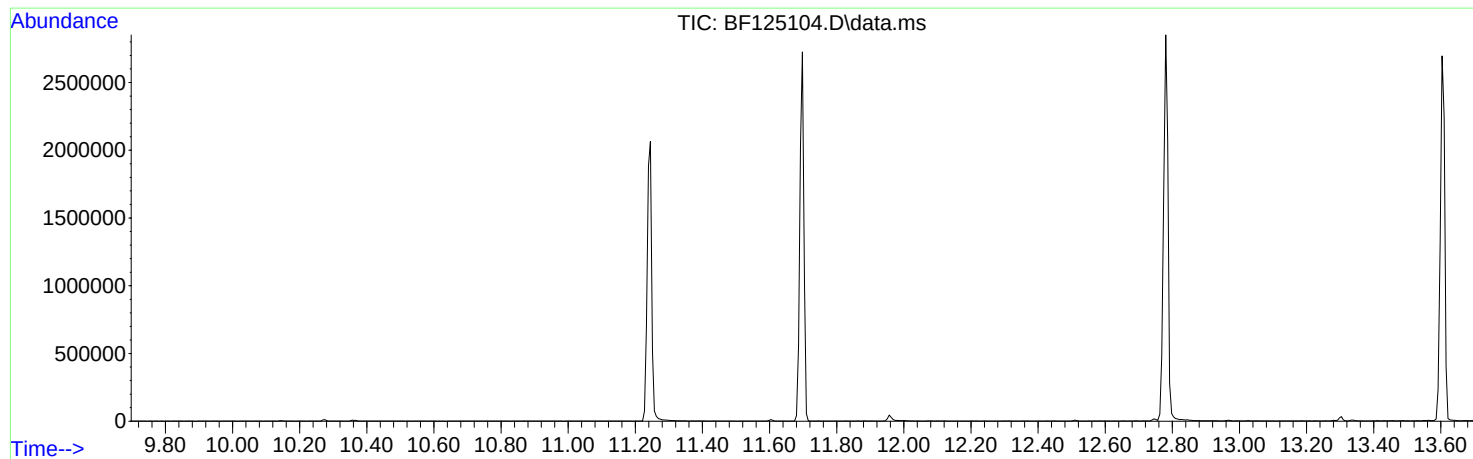




AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	95611	PASS
68	69	0.00	2	1.3	1021	PASS
69	198	0.00	100	35.1	76357	PASS
70	69	0.00	2	0.5	375	PASS
127	198	10	80	44.0	95659	PASS
197	198	0.00	2	0.5	1043	PASS
198	198	100	100	100.0	217349	PASS
199	198	5	9	6.7	14569	PASS
275	198	10	60	27.6	59912	PASS
365	198	1	100	3.5	7589	PASS
441	198	0.01	100	16.2	35251	PASS
442	442	50	100	100.0	225984	PASS
443	442	15	24	19.0	42885	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081921\
 Data File : BF125104.D
 Acq On : 19 Aug 2021 9:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 19 12:24:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 18 17:03:50 2021
 Response via : Initial Calibration

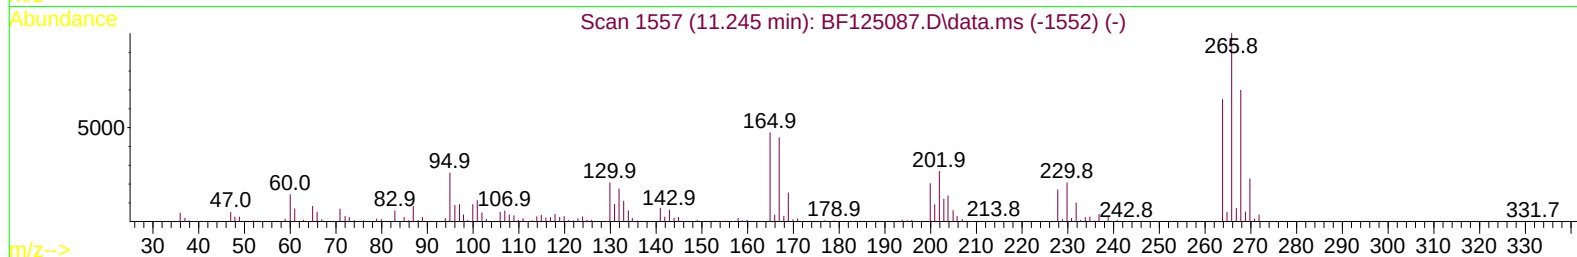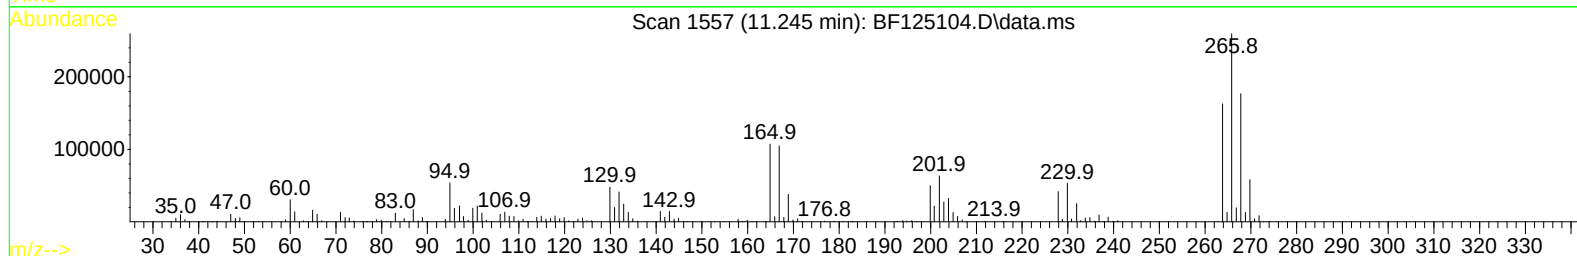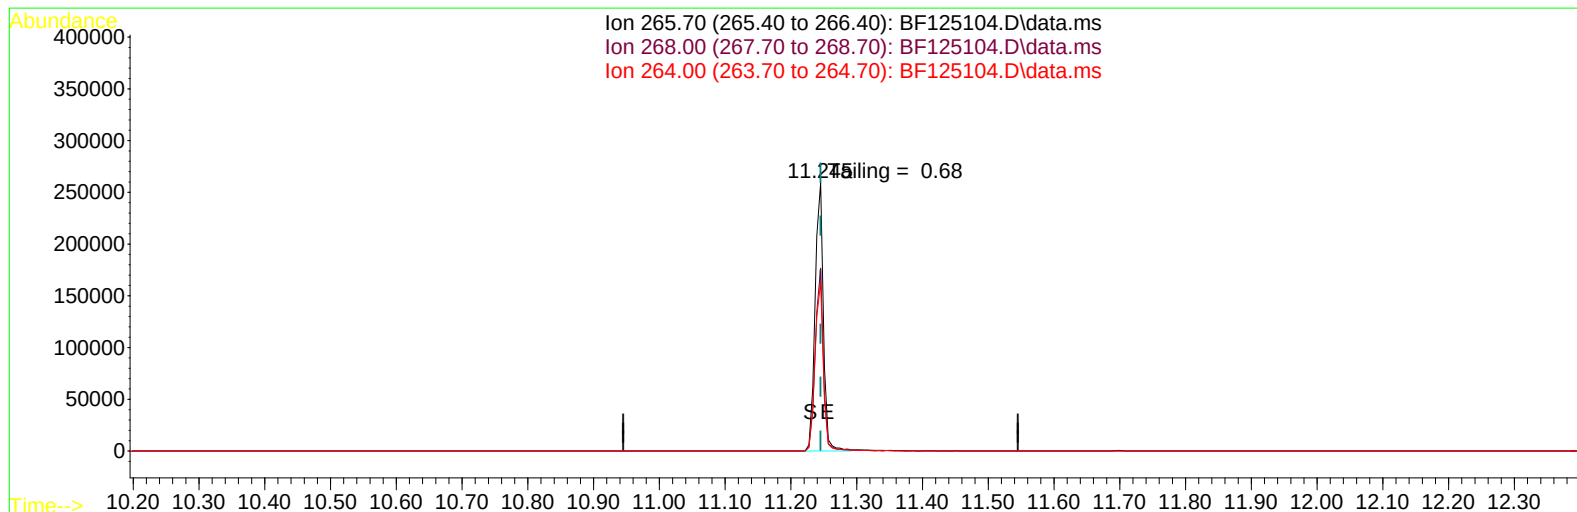

TIC: BF125104.D\data.ms

(70) Pentachlorophenol (C)

11.245min (-0.000) 37157.17 ng




response 229690

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.12
264.00	69.90	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081921\
 Data File : BF125104.D
 Acq On : 19 Aug 2021 9:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 19 12:24:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 18 17:03:50 2021
 Response via : Initial Calibration

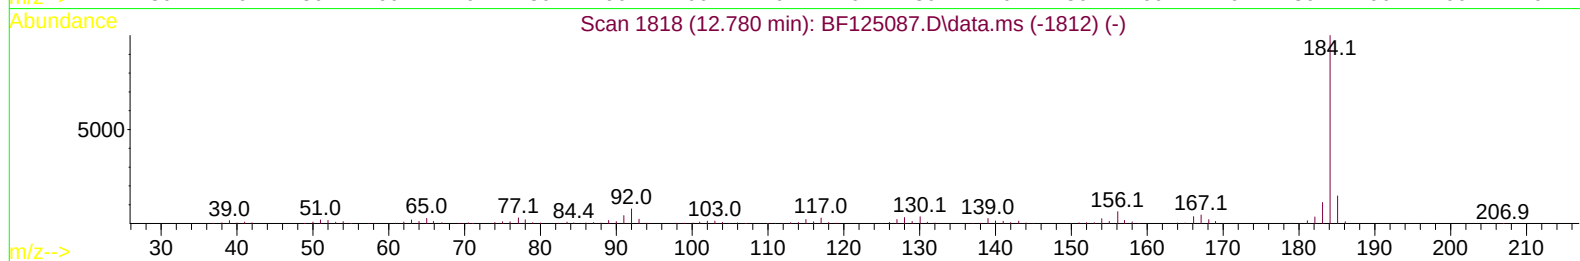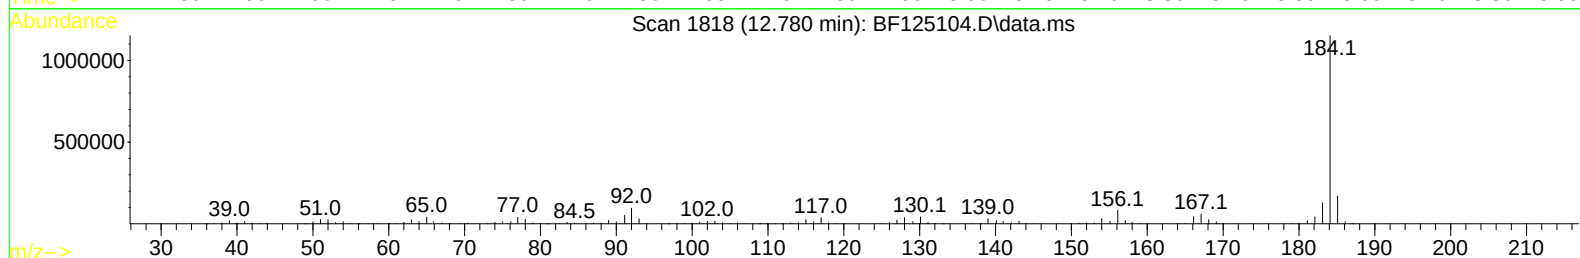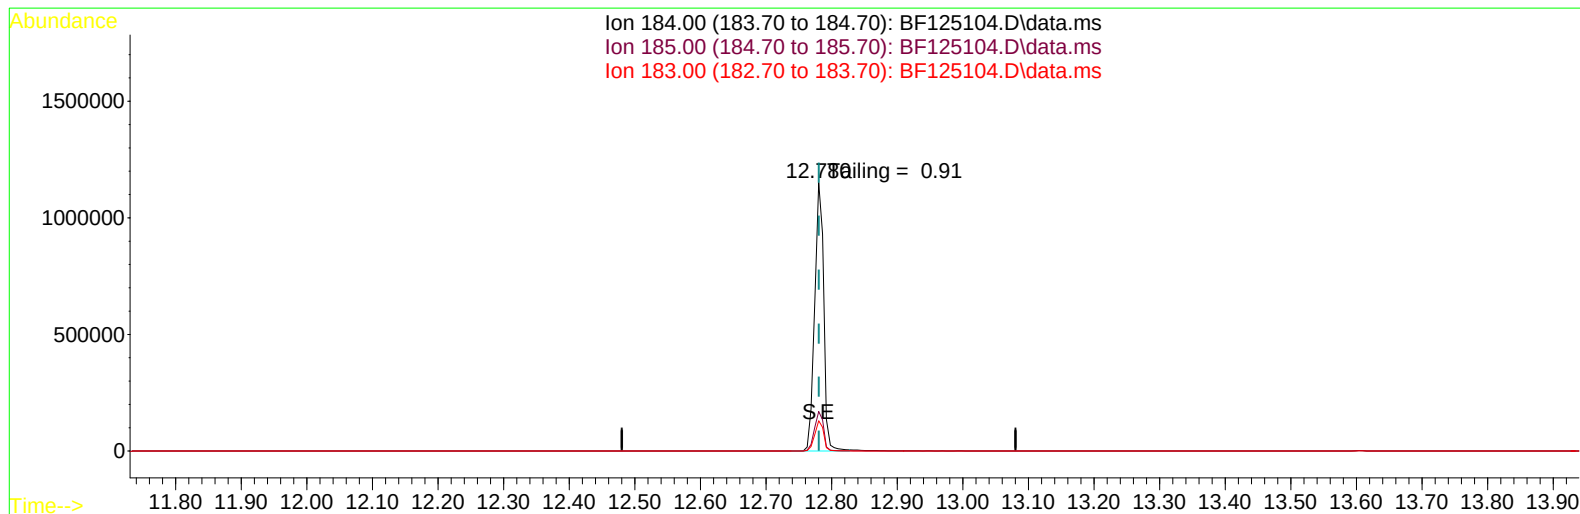

TIC: BF125104.D\data.ms

(77) Benzidine

12.780min (-0.000) 0.00 ng

response 1116179

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.77
183.00	10.10	11.28
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/19/2021	BNA_F	<u>BF125104.D</u>
Compound Name	Response	Retention Time
DDT	483530	13.6
DDD	6473	13.3
DDE	1152	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7625	491155	1.55