
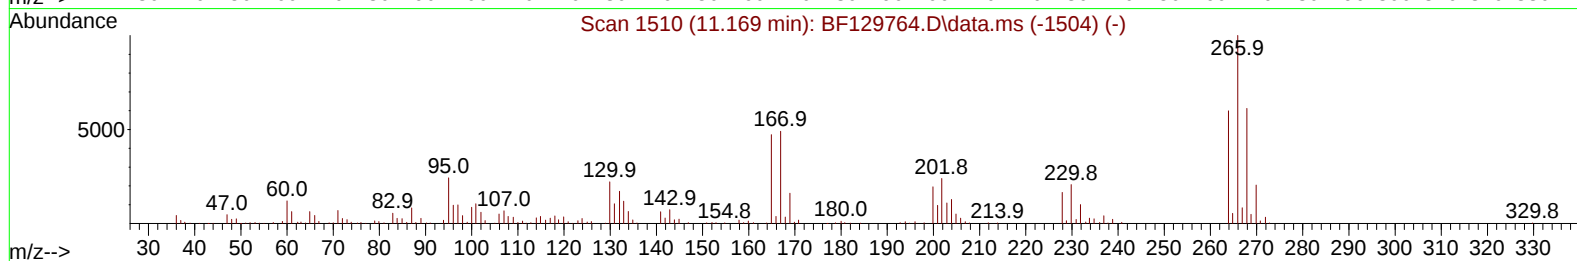
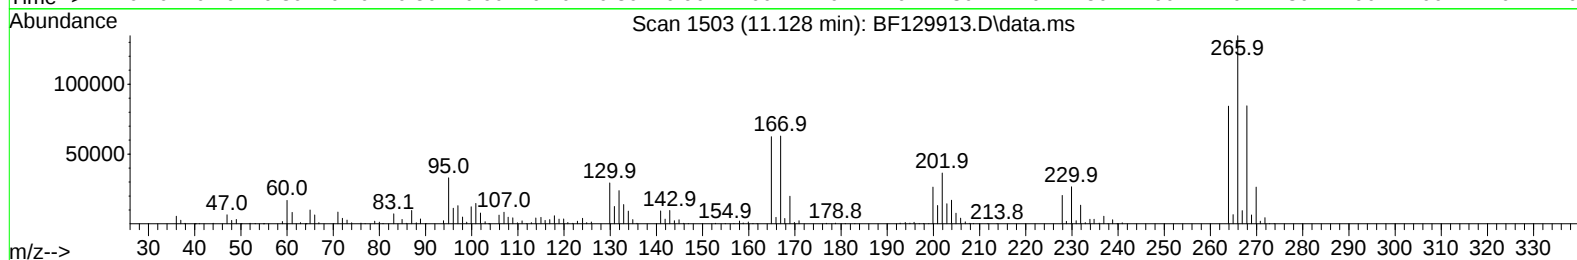


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
Data File : BF129913.D
Acq On : 19 Aug 2022 17:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 05:31:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 20 07:47:33 2022
Response via : Initial Calibration

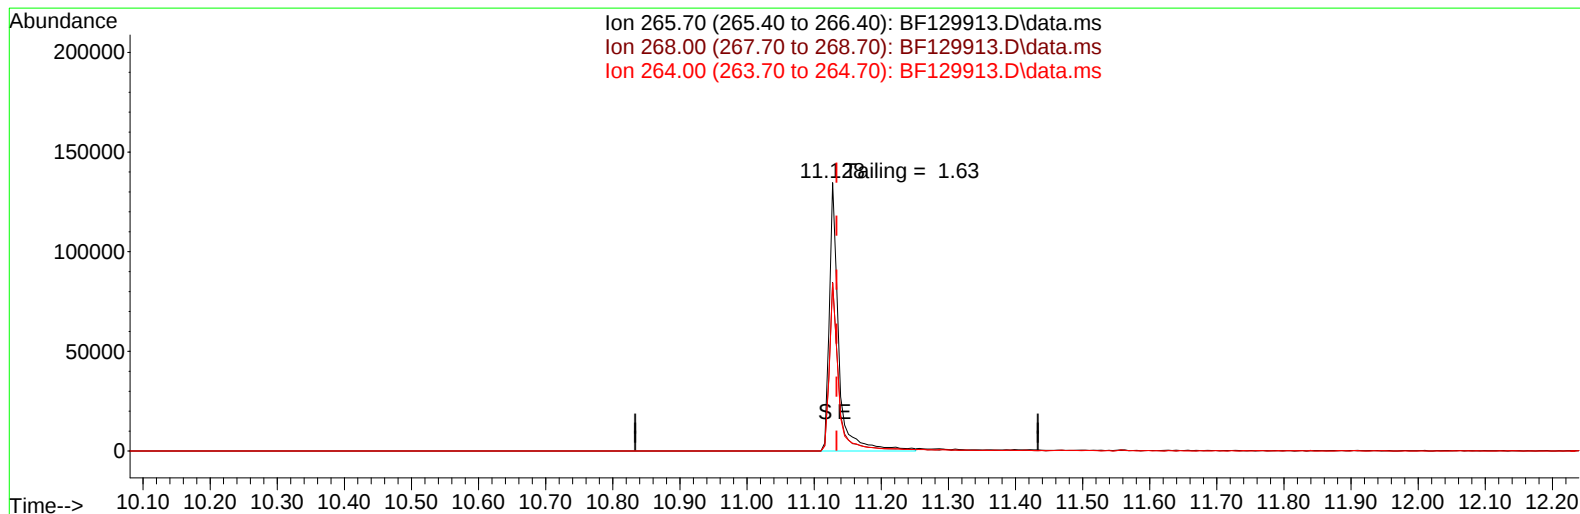

TIC: BF129913.D\data.ms

(70) Pentachlorophenol (C)




11.128min (-0.006) 371759.48 ng

response 131521

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.79
264.00	59.90	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
Data File : BF129913.D
Acq On : 19 Aug 2022 17:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 05:31:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 20 07:47:33 2022
Response via : Initial Calibration

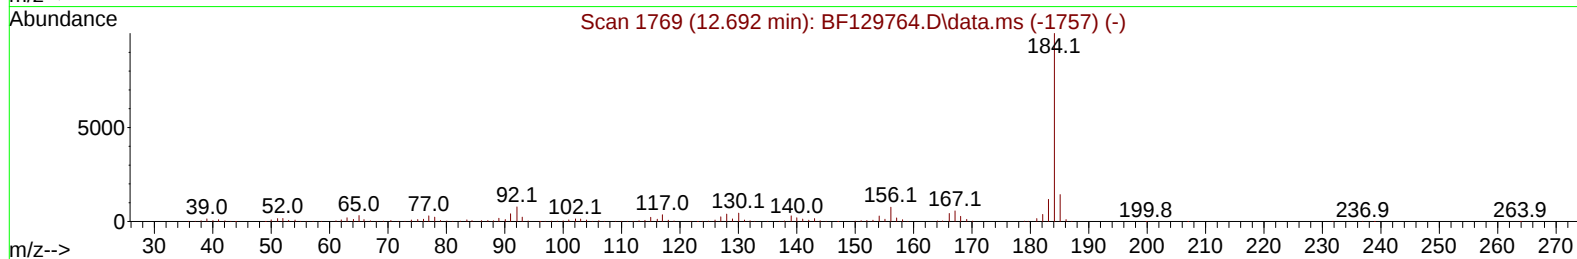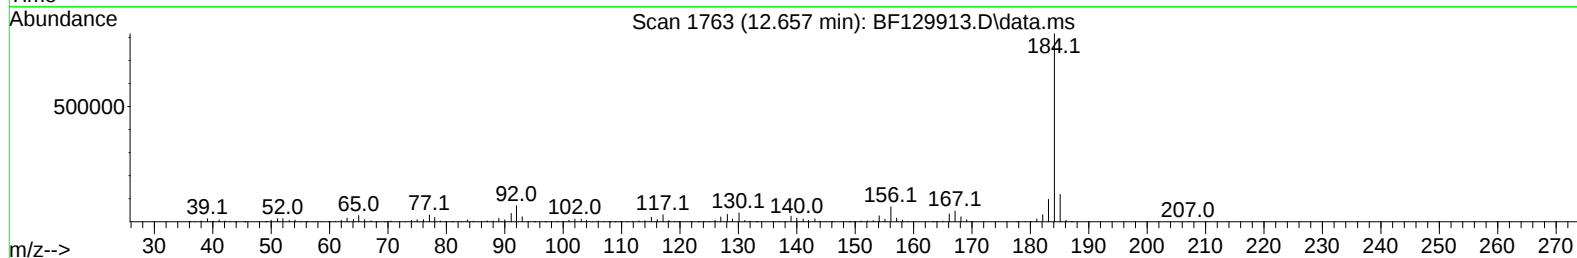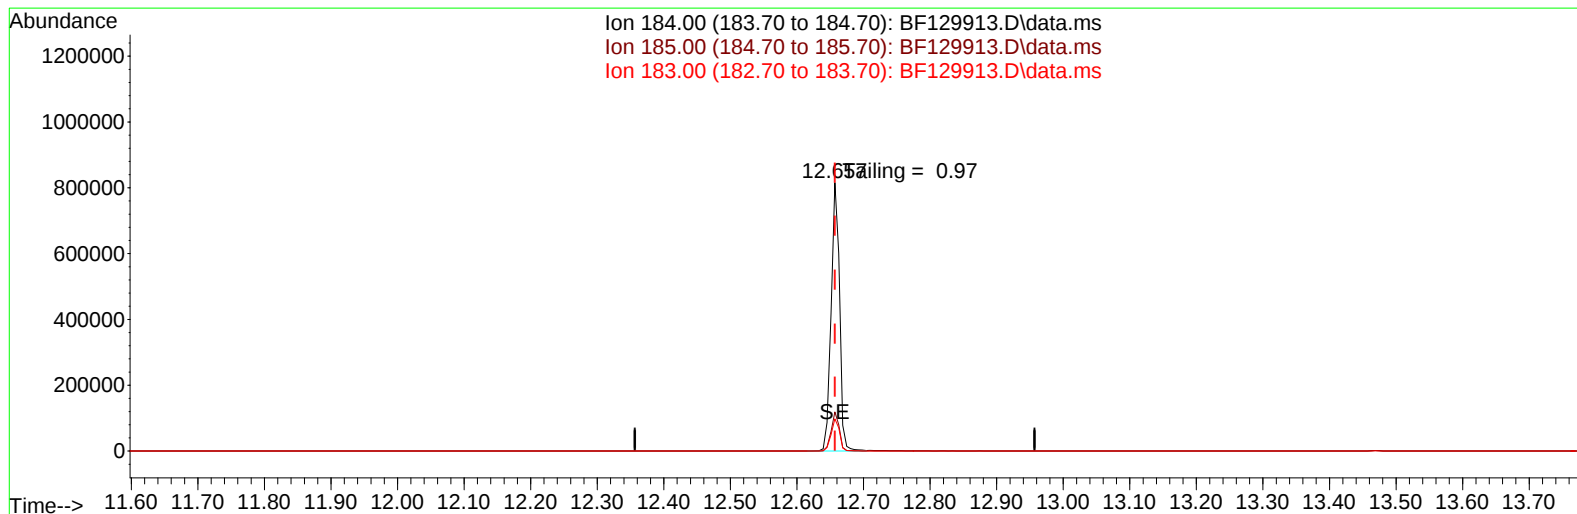

TIC: BF129913.D\data.ms

(77) Benzidine

12.657min (+ 0.000) 37835.47 ng

response 726546

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.55
183.00	11.80	11.97
0.00	0.00	0.00