

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
 Data File : BF129902.D
 Acq On : 19 Aug 2022 09:43
 Operator : CG\JU
 Sample : PB146929BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146929BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	531	535	555	rBV	3700346	3621618	78.82%	13.077%
2	6.451	703	708	725	rBV	3499858	3615367	78.69%	13.054%
3	6.793	762	766	773	rBV	901082	805086	17.52%	2.907%
4	7.363	858	863	866	rBV	2304764	2339177	50.91%	8.446%
5	8.075	979	984	987	rBV	1169666	1081687	23.54%	3.906%
6	9.151	1161	1167	1170	rBV	4616049	4432259	96.47%	16.004%
7	9.834	1277	1283	1286	rBV	1328983	1230370	26.78%	4.443%
8	10.628	1414	1418	1422	rBV	2904303	2660770	57.91%	9.607%
9	11.322	1532	1536	1540	rBV	1461195	1226684	26.70%	4.429%
10	12.910	1801	1806	1809	rBV	4724777	4594574	100.00%	16.590%
11	13.974	1983	1987	1990	rBV	1140119	1063085	23.14%	3.839%
12	14.057	1996	2001	2007	rBV	137549	172910	3.76%	0.624%
13	15.433	2228	2235	2243	rVB	645511	851498	18.53%	3.075%




Sum of corrected areas: 27695085

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
Data File : BF129902.D
Acq On : 19 Aug 2022 09:43
Operator : CG\JU
Sample : PB146929BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146929BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

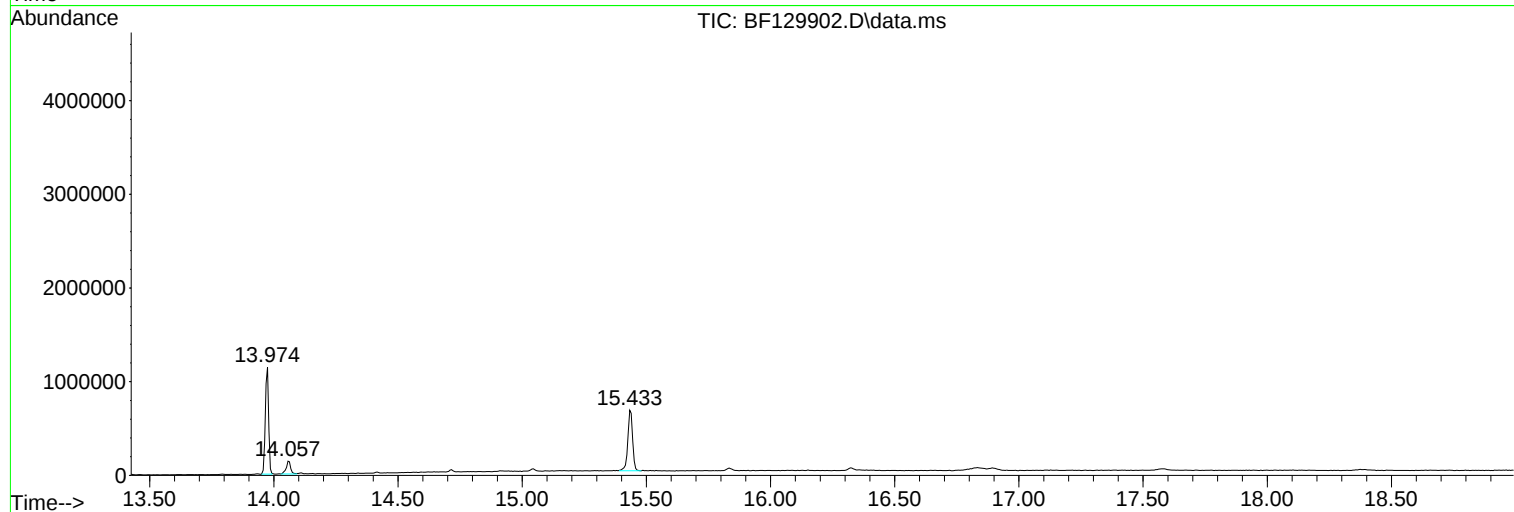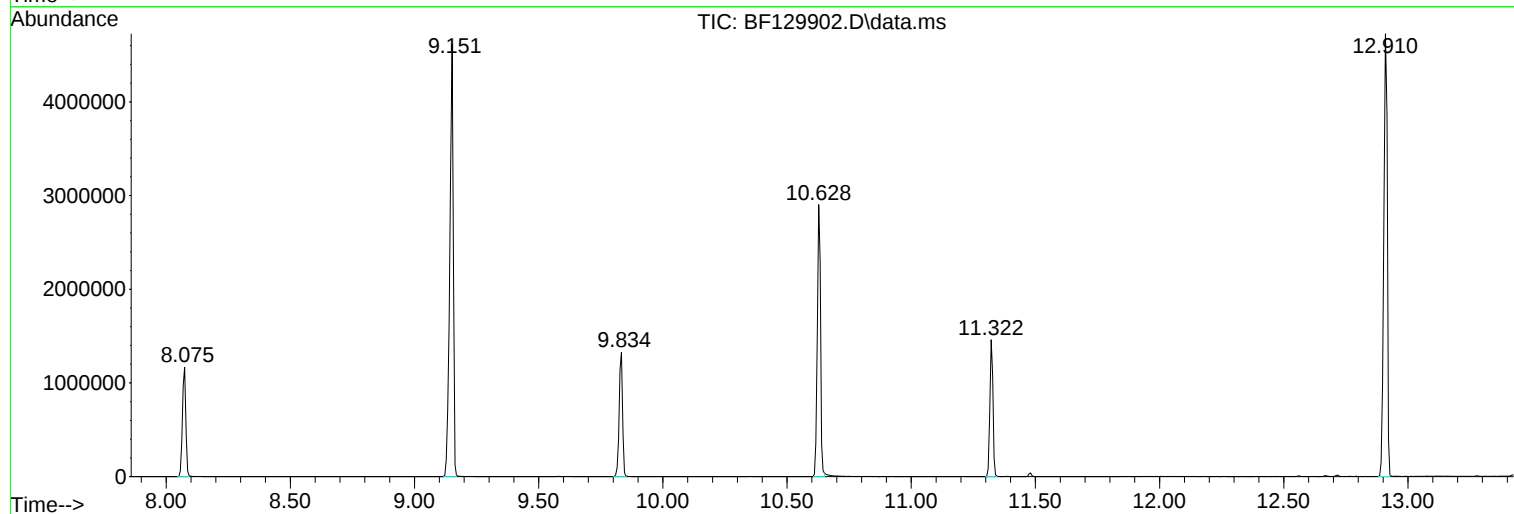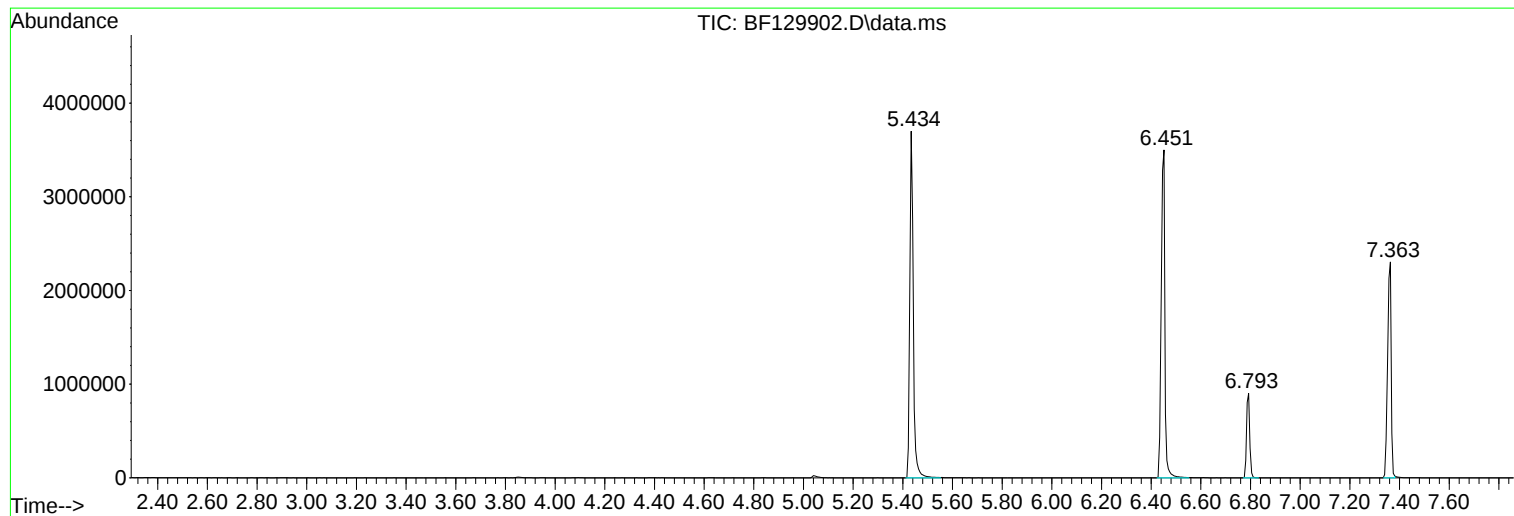

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
Data File : BF129902.D
Acq On : 19 Aug 2022 09:43
Operator : CG\JU
Sample : PB146929BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146929BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.057	3.25 ng	172910	Chrysene-d12	13.975

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
3			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	62
4			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	43
5			Cobalt, (.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	38

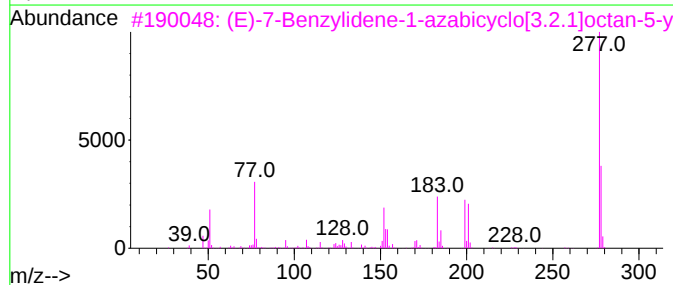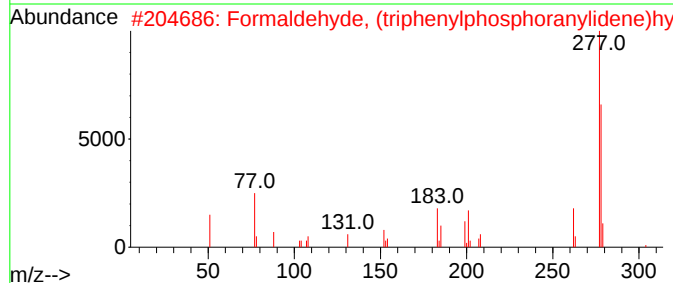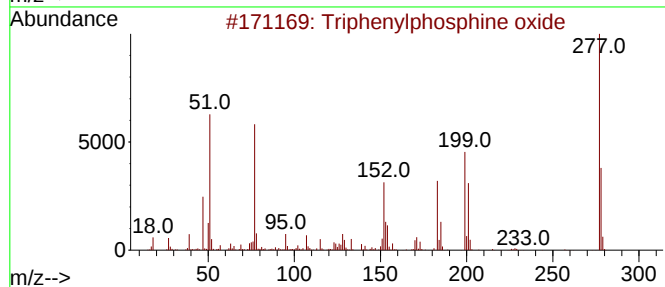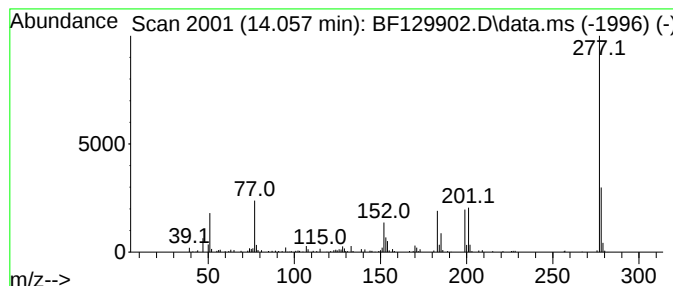

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
Data File : BF129902.D
Acq On : 19 Aug 2022 09:43
Operator : CG\JU
Sample : PB146929BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146929BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.057	3.3	ng	172910	5	13.975	1063090	20.0