
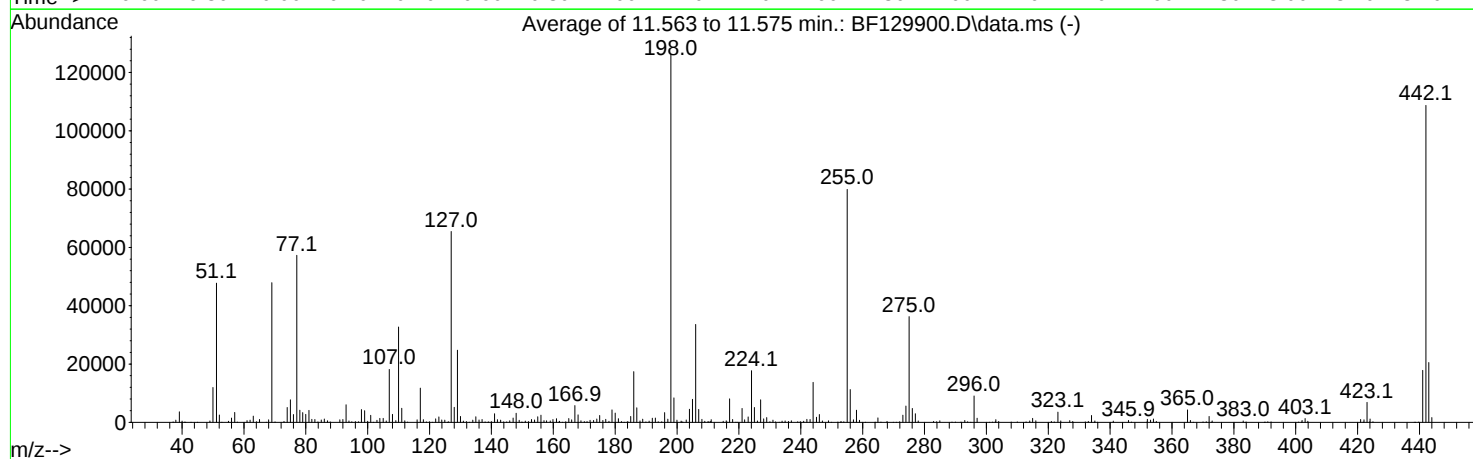


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
 Data File : BF129900.D
 Acq On : 19 Aug 2022 08:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 20 07:47:33 2022

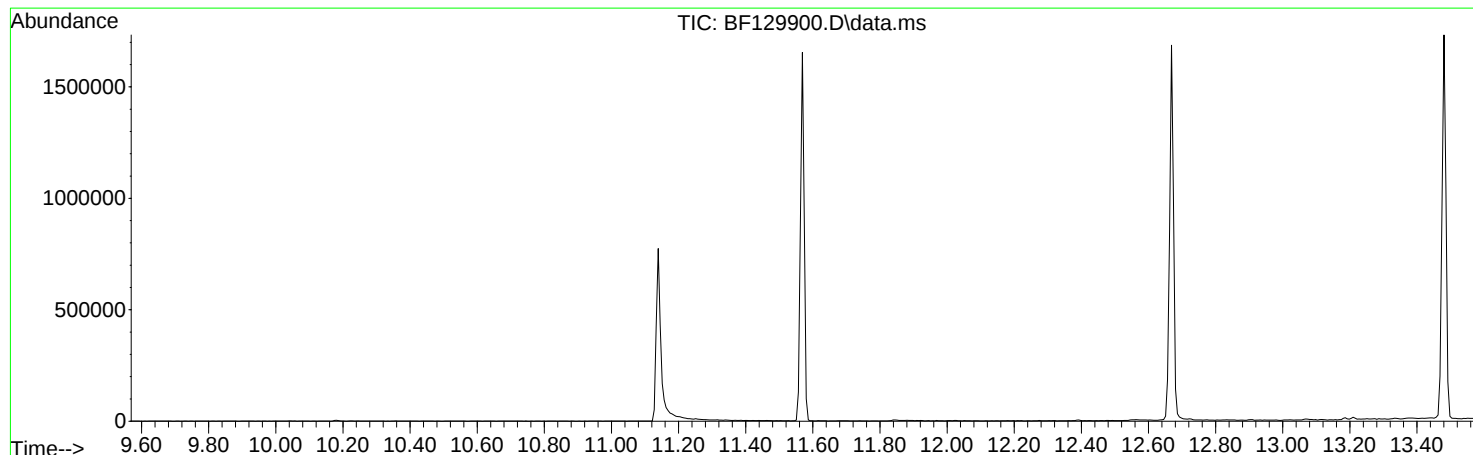

AutoFind: Scans 1577, 1578, 1579; Background Corrected with Scan 1572

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	47773	PASS
68	69	0.00	2	1.8	877	PASS
69	198	0.00	100	38.0	47896	PASS
70	69	0.00	2	0.4	197	PASS
127	198	10	80	51.9	65467	PASS
197	198	0.00	2	0.9	1083	PASS
198	198	100	100	100.0	126168	PASS
199	198	5	9	6.6	8377	PASS
275	198	10	60	28.8	36296	PASS
365	198	1	100	3.4	4279	PASS
441	198	0.01	100	14.1	17824	PASS
442	442	50	100	100.0	108733	PASS
443	442	15	24	18.9	20524	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
8/19/2022	BNA_F	<u>BF129900.D</u>
Compound Name	Response	Retention Time
DDT	276033	13.48
DDD	4160	13.21
DDE	660	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4820	280853	1.72

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
Data File : BF129900.D
Acq On : 19 Aug 2022 08:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 22 05:28:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 20 07:47:33 2022
Response via : Initial Calibration

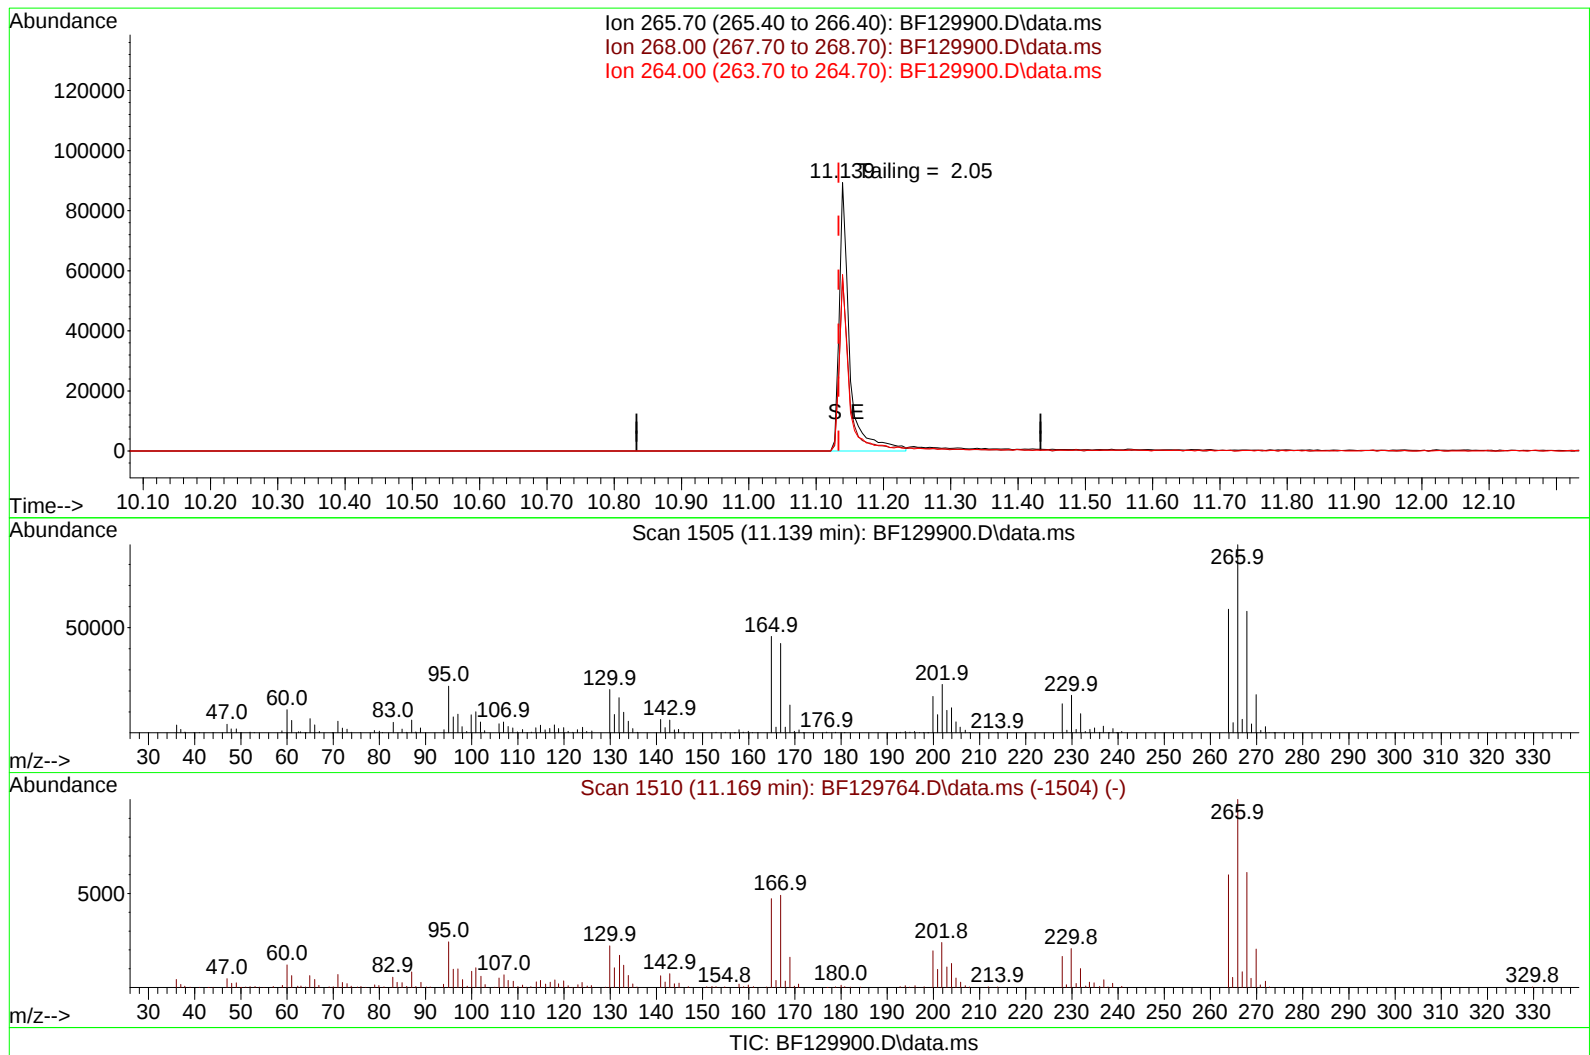

(70) Pentachlorophenol (C)

11.139min (+ 0.006) 170363.13 ng




response 94908

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.68
264.00	59.90	65.72
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\  
Data File : BF129900.D  
Acq On    : 19 Aug 2022  08:41  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 22 05:28:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 20 07:47:33 2022
Response via : Initial Calibration

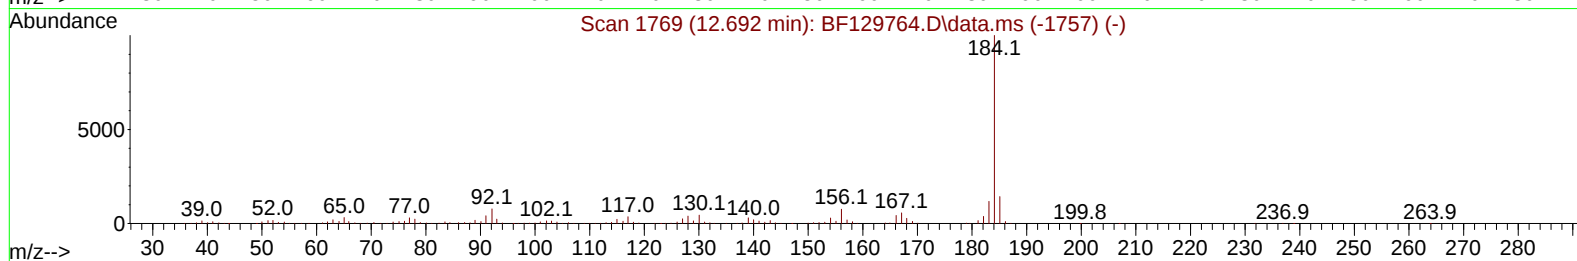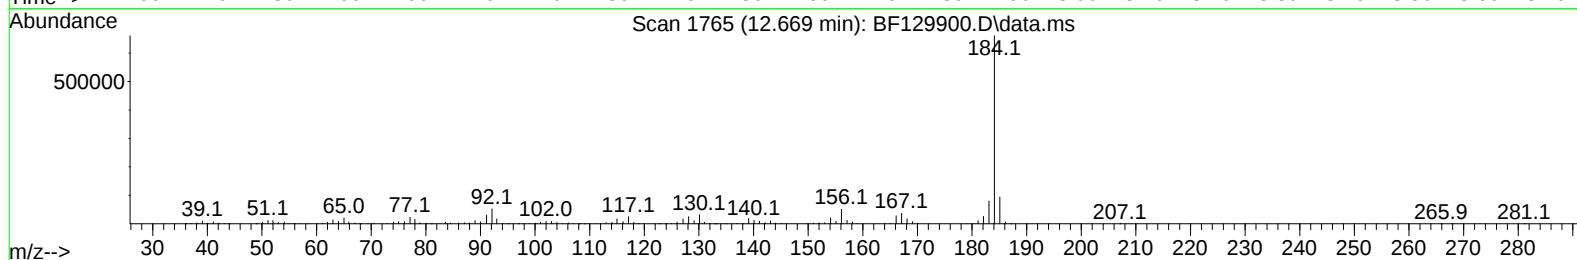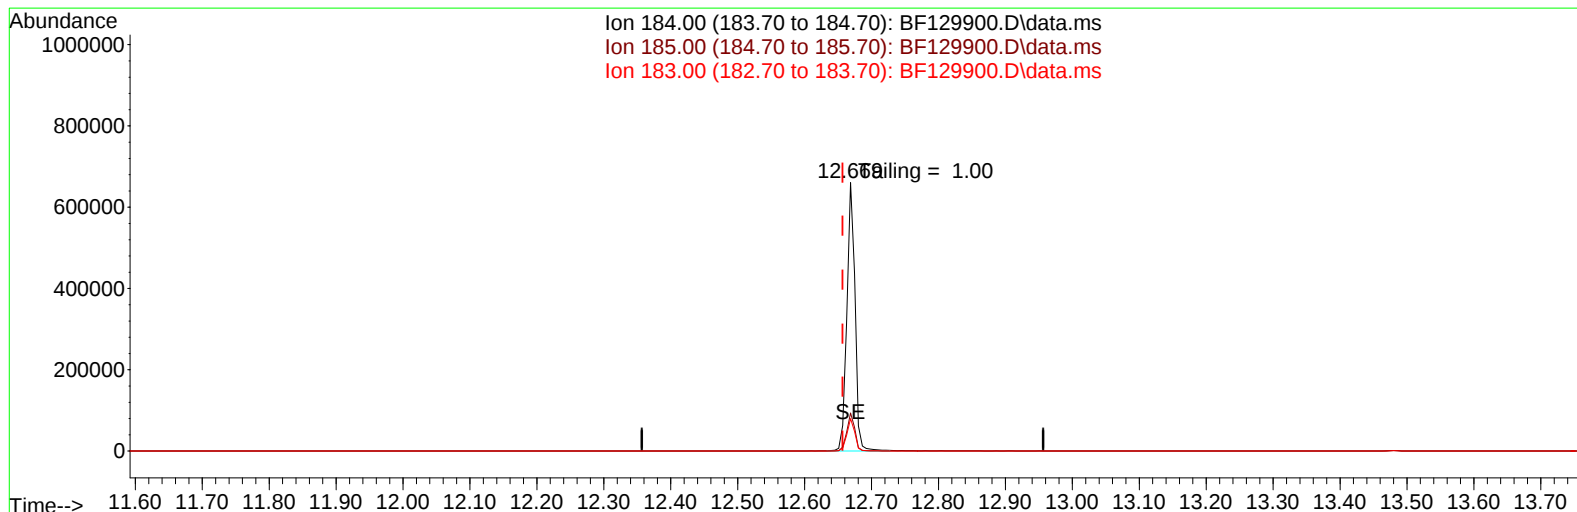

TIC: BF129900.D\data.ms

(77) Benzidine

12.669min (+ 0.012) 71470.89 ng

response **560723**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.20
183.00	11.80	12.07
0.00	0.00	0.00