


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
Data File : BF129913.D
Acq On : 19 Aug 2022 17:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 20 07:47:33 2022

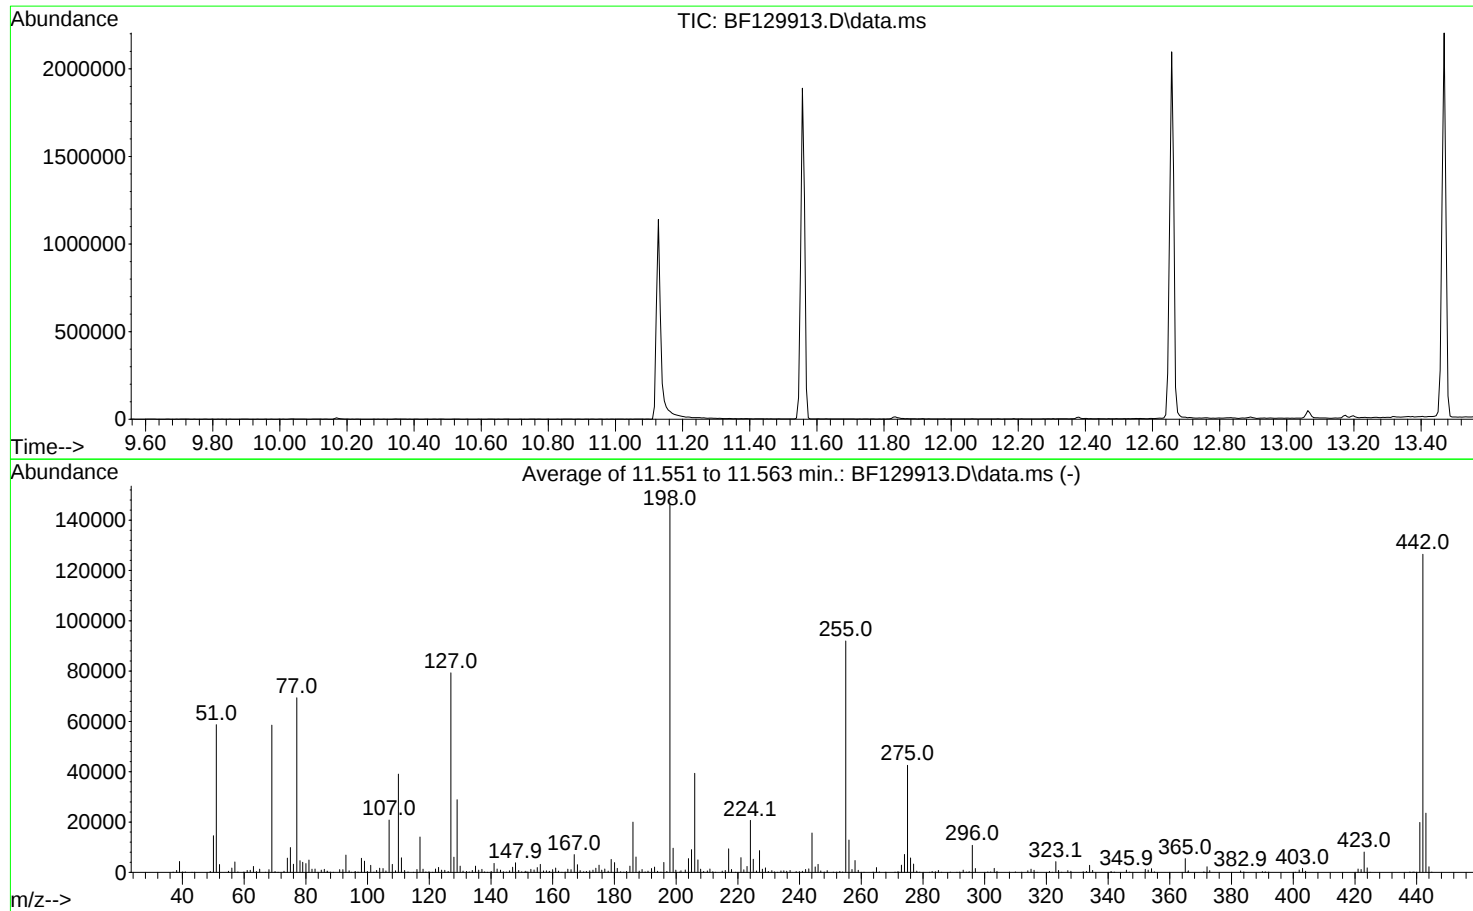

AutoFind: Scans 1575, 1576, 1577; Background Corrected with Scan 1570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	58699	PASS
68	69	0.00	2	1.8	1072	PASS
69	198	0.00	100	40.0	58525	PASS
70	69	0.00	2	0.5	321	PASS
127	198	10	80	54.3	79331	PASS
197	198	0.00	2	0.3	392	PASS
198	198	100	100	100.0	146219	PASS
199	198	5	9	6.6	9586	PASS
275	198	10	60	29.1	42560	PASS
365	198	1	100	3.7	5483	PASS
441	198	0.01	100	13.6	19827	PASS
442	442	50	100	100.0	126411	PASS
443	442	15	24	18.6	23531	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/19/2022	BNA_F	<u>BF129913.D</u>
Compound Name	Response	Retention Time
DDT	337348	13.469
DDD	5295	13.175
DDE	336	12.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5631	342979	1.64

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
Data File : BF129913.D
Acq On : 19 Aug 2022 17:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 22 05:31:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 20 07:47:33 2022
Response via : Initial Calibration

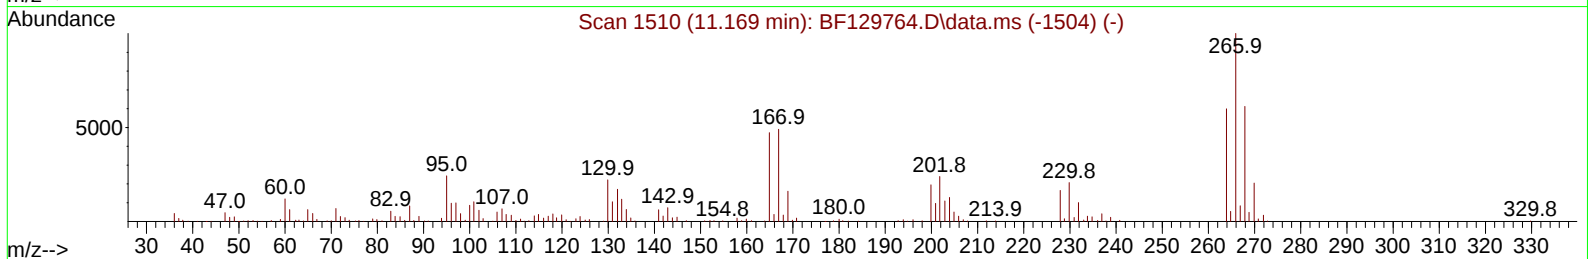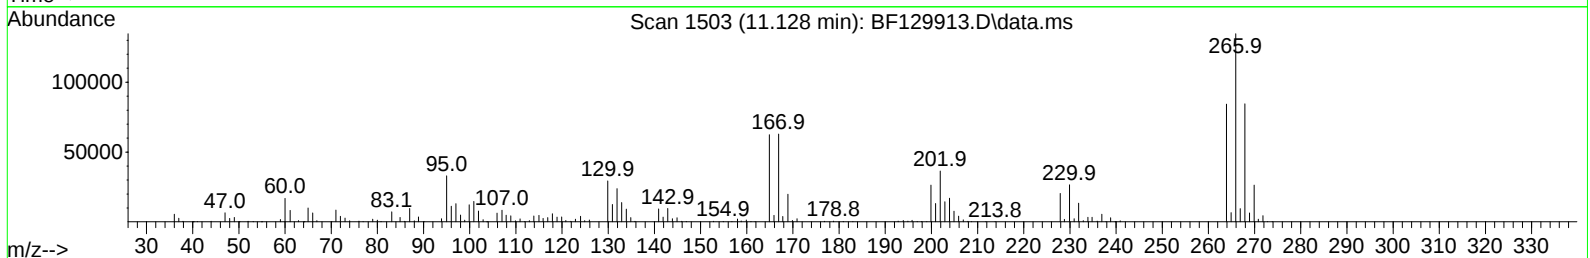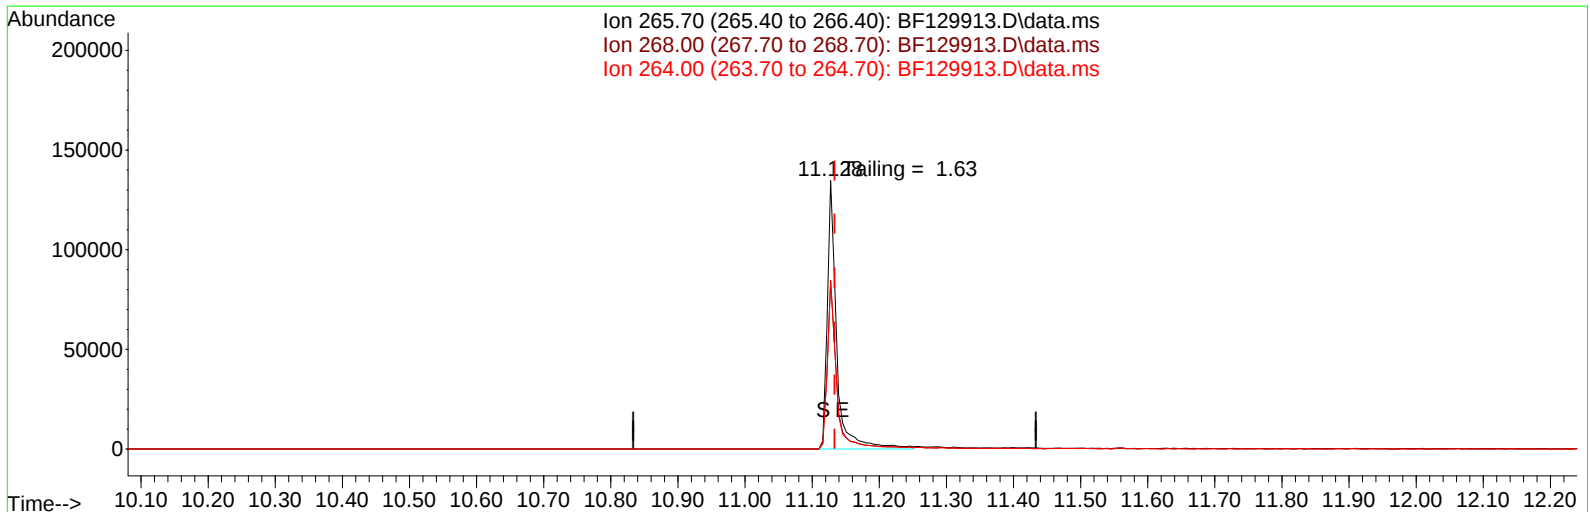

TIC: BF129913.D\data.ms

(70) Pentachlorophenol (C)

11.128min (-0.006) 371759.48 ng




response 131521

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.79
264.00	59.90	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081922\
Data File : BF129913.D
Acq On : 19 Aug 2022 17:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 22 05:31:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 20 07:47:33 2022
Response via : Initial Calibration

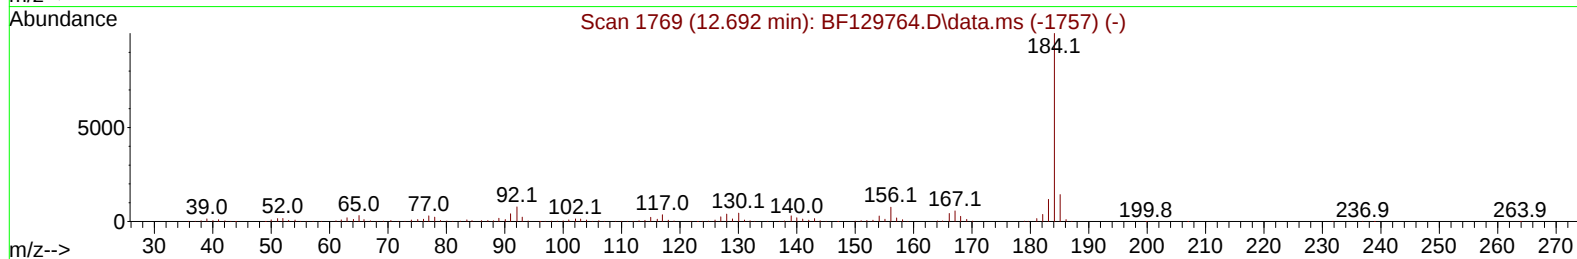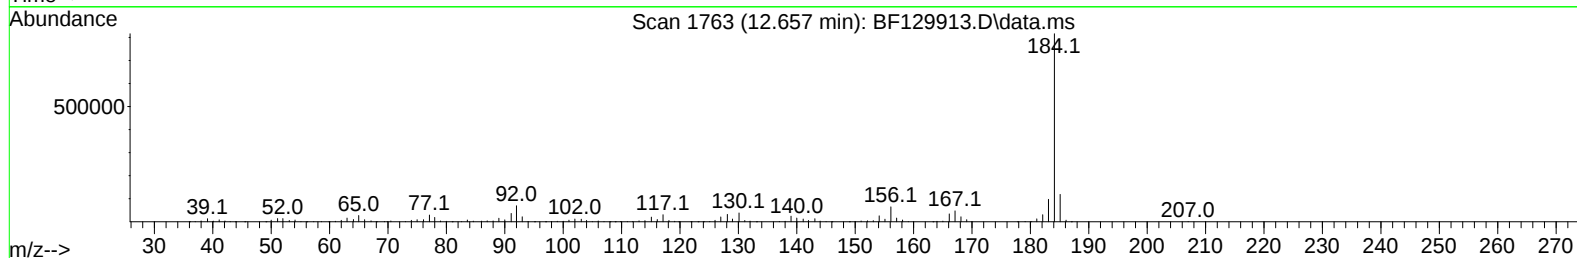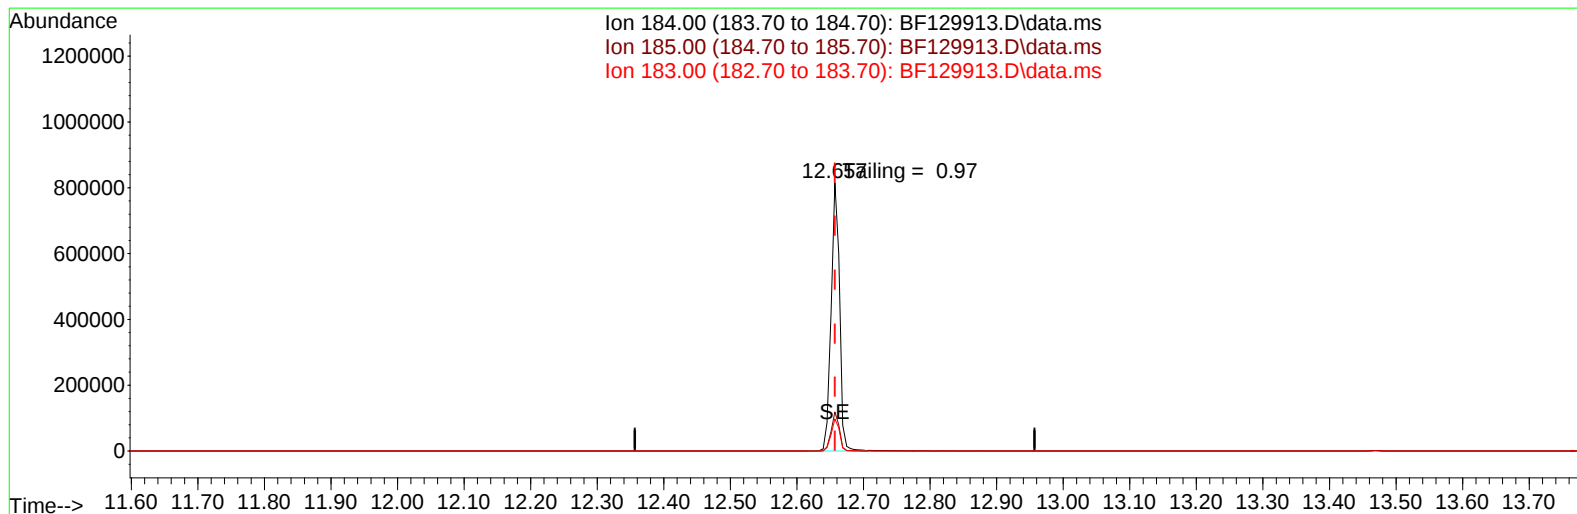

TIC: BF129913.D\data.ms

(77) Benzidine

12.657min (+ 0.000) 37835.47 ng

response 726546

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.55
183.00	11.80	11.97
0.00	0.00	0.00