
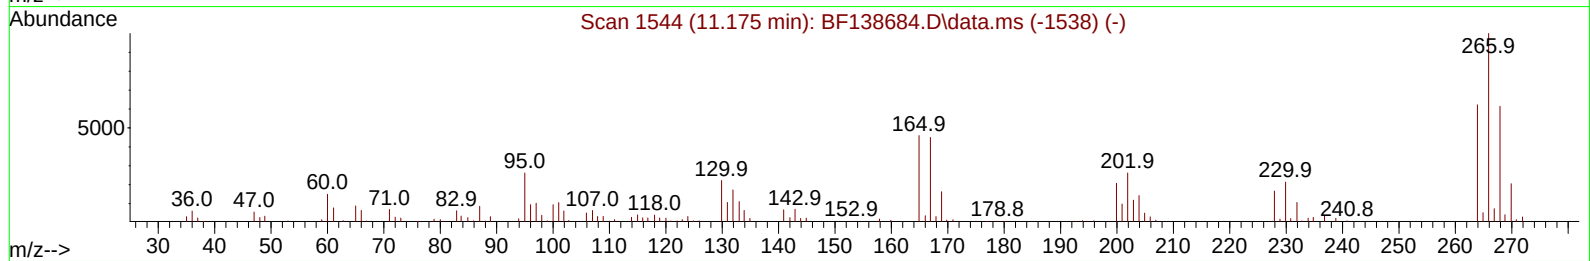
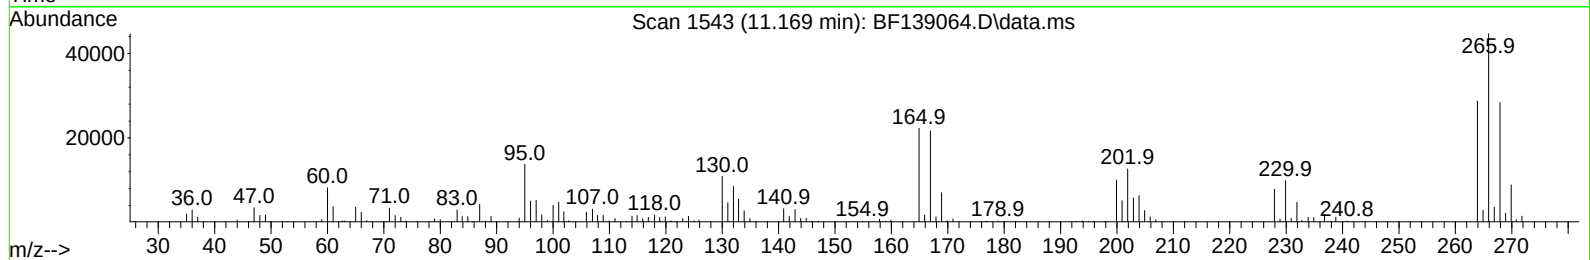


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081924\
Data File : BF139064.D
Acq On : 19 Aug 2024 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 11:09:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

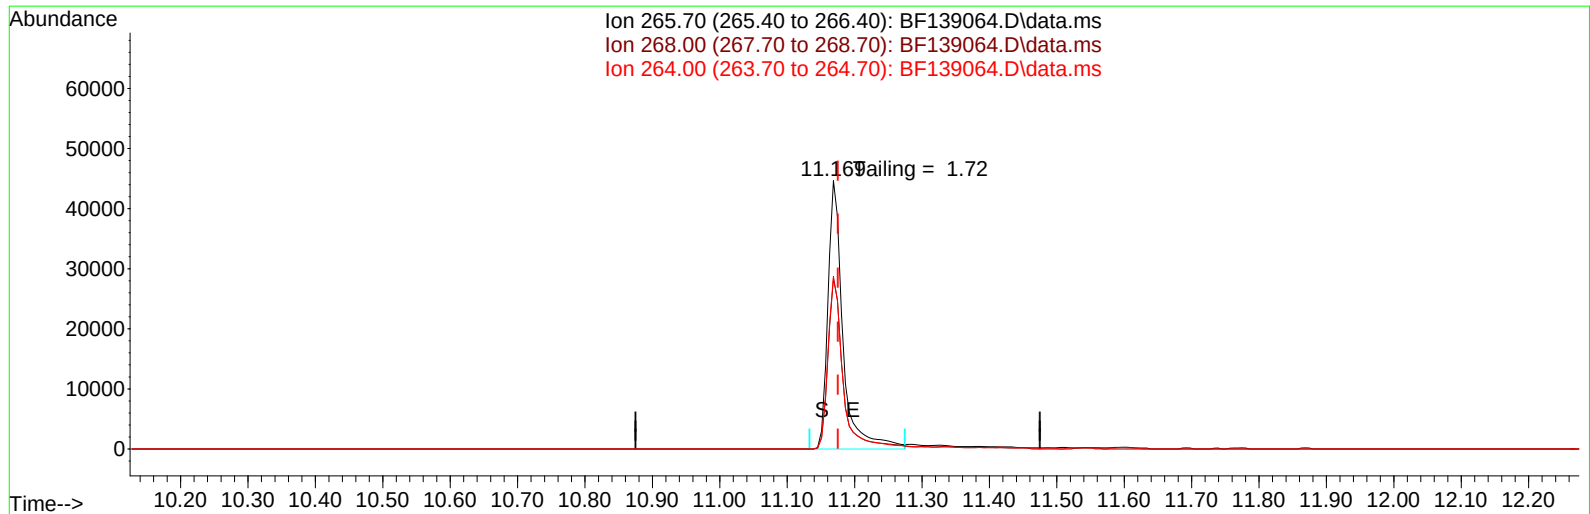

TIC: BF139064.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 65165.03 ng

response 69939

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.57
264.00	62.20	64.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081924\
Data File : BF139064.D
Acq On : 19 Aug 2024 08:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 11:09:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

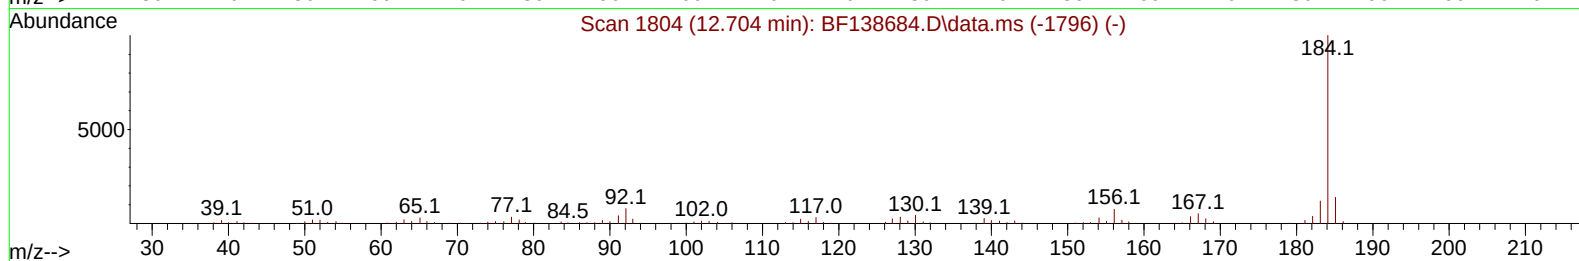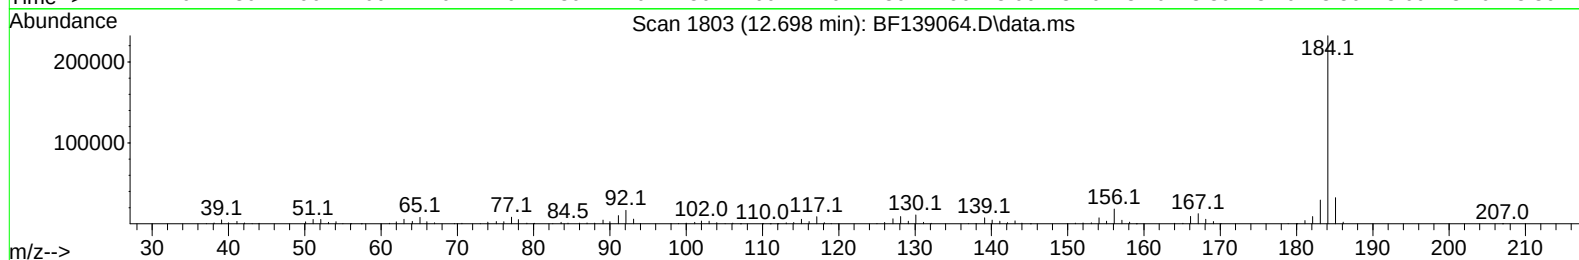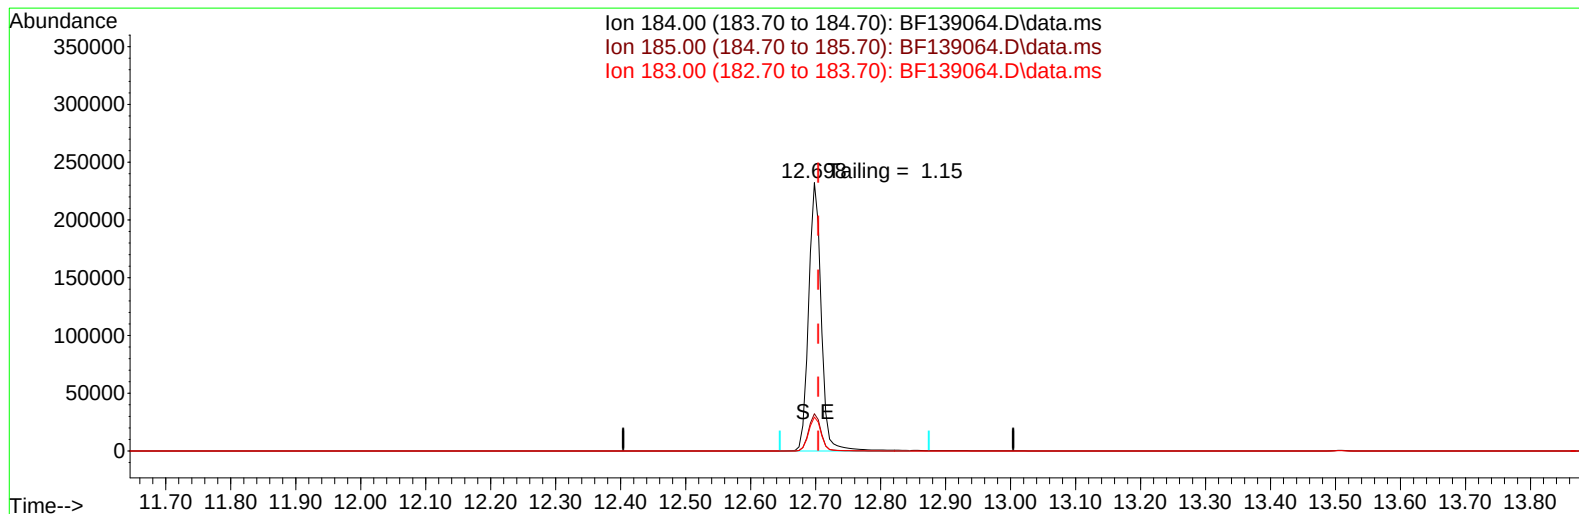

TIC: BF139064.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng m

response 313382

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.94
183.00	12.00	12.66
0.00	0.00	0.00