
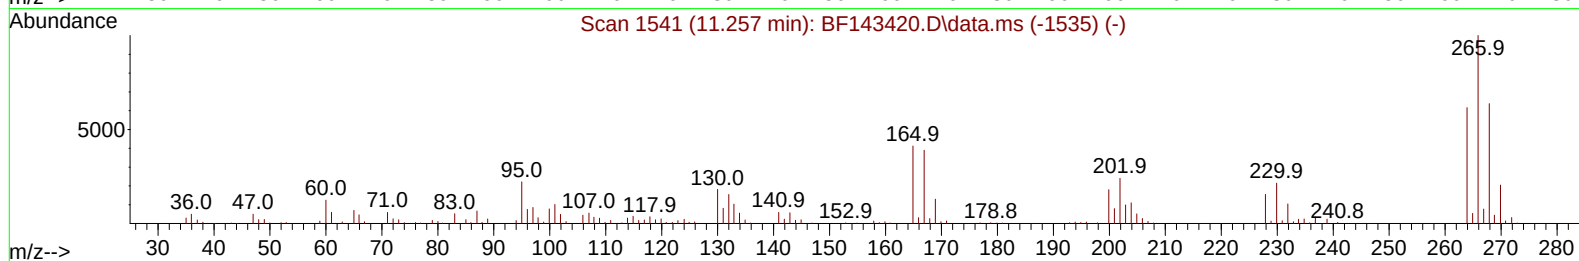
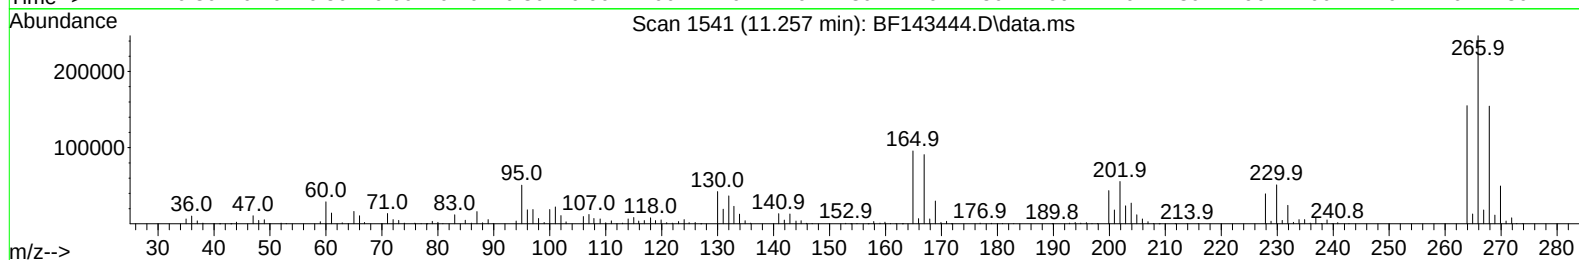


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143444.D
Acq On : 19 Aug 2025 08:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 12:05:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 18 04:40:19 2025
Response via : Initial Calibration

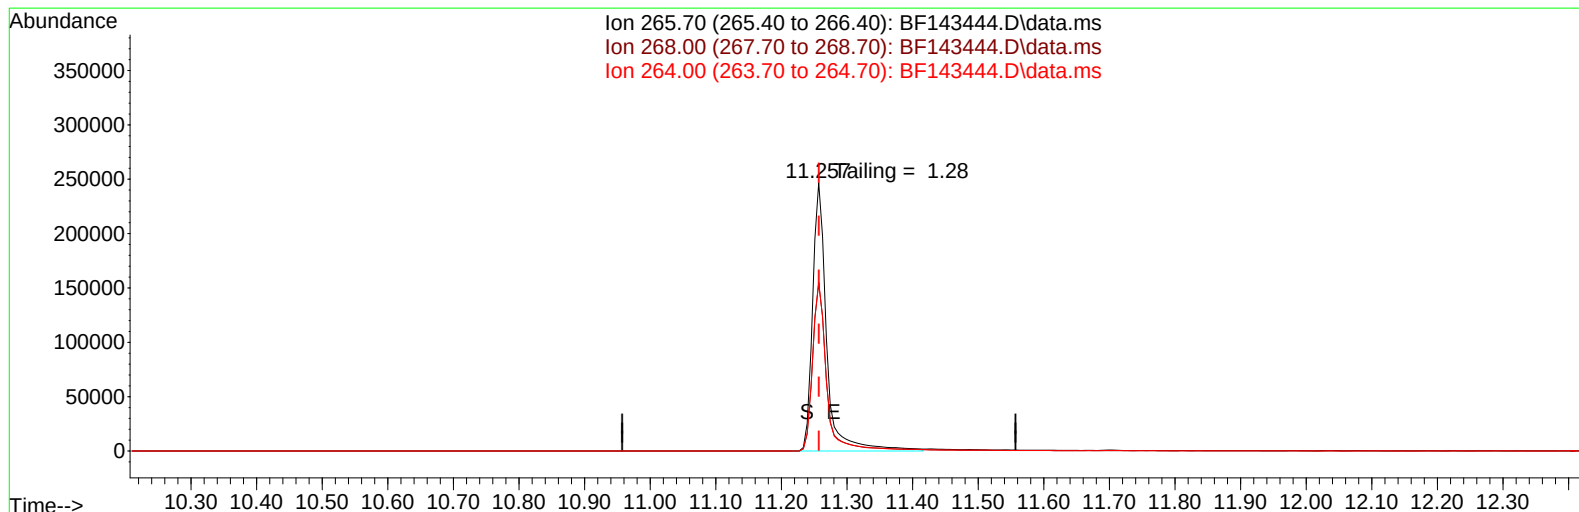

TIC: BF143444.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.000) 503335.09 ng

response 372359

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.61
264.00	61.60	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143444.D
Acq On : 19 Aug 2025 08:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 12:05:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 18 04:40:19 2025
Response via : Initial Calibration

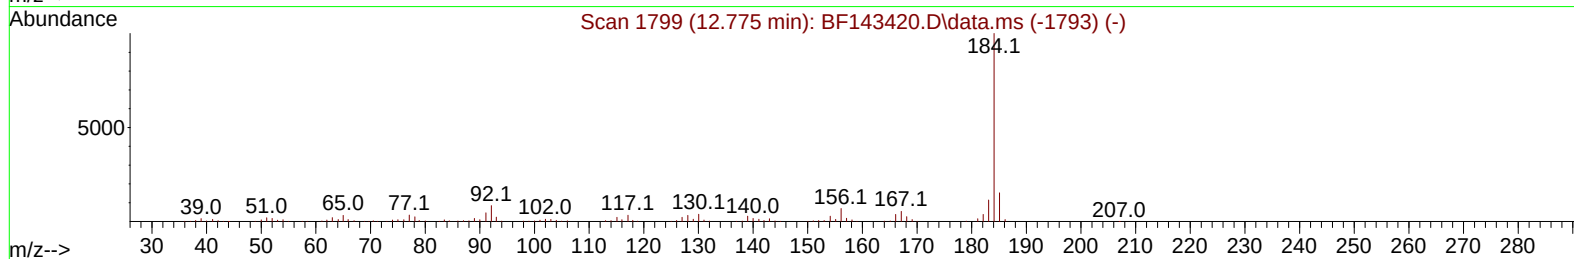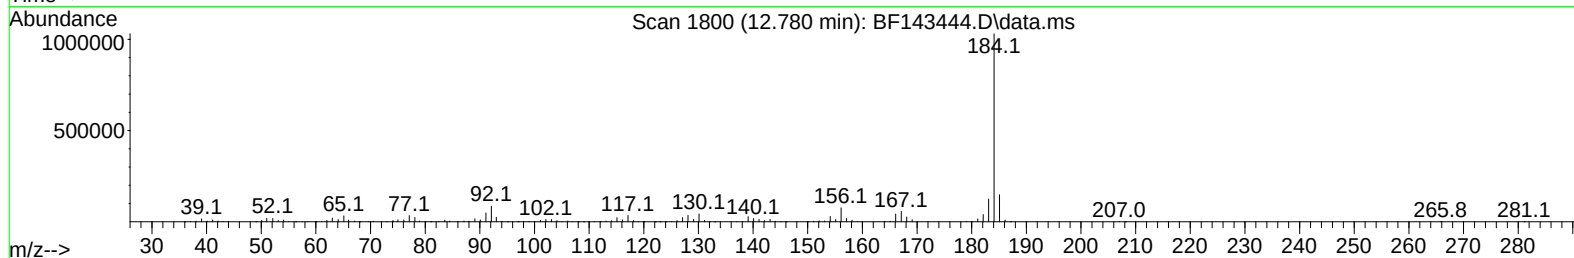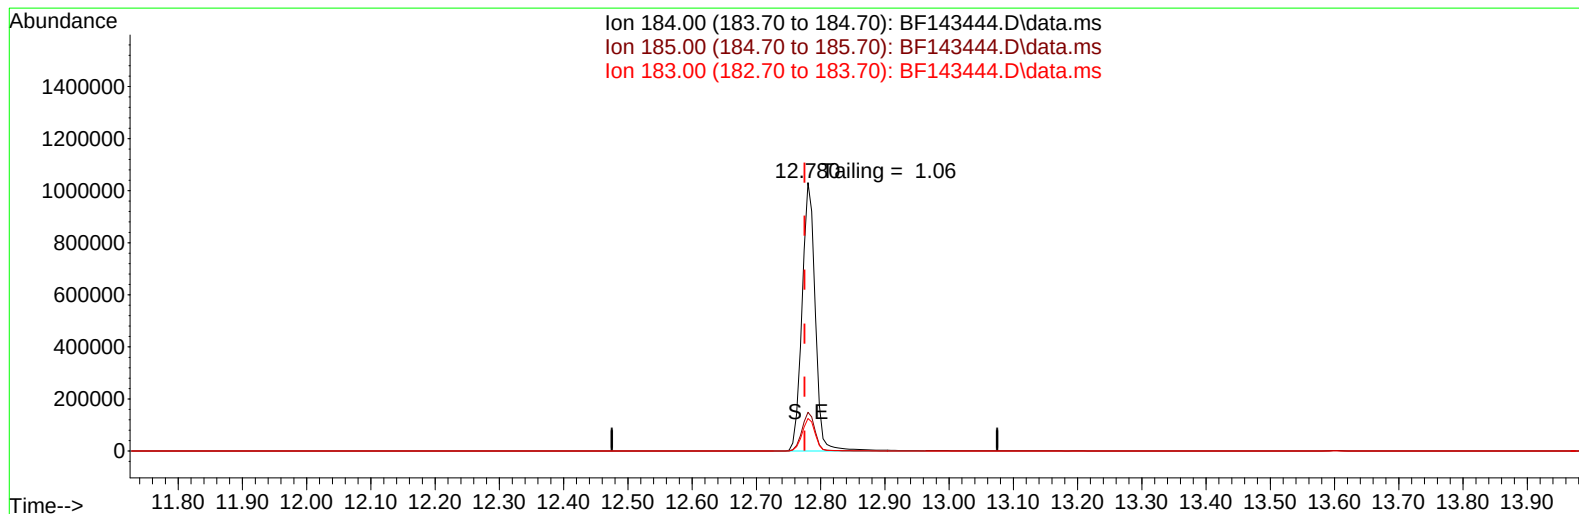

TIC: BF143444.D\data.ms

(77) Benzidine

12.780min (+ 0.005) 257789.28 ng

response 1485742

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.41
183.00	11.50	12.11
0.00	0.00	0.00