

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
 Data File : BF143453.D
 Acq On : 19 Aug 2025 13:30
 Operator : RC/JU
 Sample : Q2879-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP05-081425

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.228	3	6	15	rVB	509327	749943	16.15%	2.069%
2	5.151	495	503	515	rVB	114410	177613	3.83%	0.490%
3	5.563	567	573	592	rBV	1072618	1488914	32.07%	4.109%
4	6.557	737	742	753	rBV	1049338	1370329	29.51%	3.781%
5	6.928	799	805	815	rBV	436306	554083	11.93%	1.529%
6	7.481	893	899	909	rBV	740696	949587	20.45%	2.620%
7	8.204	1015	1022	1030	rBV	494183	646267	13.92%	1.783%
8	9.275	1199	1204	1213	rBV	1157105	1477787	31.83%	4.078%
9	9.957	1315	1320	1325	rBV	482565	630654	13.58%	1.740%
10	10.257	1366	1371	1381	rBV	137126	181251	3.90%	0.500%
11	10.669	1436	1441	1447	rBV	130793	179643	3.87%	0.496%
12	10.745	1449	1454	1460	rBV	715802	951403	20.49%	2.625%
13	10.804	1460	1464	1469	rVB2	31822	62704	1.35%	0.173%
14	10.980	1490	1494	1499	rVB2	51168	72616	1.56%	0.200%
15	11.445	1568	1573	1580	rBV2	548138	972187	20.94%	2.683%
16	11.580	1592	1596	1600	rVB	157920	193896	4.18%	0.535%
17	11.675	1607	1612	1619	rBV2	29401	54342	1.17%	0.150%
18	11.974	1658	1663	1674	rVV3	425409	720642	15.52%	1.989%
19	12.063	1674	1678	1685	rVB	54345	95937	2.07%	0.265%
20	12.145	1689	1692	1697	rVB3	56039	81367	1.75%	0.225%
21	12.498	1749	1752	1756	rBV2	38894	59653	1.28%	0.165%
22	12.592	1764	1768	1775	rBV2	101980	176260	3.80%	0.486%
23	12.663	1775	1780	1792	rBV2	517454	1320409	28.44%	3.644%
24	12.757	1793	1796	1804	rVB	108517	168471	3.63%	0.465%
25	12.886	1812	1818	1825	rBV	390138	614658	13.24%	1.696%
26	13.027	1837	1842	1850	rVB	1579782	2018731	43.48%	5.571%
27	13.392	1901	1904	1907	rBV	73671	113384	2.44%	0.313%
28	13.463	1913	1916	1920	rBV3	162541	239934	5.17%	0.662%
29	13.604	1936	1940	1945	rBV2	432184	637923	13.74%	1.760%
30	13.927	1992	1995	2005	rVB2	442765	734599	15.82%	2.027%
31	14.086	2017	2022	2030	rVB2	730546	1242257	26.75%	3.428%
32	14.551	2096	2101	2118	rVB3	492827	1172118	25.24%	3.234%
33	14.933	2163	2166	2172	rVB	315827	430807	9.28%	1.189%
34	15.145	2198	2202	2203	rBV	170229	233706	5.03%	0.645%
35	15.204	2208	2212	2216	rVB	1340687	1835596	39.53%	5.065%
36	15.580	2271	2276	2291	rBV	371184	729583	15.71%	2.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143453.D
Acq On : 19 Aug 2025 13:30
Operator : RC/JU
Sample : Q2879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP05-081425

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.045	2349	2355	2361	rVB	1028034	1777601	38.28%	4.905%
38	16.327	2399	2403	2417	rVB2	339007	727476	15.67%	2.007%
39	17.756	2632	2646	2656	rBV4	1108848	4643323	100.00%	12.813%
40	17.933	2672	2676	2684	rVB	336550	733344	15.79%	2.024%
41	18.198	2714	2721	2731	rBV	632382	2122680	45.71%	5.858%
42	18.562	2775	2783	2802	rBV7	515791	2894409	62.33%	7.987%




Sum of corrected areas: 36238087

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143453.D
Acq On : 19 Aug 2025 13:30
Operator : RC/JU
Sample : Q2879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP05-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

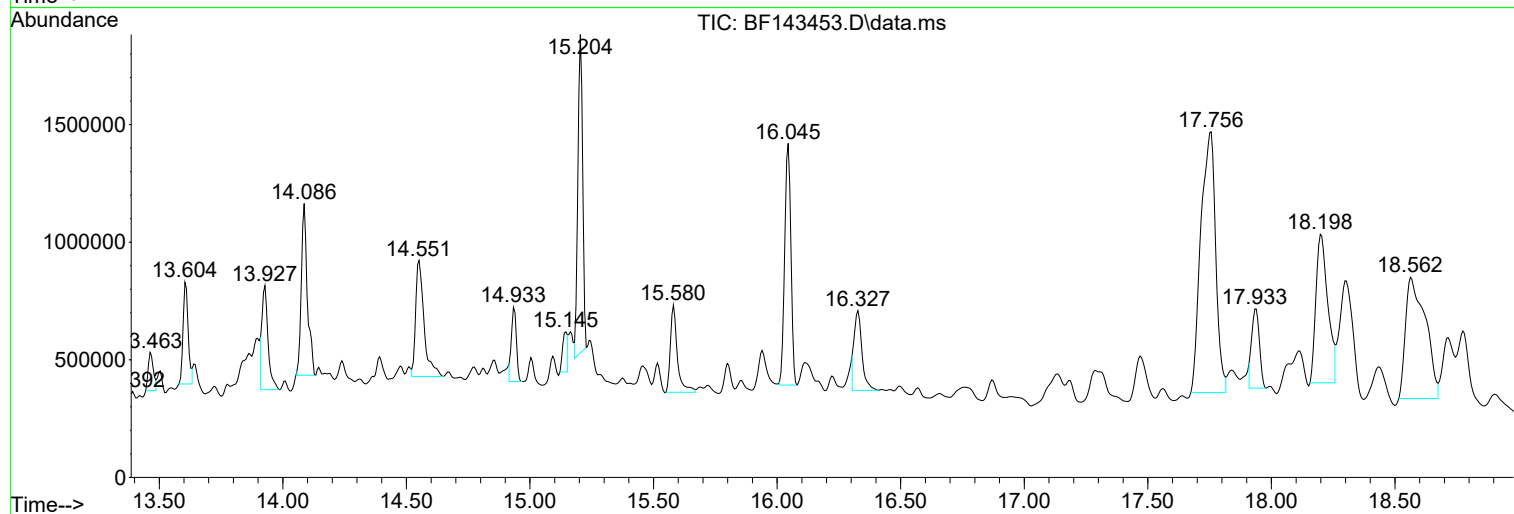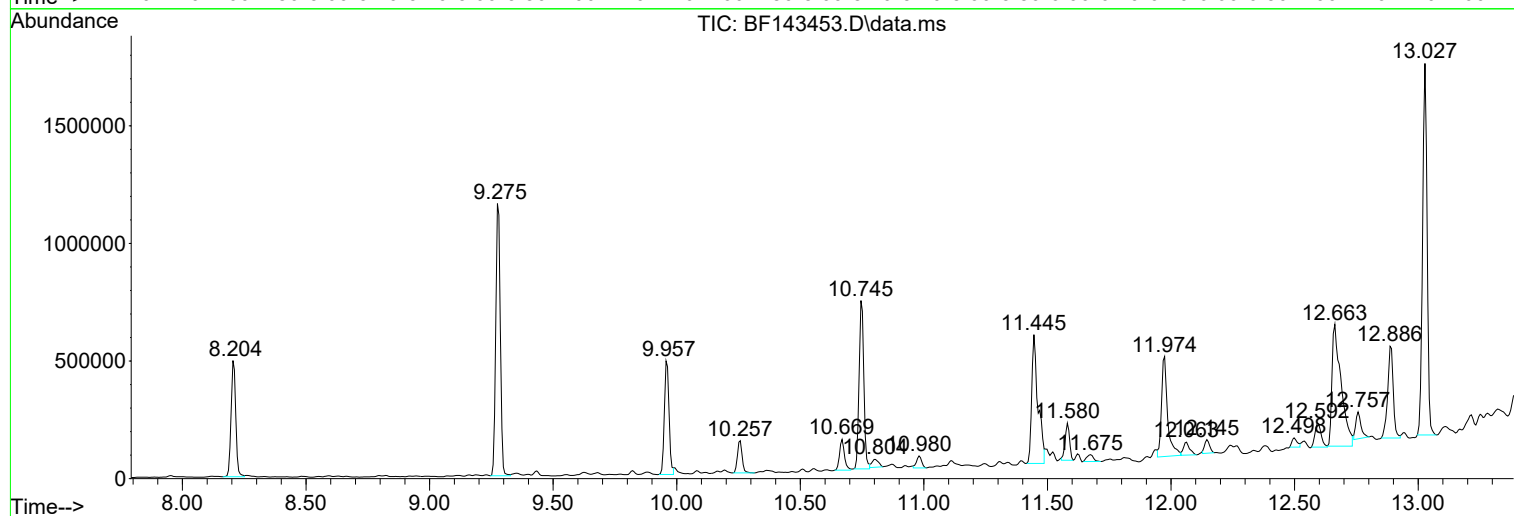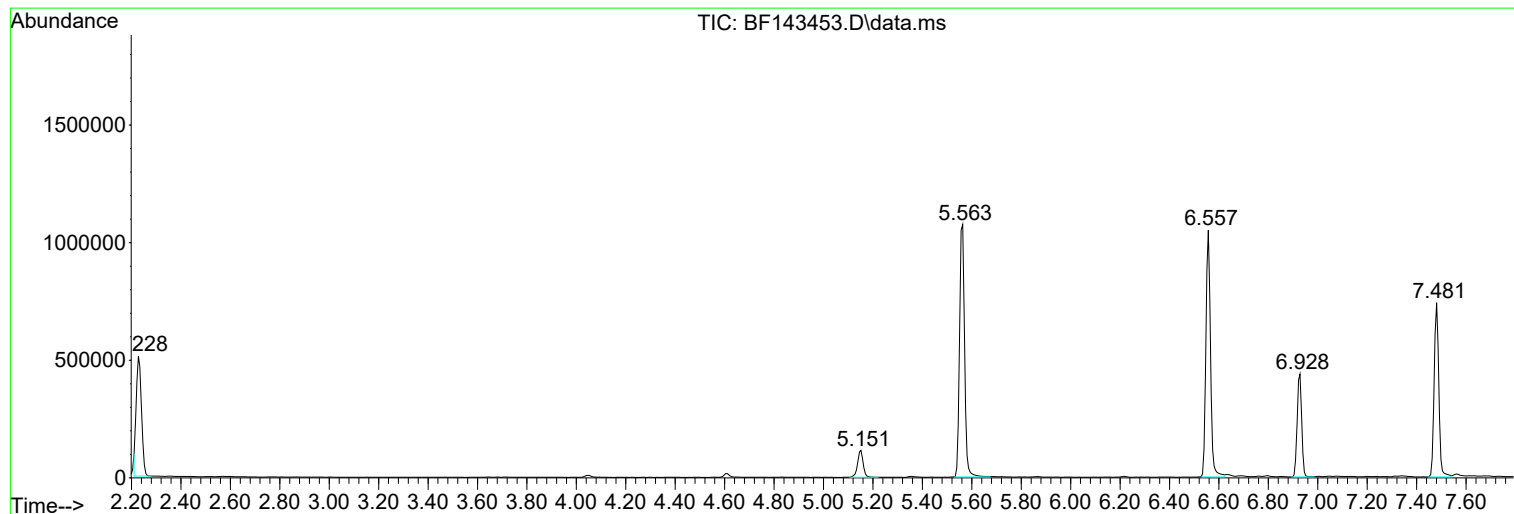

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143453.D
Acq On : 19 Aug 2025 13:30
Operator : RC/JU
Sample : Q2879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP05-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143453.D
Acq On : 19 Aug 2025 13:30
Operator : RC/JU
Sample : Q2879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP05-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------