

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
 Data File : BF143457.D
 Acq On : 19 Aug 2025 15:26
 Operator : RC/JU
 Sample : Q2879-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP09-081425

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.234	3	7	17	rVB	469209	727241	17.68%	2.572%
2	5.151	494	503	514	rBV2	88779	134269	3.26%	0.475%
3	5.563	568	573	587	rBV	848361	1128938	27.44%	3.992%
4	6.563	737	743	754	rBV	769034	1060025	25.77%	3.749%
5	6.928	800	805	812	rBV	534978	658145	16.00%	2.327%
6	7.481	894	899	910	rBV	522356	676192	16.44%	2.391%
7	8.210	1015	1023	1030	rBV	572961	741333	18.02%	2.622%
8	9.281	1199	1205	1212	rBV	912139	1153503	28.04%	4.079%
9	9.963	1315	1321	1337	rBV	570021	760621	18.49%	2.690%
10	10.669	1437	1441	1446	rBV	85613	115950	2.82%	0.410%
11	10.751	1450	1455	1464	rVB	497116	661045	16.07%	2.338%
12	10.986	1491	1495	1499	rVB2	42621	57691	1.40%	0.204%
13	11.445	1568	1573	1580	rBV	577057	886952	21.56%	3.137%
14	11.498	1580	1582	1585	rVB	50852	52934	1.29%	0.187%
15	11.974	1658	1663	1674	rVV2	329842	528192	12.84%	1.868%
16	12.145	1689	1692	1701	rVB5	39653	67791	1.65%	0.240%
17	12.592	1763	1768	1775	rBV	149678	228953	5.57%	0.810%
18	12.663	1776	1780	1792	rBV2	247854	624162	15.17%	2.207%
19	12.757	1793	1796	1804	rVB	98378	151789	3.69%	0.537%
20	12.892	1815	1819	1825	rVB	157464	214066	5.20%	0.757%
21	13.027	1837	1842	1850	rBV	1133101	1471841	35.78%	5.205%
22	13.392	1900	1904	1909	rBV2	160754	286531	6.96%	1.013%
23	13.469	1914	1917	1921	rVB3	101282	164733	4.00%	0.583%
24	13.898	1986	1990	1991	rBV2	186246	248862	6.05%	0.880%
25	14.092	2018	2023	2030	rVB2	591644	919073	22.34%	3.250%
26	14.551	2097	2101	2108	rBV2	493435	837236	20.35%	2.961%
27	14.939	2163	2167	2174	rVB	381763	542447	13.19%	1.918%
28	15.204	2208	2212	2217	rBV	981463	1392143	33.84%	4.923%
29	15.586	2272	2277	2284	rBV	319180	561261	13.64%	1.985%
30	16.045	2350	2355	2361	rVB	679729	1153742	28.04%	4.080%
31	16.327	2400	2403	2417	rVB	321020	654475	15.91%	2.314%
32	17.756	2633	2646	2657	rBV4	911995	4113929	100.00%	14.548%
33	17.945	2673	2678	2685	rVB	341359	771004	18.74%	2.727%
34	18.204	2715	2722	2733	rBV	611853	1938743	47.13%	6.856%
35	18.568	2776	2784	2802	rBV5	438223	2242684	54.51%	7.931%
36	18.715	2805	2809	2815	rBV3	162642	349441	8.49%	1.236%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143457.D
Acq On : 19 Aug 2025 15:26
Operator : RC/JU
Sample : Q2879-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP09-081425

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 28277937

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143457.D
Acq On : 19 Aug 2025 15:26
Operator : RC/JU
Sample : Q2879-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP09-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

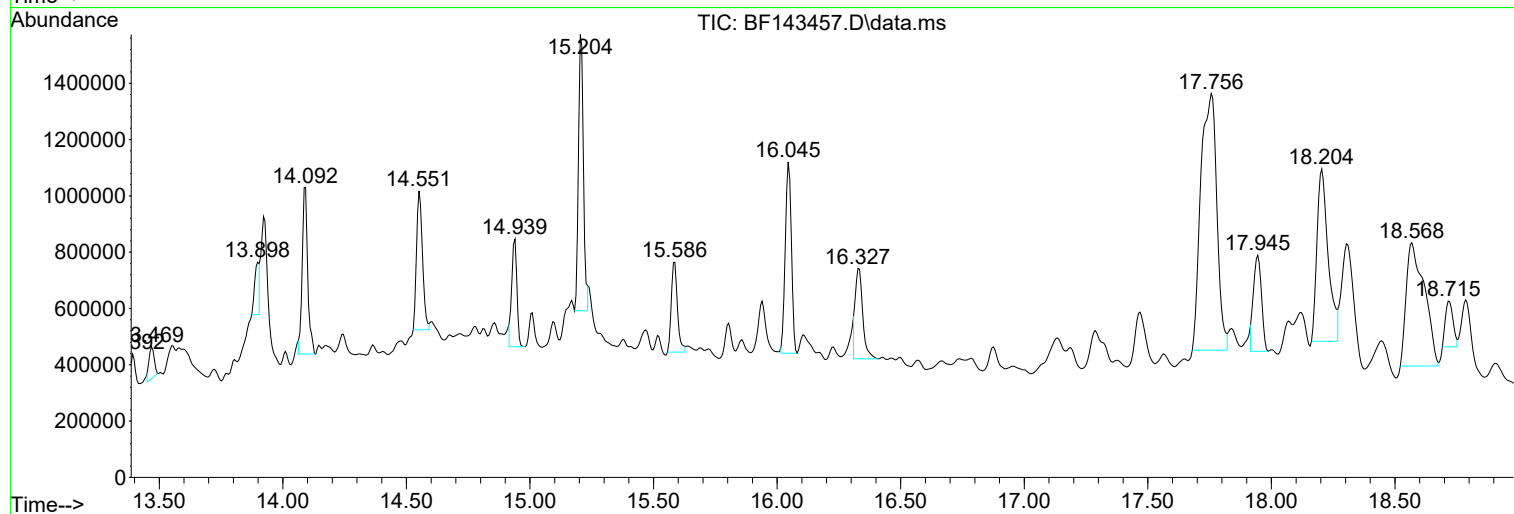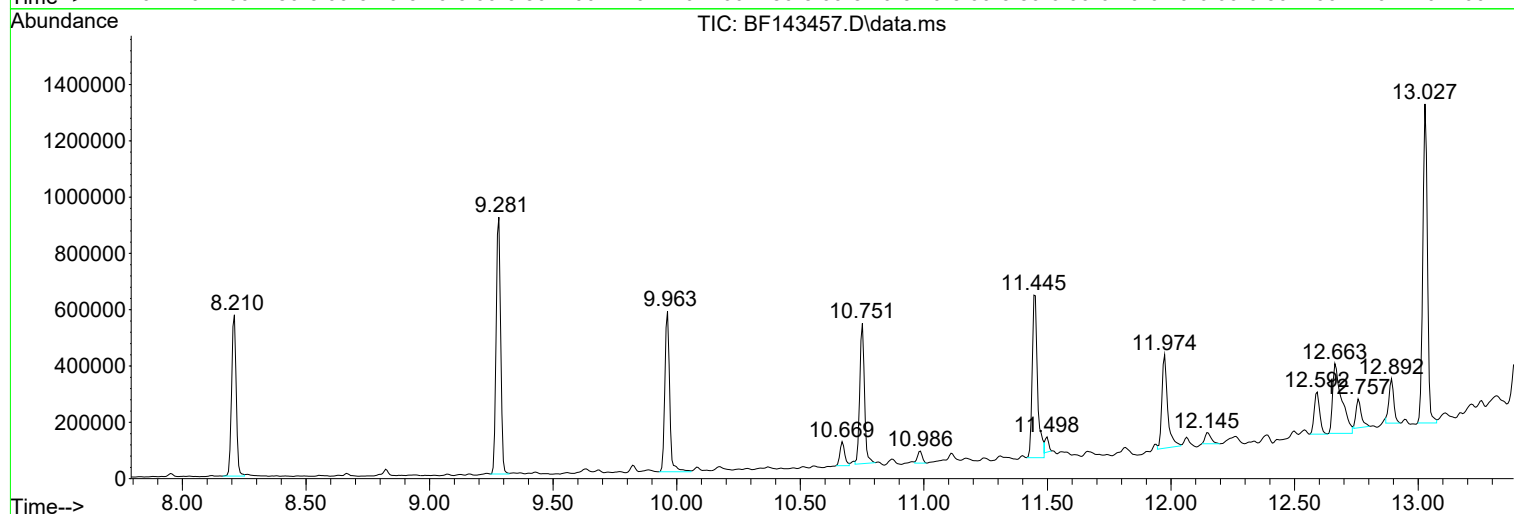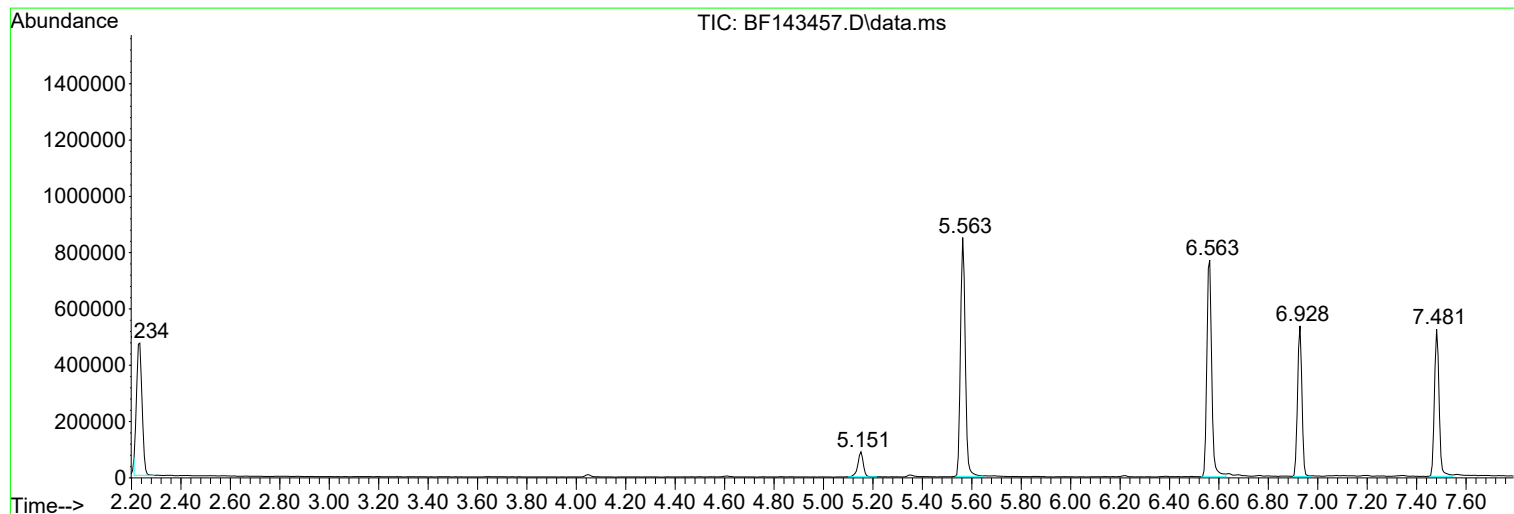

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143457.D
Acq On : 19 Aug 2025 15:26
Operator : RC/JU
Sample : Q2879-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP09-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143457.D
Acq On : 19 Aug 2025 15:26
Operator : RC/JU
Sample : Q2879-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP09-081425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------