
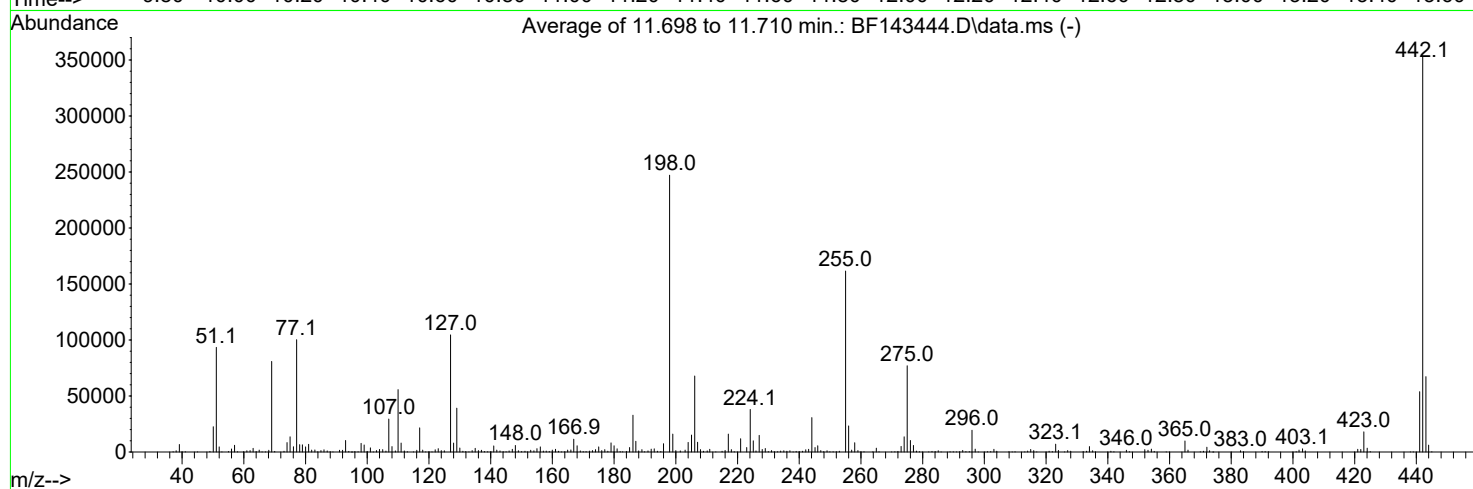


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081925\  
Data File : BF143444.D  
Acq On : 19 Aug 2025 08:39  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081525.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Mon Aug 18 04:40:19 2025

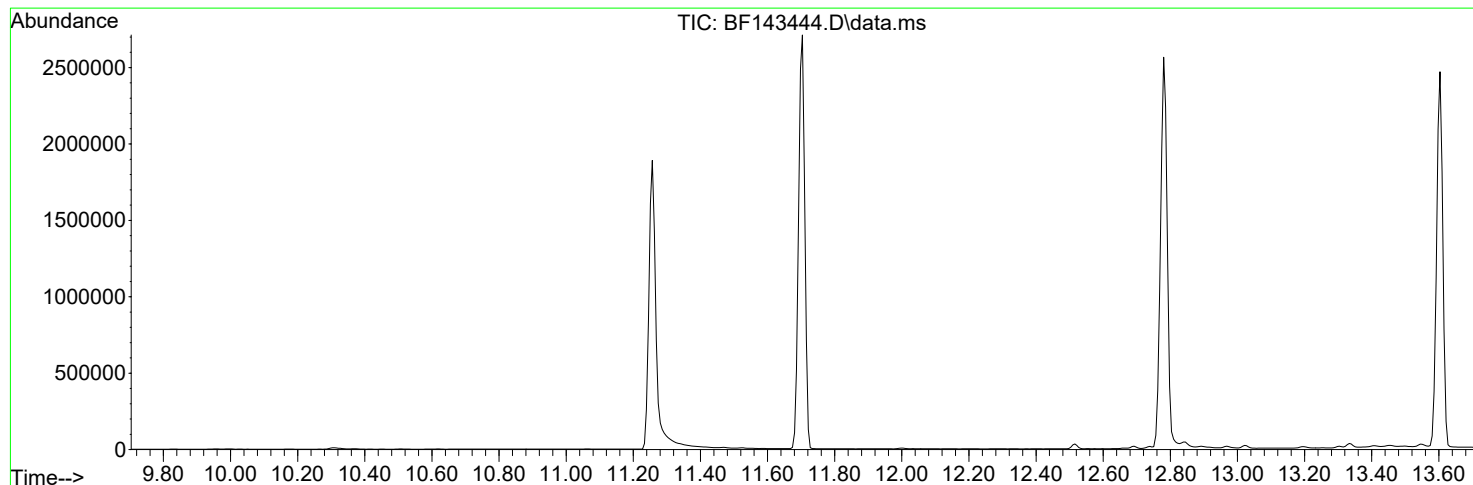

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1609

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 68             | 69              | 0.00            | 2               | 1.9          | 1571       | PASS                |
| 69             | 69              | 100             | 100             | 100.0        | 80784      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 567        | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 247168     | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 16017      | PASS                |
| 365            | 198             | 1               | 100             | 4.0          | 9857       | PASS                |
| 441            | 443             | 0.01            | 150             | 80.1         | 53915      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 352491     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 67315      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/19/2025     | BNA_F            | <u>BF143444.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 634271           | 13.604             |
| DDD           | 11218            | 13.333             |
| DDE           | 3577             | 12.968             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 14795         | 649066           | 2.28               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081925\  
Data File : BF143444.D  
Acq On : 19 Aug 2025 08:39  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 19 12:05:45 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 18 04:40:19 2025  
Response via : Initial Calibration

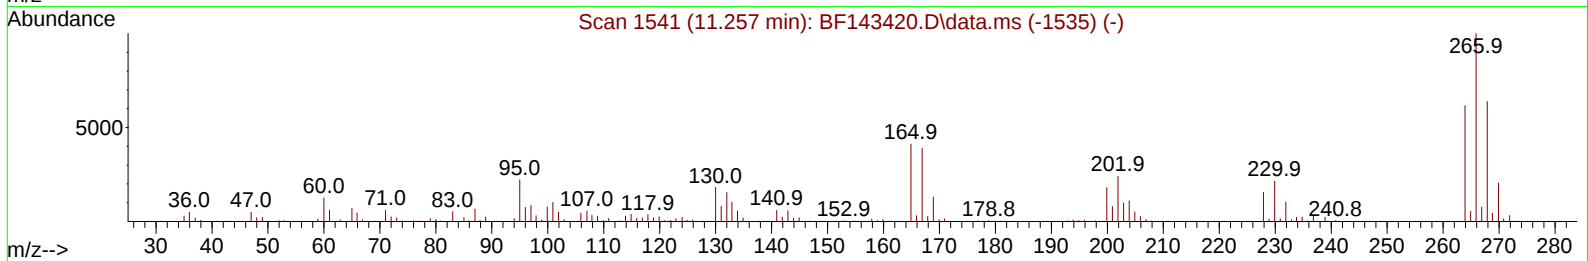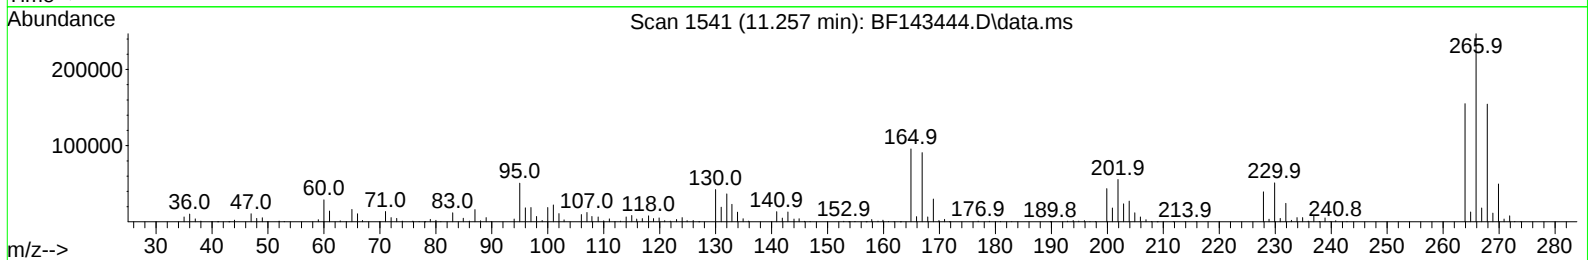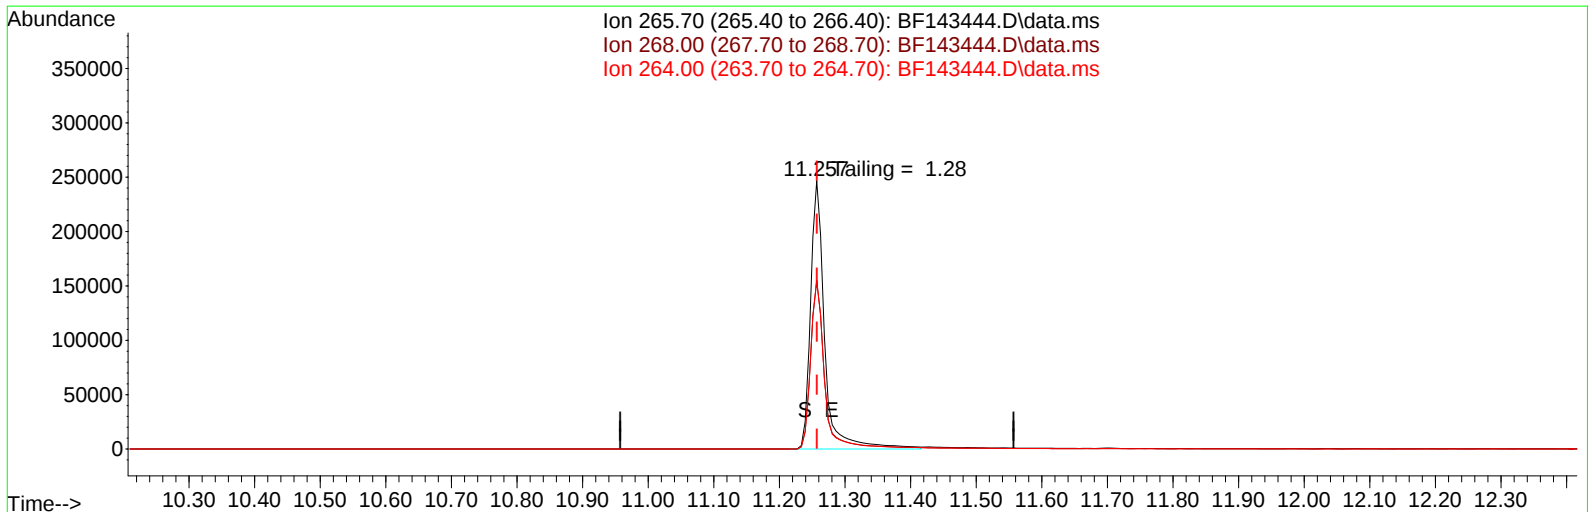

TIC: BF143444.D\data.ms

**(70) Pentachlorophenol (C)**

**11.257min (-0.000) 503335.09 ng**




**response 372359**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 62.61  |
| 264.00 | 61.60  | 62.87  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081925\  
Data File : BF143444.D  
Acq On : 19 Aug 2025 08:39  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 19 12:05:45 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 18 04:40:19 2025  
Response via : Initial Calibration

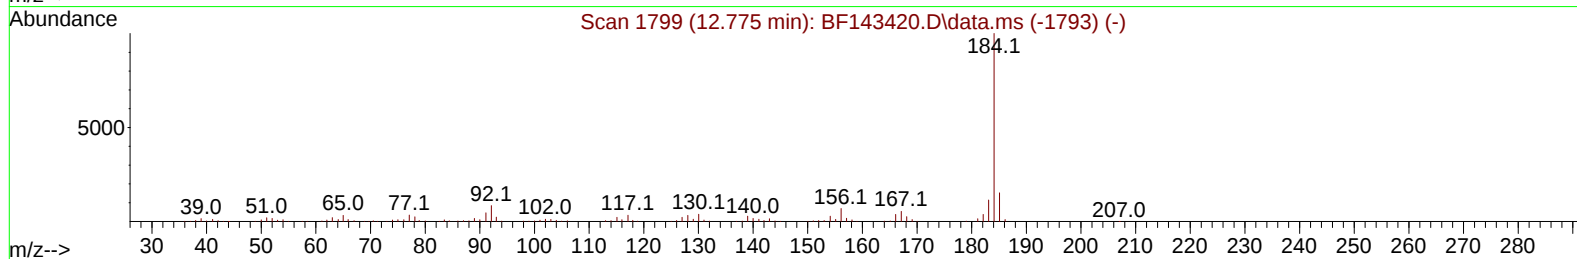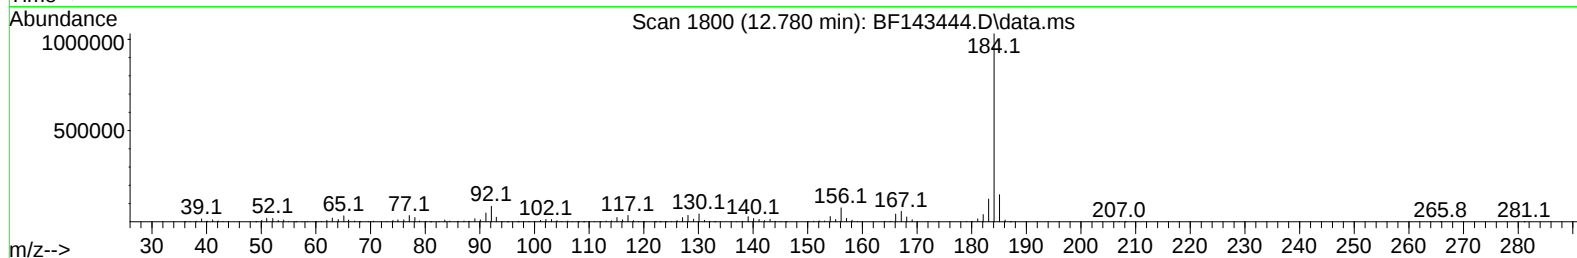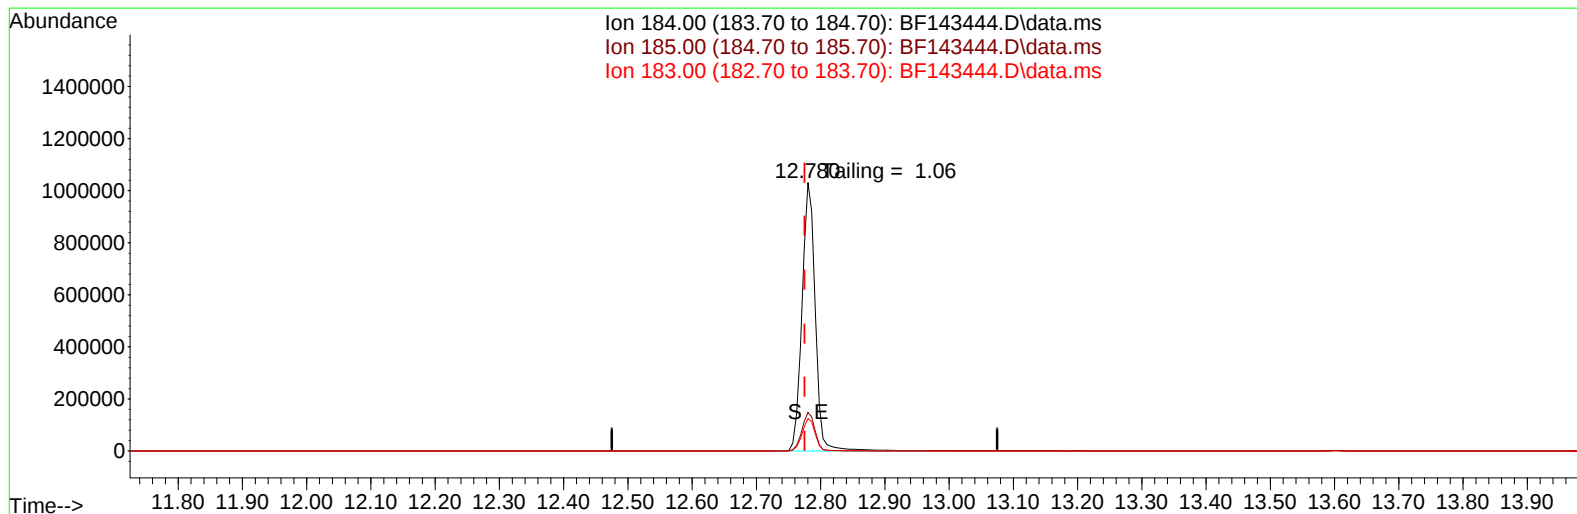

TIC: BF143444.D\data.ms

**(77) Benzidine**

**12.780min (+ 0.005) 257789.28 ng**

**response 1485742**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.20  | 14.41  |
| 183.00 | 11.50  | 12.11  |
| 0.00   | 0.00   | 0.00   |