
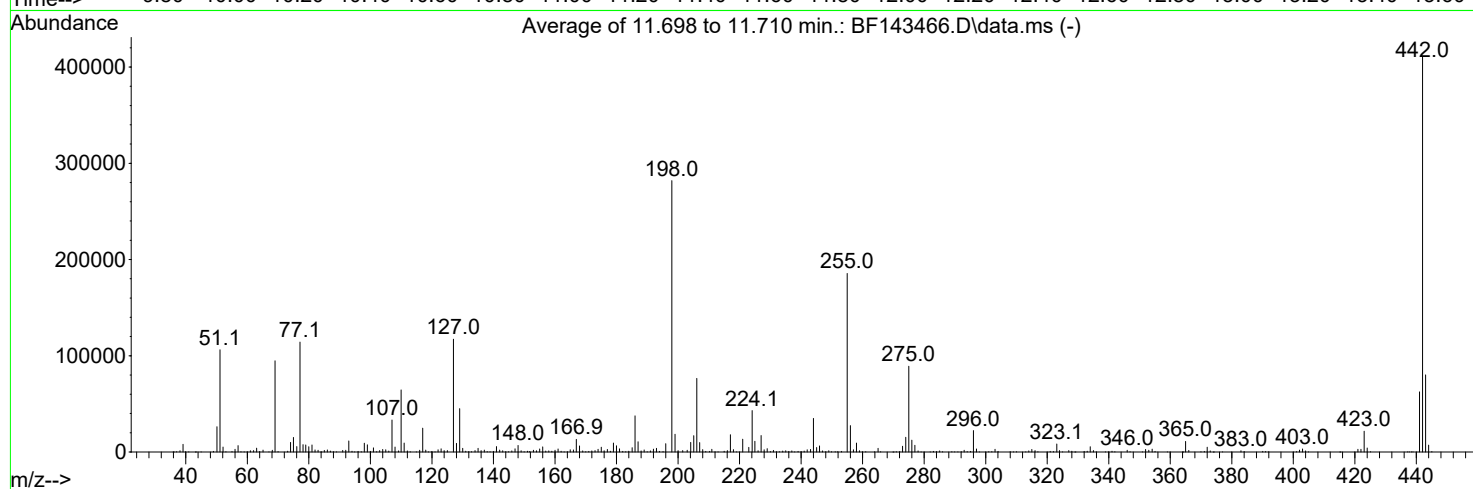


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143466.D
Acq On : 19 Aug 2025 20:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 18 04:40:19 2025

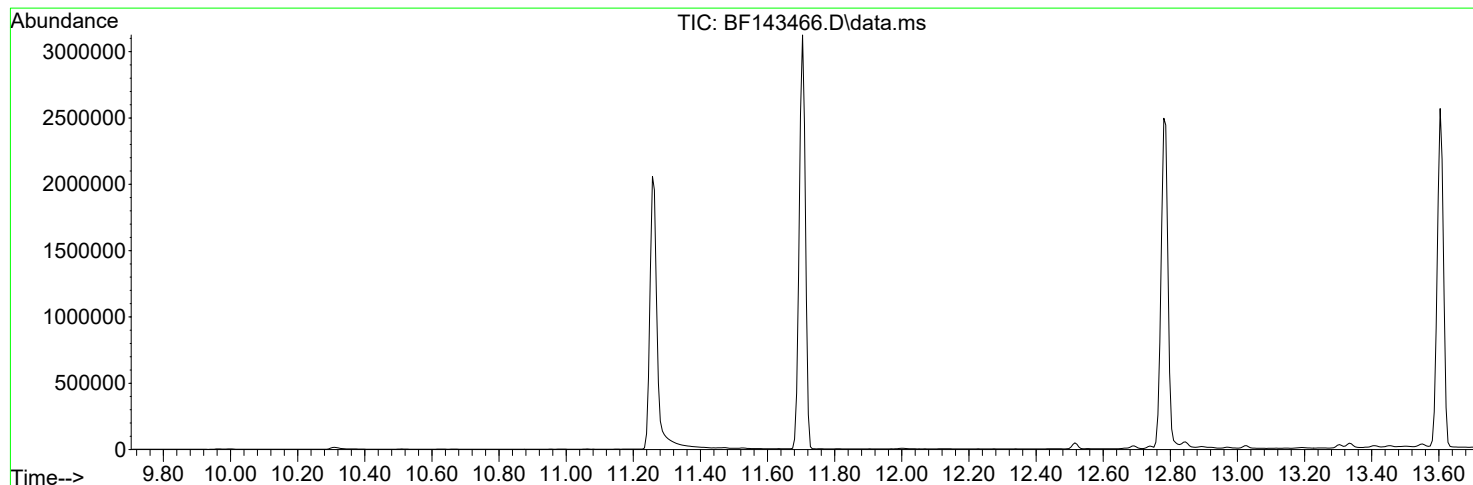

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	1869	PASS
69	69	100	100	100.0	94701	PASS
70	69	0.00	2	0.6	578	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	281899	PASS
199	198	5	9	6.5	18400	PASS
365	198	1	100	3.9	10977	PASS
441	443	0.01	150	78.2	62600	PASS
442	442	100	100	100.0	410240	PASS
443	442	15	24	19.5	80075	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/19/2025	BNA_F	<u>BF143466.D</u>
Compound Name	Response	Retention Time
DDT	668194	13.604
DDD	15521	13.333
DDE	54	12.557
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15575	683769	2.28

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143466.D
Acq On : 19 Aug 2025 20:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 20 01:26:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 18 04:40:19 2025
Response via : Initial Calibration

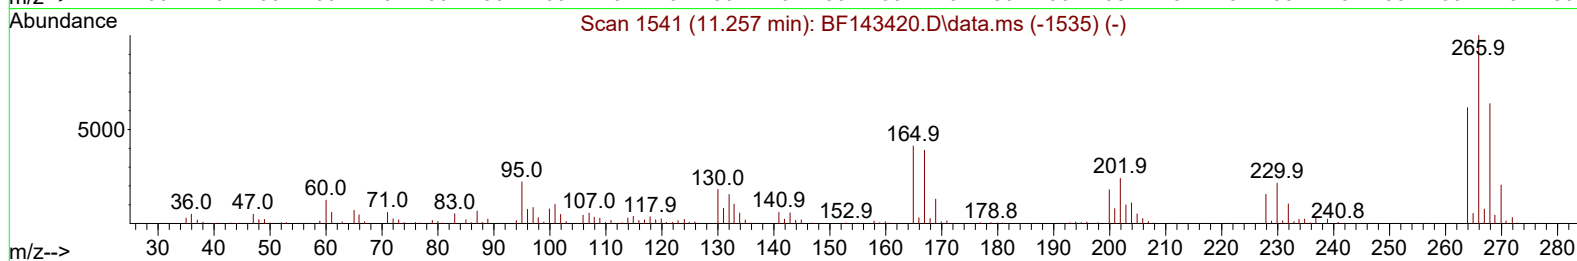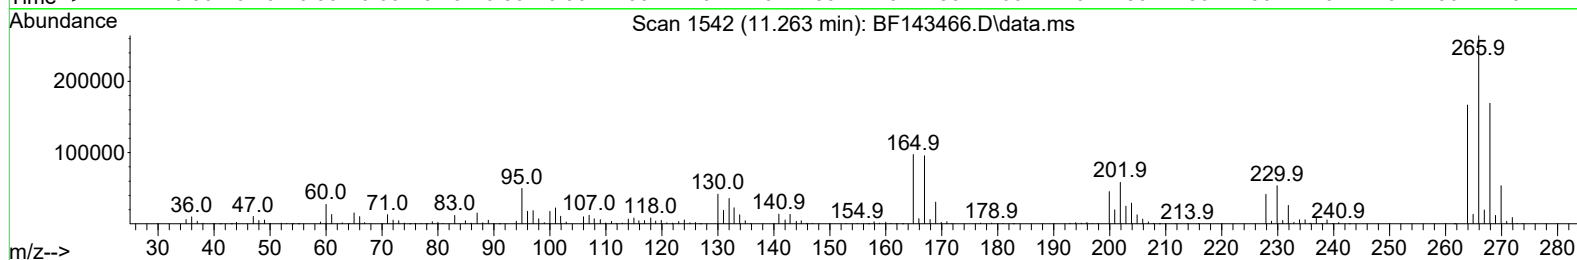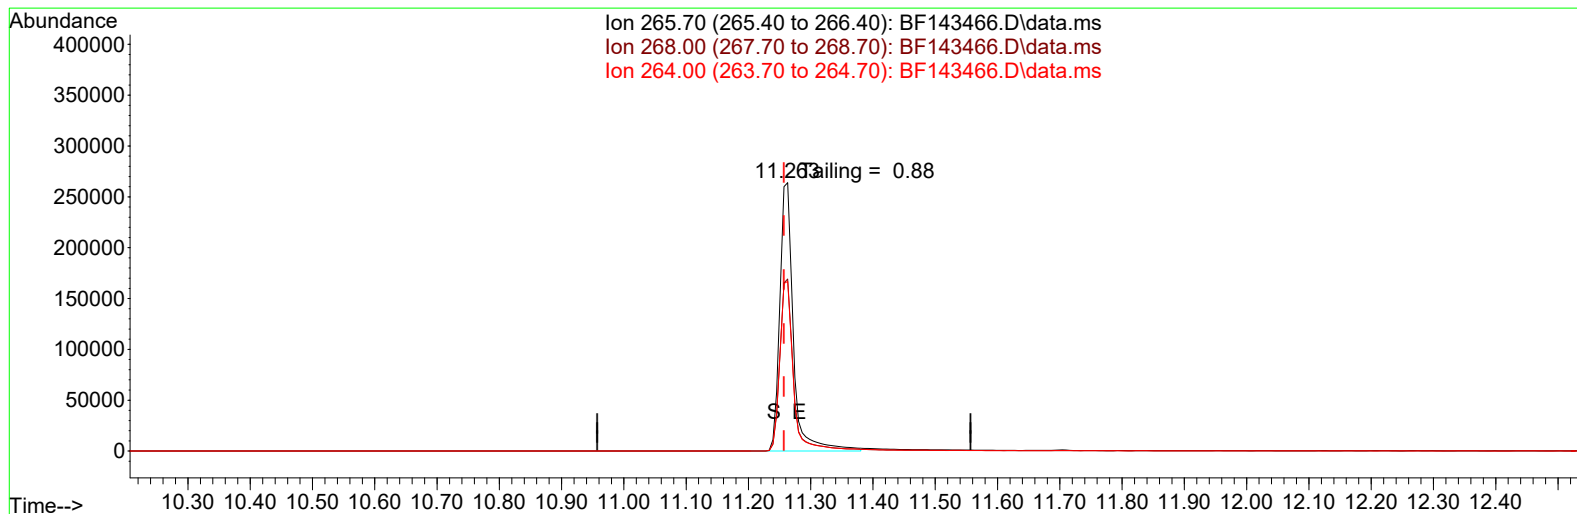

TIC: BF143466.D\data.ms

(70) Pentachlorophenol (C)

11.263min (+ 0.006) 121521.13 ng




response 416623

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.12
264.00	61.60	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081925\
Data File : BF143466.D
Acq On : 19 Aug 2025 20:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 20 01:26:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 18 04:40:19 2025
Response via : Initial Calibration

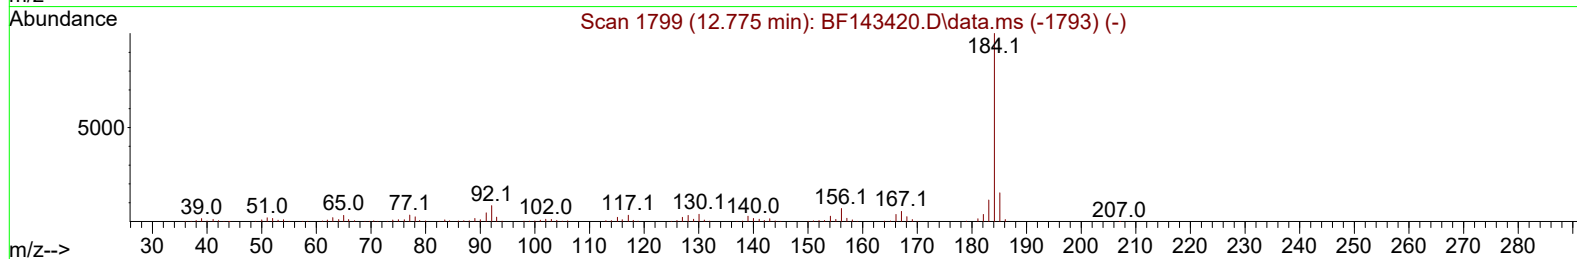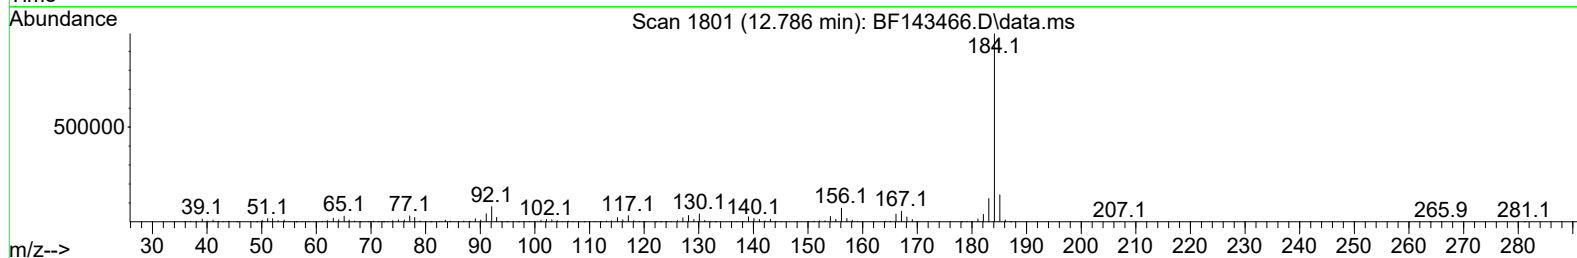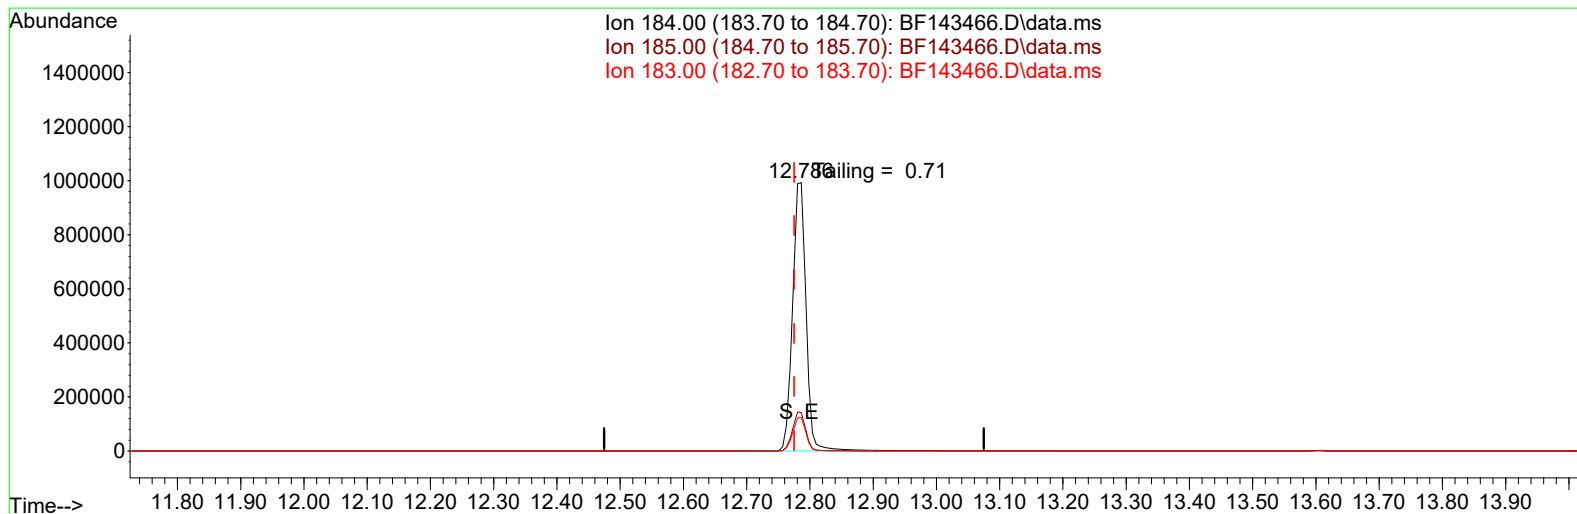

TIC: BF143466.D\data.ms

(77) Benzidine

12.786min (+ 0.011) 116017.64 ng

response 1475893

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.35
183.00	11.50	12.39
0.00	0.00	0.00