

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082015\
 Data File : BF081137.D
 Acq On : 20 Aug 2015 21:44
 Operator : UM/IZ
 Sample : PB85121BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB85121BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.710	243	247	260	rBV	613439	1066177	58.30%	6.541%
2	5.156	283	286	288	rBV	1703930	1804285	98.65%	11.069%
3	6.219	376	379	382	rBV	1400270	1616140	88.37%	9.915%
4	6.344	387	390	392	rBV	1410284	1768074	96.67%	10.847%
5	6.573	408	410	412	rBV	519899	437140	23.90%	2.682%
6	6.733	421	424	426	rBV	1130365	1317575	72.04%	8.083%
7	7.145	457	460	462	rBV	1129164	1193487	65.26%	7.322%
8	7.865	520	523	525	rBV	423462	553856	30.28%	3.398%
9	8.939	614	617	620	rBV	1648039	1768989	96.72%	10.853%
10	9.602	673	675	678	rBV	509851	581935	31.82%	3.570%
11	10.391	741	744	746	rBV	902988	899202	49.17%	5.517%
12	11.076	801	804	806	rBV	729792	613597	33.55%	3.764%
13	12.665	940	943	945	rBV	1909305	1828911	100.00%	11.220%
14	13.694	1030	1033	1035	rBV	539732	511728	27.98%	3.139%
15	15.031	1147	1150	1153	rBV	317978	338831	18.53%	2.079%


Sum of corrected areas: 16299927

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082015\
Data File : BF081137.D
Acq On : 20 Aug 2015 21:44
Operator : UM/IZ
Sample : PB85121BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85121BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

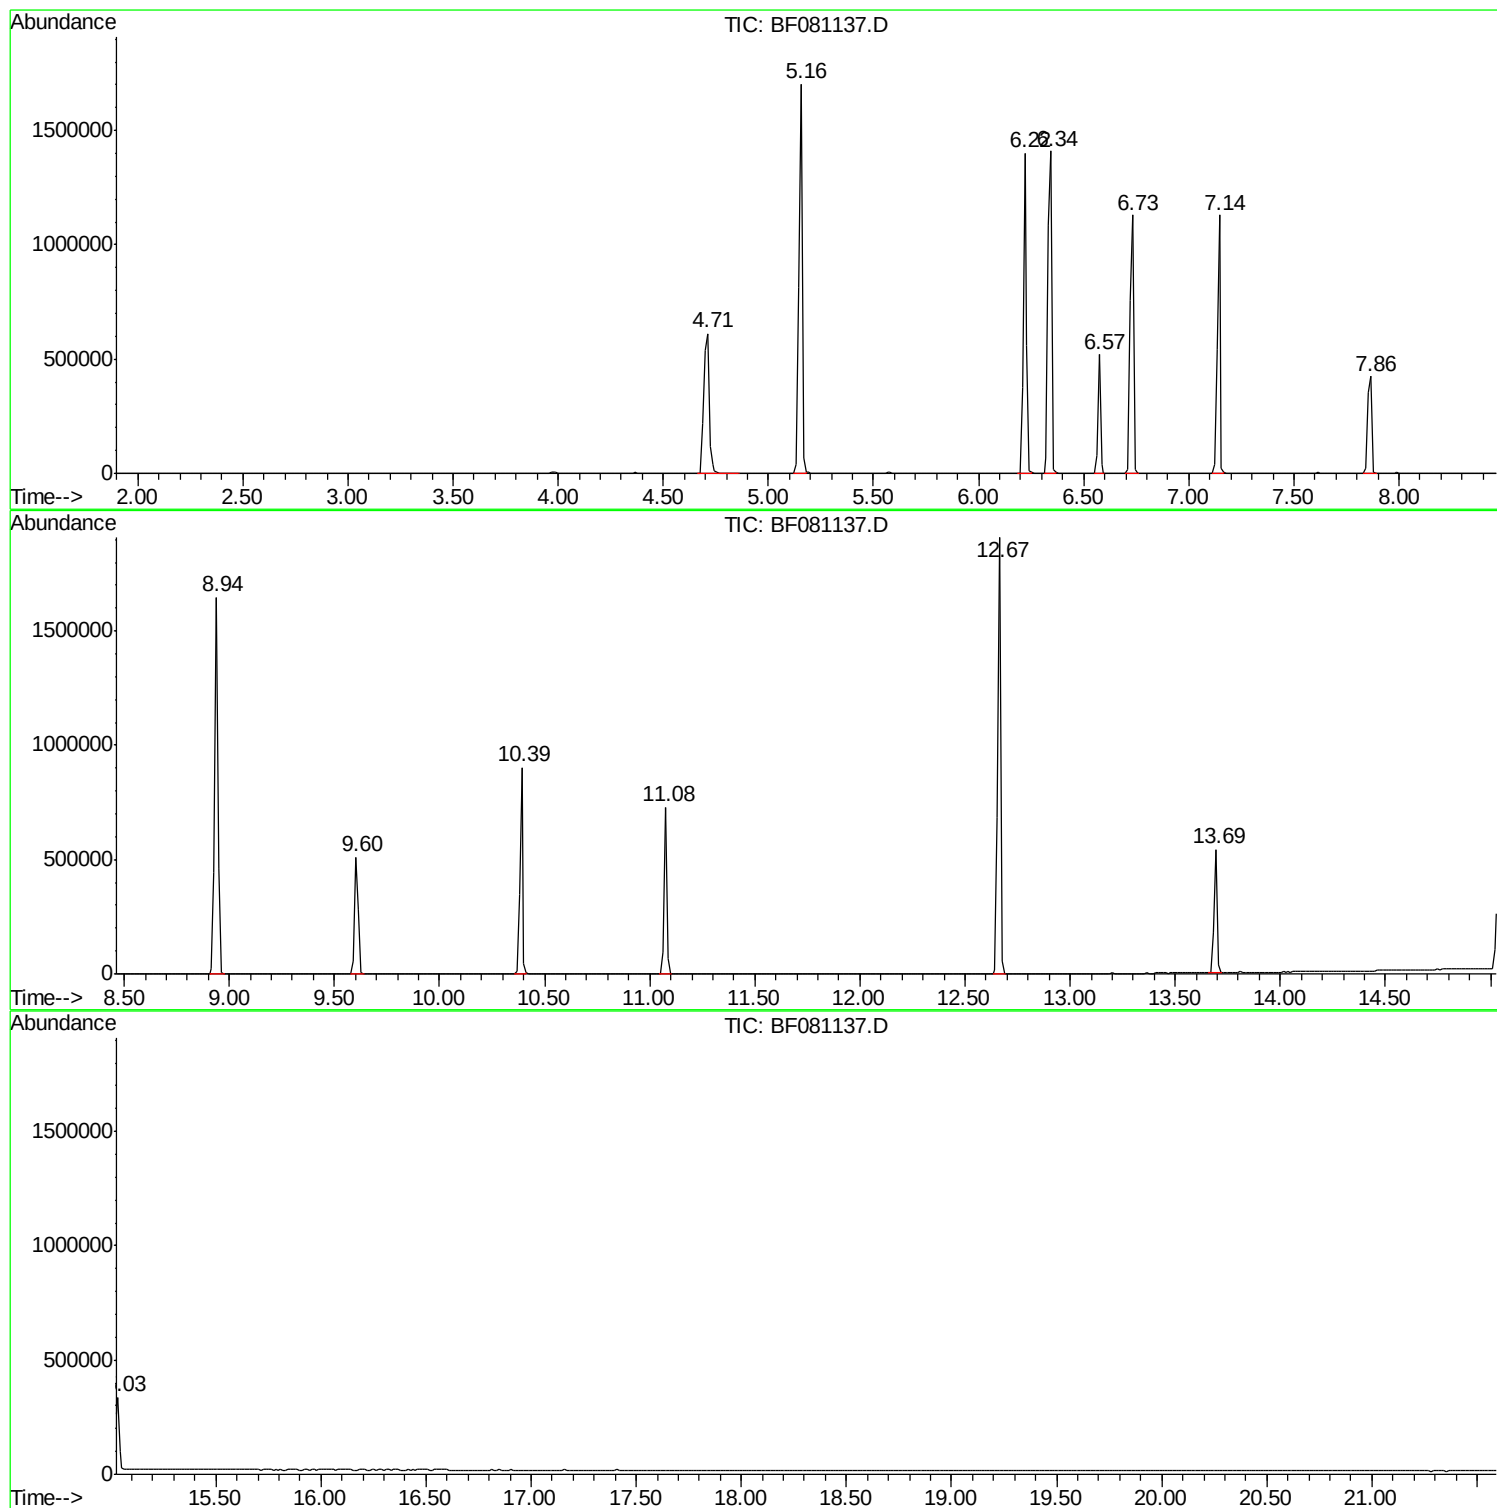

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082015\
Data File : BF081137.D
Acq On : 20 Aug 2015 21:44
Operator : UM/IZ
Sample : PB85121BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85121BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown4.71 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.71	48.78 ng	1066180	1,4-Dichlorobenzene-d4	6.57

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	33
3			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
4			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
5			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23

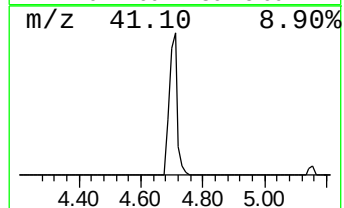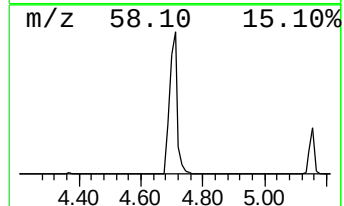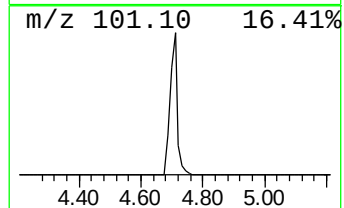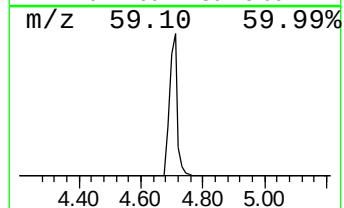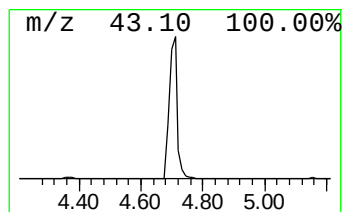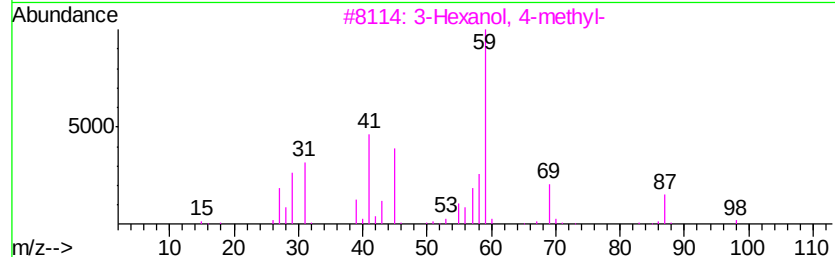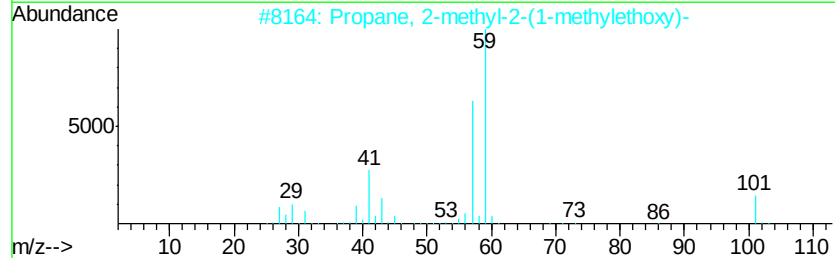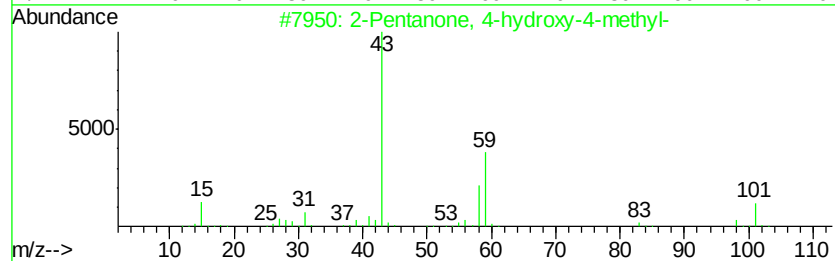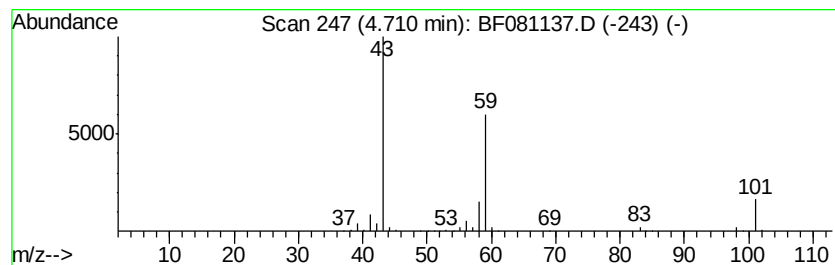

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082015\
Data File : BF081137.D
Acq On : 20 Aug 2015 21:44
Operator : UM/IZ
Sample : PB85121BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85121BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.34 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.34	80.89 ng	1768070	1,4-Dichlorobenzene-d4	6.57

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9
5		Xenon	132	Xe	007440-63-3	9

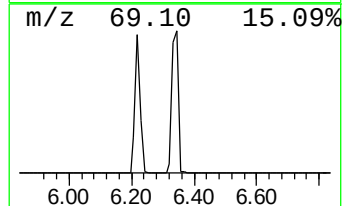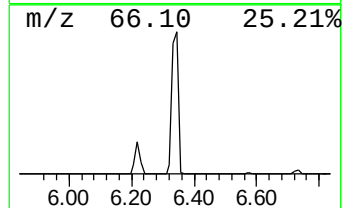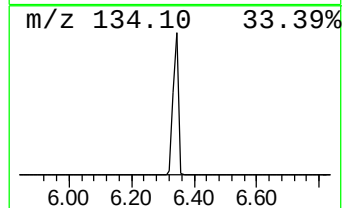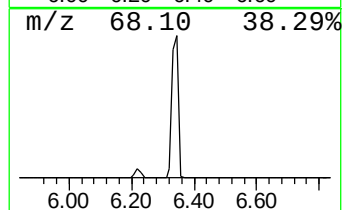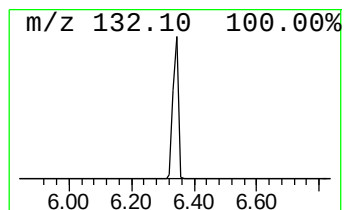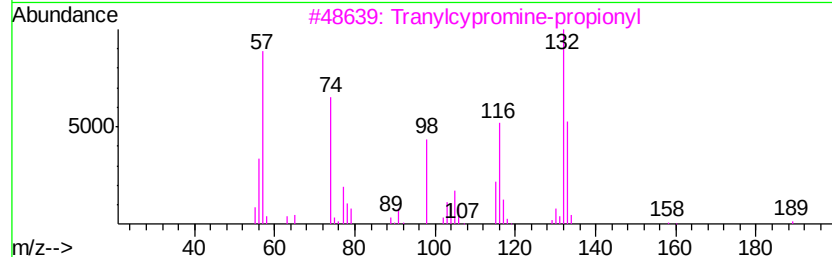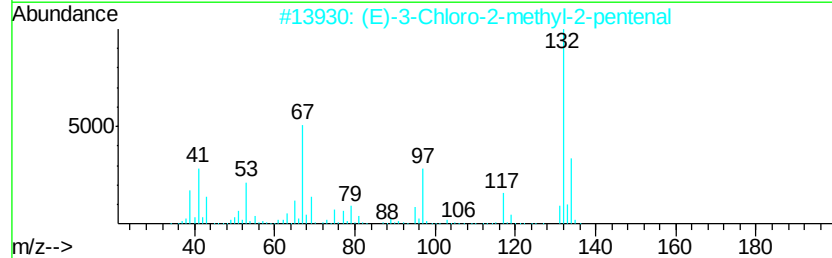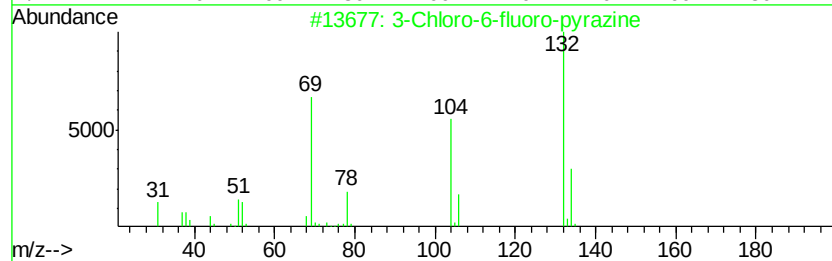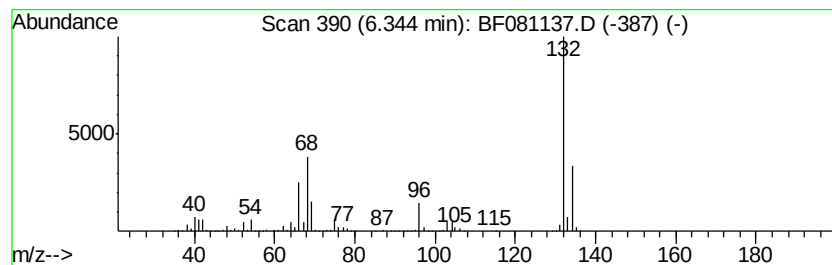

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082015\
Data File : BF081137.D
Acq On : 20 Aug 2015 21:44
Operator : UM/IZ
Sample : PB85121BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85121BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown4.71	4.71	48.8	ng	1066180	1	6.57	437140	20.0
unknown6.34	6.34	80.9	ng	1768070	1	6.57	437140	20.0