


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082015\
Data File : BF081125.D
Acq On : 20 Aug 2015 15:28
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 20 11:22:13 2015

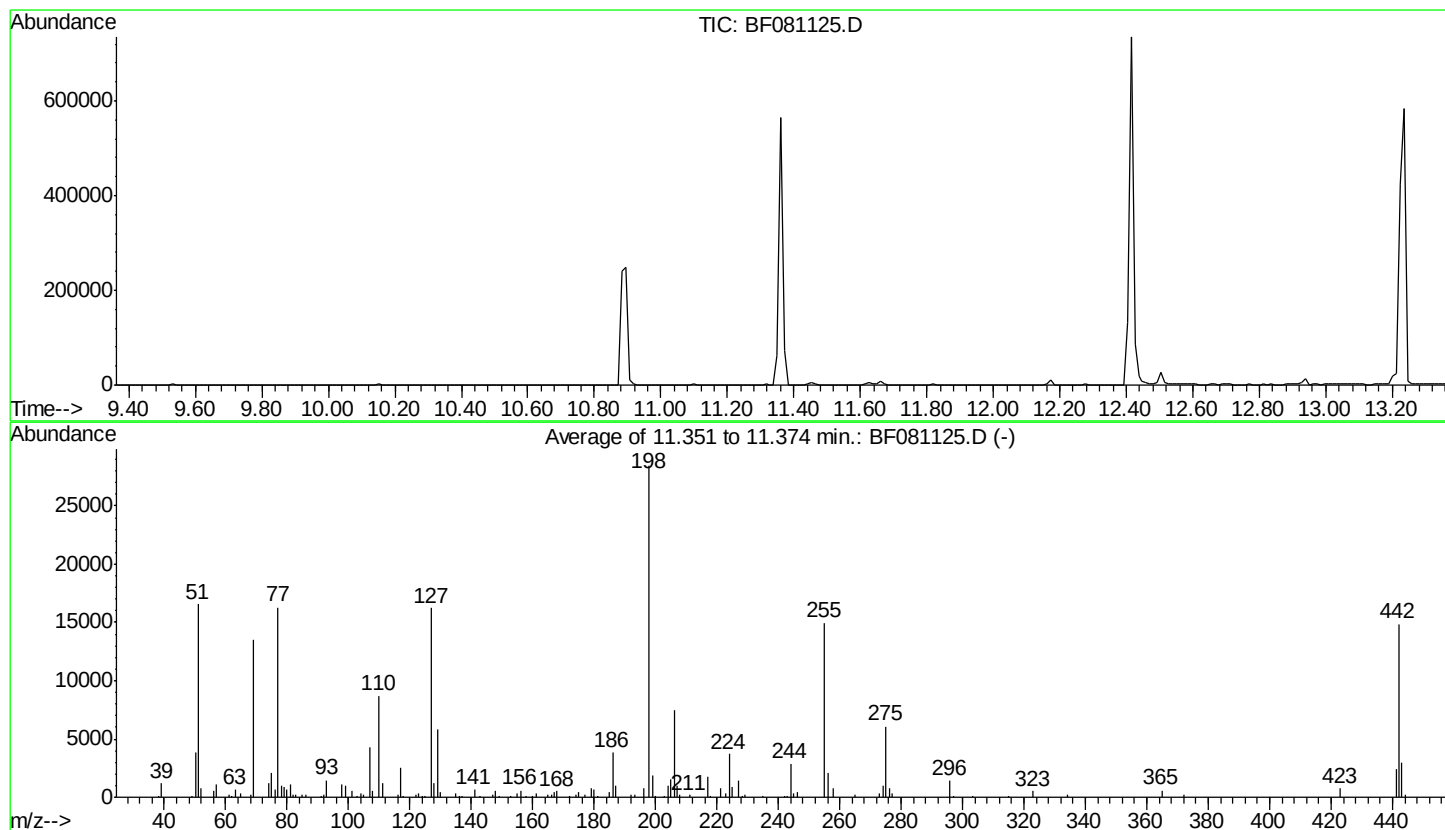

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.2	16545	PASS
68	69	0.00	2	1.3	176	PASS
69	198	0.00	100	47.5	13523	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.0	16209	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28452	PASS
199	198	5	9	6.6	1877	PASS
275	198	10	60	21.4	6084	PASS
365	198	1	100	2.1	594	PASS
441	442	0.01	24	16.1	2396	PASS
442	198	50	100	52.3	14874	PASS
443	442	15	24	19.9	2966	PASS