

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082021\
 Data File : BF125132.D
 Acq On : 20 Aug 2021 13:40
 Operator : JU/CG
 Sample : M3447-01 2X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TR-05-081721

Manual Integrations
 APPROVED

mohammad
 8/23/2021 12:26:10 PM

Quant Time: Aug 20 14:03:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 18 17:03:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.916	152	182778	20.000	ng	0.00
21) Naphthalene-d8	8.204	136	693011	20.000	ng	# 0.00
39) Acenaphthene-d10	9.957	164	358381	20.000	ng	0.00
64) Phenanthrene-d10	11.445	188	581890	20.000	ng	0.00
76) Chrysene-d12	14.086	240	392403	20.000	ng	# 0.00
86) Perylene-d12	15.586	264	346830	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.522	112	330444	27.364	ng	-0.01
7) Phenol-d6	6.528	99	414137	26.517	ng	-0.01
23) Nitrobenzene-d5	7.475	82	276156	20.061	ng	-0.01
42) 2,4,6-Tribromophenol	10.739	330	101936	28.494	ng	-0.01
45) 2-Fluorobiphenyl	9.274	172	544602	21.179	ng	0.00
79) Terphenyl-d14	13.027	244	475547	19.306	ng	0.00
Target Compounds						Qvalue
71) Phenanthrene	11.468	178	268174	8.364	ng	99
72) Anthracene	11.515	178	69655	2.204	ng	98
75) Fluoranthene	12.657	202	612673	19.258	ng	98
78) Pyrene	12.886	202	570929	16.961	ng	95
81) Benzo(a)anthracene	14.074	228	303053	10.719	ng	96
83) Chrysene	14.109	228	275968	9.870	ng	95
87) Indeno(1,2,3-cd)pyrene	17.092	276	121581	4.866	ng	# 88
88) Benzo(b)fluoranthene	15.145	252	382760m	15.106	ng	
89) Benzo(k)fluoranthene	15.168	252	119773m	5.066	ng	
90) Benzo(a)pyrene	15.521	252	254091	11.352	ng	96
92) Benzo(g,h,i)perylene	17.550	276	110695m	5.315	ng	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082021\
Data File : BF125132.D
Acq On : 20 Aug 2021 13:40
Operator : JU/CG
Sample : M3447-01 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampled :
TR-05-081721

Manual Integrations
APPROVED

mohammad
8/23/2021 12:26:10 PM

Quant Time: Aug 20 14:03:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 17:03:50 2021
Response via : Initial Calibration

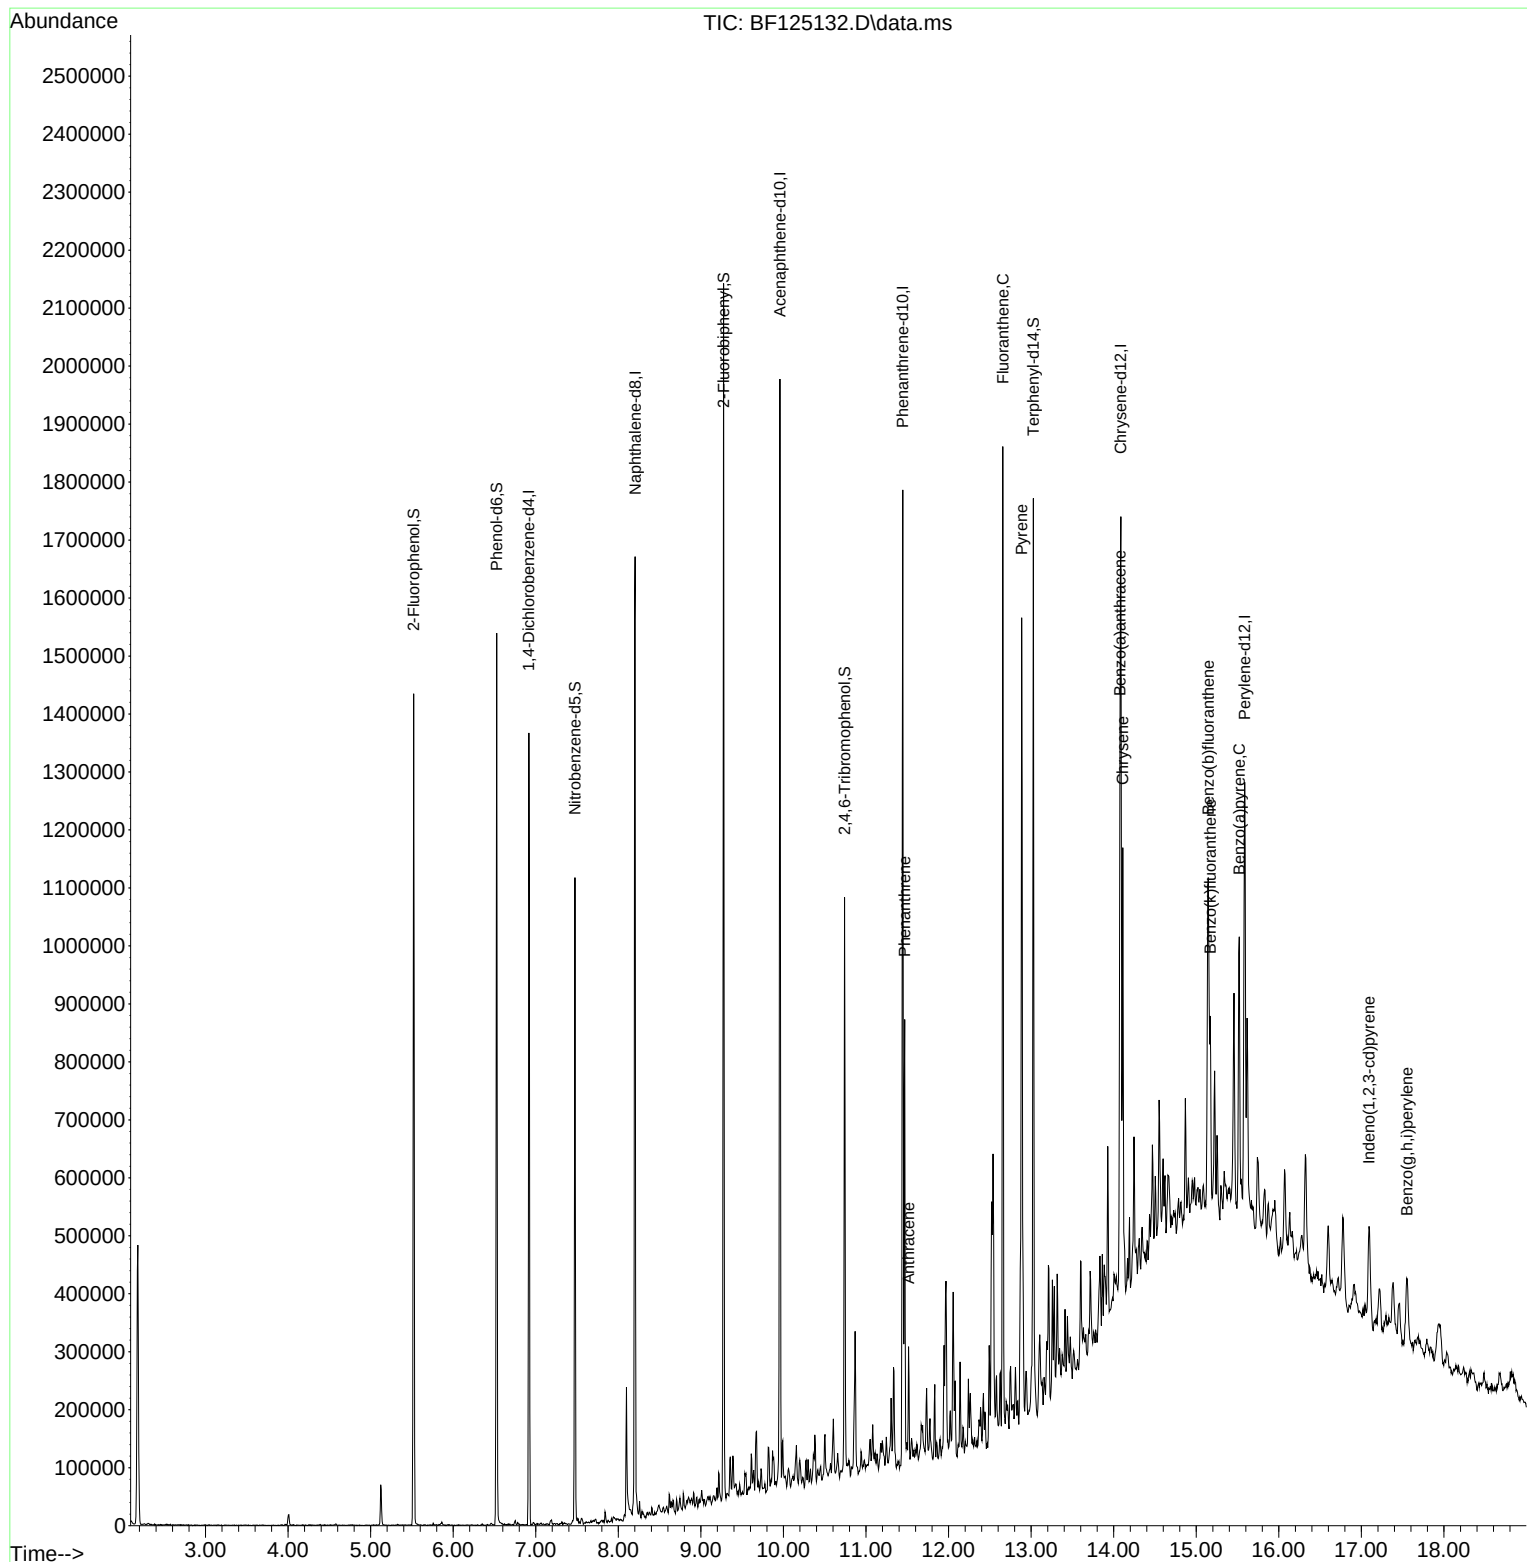







#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.916 min Scan# 821
Delta R.T. -0.006 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40

Tgt Ion:152 Resp: 182778
Ion Ratio Lower Upper
152 100
150 155.5 117.6 176.4
115 64.2 47.1 70.7

Instrument :
BNA_F
ClientSampled :
TR-05-081721




Manual Integrations
APPROVED


mohammad
8/23/2021 12:26:10 PM

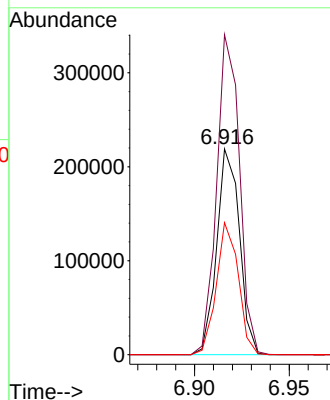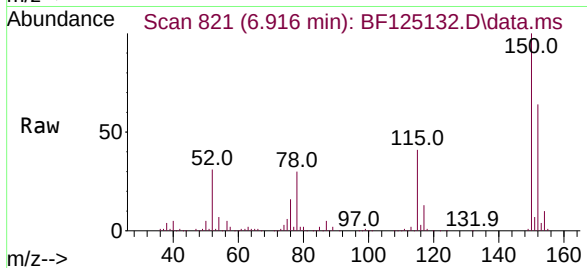

#5
2-Fluorophenol
Concen: 27.364 ng
RT: 5.522 min Scan# 584
Delta R.T. -0.012 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40


Tgt Ion:112 Resp: 330444
Ion Ratio Lower Upper
112 100
64 71.2 44.2 66.2#
63 37.4 26.2 39.2

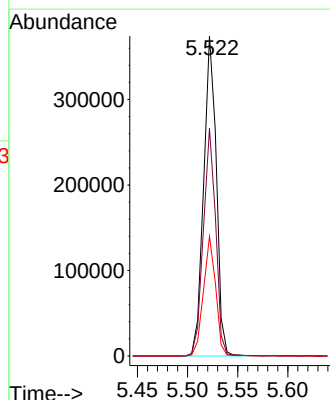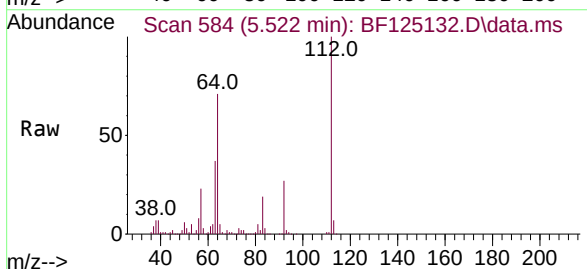

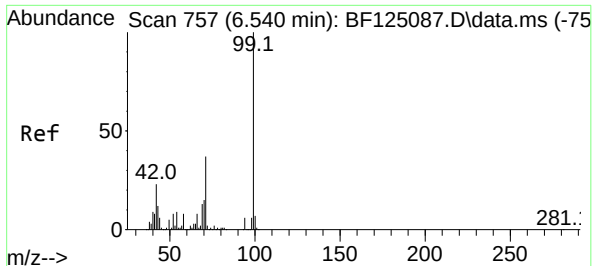

#7
Phenol-d6
Concen: 26.517 ng
RT: 6.528 min Scan# 755
Delta R.T. -0.012 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40




Instrument :
BNA_F
ClientSampleId :
TR-05-081721

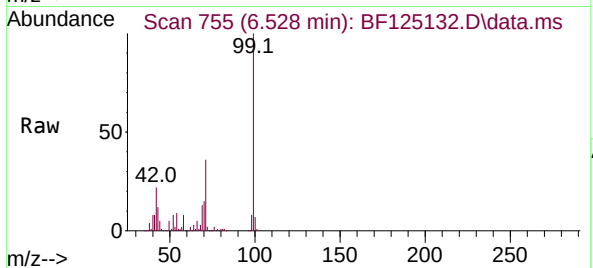


Tgt Ion: 99 Resp: 414137
Ion Ratio Lower Upper
99 100
42 22.4 23.5 35.3#
71 35.7 25.6 38.4

Manual Integrations
APPROVED



mohammad
8/23/2021 12:26:10 PM

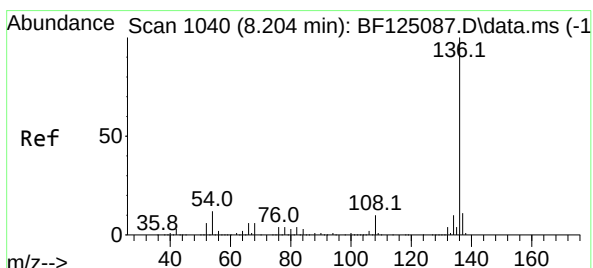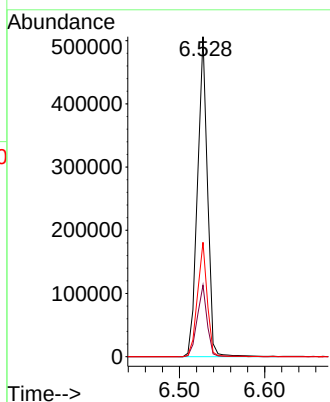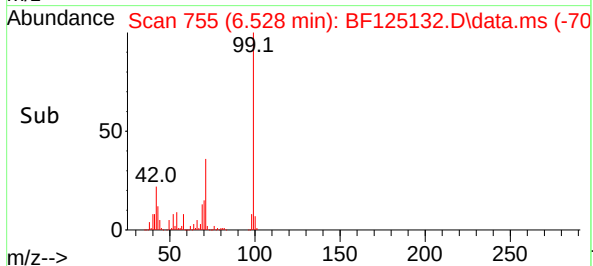


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.204 min Scan# 1040
Delta R.T. -0.000 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40

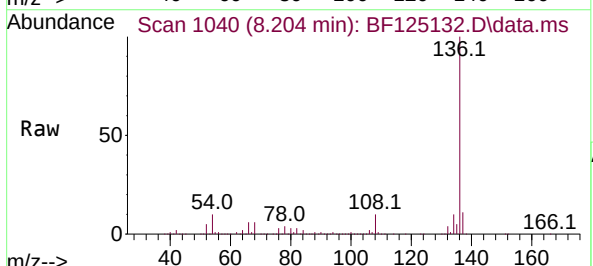


Tgt Ion: 136 Resp: 693011
Ion Ratio Lower Upper
136 100
137 11.1 9.8 14.6
54 10.2 6.4 9.6#
68 5.6 3.3 4.9#

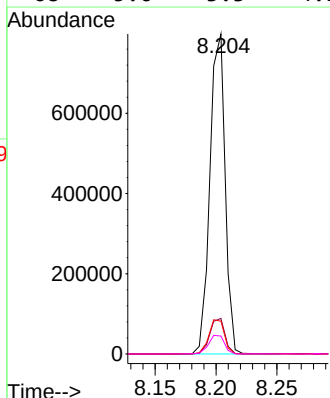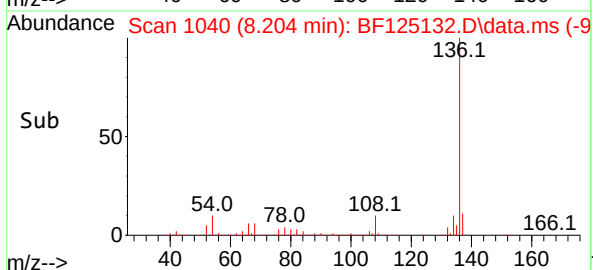

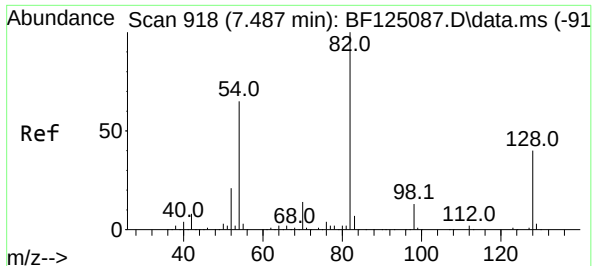

#23
Nitrobenzene-d5
Concen: 20.061 ng
RT: 7.475 min Scan# 916
Delta R.T. -0.012 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40




Instrument :
BNA_F
ClientSampleId :
TR-05-081721

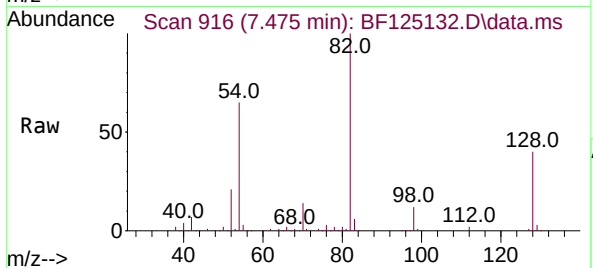


Tgt Ion: 82 Resp: 276156
Ion Ratio Lower Upper
82 100
128 39.9 40.6 60.8#
54 64.9 49.6 74.4

Manual Integrations
APPROVED



mohammad
8/23/2021 12:26:10 PM

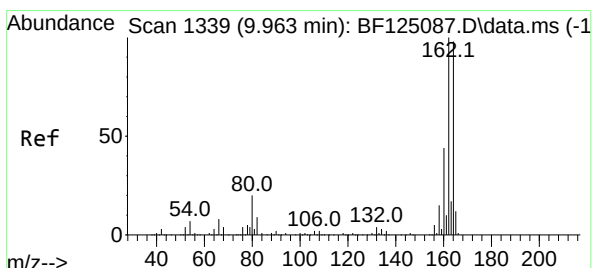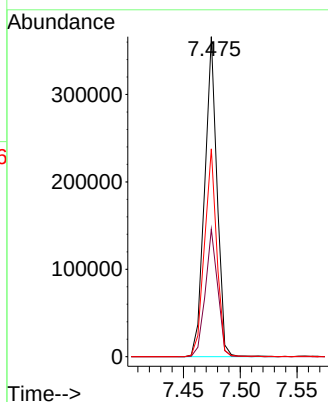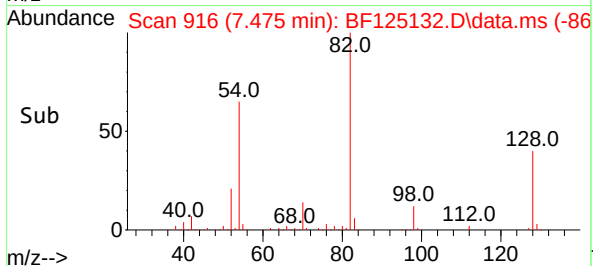


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.957 min Scan# 1338
Delta R.T. -0.006 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40

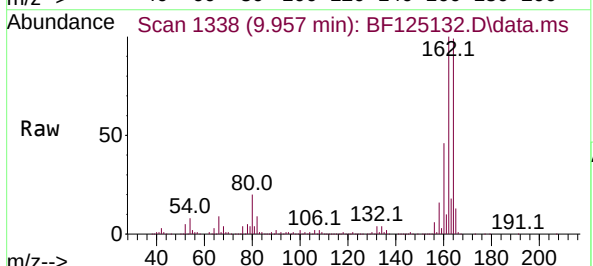

Tgt Ion: 164 Resp: 358381
Ion Ratio Lower Upper
164 100
162 101.0 81.3 121.9
160 46.0 38.0 57.0

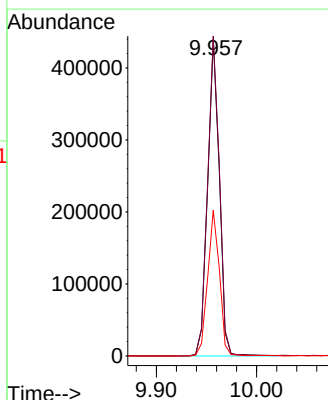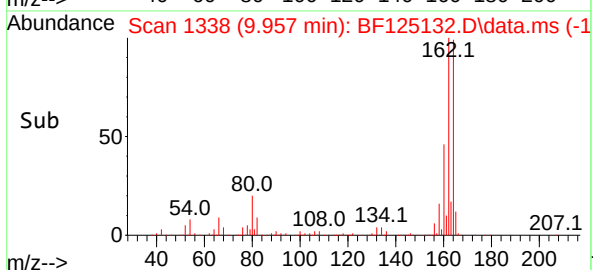







#42
2,4,6-Tribromophenol
Concen: 28.494 ng
RT: 10.739 min Scan# 1471
Delta R.T. -0.012 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40

Tgt Ion: 330 Resp: 101936
Ion Ratio Lower Upper
330 100
332 93.1 76.2 114.4
141 36.3 44.6 66.8#

Instrument :
BNA_F
ClientSampleId :
TR-05-081721




Manual Integrations
APPROVED


mohammad
8/23/2021 12:26:10 PM

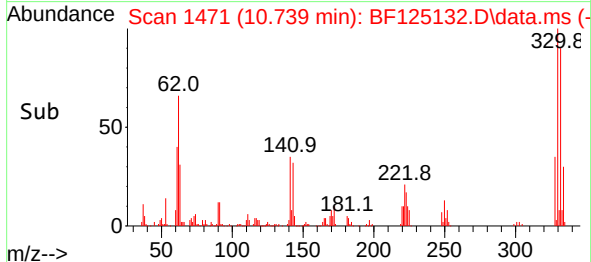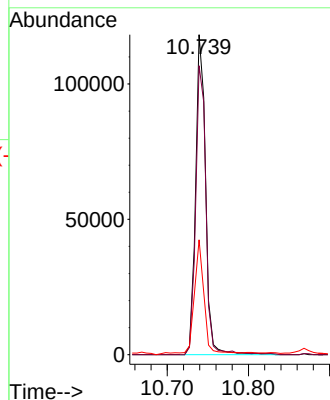

#45
2-Fluorobiphenyl
Concen: 21.179 ng
RT: 9.274 min Scan# 1222
Delta R.T. -0.006 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40


Tgt Ion: 172 Resp: 544602
Ion Ratio Lower Upper
172 100
171 33.6 26.5 39.7
170 23.3 18.8 28.2

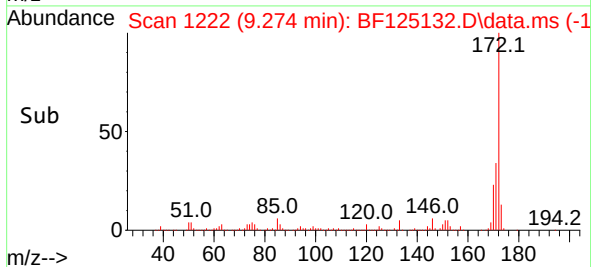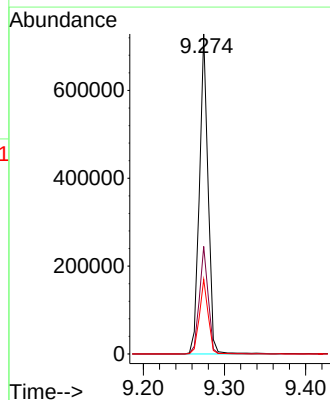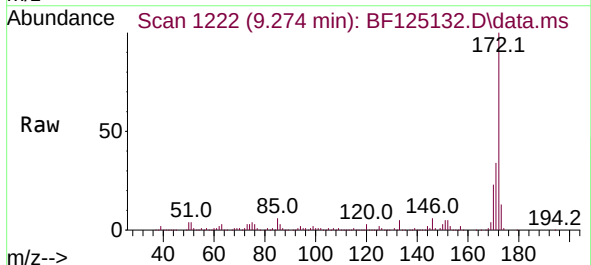



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.445 min Scan# 1591
Delta R.T. -0.000 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40




Instrument :
BNA_F
ClientSampleId :
TR-05-081721




Tgt Ion:188 Resp: 581890
Ion Ratio Lower Upper
188 100
94 8.7 6.7 10.1
80 9.4 7.5 11.3

Manual Integrations
APPROVED



mohammad
8/23/2021 12:26:10 PM

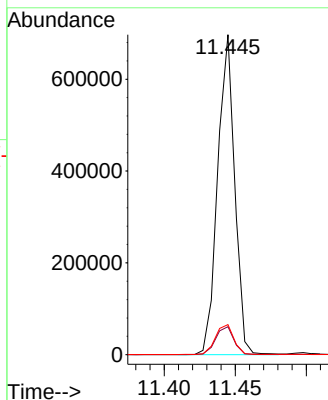


#71
Phenanthrene
Concen: 8.364 ng
RT: 11.468 min Scan# 1595
Delta R.T. -0.006 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40




Tgt Ion:178 Resp: 268174
Ion Ratio Lower Upper
178 100
176 19.2 14.7 22.1
179 14.6 11.5 17.3

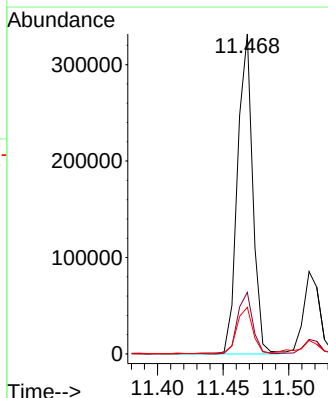



#72
 Anthracene
 Concen: 2.204 ng
 RT: 11.515 min Scan# 1603
 Delta R.T. -0.012 min
 Lab File: BF125132.D
 Acq: 20 Aug 2021 13:40




Instrument :
 BNA_F
 ClientSampled :
 TR-05-081721




Tgt Ion:178 Resp: 69655
 Ion Ratio Lower Upper
 178 100
 176 17.6 14.3 21.5
 179 16.5 12.2 18.4

Manual Integrations
 APPROVED



mohammad
 8/23/2021 12:26:10 PM

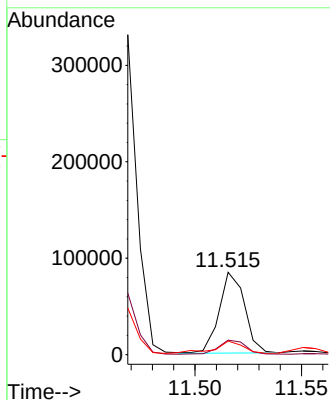


#75
 Fluoranthene
 Concen: 19.258 ng
 RT: 12.657 min Scan# 1797
 Delta R.T. -0.006 min
 Lab File: BF125132.D
 Acq: 20 Aug 2021 13:40




Tgt Ion:202 Resp: 612673
 Ion Ratio Lower Upper
 202 100
 101 10.9 0.0 30.7
 203 17.5 0.0 36.3

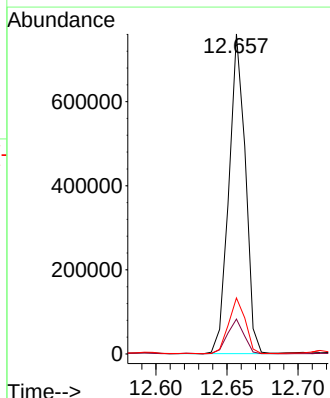





#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.086 min Scan# 2040
Delta R.T. -0.000 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40




Tgt Ion:240 Resp: 392403
Ion Ratio Lower Upper
240 100
120 9.6 10.8 16.2#
236 25.6 21.6 32.4

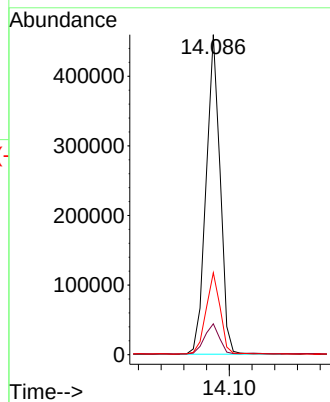


Instrument :
BNA_F
ClientSampleId :
TR-05-081721

Manual Integrations
APPROVED



mohammad
8/23/2021 12:26:10 PM




#78
Pyrene
Concen: 16.961 ng
RT: 12.886 min Scan# 1836
Delta R.T. -0.006 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40

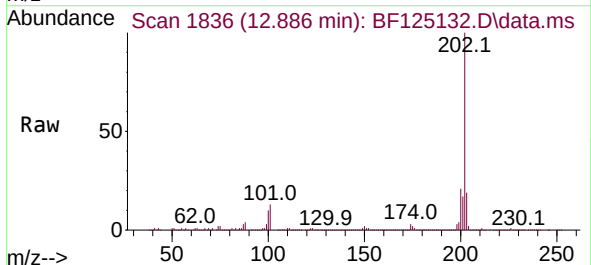


Tgt Ion:202 Resp: 570929
Ion Ratio Lower Upper
202 100
200 21.3 15.3 22.9
203 18.5 13.4 20.0

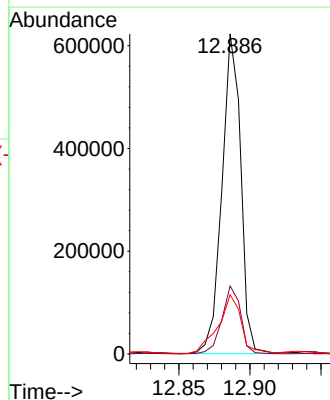
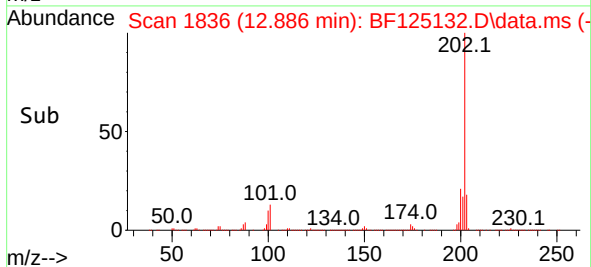




#79
 Terphenyl-d14
 Concen: 19.306 ng
 RT: 13.027 min Scan# 1860
 Delta R.T. -0.006 min
 Lab File: BF125132.D
 Acq: 20 Aug 2021 13:40




Tgt Ion:244 Resp: 475547
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.9 8.9
 122 9.2 9.0 13.4

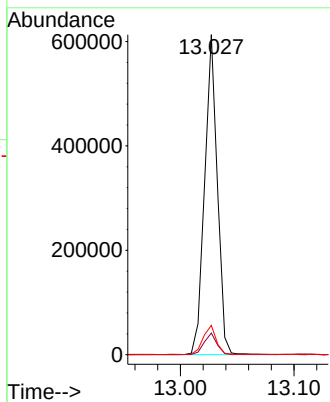


Instrument :
 BNA_F
 ClientSampleId :
 TR-05-081721

Manual Integrations
 APPROVED



mohammad
 8/23/2021 12:26:10 PM




#81
 Benzo(a)anthracene
 Concen: 10.719 ng
 RT: 14.074 min Scan# 2038
 Delta R.T. -0.006 min
 Lab File: BF125132.D
 Acq: 20 Aug 2021 13:40

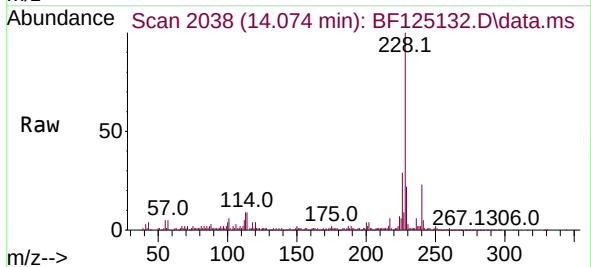


Tgt Ion:228 Resp: 303053
 Ion Ratio Lower Upper
 228 100
 226 28.7 21.6 32.4
 229 22.0 15.6 23.4


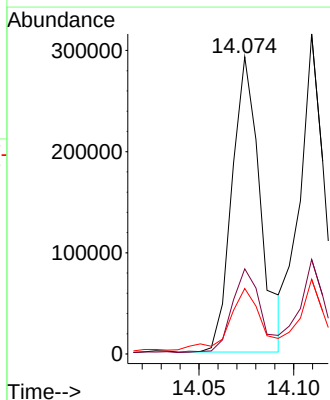
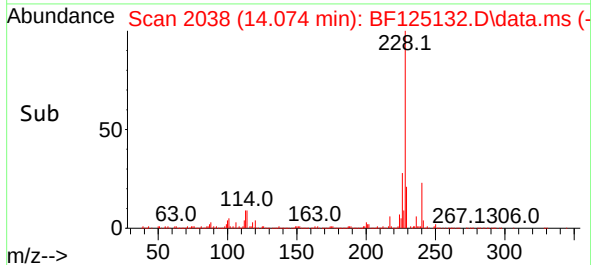





#83
Chrysene
Concen: 9.870 ng
RT: 14.109 min Scan# 2044
Delta R.T. -0.006 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40





Tgt Ion:228 Resp: 275968
Ion Ratio Lower Upper
228 100
226 29.6 22.6 34.0
229 23.4 15.9 23.9

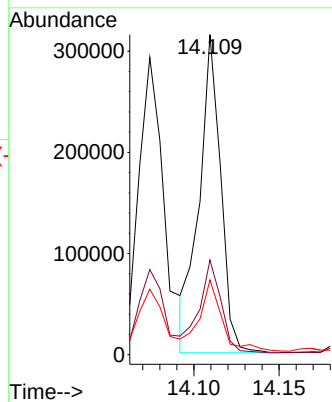

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.586 min Scan# 2295
Delta R.T. 0.006 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40

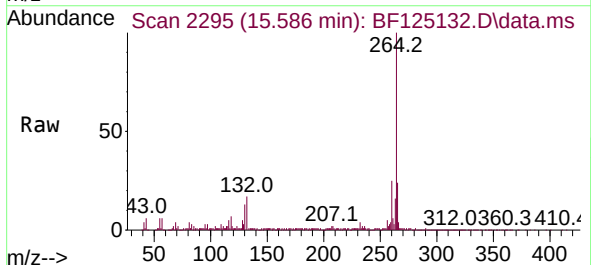


Tgt Ion:264 Resp: 346830
Ion Ratio Lower Upper
264 100
260 24.8 19.6 29.4
265 23.7 17.2 25.8

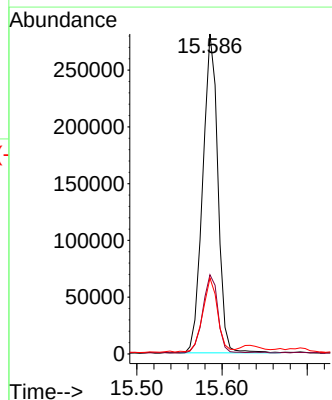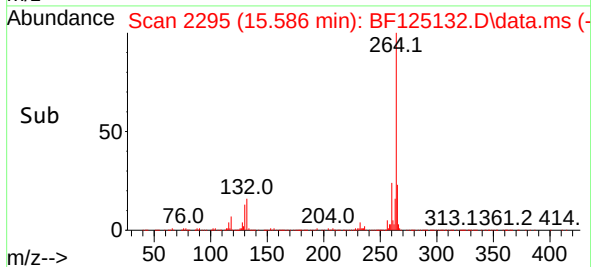

Instrument :
BNA_F
ClientSampleId :
TR-05-081721

Manual Integrations
APPROVED

mohammad
8/23/2021 12:26:10 PM







#87
Indeno(1,2,3-cd)pyrene
Concen: 4.866 ng
RT: 17.092 min Scan# 2551
Delta R.T. -0.000 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40

Tgt Ion: 276 Resp: 121581
Ion Ratio Lower Upper
276 100
138 19.2 24.1 36.1#
277 23.2 18.8 28.2

Instrument :
BNA_F
ClientSampleId :
TR-05-081721




Manual Integrations
APPROVED


mohammad
8/23/2021 12:26:10 PM

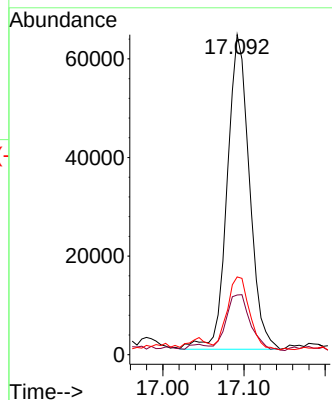

#88
Benzo(b)fluoranthene
Concen: 15.106 ng m
RT: 15.145 min Scan# 2220
Delta R.T. -0.000 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40

Tgt Ion: 252 Resp: 382760
Ion Ratio Lower Upper
252 100
253 22.3 16.8 25.2
125 10.3 9.8 14.8

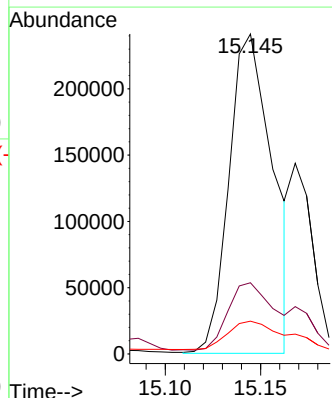



#89

Benzo(k)fluoranthene

Concen: 5.066 ng m

RT: 15.168 min Scan# 2224

Delta R.T. -0.006 min

Lab File: BF125132.D

Acq: 20 Aug 2021 13:40

Tgt Ion:252 Resp: 119773

Ion Ratio Lower Upper

252 100

253 24.8 17.8 26.8

125 10.4 7.2 10.8

Instrument :

BNA_F

ClientSampleId :





TR-05-081721

Manual Integrations

APPROVED

mohammad

8/23/2021 12:26:10 PM

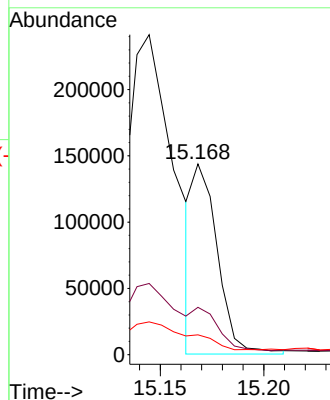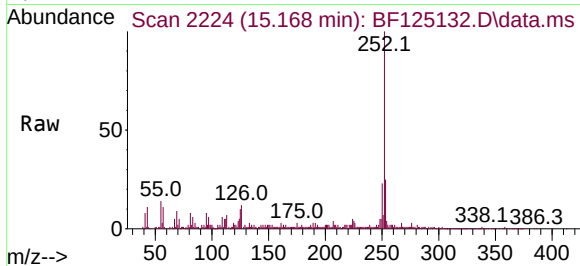

#90

Benzo(a)pyrene

Concen: 11.352 ng

RT: 15.521 min Scan# 2284

Delta R.T. -0.000 min

Lab File: BF125132.D

Acq: 20 Aug 2021 13:40




Tgt Ion:252 Resp: 254091


Ion Ratio Lower Upper

252 100


253 21.5 18.4 27.6

125 10.0 9.9 14.9

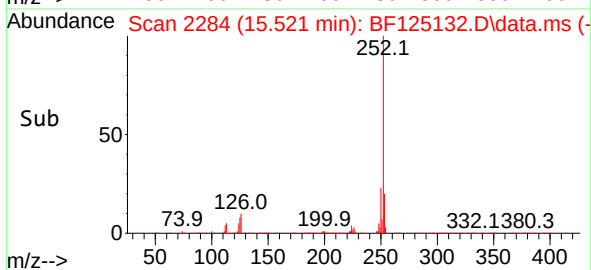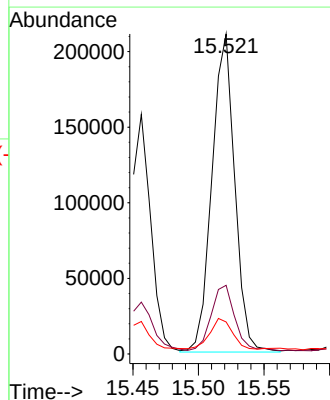
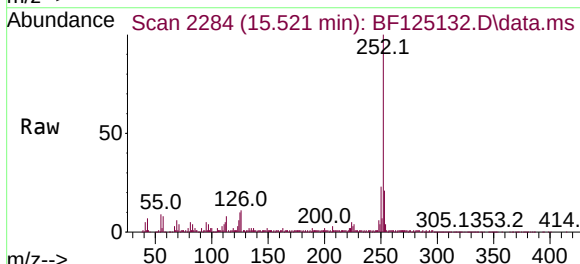


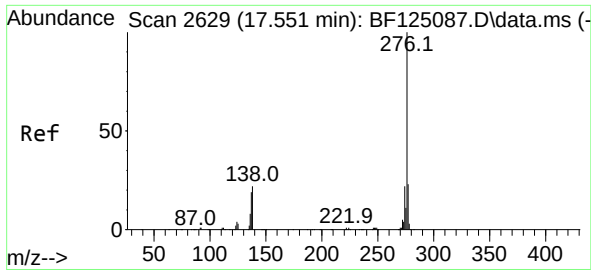

#92
Benzo(g,h,i)perylene
Concen: 5.315 ng m
RT: 17.550 min Scan# 2629
Delta R.T. -0.000 min
Lab File: BF125132.D
Acq: 20 Aug 2021 13:40

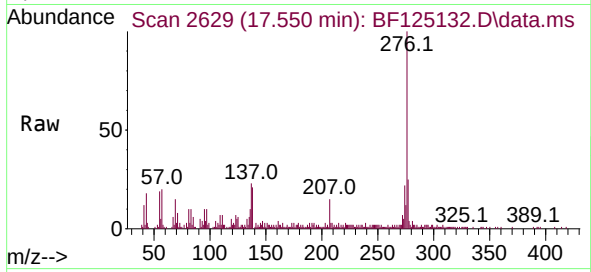

Tgt Ion: 276 Resp: 110695
Ion Ratio Lower Upper
276 100
277 25.2 22.0 33.0
138 21.0 22.2 33.4#

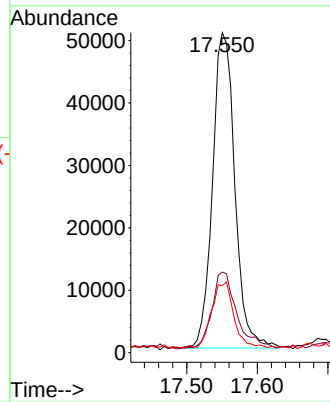

Instrument :
BNA_F
ClientSampleId :
TR-05-081721

Manual Integrations
APPROVED

mohammad
8/23/2021 12:26:10 PM