
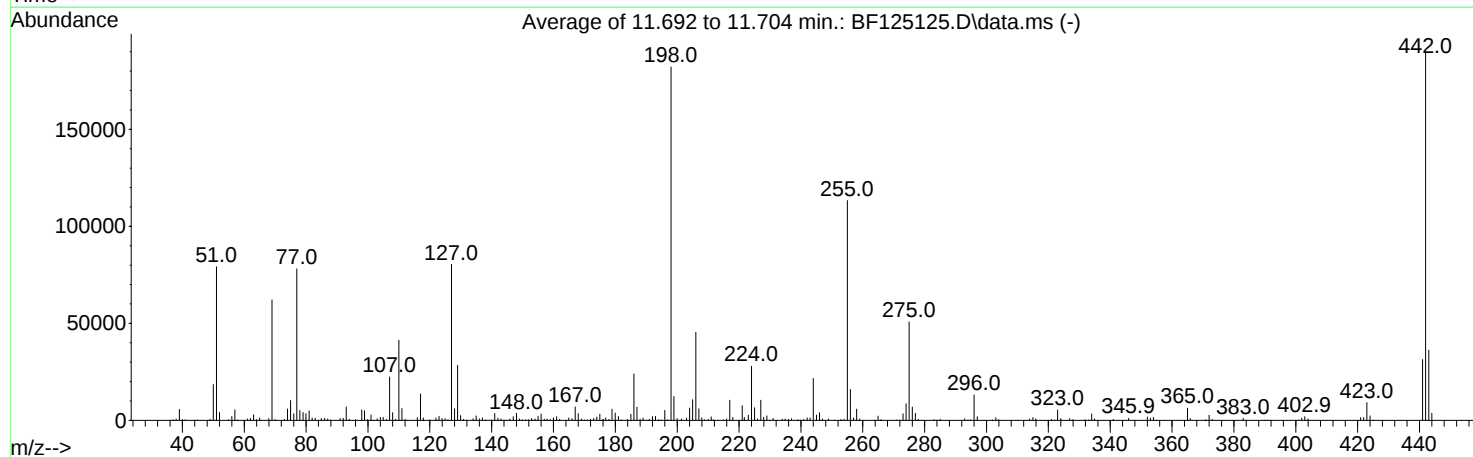


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082021\
 Data File : BF125125.D
 Acq On : 20 Aug 2021 9:09
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 18 17:03:50 2021

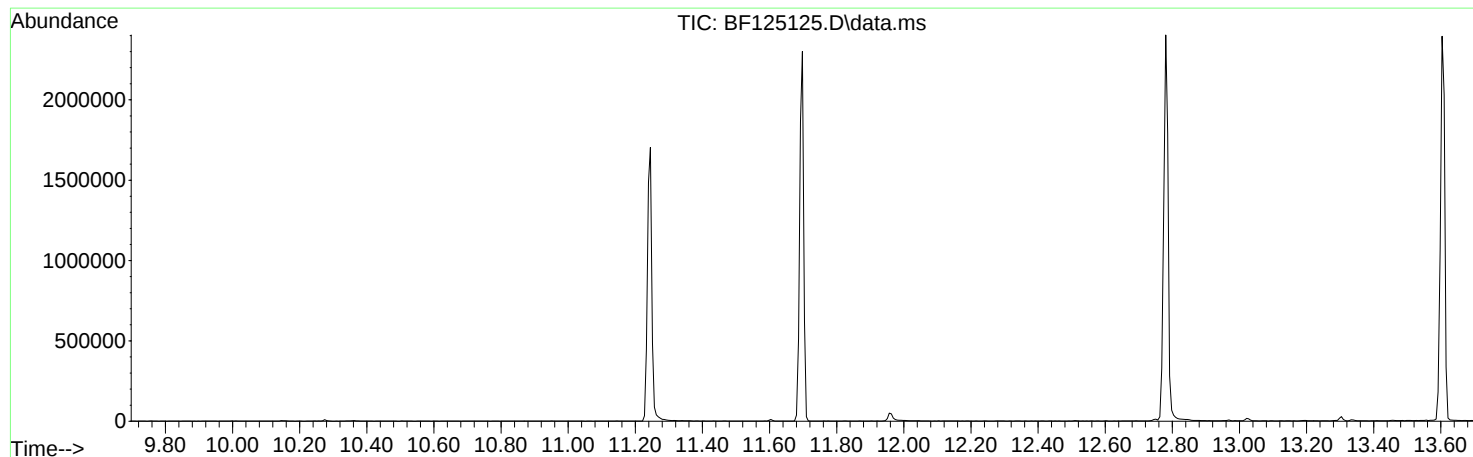

AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	79166	PASS
68	69	0.00	2	1.5	935	PASS
69	198	0.00	100	34.1	62110	PASS
70	69	0.00	2	0.5	323	PASS
127	198	10	80	44.1	80371	PASS
197	198	0.00	2	0.2	304	PASS
198	198	100	100	100.0	182056	PASS
199	198	5	9	6.7	12269	PASS
275	198	10	60	27.9	50728	PASS
365	198	1	100	3.4	6252	PASS
441	198	0.01	100	17.2	31349	PASS
442	442	50	100	100.0	189597	PASS
443	442	15	24	19.1	36173	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/20/2021	BNA_F	<u>BF125125.D</u>
Compound Name	Response	Retention Time
DDT	425050	13.6
DDD	5228	13.3
DDE	905	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6133	431183	1.42

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082021\
Data File : BF125125.D
Acq On : 20 Aug 2021 9:09
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 20 10:53:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 17:03:50 2021
Response via : Initial Calibration

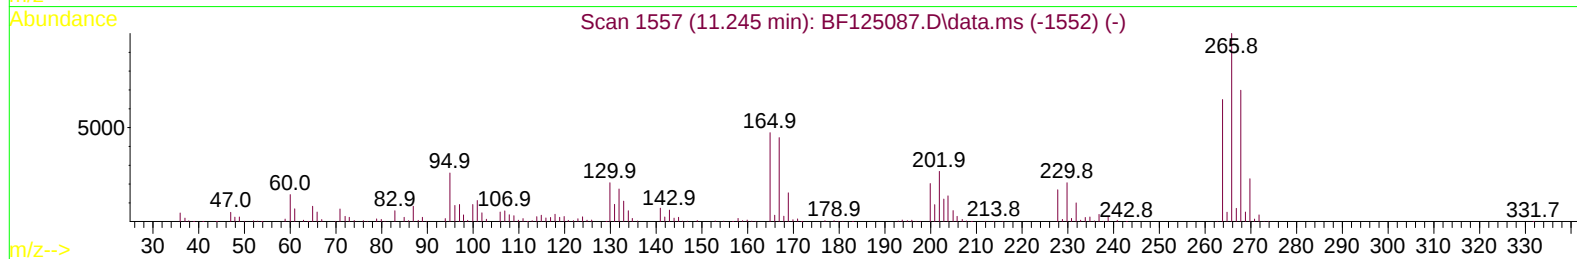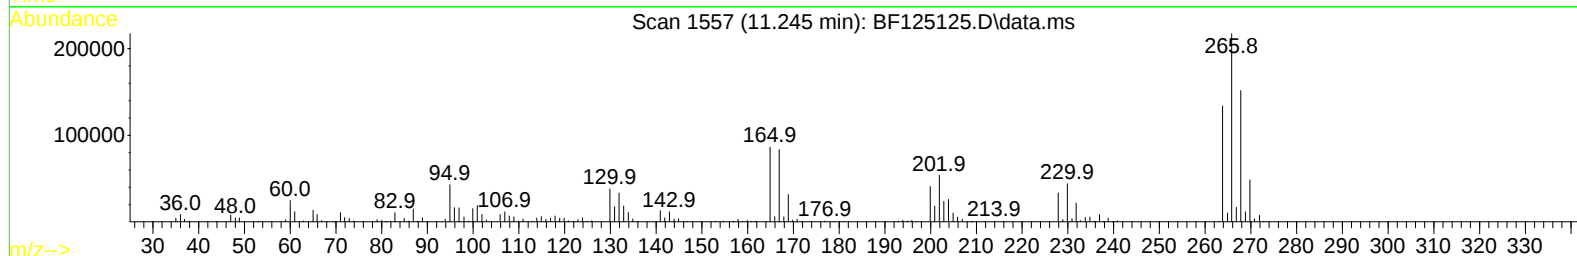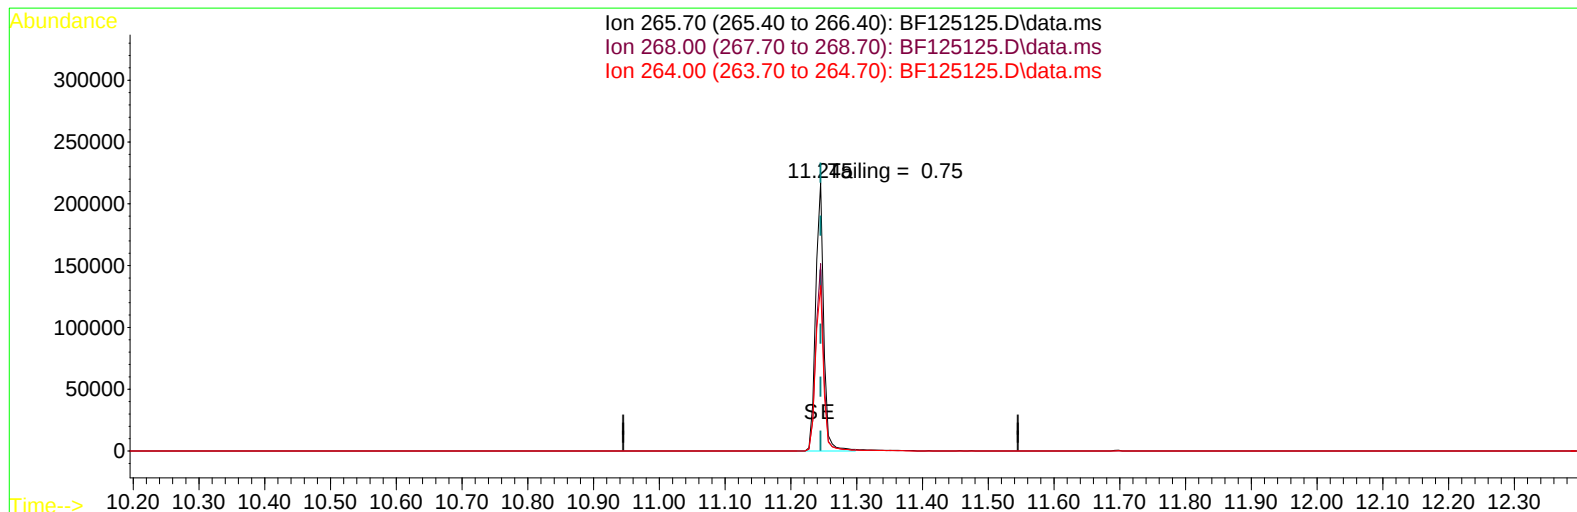

TIC: BF125125.D\data.ms

(70) Pentachlorophenol (C)

11.245min (-0.000) 32883.56 ng




response 186669

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	69.82
264.00	69.90	61.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082021\
Data File : BF125125.D
Acq On : 20 Aug 2021 9:09
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 20 10:53:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 17:03:50 2021
Response via : Initial Calibration

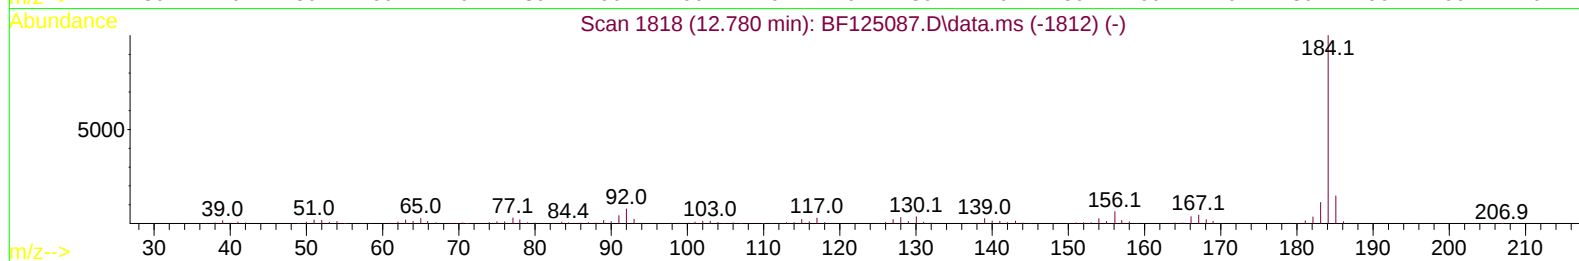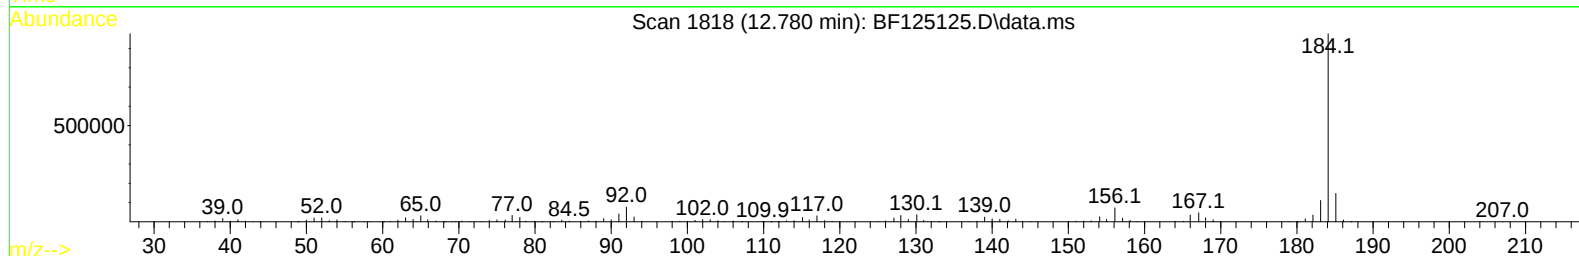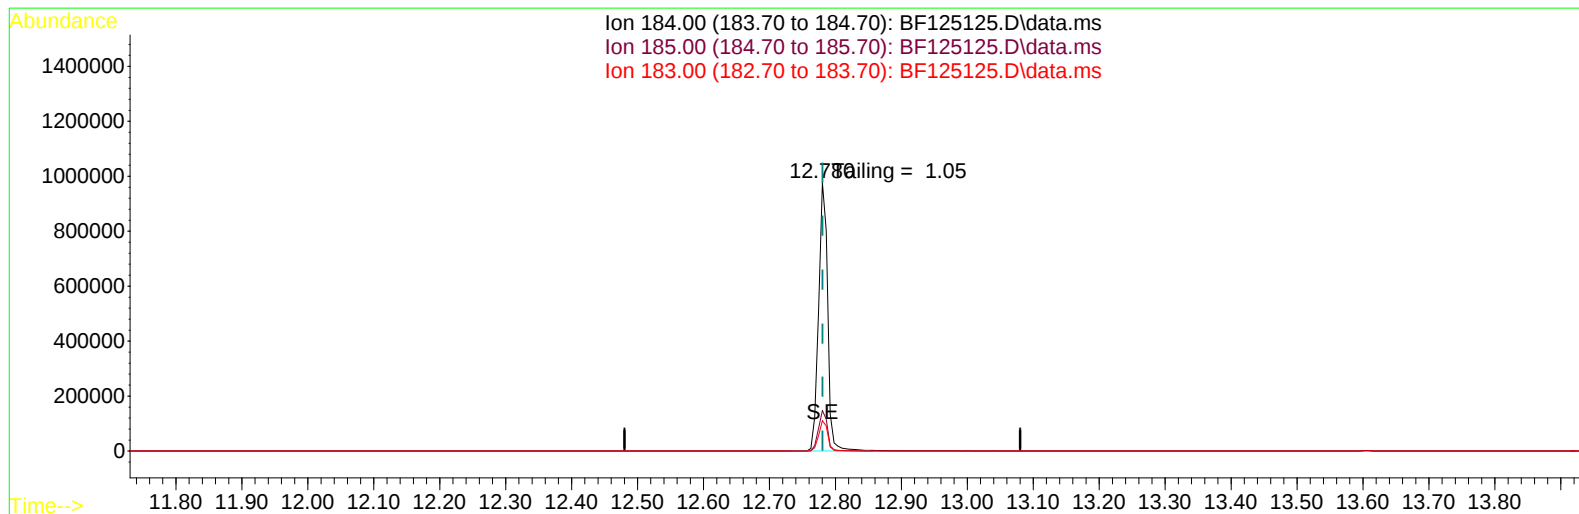

TIC: BF125125.D\data.ms

(77) Benzidine

12.780min (-0.000) 0.00 ng

response 940656

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	15.08
183.00	10.10	11.36
0.00	0.00	0.00