

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082115\
 Data File : BF081156.D
 Acq On : 21 Aug 2015 20:47
 Operator : UM/IZ
 Sample : G3363-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Aug 21 23:31:34 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 21 23:26:22 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.55	152	60149	20.00	ng	-0.01
21) Naphthalene-d8	7.84	136	252276	20.00	ng	0.00
38) Acenaphthene-d10	9.58	164	112528	20.00	ng	-0.01
63) Phenanthrene-d10	11.05	188	238894	20.00	ng	0.00
75) Chrysene-d12	13.66	240	166765	20.00	ng	-0.01
86) Perylene-d12	15.00	264	130677	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.13	112	484439	121.14	ng	0.02
7) Phenol-d6	6.21	99	560405	107.40	ng	0.00
23) Nitrobenzene-d5	7.12	82	425956	77.13	ng	-0.01
41) 2,4,6-Tribromophenol	10.37	330	126870	130.06	ng	0.00
44) 2-Fluorobiphenyl	8.92	172	709548	82.62	ng	-0.01
78) Terphenyl-d14	12.64	244	751662	96.63	ng	0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.12	70	55772	15.43	ng	# 70
50) 2,6-Dinitrotoluene	9.58	165	14449	7.26	ng	# 22
56) 2,4-Dinitrotoluene	9.58	165	14449	5.48	ng	# 17
66) 4-Bromophenyl-phenylether	10.37	248	10231	4.36	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082115\
Data File : BF081156.D
Acq On : 21 Aug 2015 20:47
Operator : UM/IZ
Sample : G3363-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Aug 21 23:31:34 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 21 23:26:22 2015
Response via : Initial Calibration

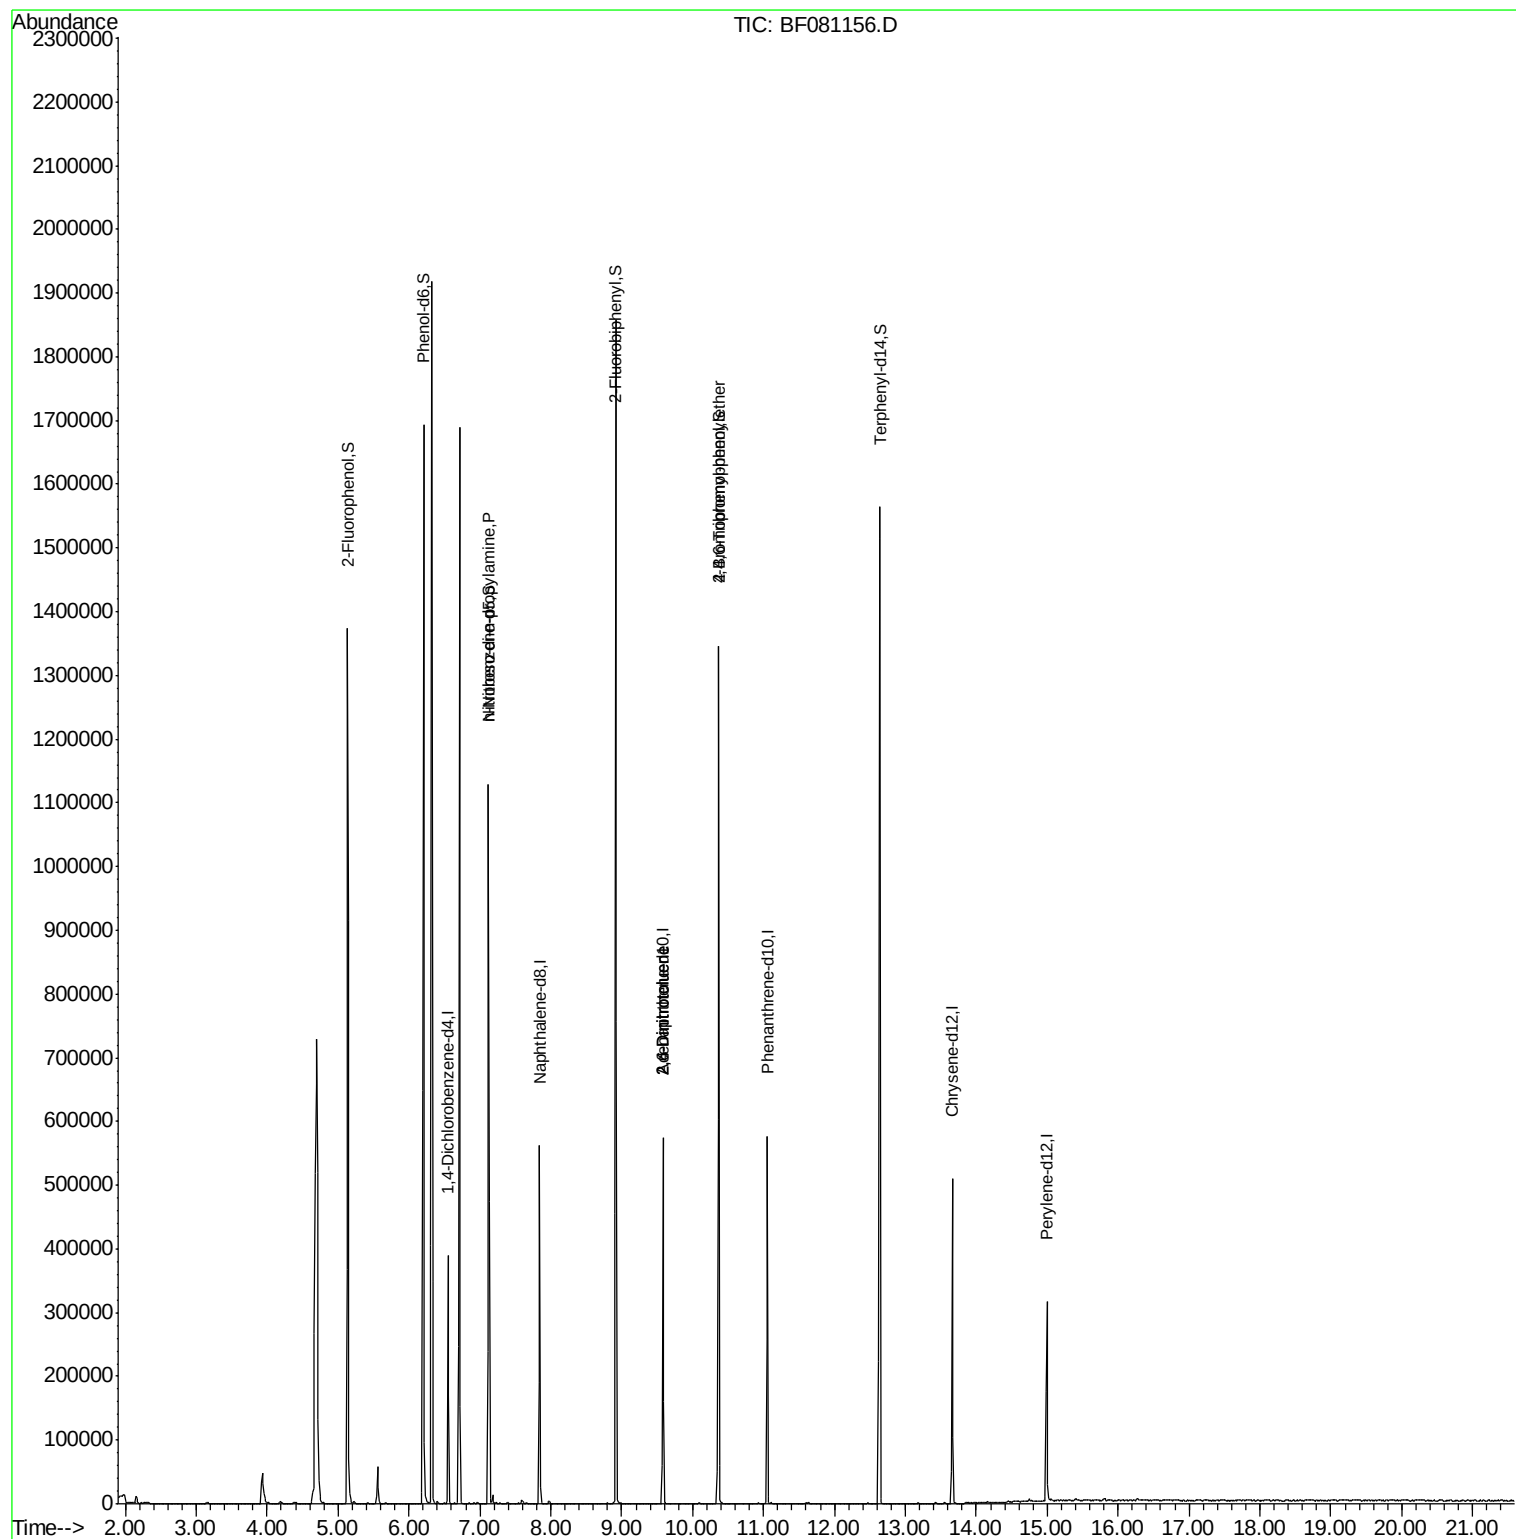

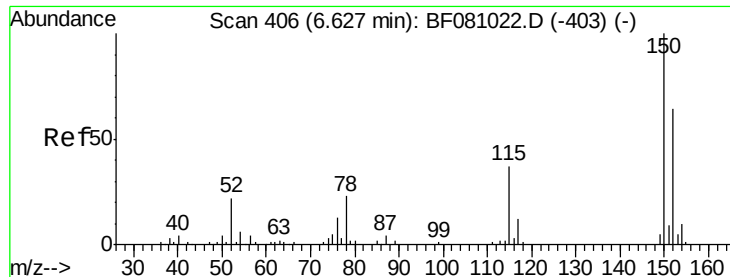


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.55 min Scan# 408
Delta R.T. -0.01 min
Lab File: BF081156.D
Acq: 21 Aug 2015 20:47

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 60149
Ion Ratio Lower Upper
152 100
150 157.9 123.8 185.6
115 71.8 52.1 78.1

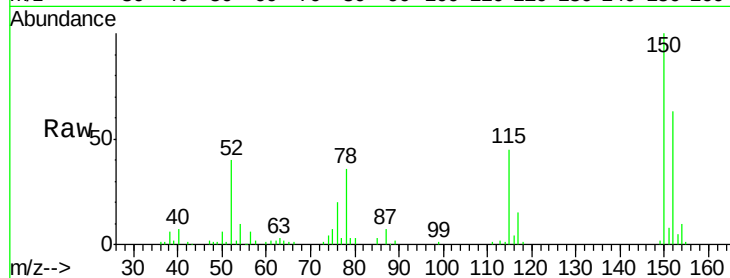


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

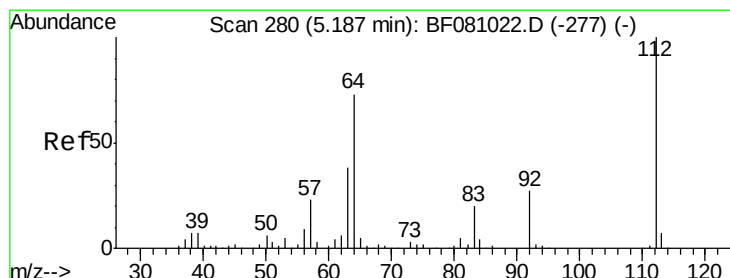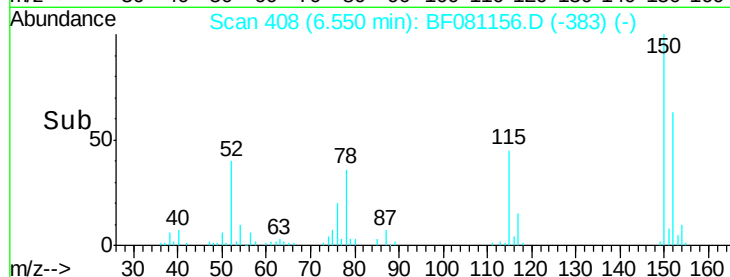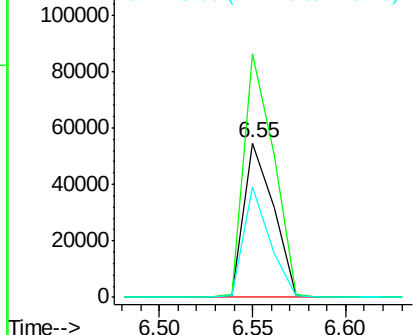



#5


2-Fluorophenol
Concen: 121.14 ng
RT: 5.13 min Scan# 284
Delta R.T. 0.02 min
Lab File: BF081156.D
Acq: 21 Aug 2015 20:47

Tgt Ion:112 Resp: 484439
Ion Ratio Lower Upper
112 100
64 79.1 66.9 100.3
63 42.8 38.1 57.1

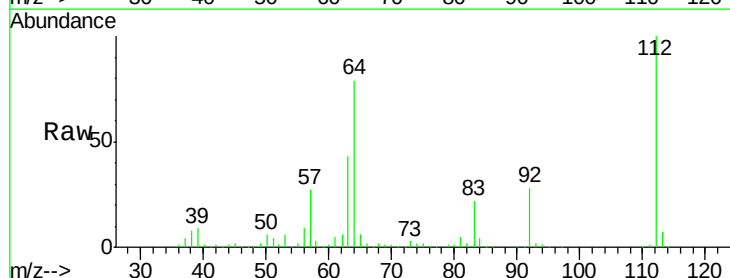

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

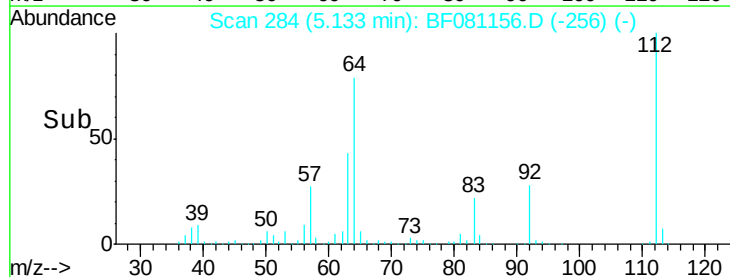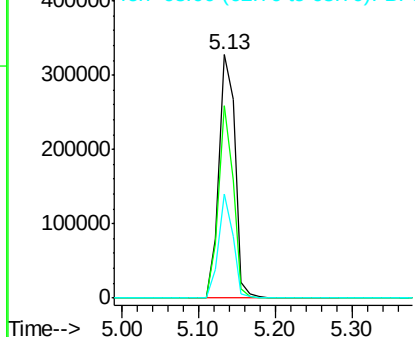

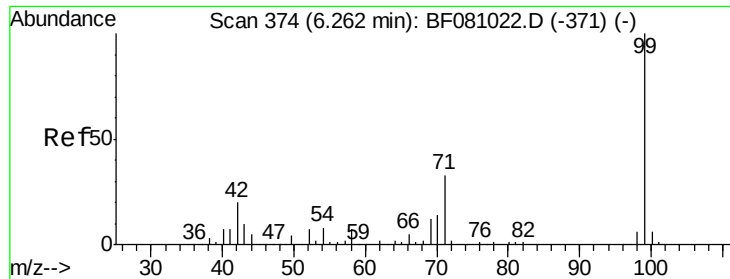

#7

Phenol-d6

Concen: 107.40 ng

RT: 6.21 min Scan# 378

Delta R.T. -0.00 min

Lab File: BF081156.D

Acq: 21 Aug 2015 20:47

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 560405

Ion Ratio Lower Upper

99 100

42 23.4 19.6 29.4




71 36.6 31.2 46.8

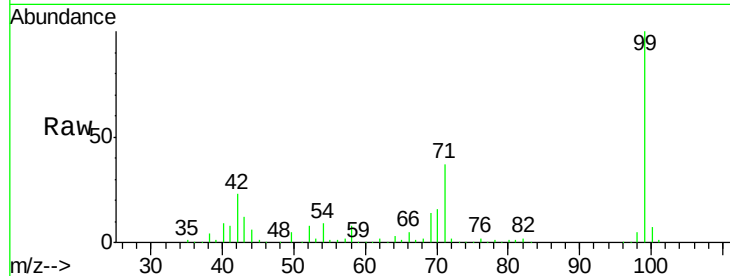

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

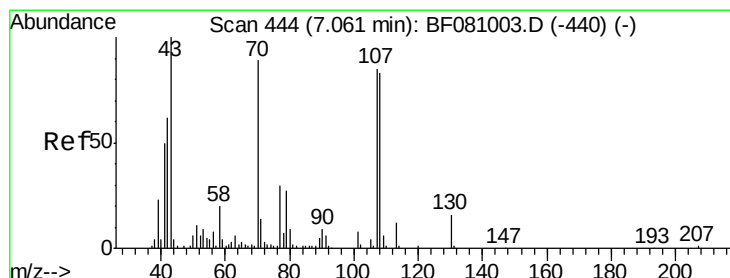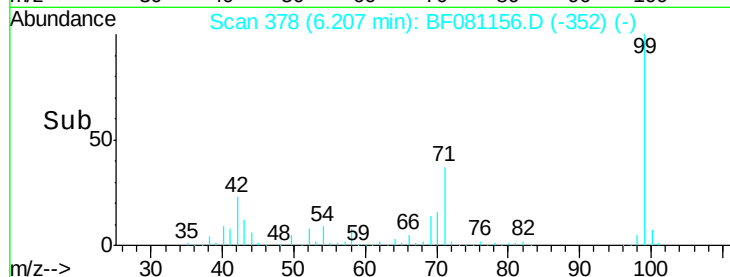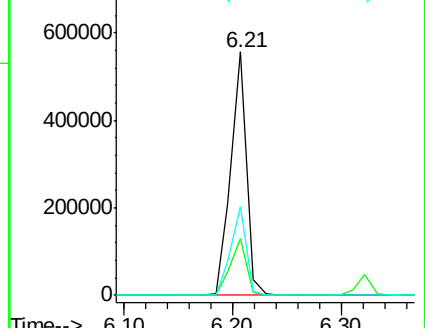

#19

n-Nitroso-di-n-propylamine

Concen: 15.43 ng

RT: 7.12 min Scan# 458

Delta R.T. 0.13 min

Lab File: BF081156.D

Acq: 21 Aug 2015 20:47

Tgt Ion: 70 Resp: 55772


Ion Ratio Lower Upper

70 100

42 55.2 65.0 97.4#

101 0.0 7.4 11.2#

130 2.0 13.0 19.4#


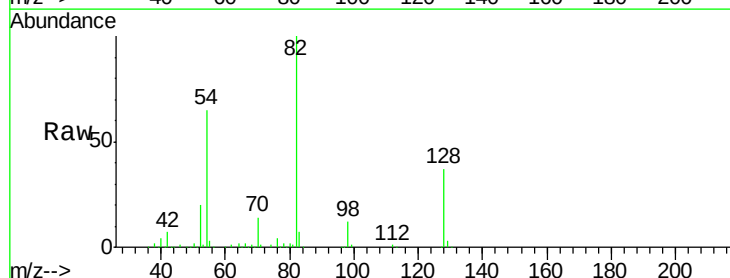



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0



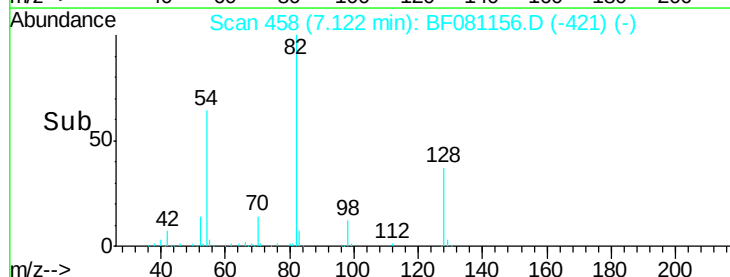
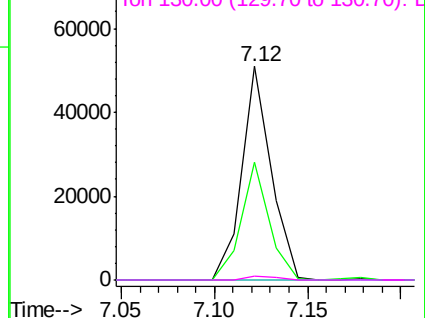


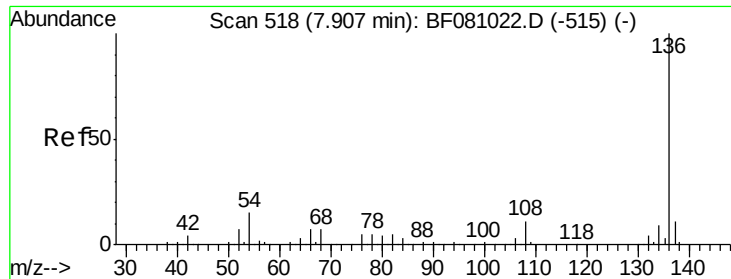

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.84 min Scan# 521
Delta R.T. -0.00 min
Lab File: BF081156.D
Acq: 21 Aug 2015 20:47




Instrument :
BNA_F
ClientSampleId :


Tot Ion:	136	Resp:	252276
Ion	Ratio	Lower	Upper
136	100		
137	10.4	8.2	12.2
54	10.3	7.7	11.5
68	5.5	3.4	5.2#

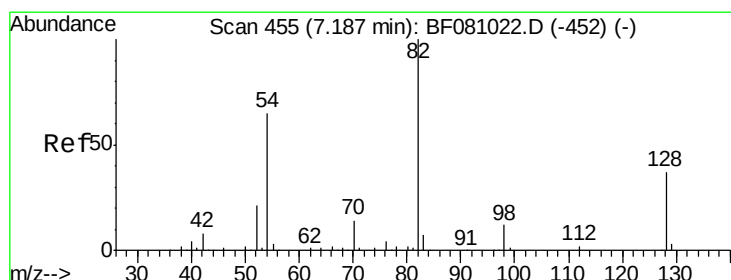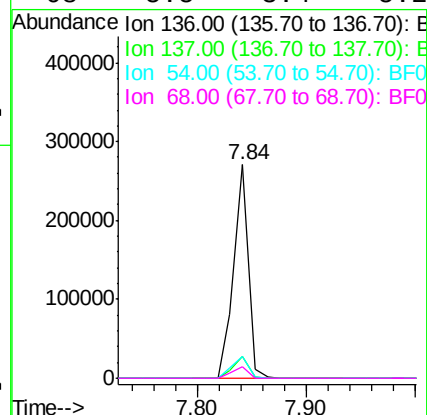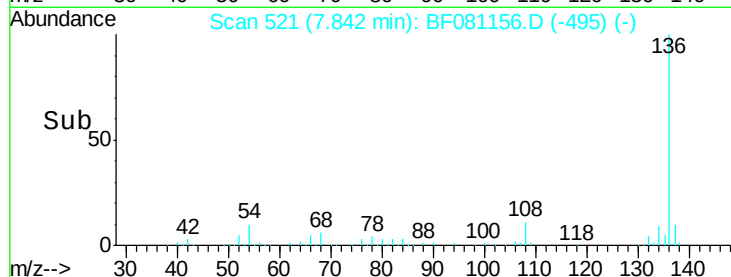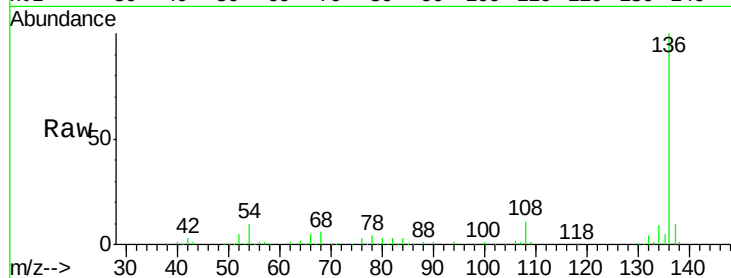

#23
Nitrobenzene-d5
Concen: 77.13 ng
RT: 7.12 min Scan# 458
Delta R.T. -0.01 min
Lab File: BF081156.D
Acq: 21 Aug 2015 20:47

Tgt Ion:	82	Resp:	425956
Ion	Ratio	Lower	Upper
82	100		
128	37.0	28.6	42.8
54	65.3	55.1	82.7

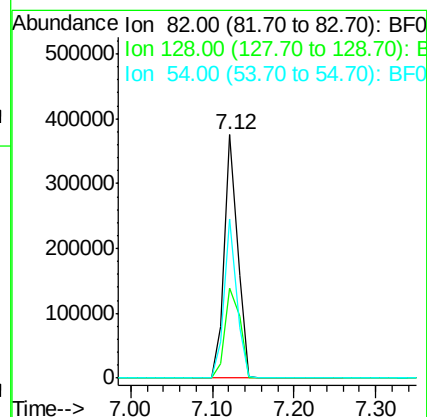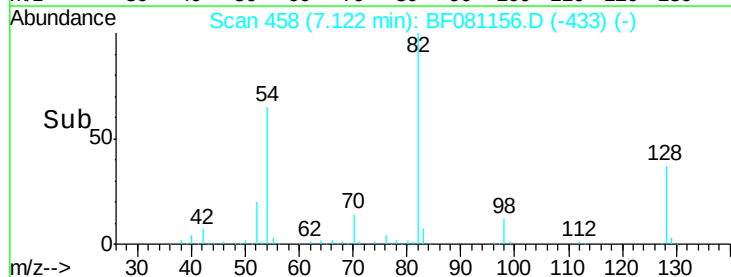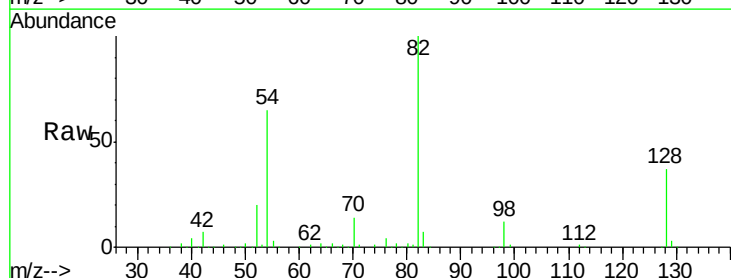


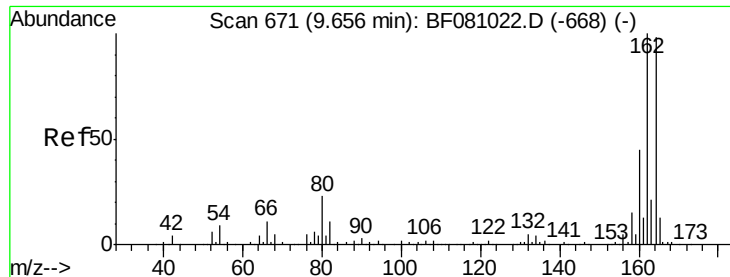




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.58 min Scan# 673
 Delta R.T. -0.01 min
 Lab File: BF081156.D
 Acq: 21 Aug 2015 20:47

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:164 Resp: 112528
 Ion Ratio Lower Upper
 164 100
 162 102.7 83.8 125.8
 160 46.7 39.8 59.8

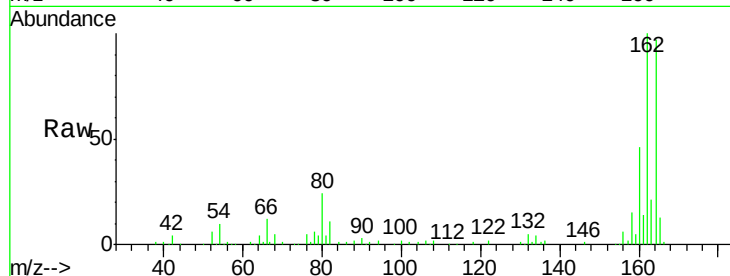


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

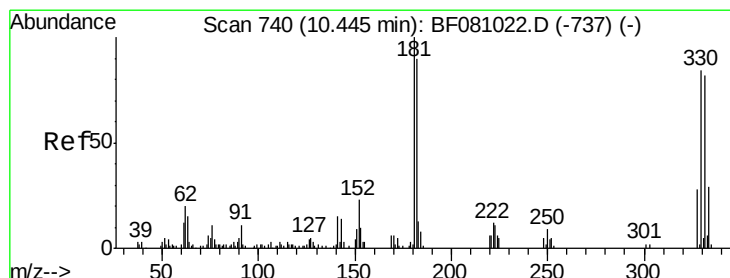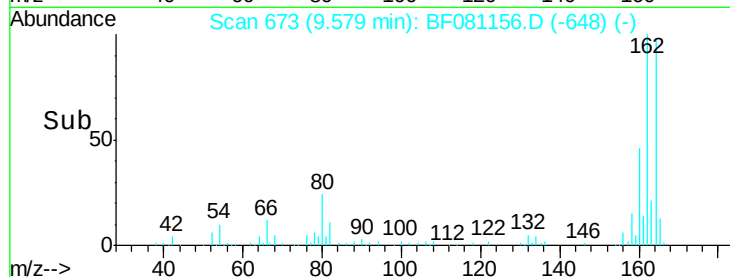
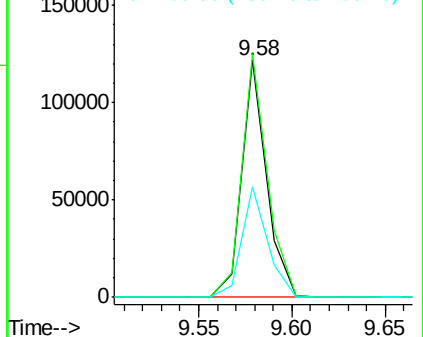



#41
 2,4,6-Tribromophenol
 Concen: 130.06 ng
 RT: 10.37 min Scan# 742
 Delta R.T. -0.00 min
 Lab File: BF081156.D
 Acq: 21 Aug 2015 20:47

Tgt Ion:330 Resp: 126870
 Ion Ratio Lower Upper
 330 100
 332 95.0 77.3 115.9
 141 55.7 44.9 67.3

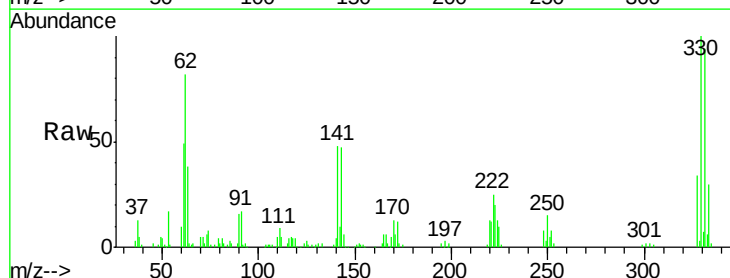

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



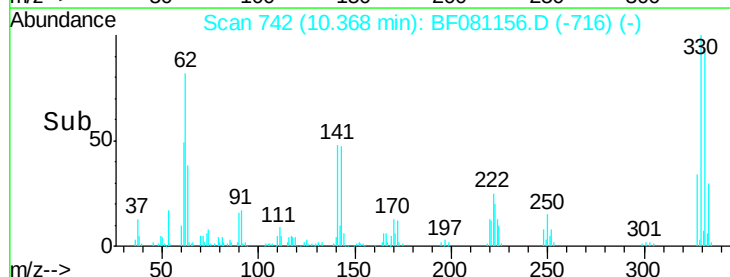
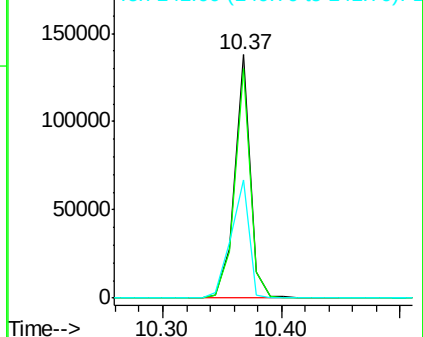


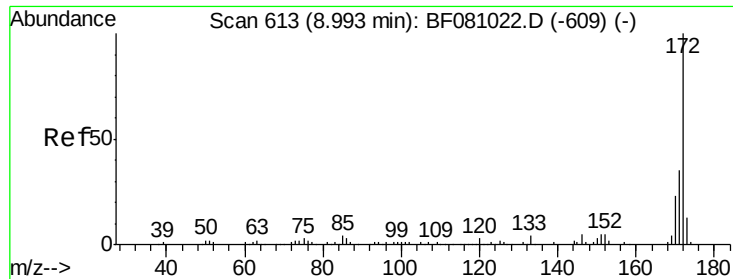

#44
2-Fluorobiphenyl
Concen: 82.62 ng
RT: 8.92 min Scan# 615
Delta R.T. -0.01 min
Lab File: BF081156.D
Acq: 21 Aug 2015 20:47




Instrument :
BNA_F
ClientSampleId :


Tot Ion:172 Resp: 709548
Ion Ratio Lower Upper
172 100
171 35.3 28.9 43.3
170 24.3 19.4 29.2

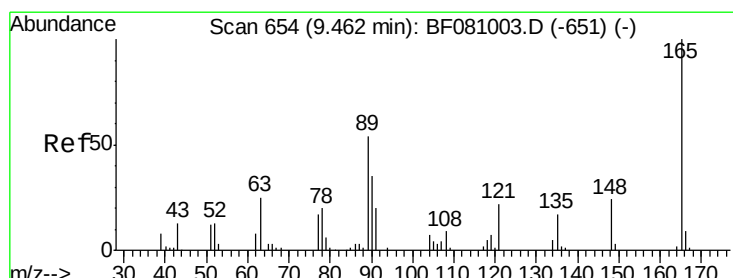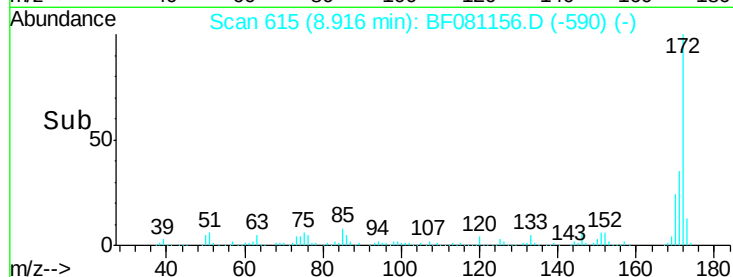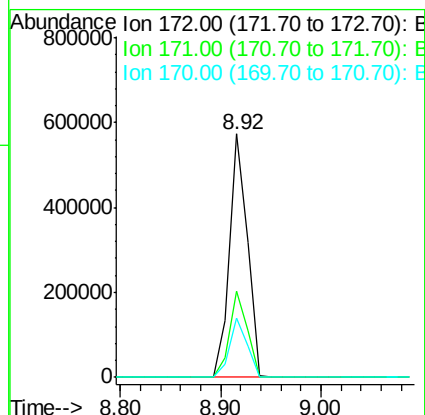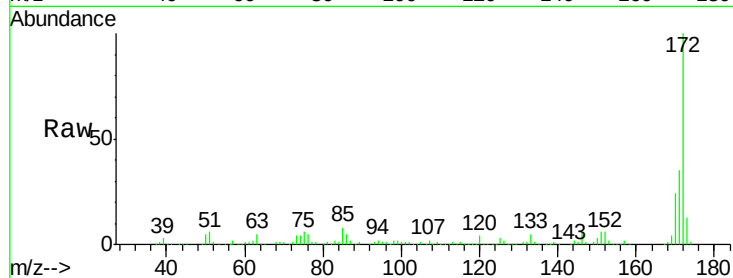

#50
2,6-Dinitrotoluene
Concen: 7.26 ng
RT: 9.58 min Scan# 673
Delta R.T. 0.19 min
Lab File: BF081156.D
Acq: 21 Aug 2015 20:47

Tgt Ion:165 Resp: 14449
Ion Ratio Lower Upper
165 100
63 2.1 49.5 74.3#
89 0.0 47.6 71.4#


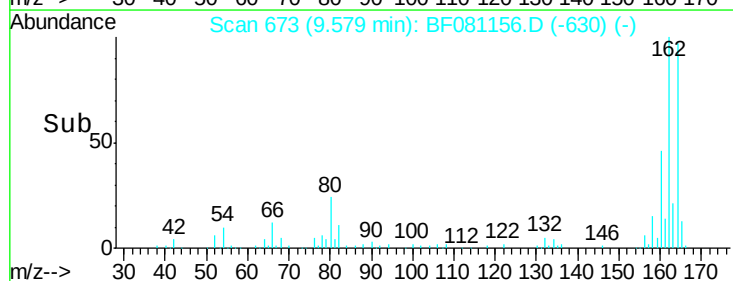
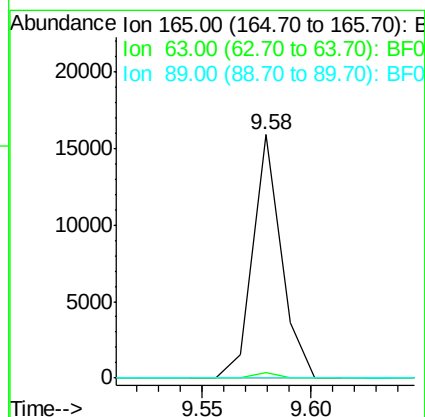
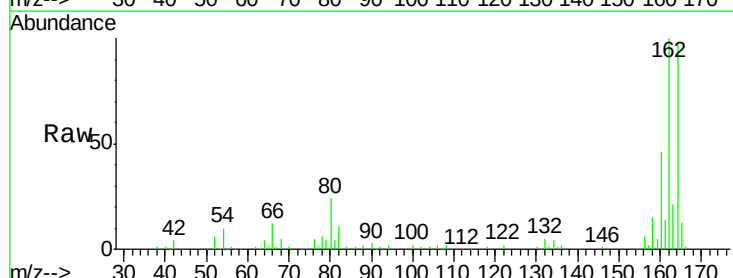


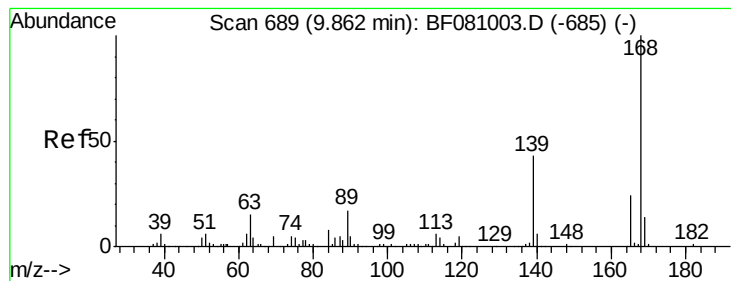

#56
 2,4-Dinitrotoluene
 Concen: 5.48 ng
 RT: 9.58 min Scan# 673
 Delta R.T. -0.21 min
 Lab File: BF081156.D
 Acq: 21 Aug 2015 20:47




Instrument :
 BNA_F
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
165	100		
63	2.1	52.2	78.4#
89	0.0	60.1	90.1#
182	0.0	1.8	2.6#

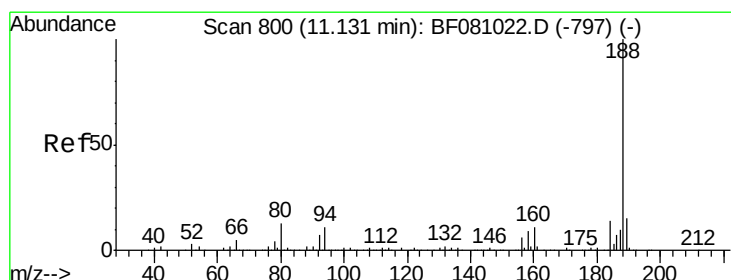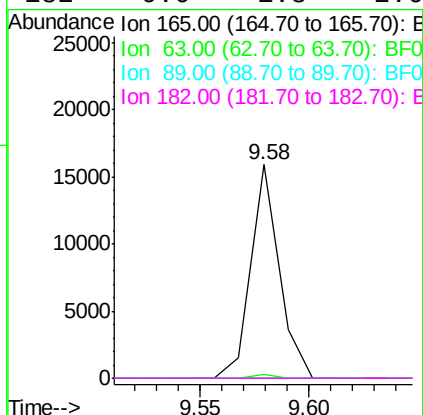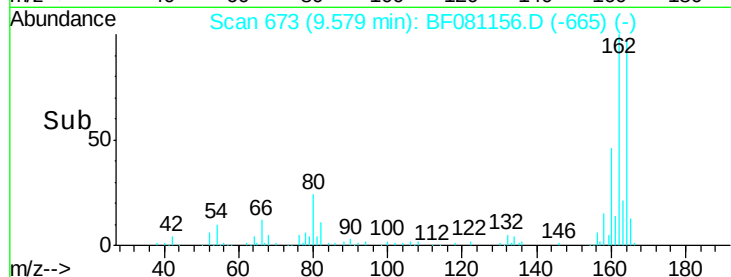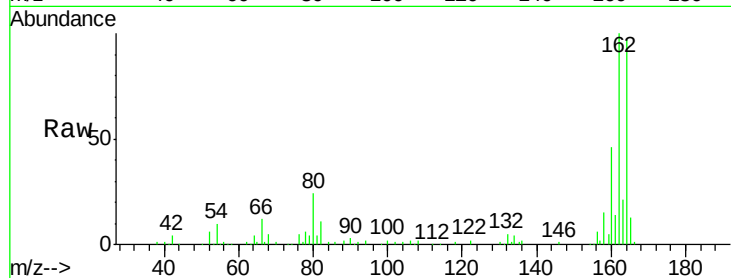

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.05 min Scan# 802
 Delta R.T. -0.00 min
 Lab File: BF081156.D
 Acq: 21 Aug 2015 20:47

Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.6	8.2	12.2#
80	7.6	9.5	14.3#

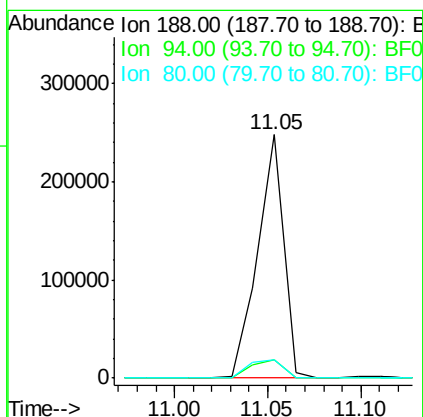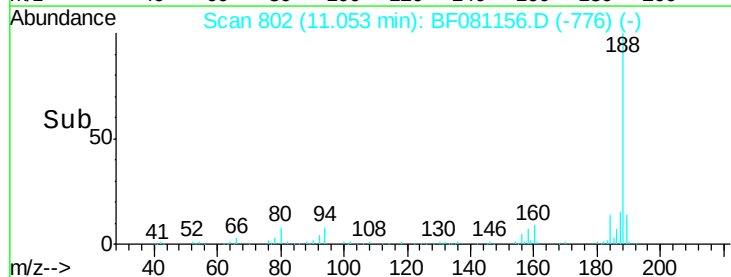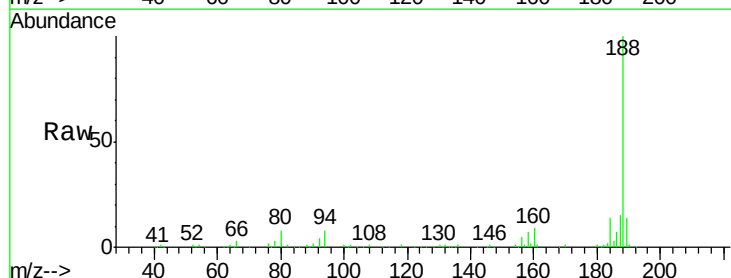


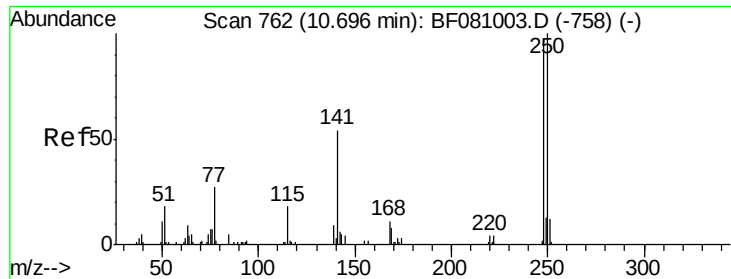




#66
4-Bromophenyl-phenylether
Concen: 4.36 ng
RT: 10.37 min Scan# 742
Delta R.T. -0.24 min
Lab File: BF081156.D
Acq: 21 Aug 2015 20:47

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 10231
Ion Ratio Lower Upper
248 100
250 192.2 77.8 116.6#
141 608.0 39.8 59.6#

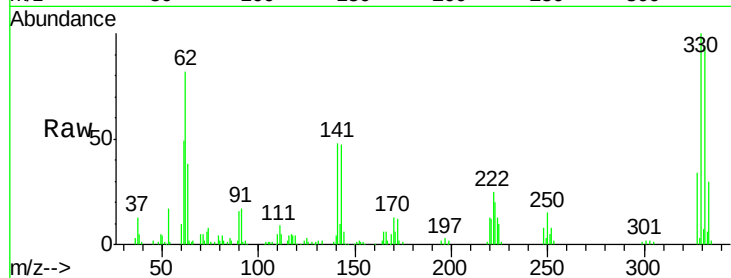


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

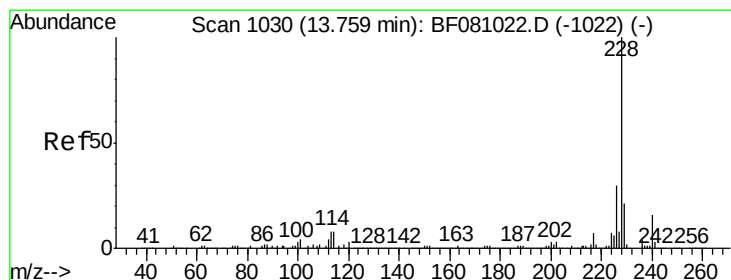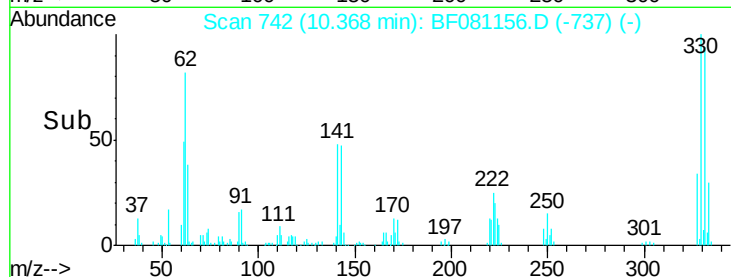
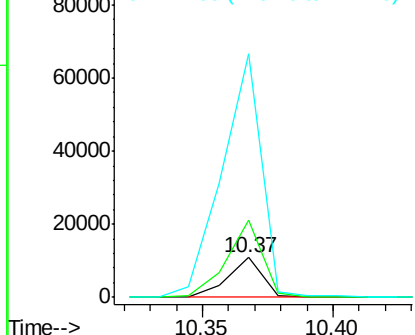



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.66 min Scan# 1030
Delta R.T. -0.01 min
Lab File: BF081156.D
Acq: 21 Aug 2015 20:47

Tgt Ion:240 Resp: 166765
Ion Ratio Lower Upper
240 100
120 13.9 5.6 8.4#
236 26.2 20.6 30.8

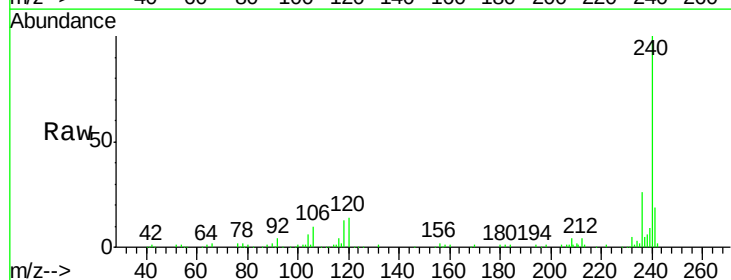

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

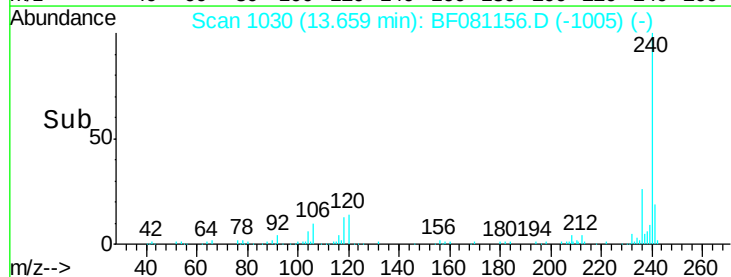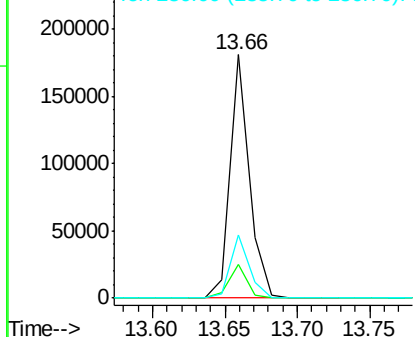


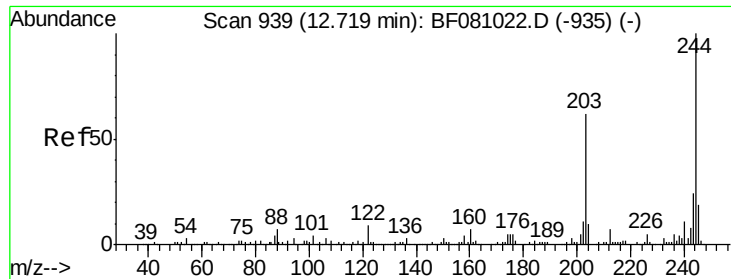




#78
 Terphenyl-d14
 Concen: 96.63 ng
 RT: 12.64 min Scan# 941
 Delta R.T. 0.01 min
 Lab File: BF081156.D
 Acq: 21 Aug 2015 20:47

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:244 Resp: 751662
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.8 8.8
 122 6.6 8.2 12.4#

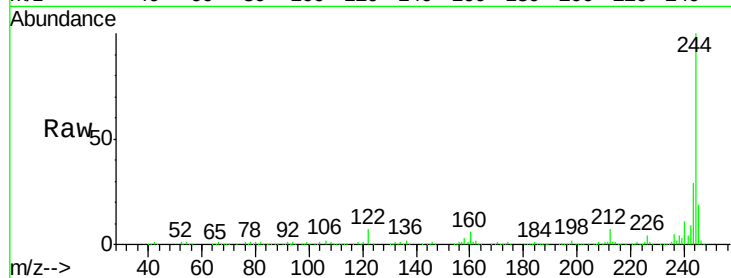


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

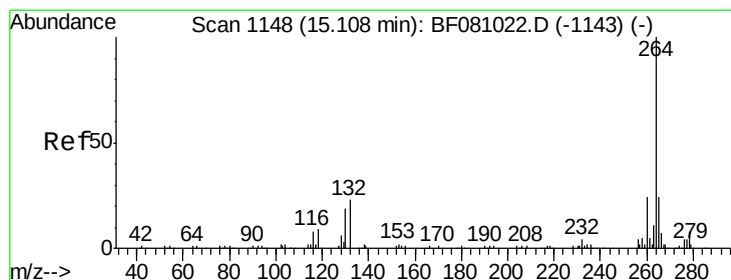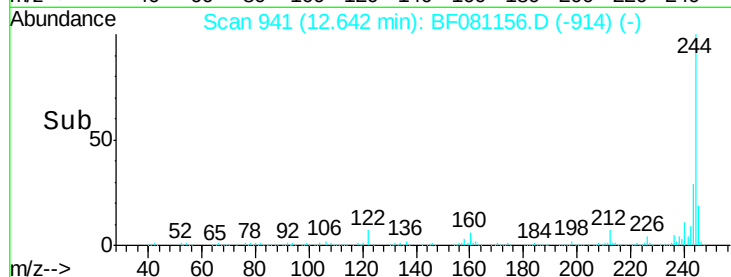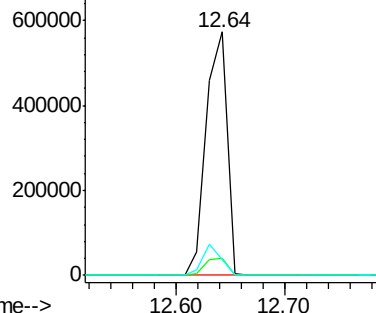

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.00 min Scan# 1147
 Delta R.T. -0.00 min
 Lab File: BF081156.D
 Acq: 21 Aug 2015 20:47

Tgt Ion:264 Resp: 130677
 Ion Ratio Lower Upper
 264 100
 260 23.8 19.6 29.4
 265 20.9 17.5 26.3

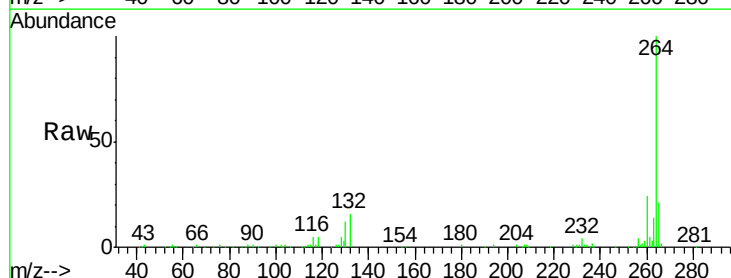

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

