
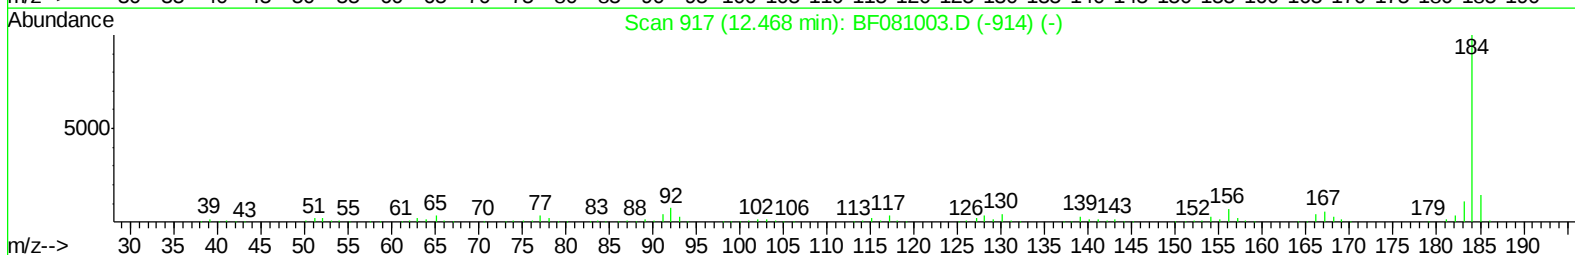
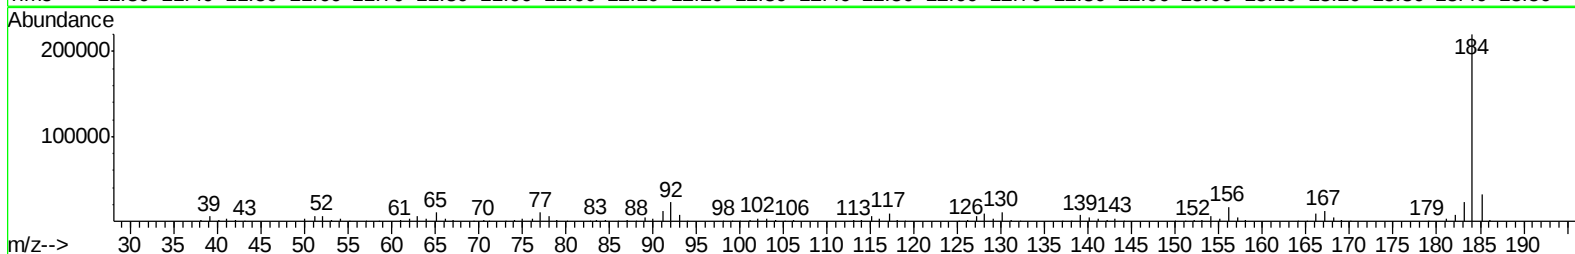


Data Path : Z:\HPCHEM1\BNA_F\Data\BF082115\
Data File : BF081144.D
Acq On : 21 Aug 2015 14:32
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 03:59:39 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 03:32:45 2015
Response via : Initial Calibration

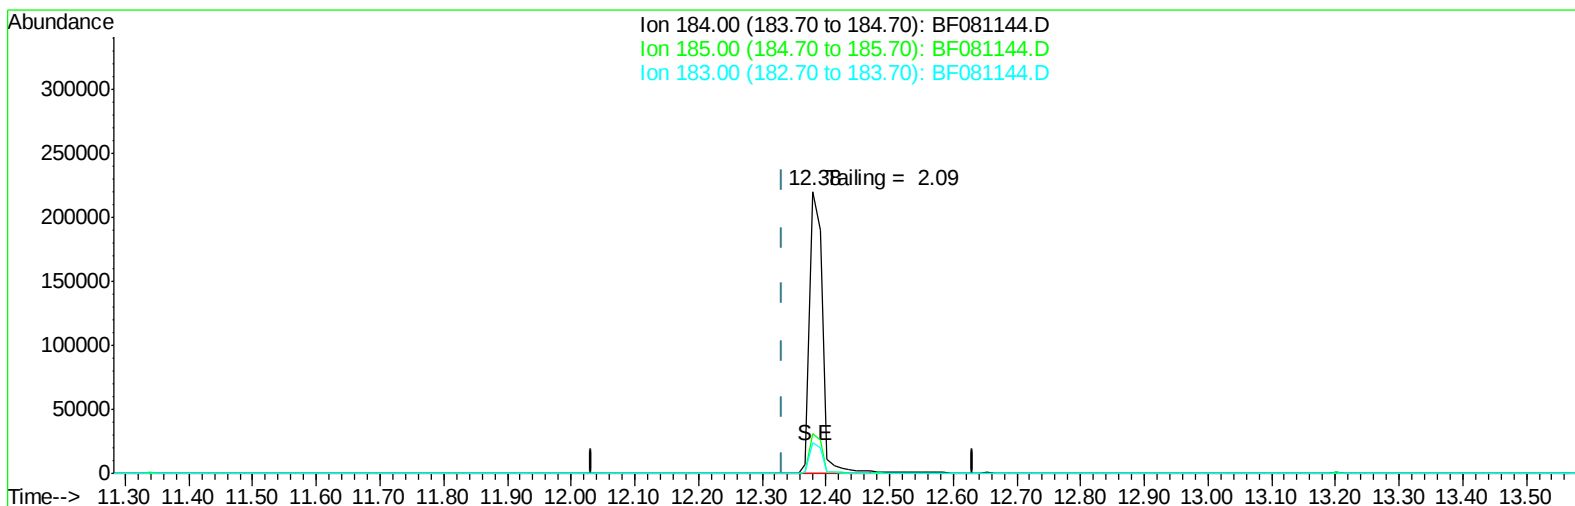

TIC: BF081144.D

(76) Benzidine




12.379min (+0.047) 0.00ng

response 313097

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.23
183.00	11.10	10.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF082115\
Data File : BF081144.D
Acq On : 21 Aug 2015 14:32
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 03:59:39 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 03:32:45 2015
Response via : Initial Calibration

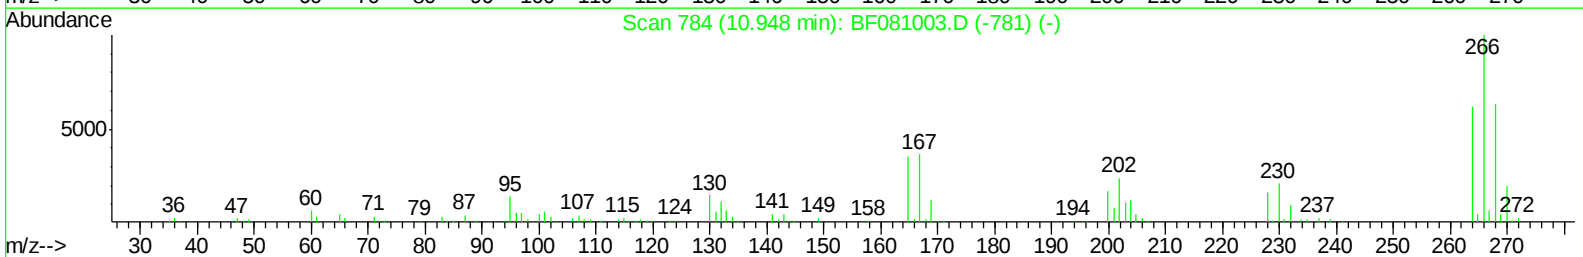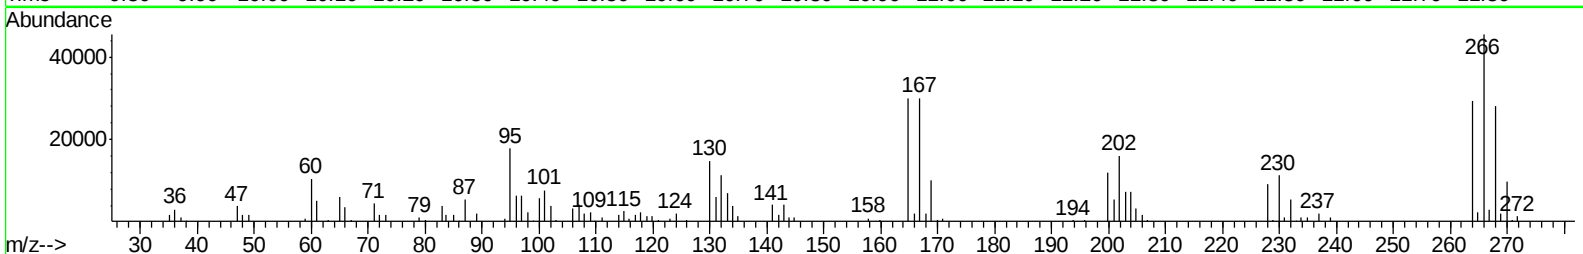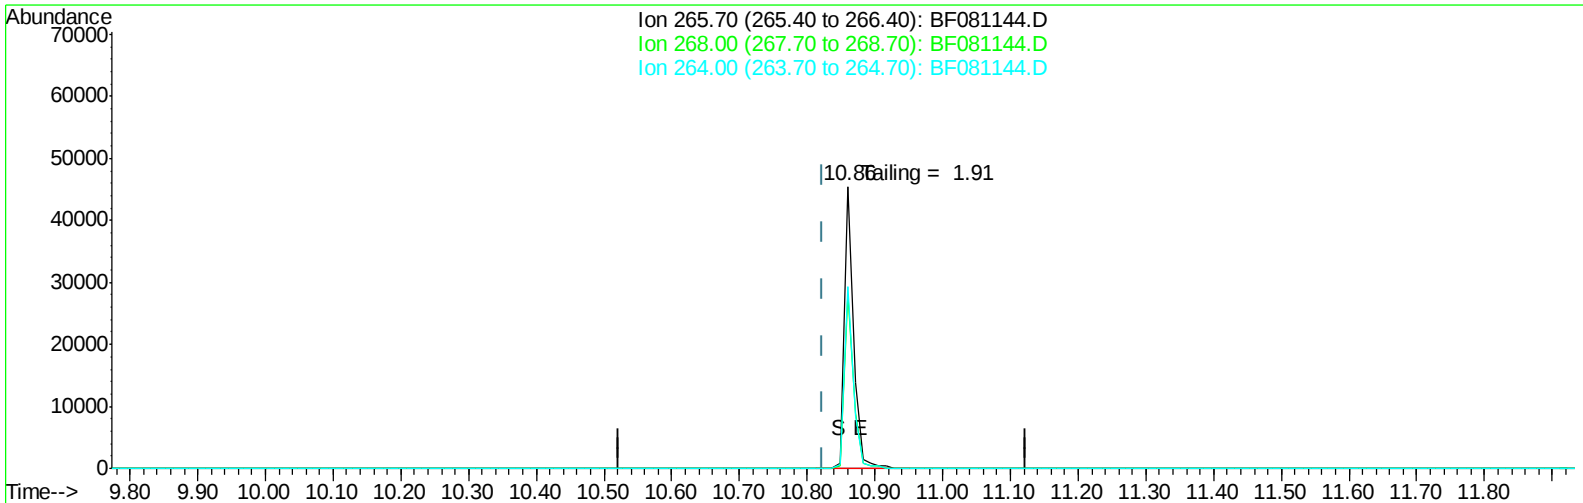

TIC: BF081144.D

(69) Pentachlorophenol (C)

10.859min (+0.036) 0.00ng

response 43353

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	61.79
264.00	63.20	64.38
0.00	0.00	0.00