


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082115\
Data File : BF081144.D
Acq On : 21 Aug 2015 14:32
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 21 23:26:22 2015

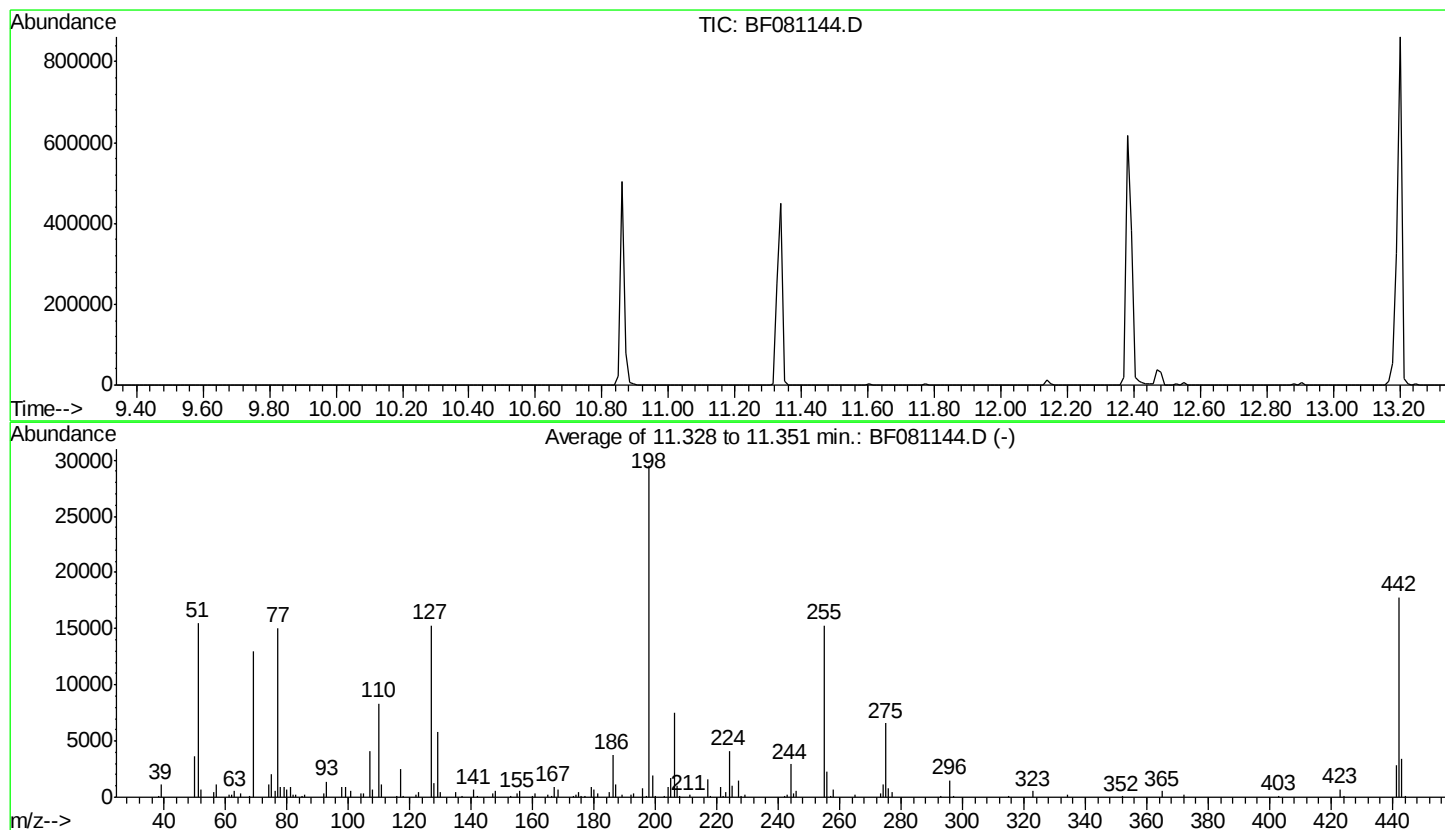

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	15522	PASS
68	69	0.00	2	1.1	145	PASS
69	198	0.00	100	43.9	12954	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.8	15288	PASS
197	198	0.00	2	0.5	147	PASS
198	198	100	100	100.0	29511	PASS
199	198	5	9	6.7	1990	PASS
275	198	10	60	22.3	6583	PASS
365	198	1	100	1.9	566	PASS
441	442	0.01	24	16.1	2857	PASS
442	198	50	100	60.3	17795	PASS
443	442	15	24	19.3	3440	PASS