
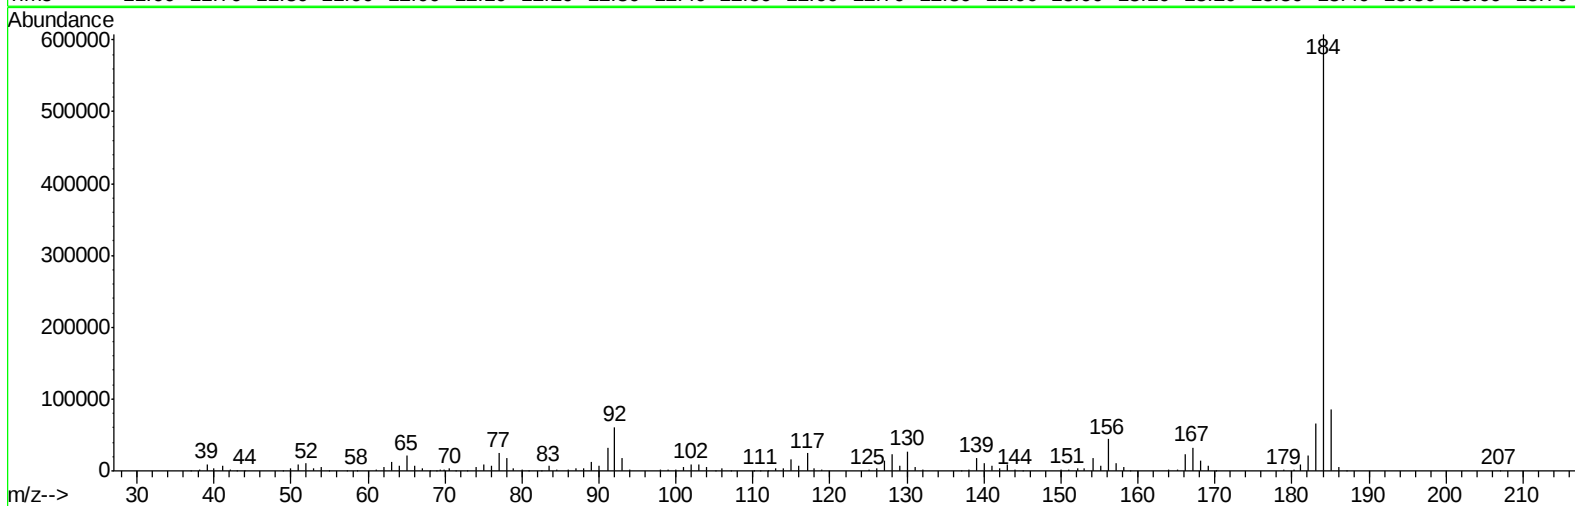


Data Path : Z:\HPCHEM1\BNA F\DATA\BF082117\
Data File : BF097895.D
Acq On : 21 Aug 2017 9:59
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 02:06:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

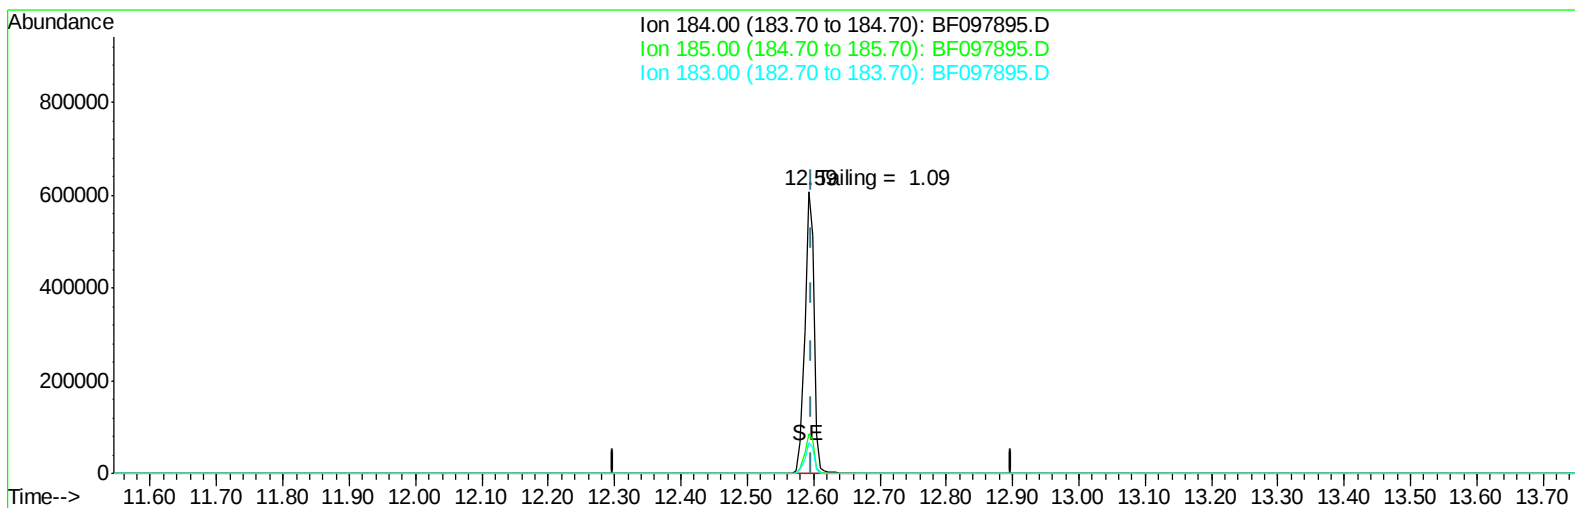

TIC: BF097895.D

(76) Benzidine



12.592min (-0.006) 2567.89ng

response 571182

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.21#
183.00	12.20	10.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082117\
Data File : BF097895.D
Acq On : 21 Aug 2017 9:59
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 02:06:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

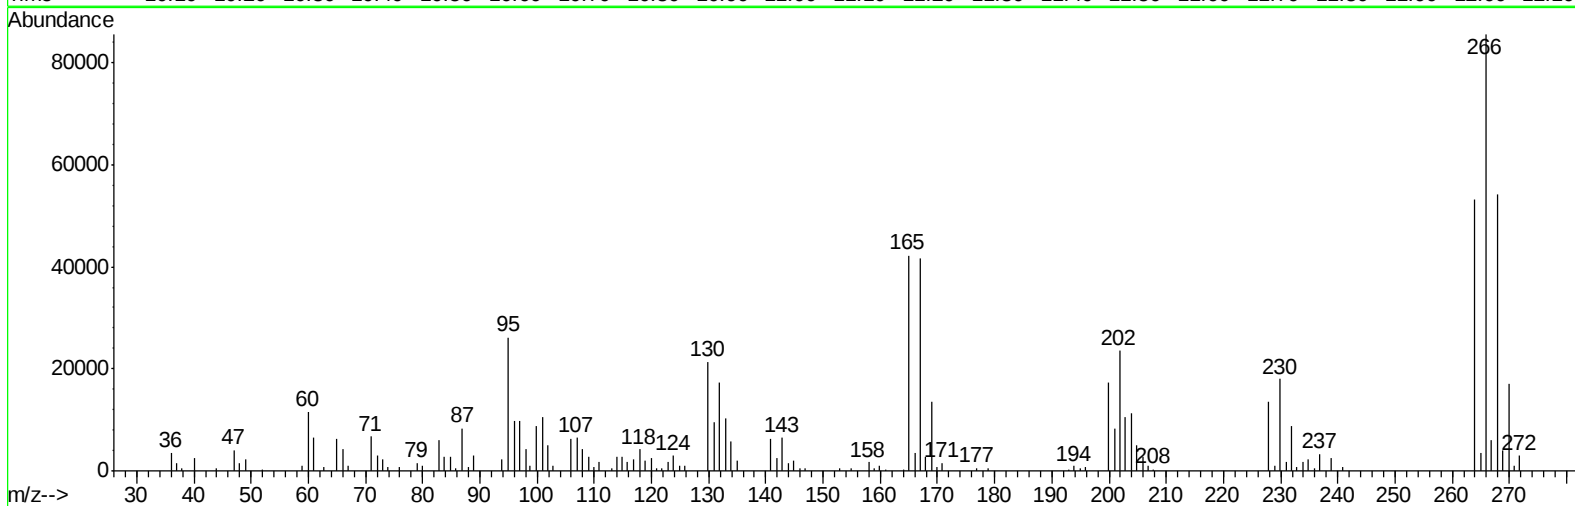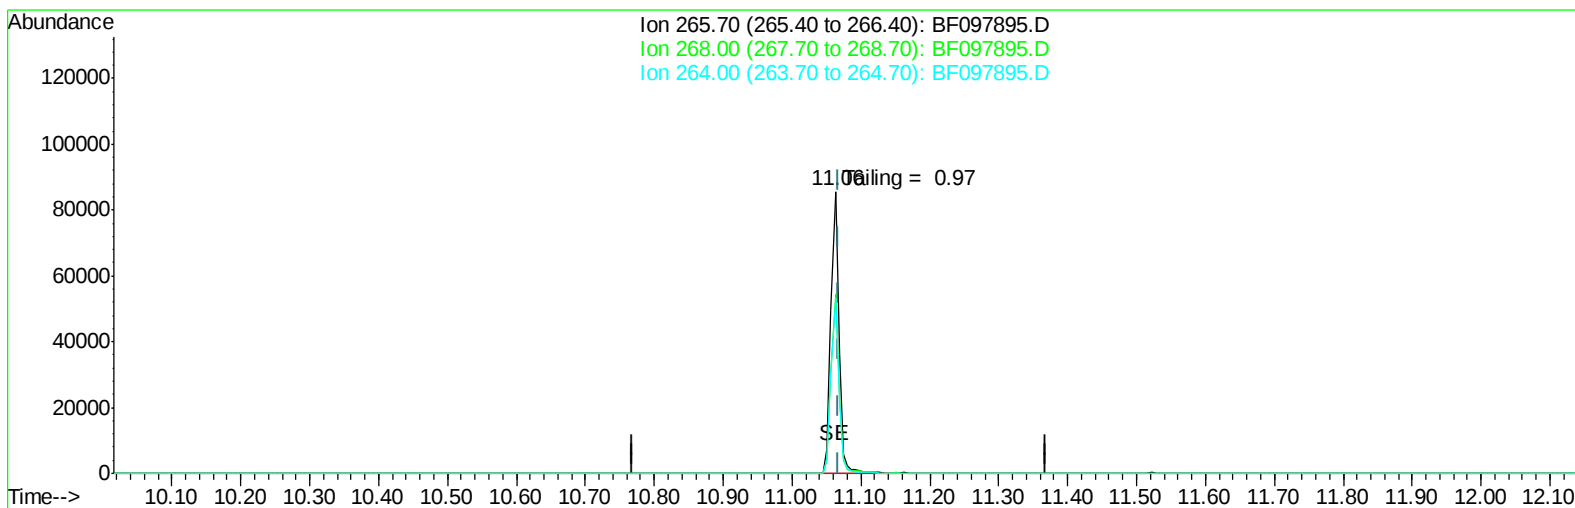

TIC: BF097895.D

(69) Pentachlorophenol (C)

11.063min (-0.006) 1046.52ng

response 67871

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.49
264.00	64.60	62.26
0.00	0.00	0.00