
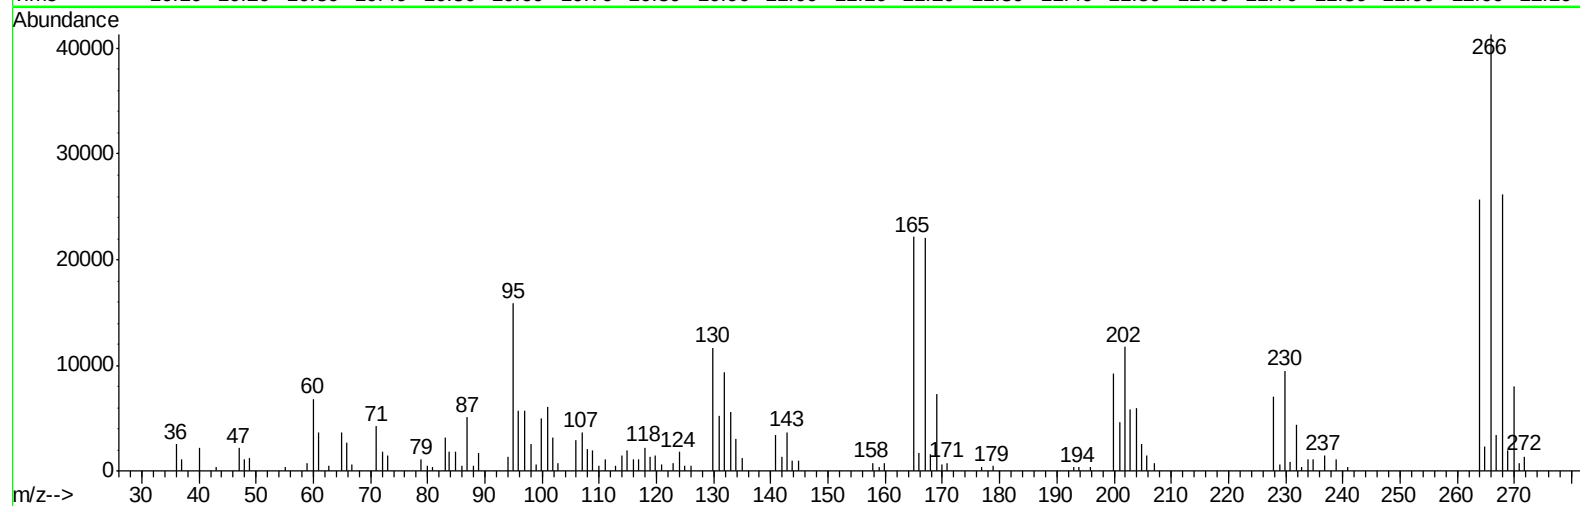


Data Path : Z:\HPCHEM1\BNA F\DATA\BF082117\
Data File : BF097934.D
Acq On : 22 Aug 2017 5:09
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 08:02:37 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

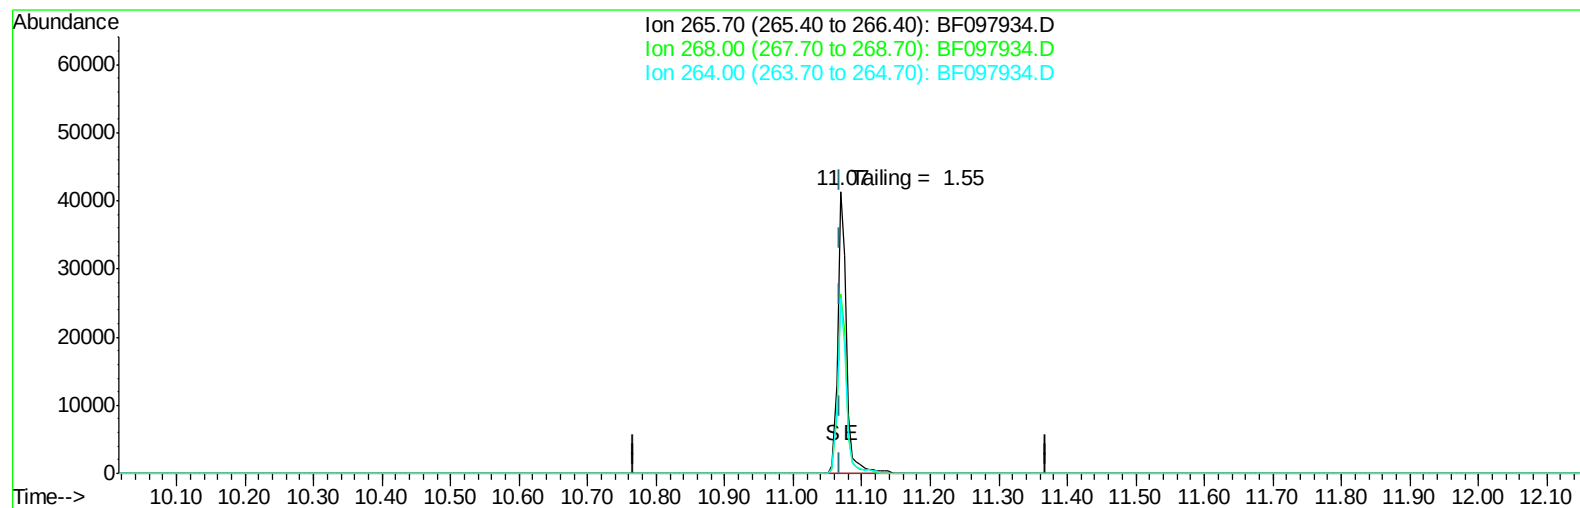

TIC: BF097934.D

(69) Pentachlorophenol (C)



11.069min (+0.000) 949.63ng

response 36950

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.47
264.00	64.60	62.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082117\
Data File : BF097934.D
Acq On : 22 Aug 2017 5:09
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 08:02:37 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

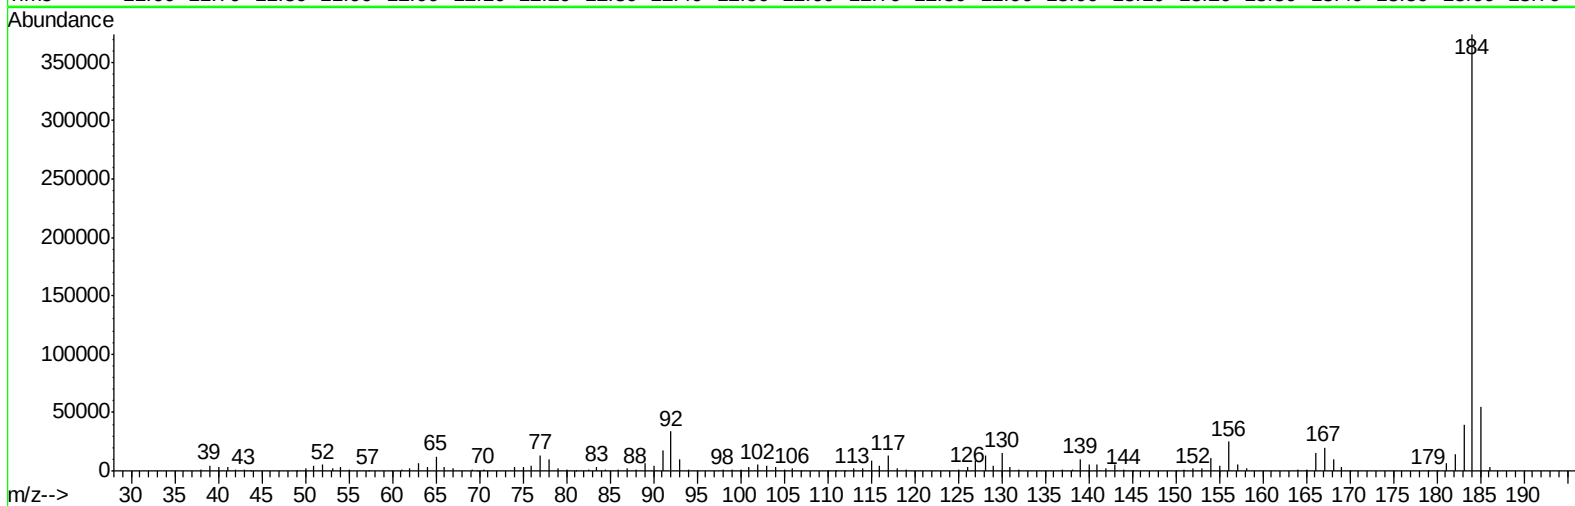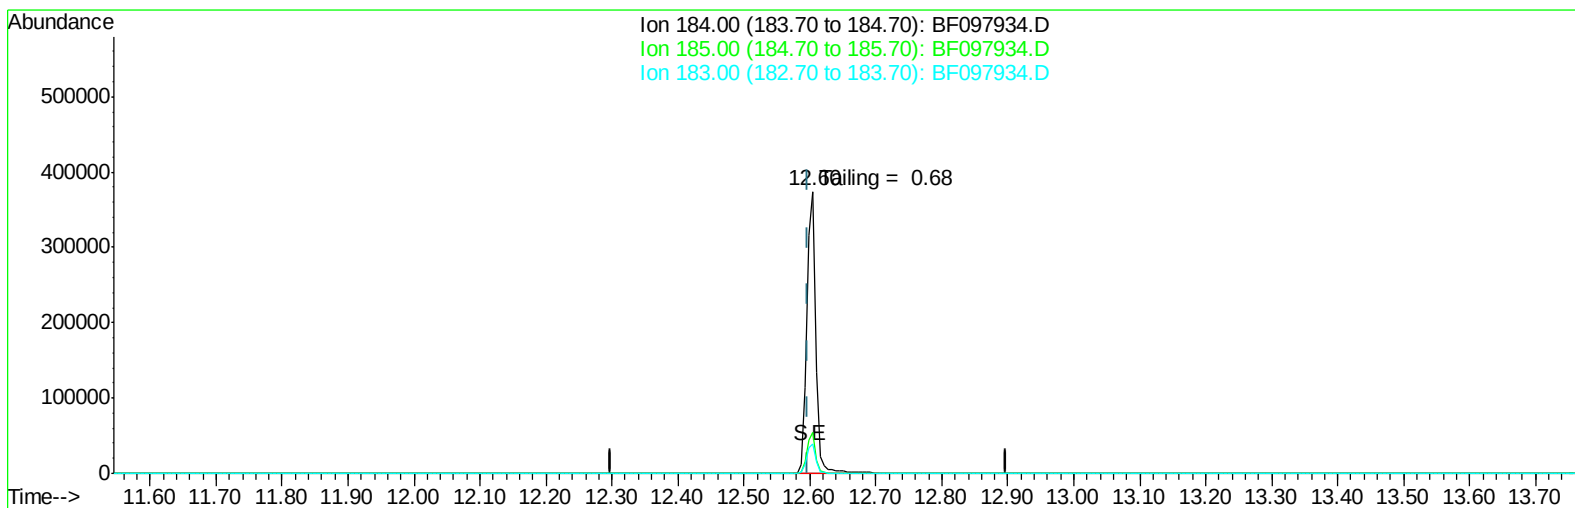

TIC: BF097934.D

(76) Benzidine

12.604min (+0.006) 2723.44ng

response 361200

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.61#
183.00	12.20	10.67
0.00	0.00	0.00