

Data Path : U:\HPCHEM1\BNA F\DATA\BF082117\
 Data File : BF097947.D
 Acq On : 22 Aug 2017 11:18
 Operator : SJ/JU
 Sample : I4900-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CONTROL-HOUSE-STAIR

Quant Time: Aug 22 13:18:26 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 21 15:59:04 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	104513	20.00	ng	0.00
21) Naphthalene-d8	8.03	136	379949	20.00	ng	0.00
38) Acenaphthene-d10	9.78	164	140479	20.00	ng	0.00
63) Phenanthrene-d10	11.26	188	244985	20.00	ng	0.00
75) Chrysene-d12	13.89	240	207881	20.00	ng	0.00
86) Perylene-d12	15.32	264	136118	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	461906	67.23	ng	0.00
7) Phenol-d6	6.38	99	811694	86.94	ng	0.00
23) Nitrobenzene-d5	7.31	82	543684	77.74	ng	-0.01
41) 2,4,6-Tribromophenol	10.57	330	56851	46.64	ng	0.00
44) 2-Fluorobiphenyl	9.11	172	764199	79.92	ng	0.00
78) Terphenyl-d14	12.85	244	593133	59.50	ng	0.00
Target Compounds						
10) Phenol	6.39	94	30115	2.758	ng	96
49) Dimethylphthalate	9.50	163	126202	12.290	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA F\DATA\BF082117\
Data File : BF097947.D
Acq On : 22 Aug 2017 11:18
Operator : SJ/JU
Sample : I4900-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-STAIR

Quant Time: Aug 22 13:18:26 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

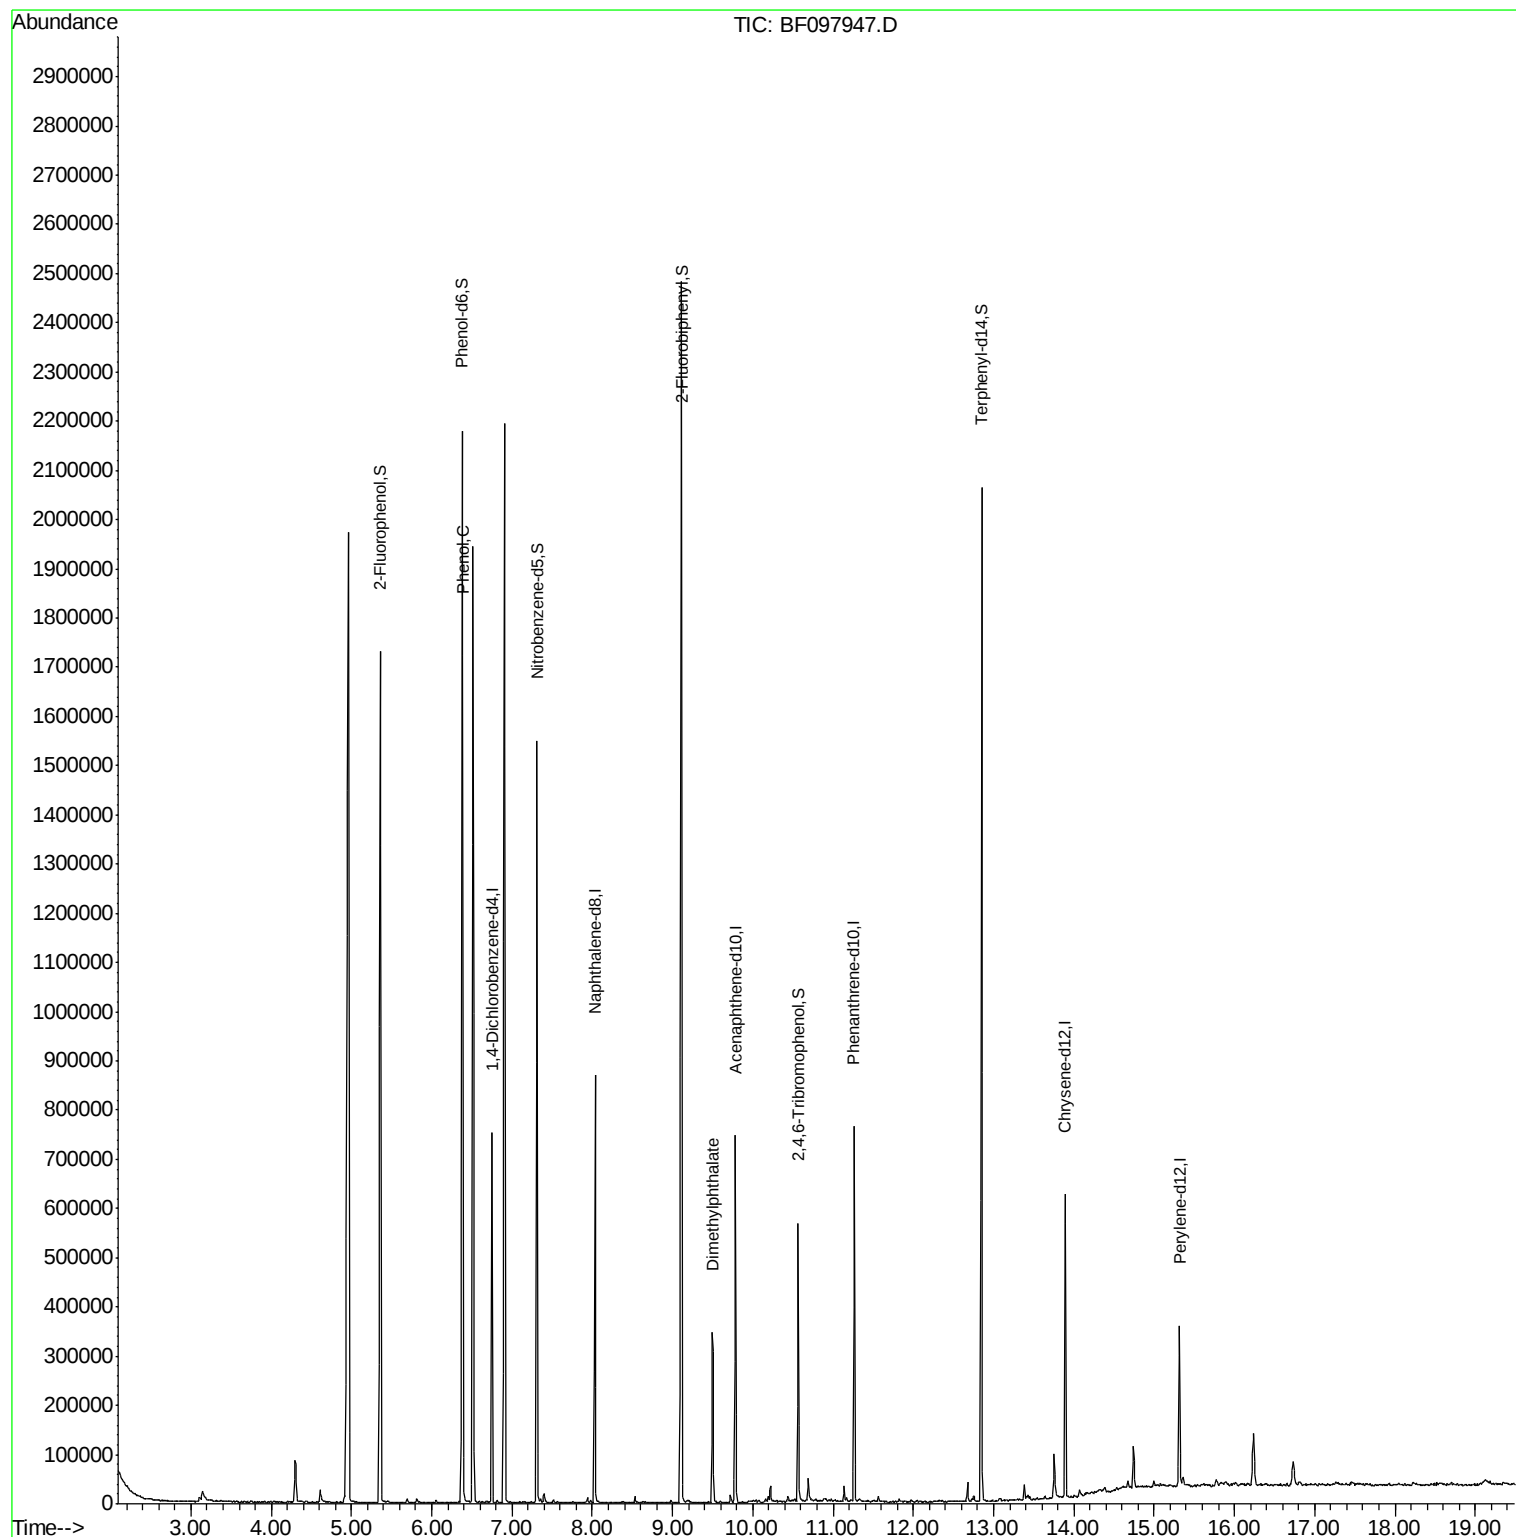




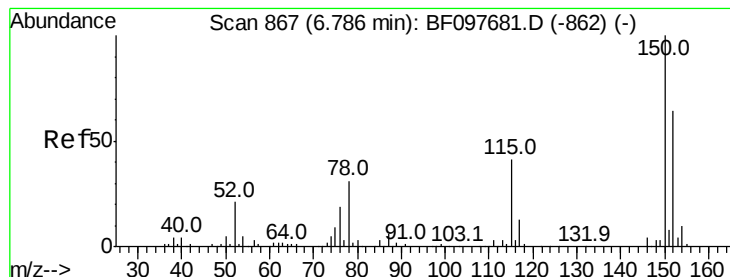


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.75 min Scan# 793
Delta R.T. 0.00 min
Lab File: BF097947.D
Acq: 22 Aug 2017 11:18

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-STAIR




Tot Ion:152 Resp: 104513
Ion Ratio Lower Upper
152 100
150 155.2 126.2 189.2
115 63.4 52.2 78.2

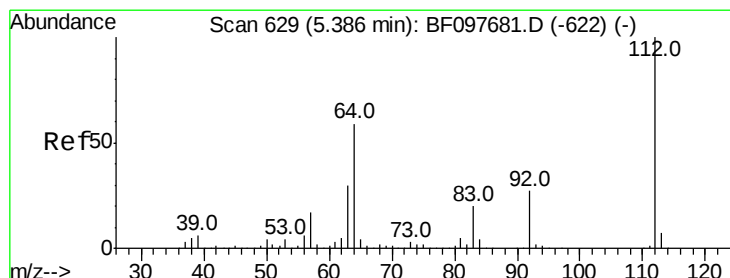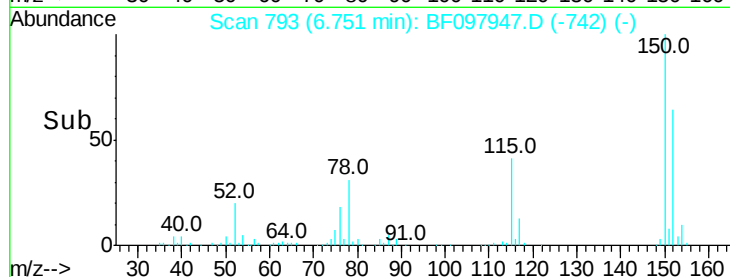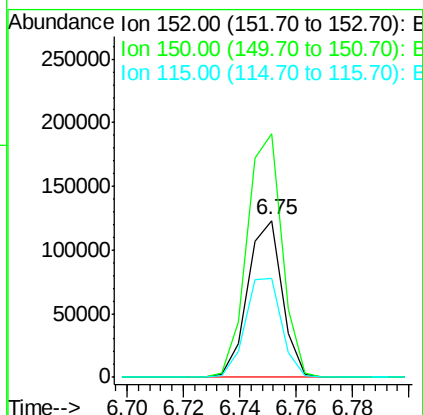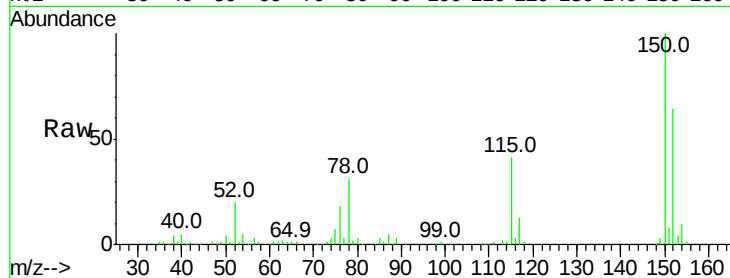


#5

2-Fluorophenol
Concen: 67.225 ng
RT: 5.36 min Scan# 556
Delta R.T. 0.01 min
Lab File: BF097947.D
Acq: 22 Aug 2017 11:18

Tgt Ion:112 Resp: 461906
Ion Ratio Lower Upper
112 100
64 61.8 46.0 69.0
63 31.5 23.4 35.0

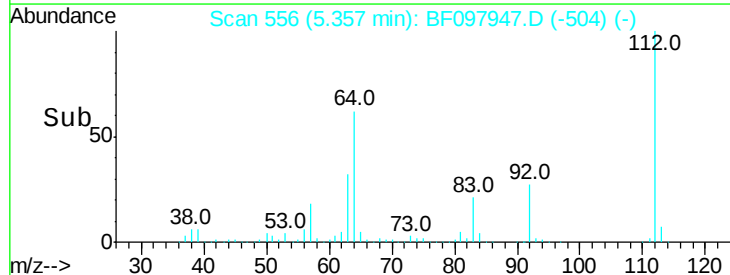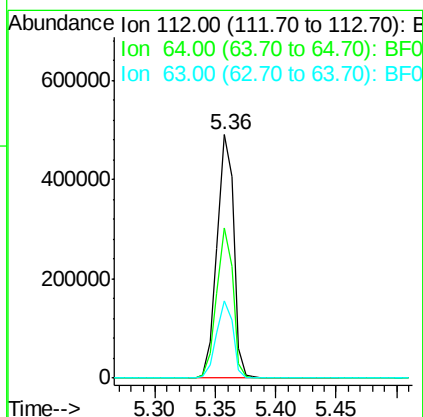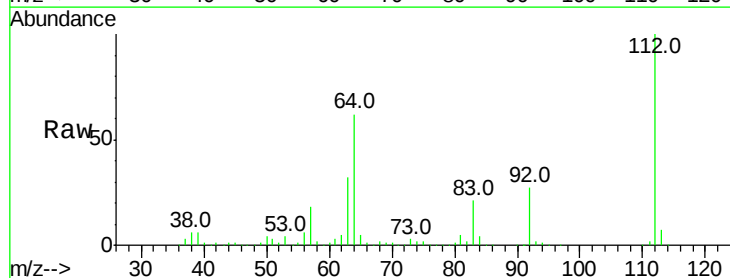

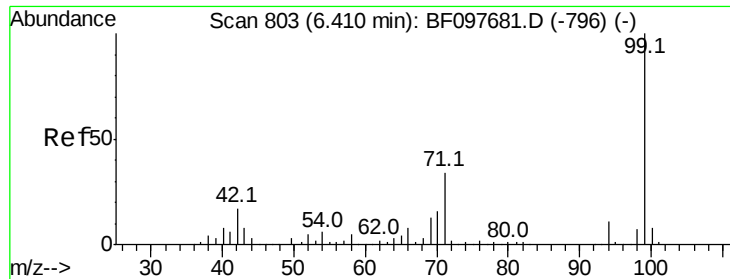

#7

Phenol-d6

Concen: 86.945 ng

RT: 6.38 min Scan# 730

Delta R.T. -0.01 min

Lab File: BF097947.D

Acq: 22 Aug 2017 11:18

Instrument :

BNA_F

ClientSampleId :

CONTROL-HOUSE-STAIR


Tot Ion: 99 Resp: 811694

Ion Ratio Lower Upper




99 100

42 16.1 13.5 20.3

71 33.4 24.5 36.7

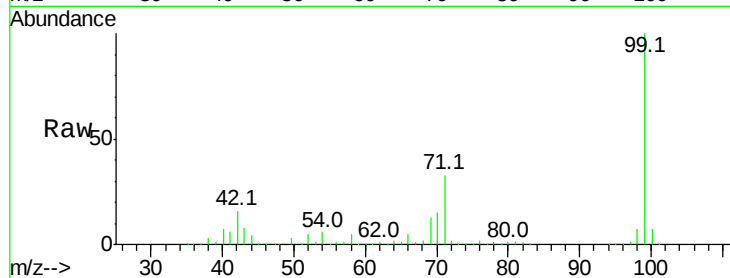

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

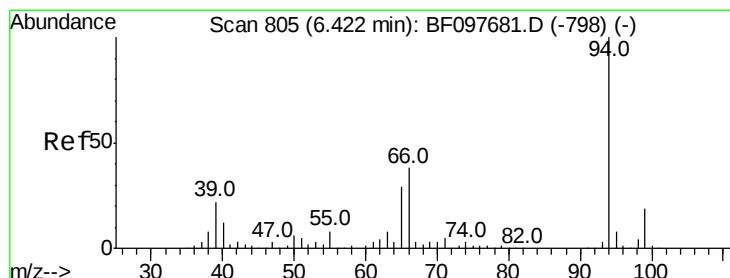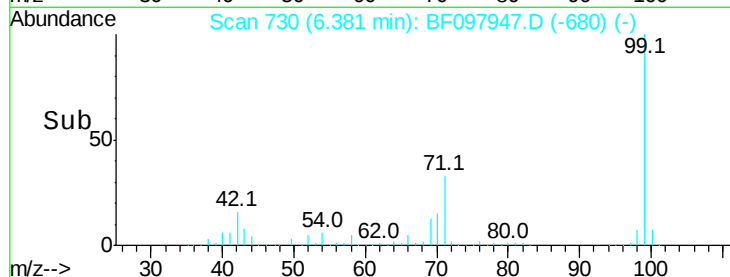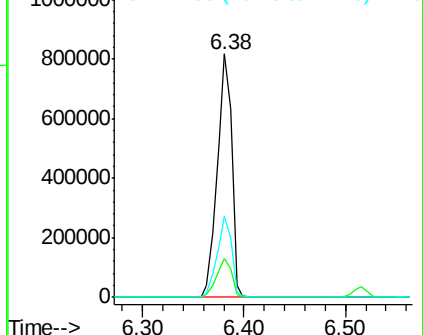

#10

Phenol

Concen: 2.758 ng

RT: 6.39 min Scan# 732

Delta R.T. -0.01 min

Lab File: BF097947.D

Acq: 22 Aug 2017 11:18


Tgt Ion: 94 Resp: 30115

Ion Ratio Lower Upper



94 100

65 30.1 9.9 49.9

66 38.8 23.1 63.1

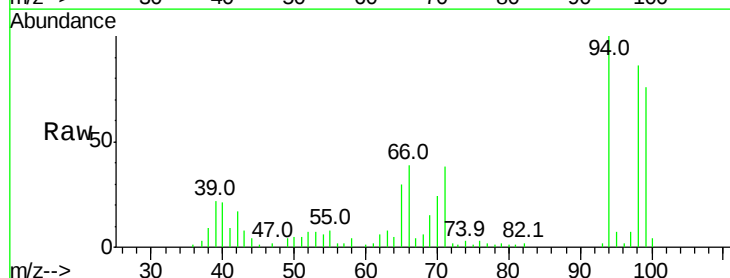

Abundance Ion 94.00 (93.70 to 94.70): BF0
Ion 65.00 (64.70 to 65.70): BF0
Ion 66.00 (65.70 to 66.70): BF0



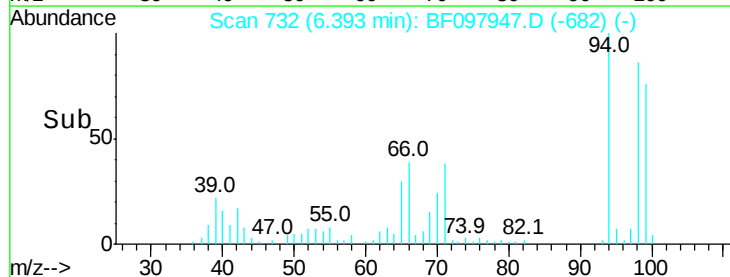
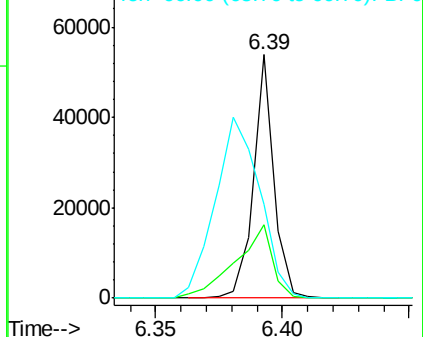




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.03 min Scan# 1011
Delta R.T. 0.00 min
Lab File: BF097947.D
Acq: 22 Aug 2017 11:18




Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-STAIR


Tot Ion:	136	Resp:	379949
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.5	12.7
54	7.0	4.9	7.3
68	6.5	4.1	6.1#

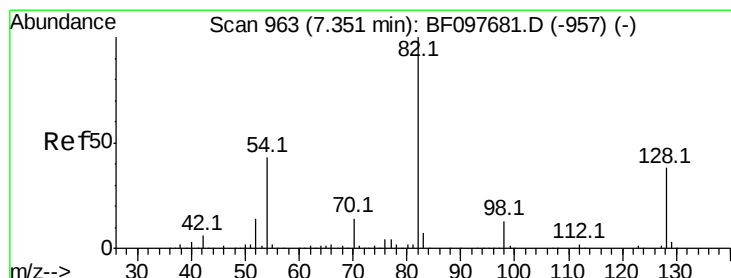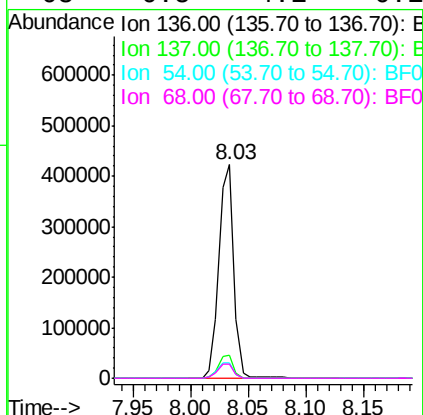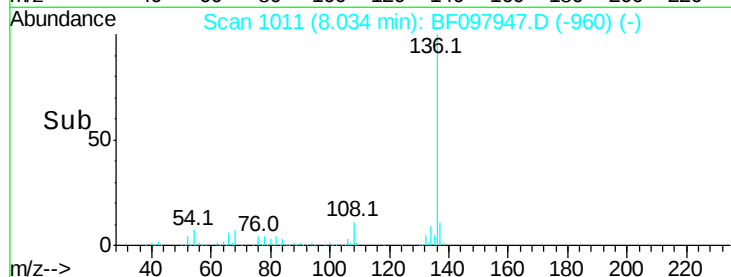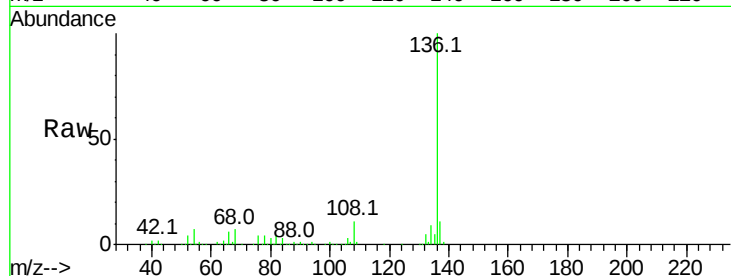

#23
Nitrobenzene-d5
Concen: 77.735 ng
RT: 7.31 min Scan# 888
Delta R.T. -0.01 min
Lab File: BF097947.D
Acq: 22 Aug 2017 11:18

Tgt Ion:	82	Resp:	543684
Ion	Ratio	Lower	Upper
82	100		
128	36.6	34.0	51.0
54	42.9	42.2	63.2


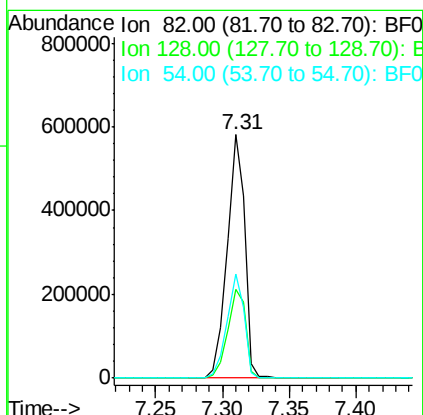
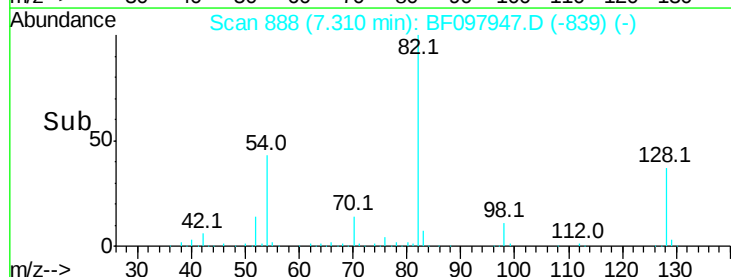



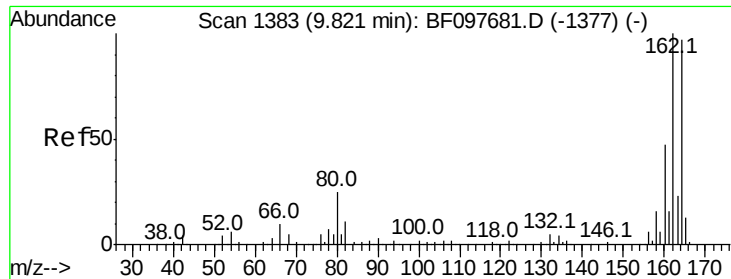

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.78 min Scan# 1308
 Delta R.T. -0.01 min
 Lab File: BF097947.D
 Acq: 22 Aug 2017 11:18




Instrument :
 BNA_F
 ClientSampleId :
 CONTROL-HOUSE-STAIR

Tot Ion:164 Resp: 140479
 Ion Ratio Lower Upper
 164 100
 162 101.1 82.6 123.8
 160 49.6 36.2 54.2

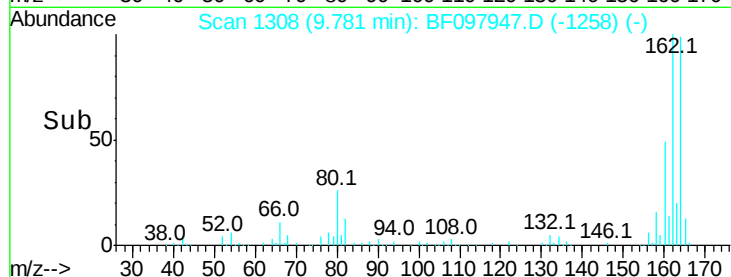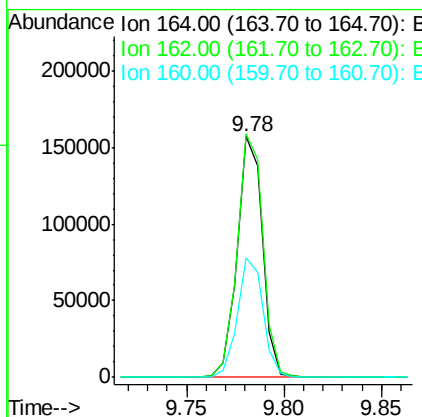

#41
 2,4,6-Tribromophenol
 Concen: 46.642 ng
 RT: 10.57 min Scan# 1442
 Delta R.T. -0.01 min
 Lab File: BF097947.D
 Acq: 22 Aug 2017 11:18

Tgt Ion:330 Resp: 56851
 Ion Ratio Lower Upper
 330 100
 332 93.8 76.6 115.0
 141 43.9 31.4 47.2


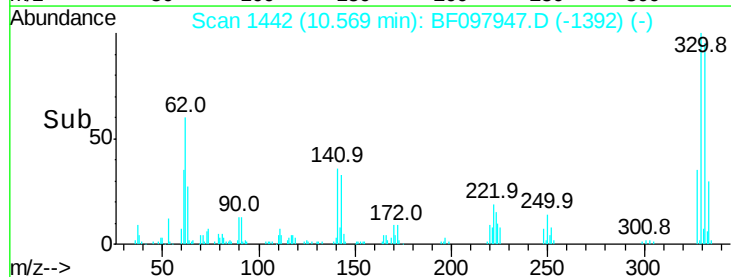
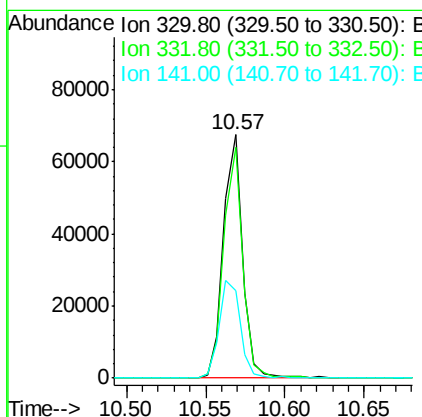





#44
2-Fluorobiphenyl
Concen: 79.924 ng
RT: 9.11 min Scan# 1194
Delta R.T. 0.00 min
Lab File: BF097947.D
Acq: 22 Aug 2017 11:18




Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-STAIR


Tot Ion:172 Resp: 764199
Ion Ratio Lower Upper
172 100
171 35.6 29.6 44.4
170 24.1 19.8 29.8

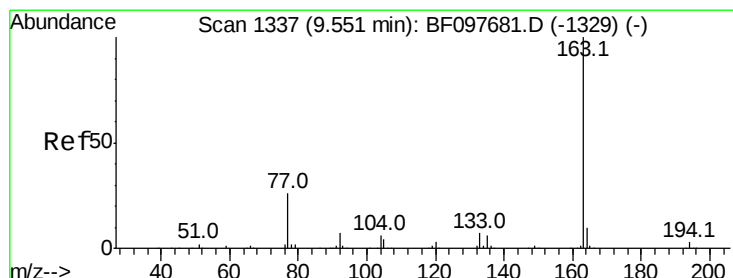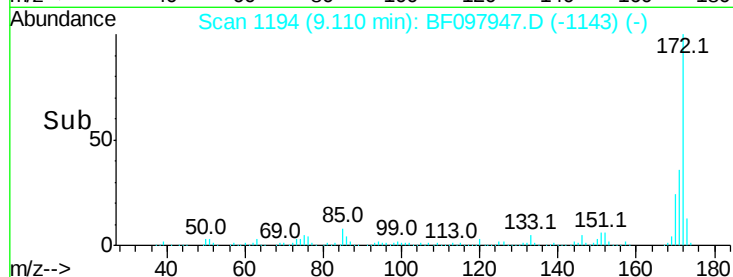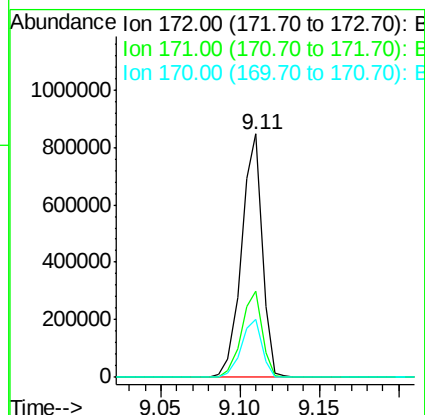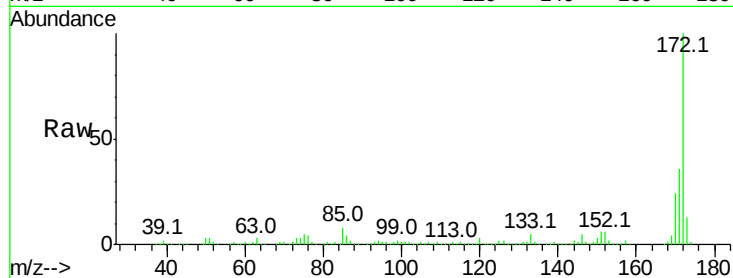

#49
Dimethylphthalate
Concen: 12.290 ng
RT: 9.50 min Scan# 1260
Delta R.T. -0.02 min
Lab File: BF097947.D
Acq: 22 Aug 2017 11:18

Tgt Ion:163 Resp: 126202
Ion Ratio Lower Upper
163 100
194 3.6 2.6 4.0
164 10.1 8.4 12.6


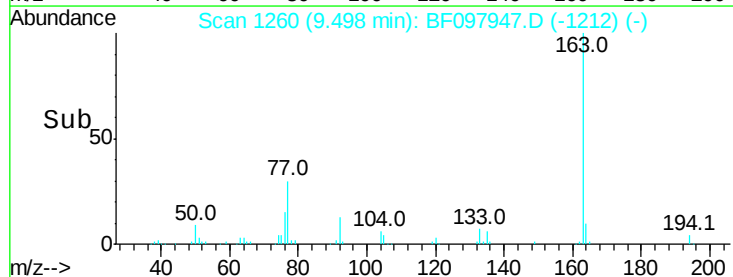
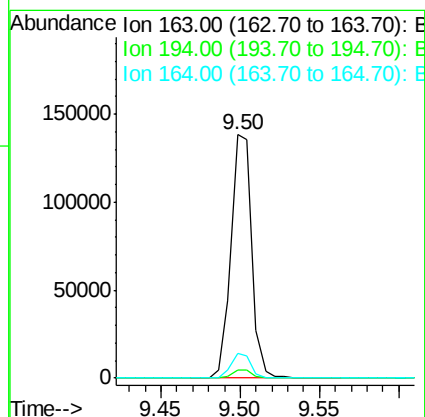
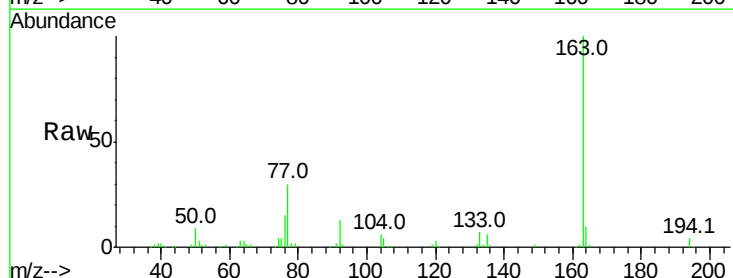


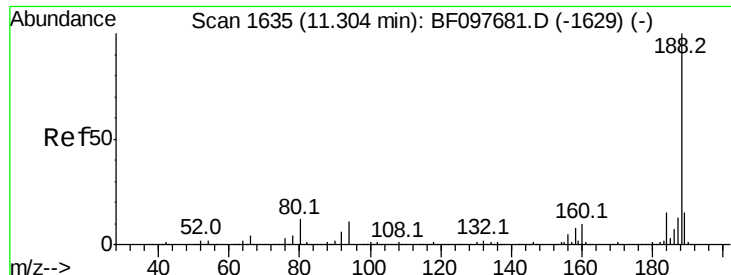

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.26 min Scan# 1560
Delta R.T. 0.00 min
Lab File: BF097947.D
Acq: 22 Aug 2017 11:18




Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-STAIR


Tot Ion:188 Resp: 244985
Ion Ratio Lower Upper
188 100
94 11.1 9.4 14.2
80 12.5 10.2 15.2

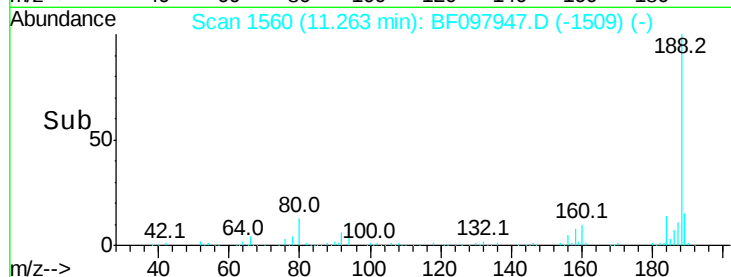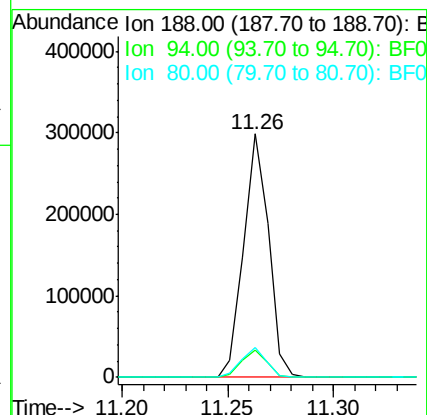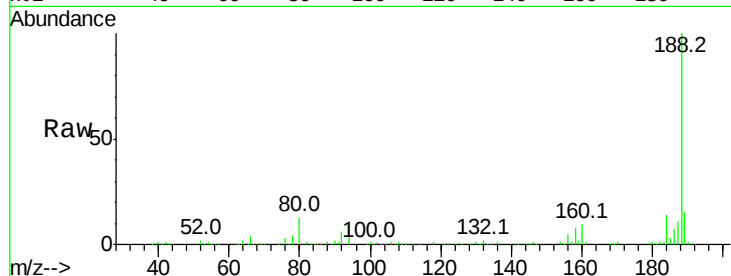

#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.89 min Scan# 2007
Delta R.T. -0.01 min
Lab File: BF097947.D
Acq: 22 Aug 2017 11:18

Tgt Ion:240 Resp: 207881
Ion Ratio Lower Upper
240 100
120 14.0 5.8 8.8#
236 26.5 20.5 30.7

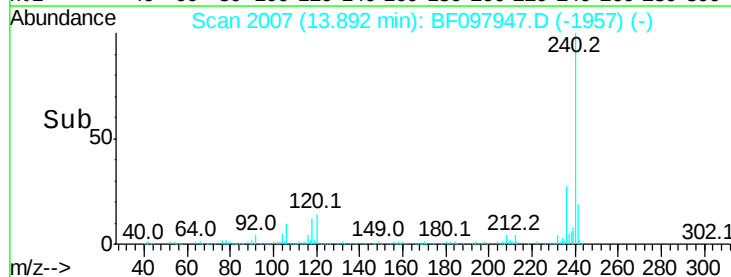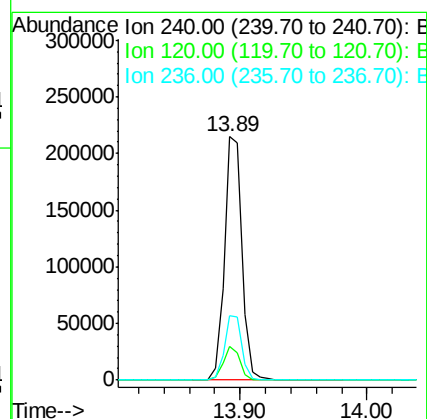

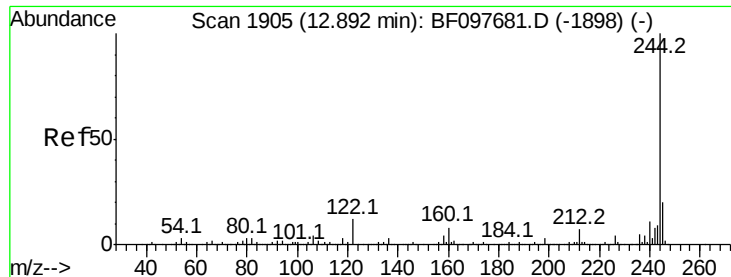

#78

Terphenyl-d14

Concen: 59.500 ng

RT: 12.85 min Scan# 1830

Delta R.T. 0.00 min

Lab File: BF097947.D

Acq: 22 Aug 2017 11:18

Instrument :

BNA_F

ClientSampleId :

CONTROL-HOUSE-STAIR


Tot Ion:244 Resp: 593133

Ion Ratio Lower Upper

244 100

212 7.3 6.0 9.0




122 13.1 10.3 15.5



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

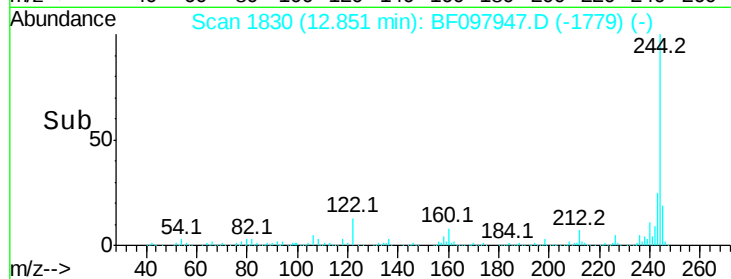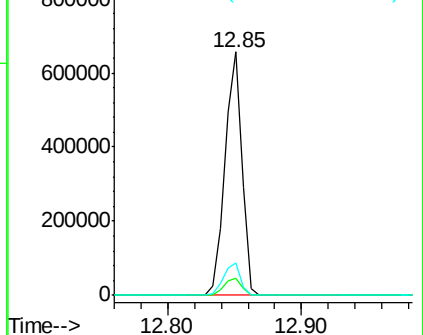

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.32 min Scan# 2249

Delta R.T. 0.01 min

Lab File: BF097947.D

Acq: 22 Aug 2017 11:18


Tgt Ion:264 Resp: 136118

Ion Ratio Lower Upper

264 100

260 23.4 19.5 29.3

265 20.6 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

