

Data Path : U:\HPCHEM1\BNA F\DATA\BF082117\
 Data File : BF097952.D
 Acq On : 22 Aug 2017 13:36
 Operator : SJ/JU
 Sample : I4900-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 220-1-CONCRETE

Quant Time: Aug 22 14:40:51 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 21 15:59:04 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	99687	20.00	ng	0.00
21) Naphthalene-d8	8.03	136	362478	20.00	ng	0.00
38) Acenaphthene-d10	9.78	164	131940	20.00	ng	0.00
63) Phenanthrene-d10	11.26	188	233224	20.00	ng	0.00
75) Chrysene-d12	13.89	240	200088	20.00	ng	0.00
86) Perylene-d12	15.32	264	128438	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	563820	86.03	ng	0.00
7) Phenol-d6	6.38	99	810260	90.99	ng	0.00
23) Nitrobenzene-d5	7.31	82	493450	73.95	ng	-0.01
41) 2,4,6-Tribromophenol	10.57	330	82367	71.95	ng	0.00
44) 2-Fluorobiphenyl	9.11	172	699811	77.93	ng	0.00
78) Terphenyl-d14	12.85	244	548858	57.20	ng	0.00
Target Compounds						
10) Phenol	6.39	94	21487	2.063	ng	98
49) Dimethylphthalate	9.50	163	111246	11.535	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA F\DATA\BF082117\
Data File : BF097952.D
Acq On : 22 Aug 2017 13:36
Operator : SJ/JU
Sample : I4900-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
220-1-CONCRETE

Quant Time: Aug 22 14:40:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

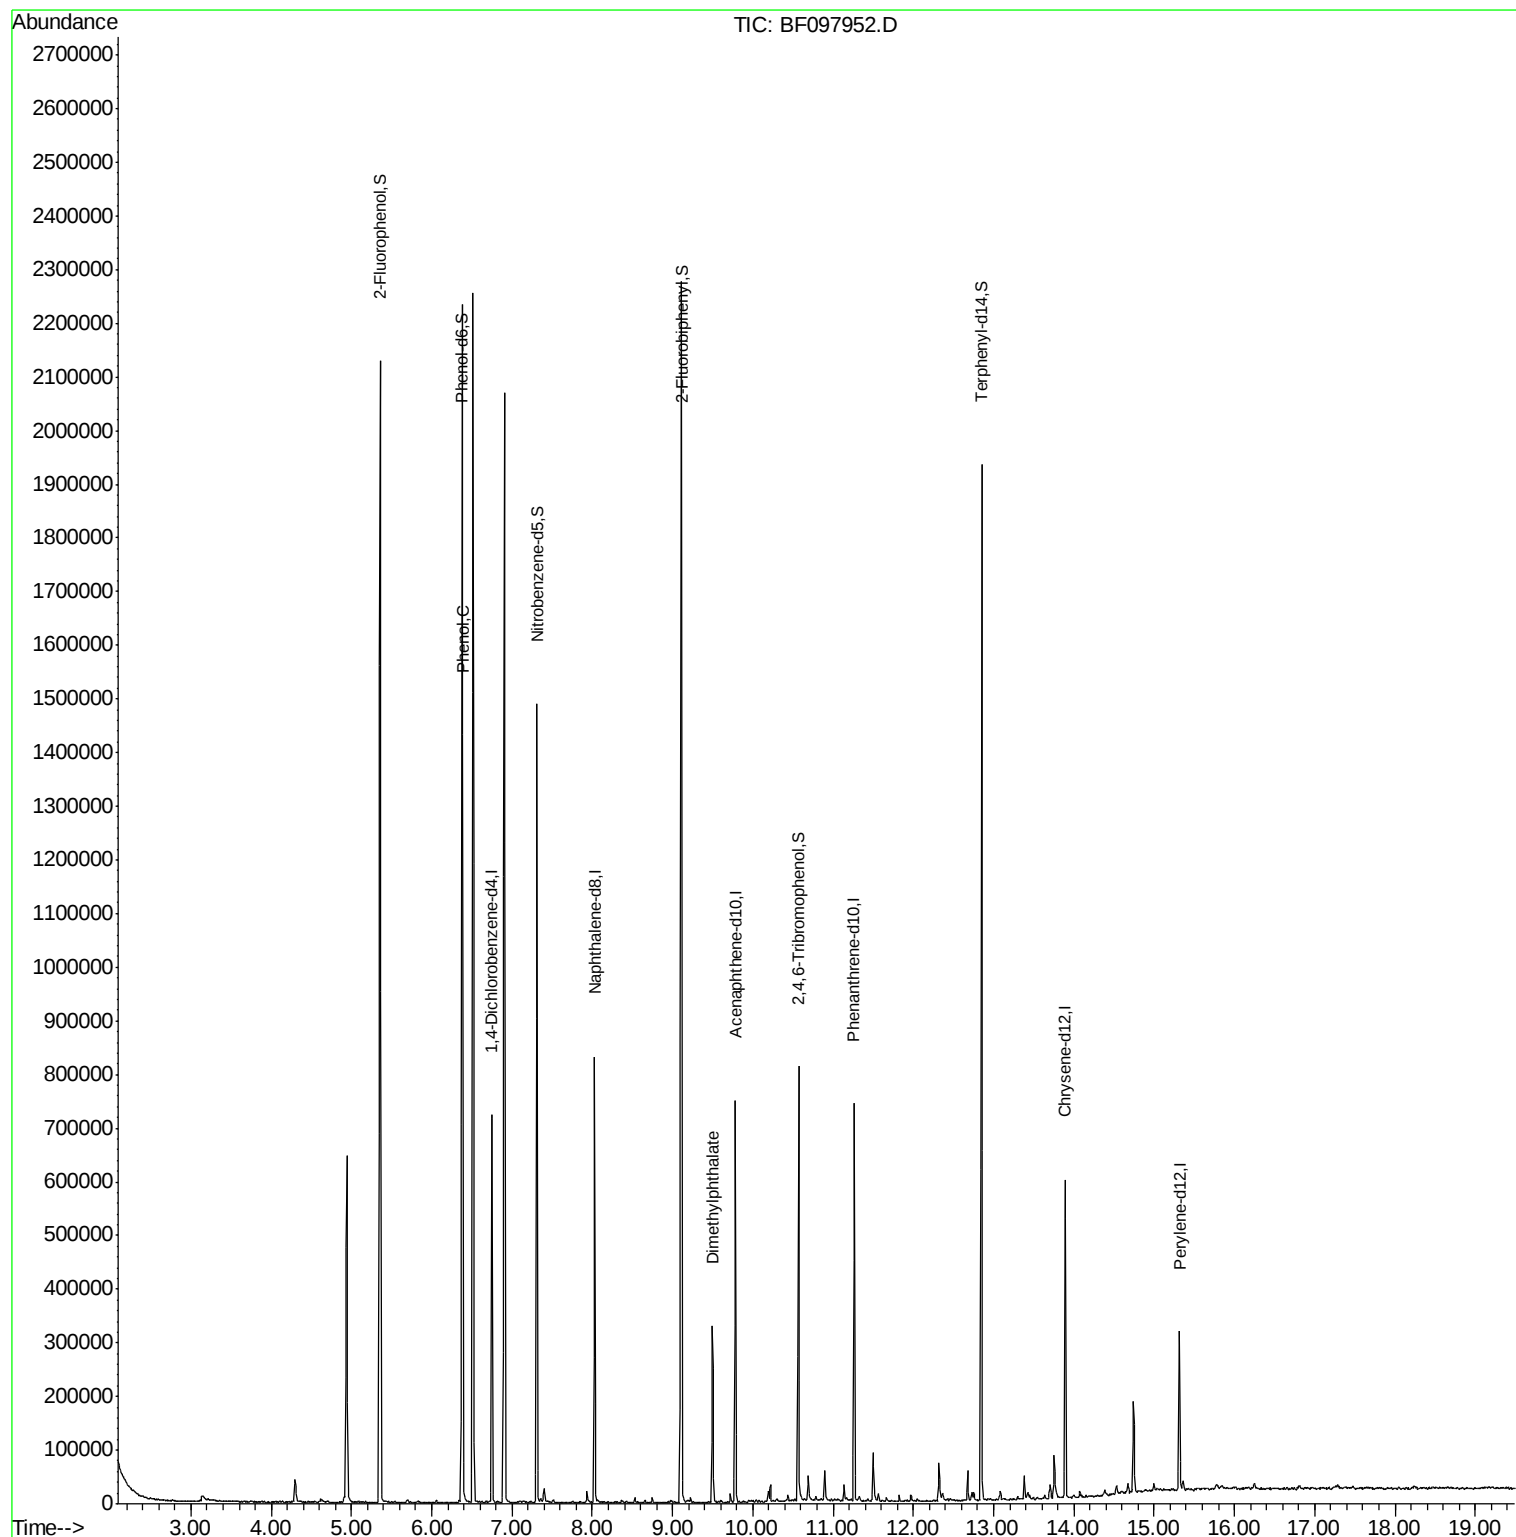

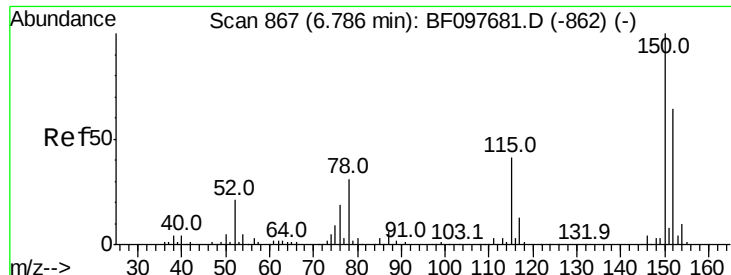


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.75 min Scan# 793
Delta R.T. 0.00 min
Lab File: BF097952.D
Acq: 22 Aug 2017 13:36

Instrument :
BNA_F
ClientSampleId :
220-1-CONCRETE

Tot Ion:152 Resp: 99687
Ion Ratio Lower Upper
152 100
150 155.5 126.2 189.2
115 61.7 52.2 78.2

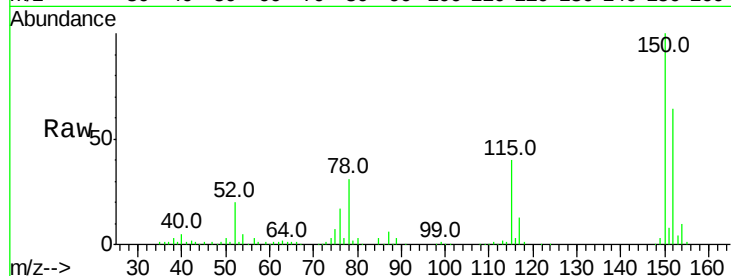


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

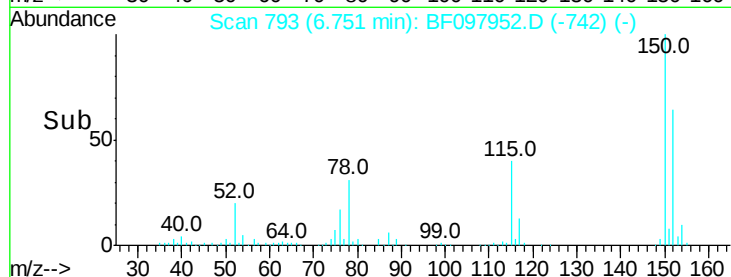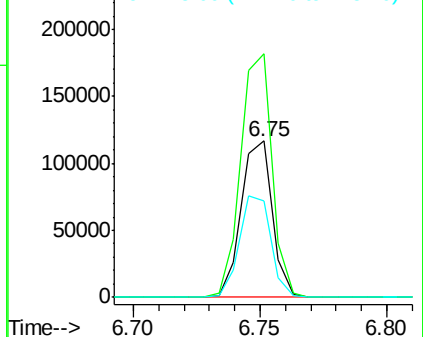



#5


2-Fluorophenol
Concen: 86.030 ng
RT: 5.36 min Scan# 556
Delta R.T. 0.01 min
Lab File: BF097952.D
Acq: 22 Aug 2017 13:36

Tgt Ion:112 Resp: 563820
Ion Ratio Lower Upper
112 100
64 59.8 46.0 69.0
63 31.2 23.4 35.0

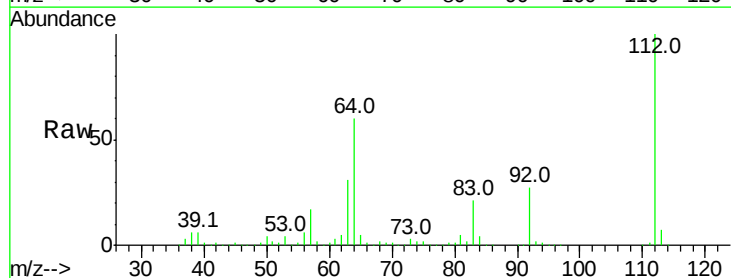

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

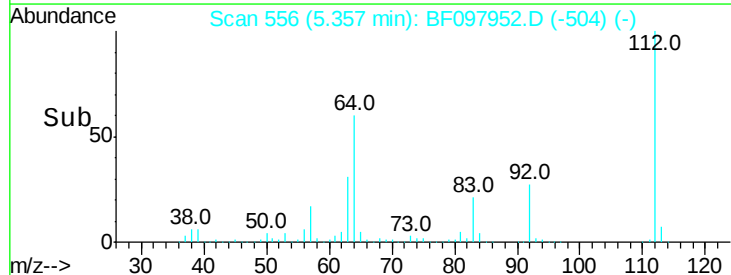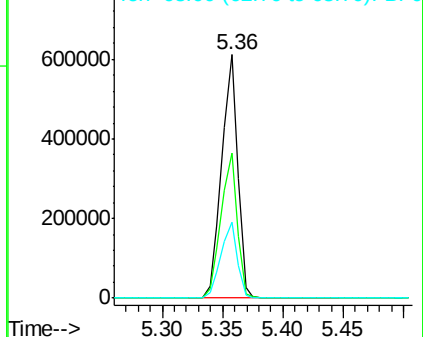

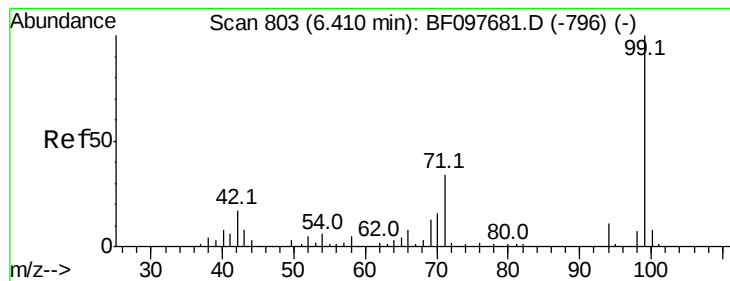

#7

Phenol-d6

Concen: 90.993 ng

RT: 6.38 min Scan# 730

Delta R.T. -0.01 min

Lab File: BF097952.D

Acq: 22 Aug 2017 13:36

Instrument :

BNA_F

ClientSampleId :

220-1-CONCRETE


Tot Ion: 99 Resp: 810260

Ion Ratio Lower Upper

99 100

42 15.7 13.5 20.3




71 33.2 24.5 36.7

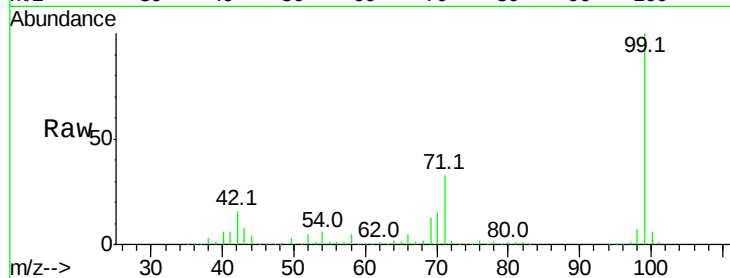

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

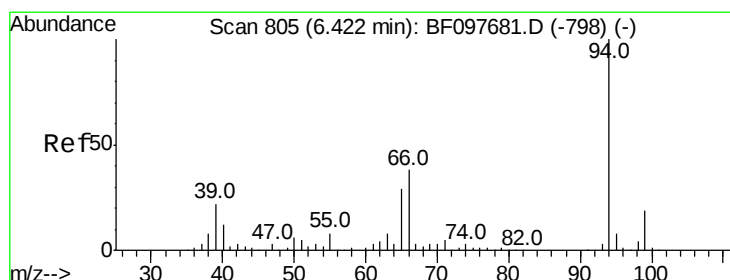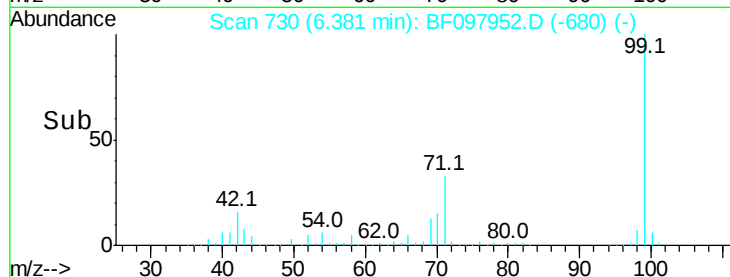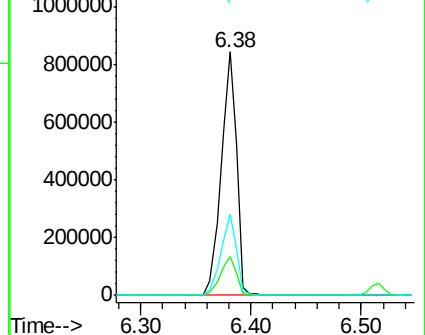

#10

Phenol

Concen: 2.063 ng

RT: 6.39 min Scan# 732

Delta R.T. -0.01 min

Lab File: BF097952.D

Acq: 22 Aug 2017 13:36


Tgt Ion: 94 Resp: 21487

Ion Ratio Lower Upper

94 100

65 30.2 9.9 49.9



66 41.1 23.1 63.1

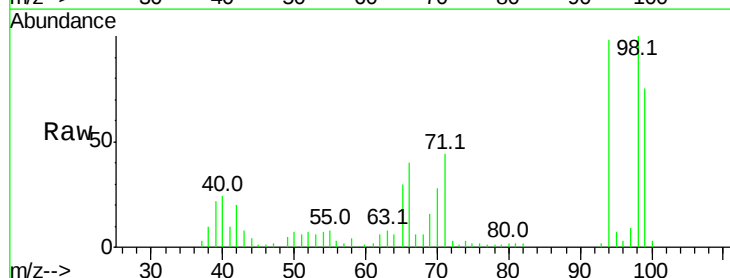

Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0



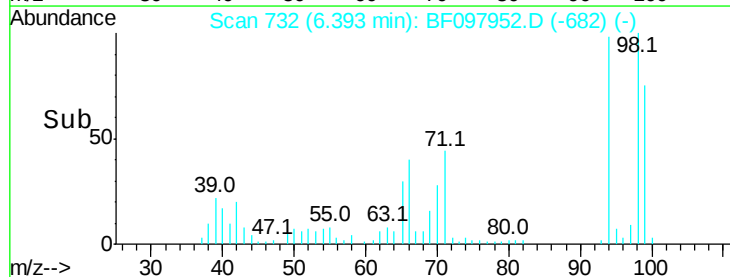
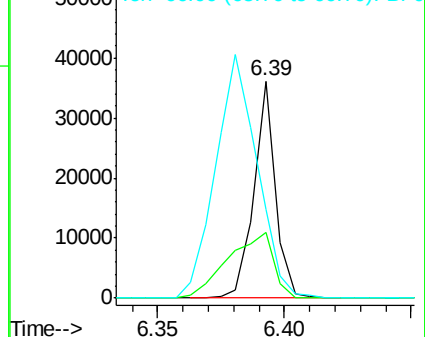




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.03 min Scan# 1011
Delta R.T. 0.00 min
Lab File: BF097952.D
Acq: 22 Aug 2017 13:36




Instrument :
BNA_F
ClientSampleId :
220-1-CONCRETE


Tot Ion:136 Resp: 362478
Ion Ratio Lower Upper
136 100
137 10.5 8.5 12.7
54 6.7 4.9 7.3
68 6.2 4.1 6.1#

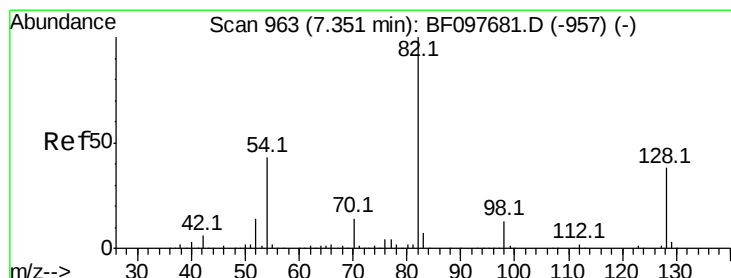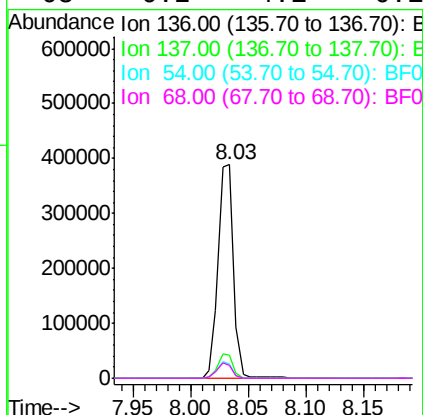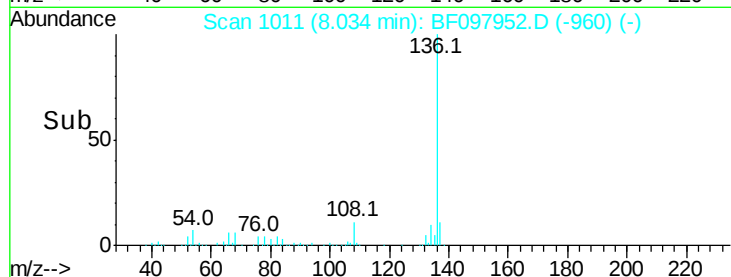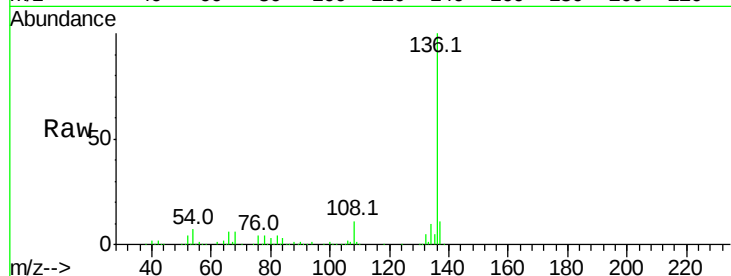

#23
Nitrobenzene-d5
Concen: 73.953 ng
RT: 7.31 min Scan# 888
Delta R.T. -0.01 min
Lab File: BF097952.D
Acq: 22 Aug 2017 13:36

Tgt Ion: 82 Resp: 493450
Ion Ratio Lower Upper
82 100
128 36.8 34.0 51.0
54 42.6 42.2 63.2

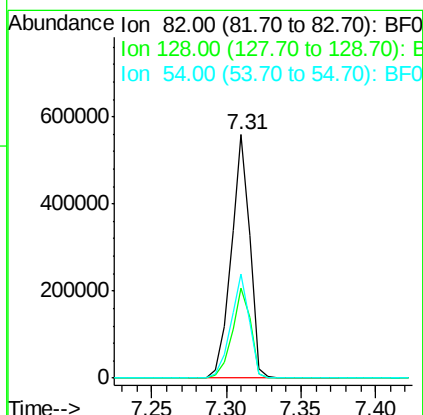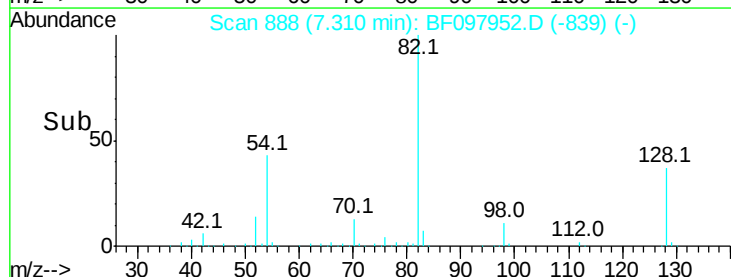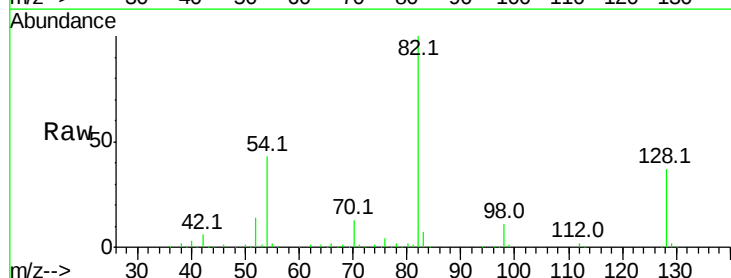


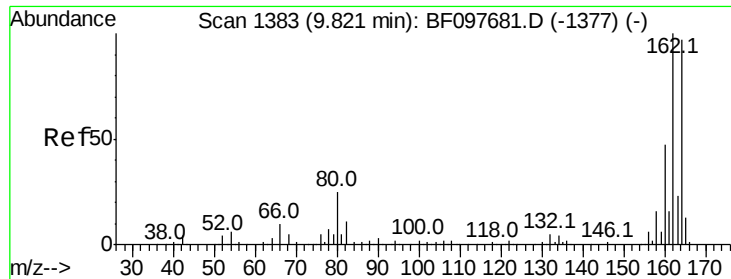




#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.78 min Scan# 1308
 Delta R.T. -0.01 min
 Lab File: BF097952.D
 Acq: 22 Aug 2017 13:36

Instrument :
 BNA_F
 ClientSampleId :
 220-1-CONCRETE

Tot Ion:164 Resp: 131940
 Ion Ratio Lower Upper
 164 100
 162 103.7 82.6 123.8
 160 47.8 36.2 54.2

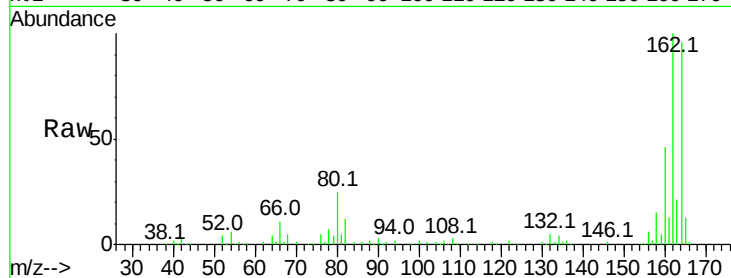


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

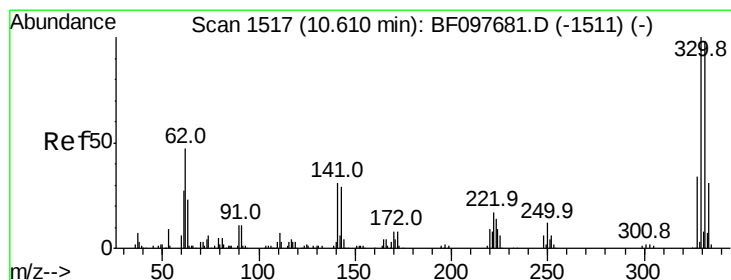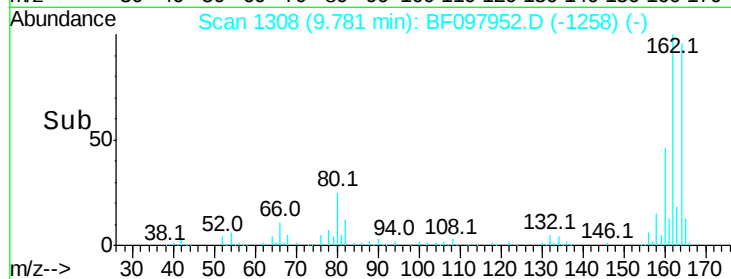
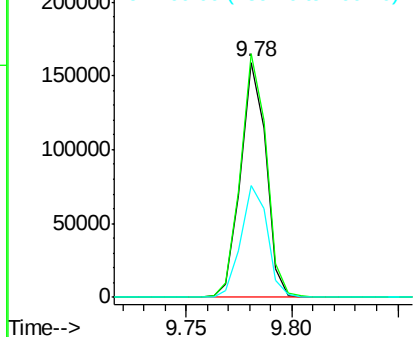


#41
 2,4,6-Tribromophenol
 Concen: 71.949 ng
 RT: 10.57 min Scan# 1442
 Delta R.T. -0.01 min
 Lab File: BF097952.D
 Acq: 22 Aug 2017 13:36

Tgt Ion:330 Resp: 82367
 Ion Ratio Lower Upper
 330 100
 332 95.9 76.6 115.0
 141 43.1 31.4 47.2

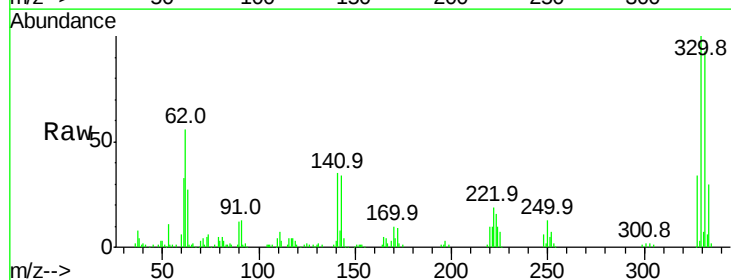

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



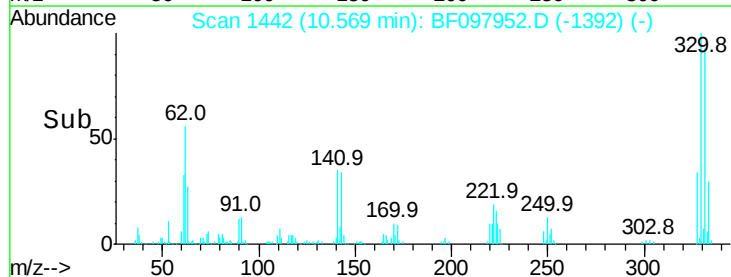
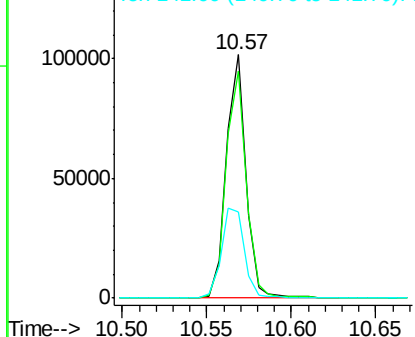




#44
 2-Fluorobiphenyl
 Concen: 77.927 ng
 RT: 9.11 min Scan# 1194
 Delta R.T. 0.00 min
 Lab File: BF097952.D
 Acq: 22 Aug 2017 13:36




Instrument :
 BNA_F
 ClientSampleId :
 220-1-CONCRETE


Tot Ion:172 Resp: 699811
 Ion Ratio Lower Upper
 172 100
 171 35.6 29.6 44.4
 170 24.5 19.8 29.8

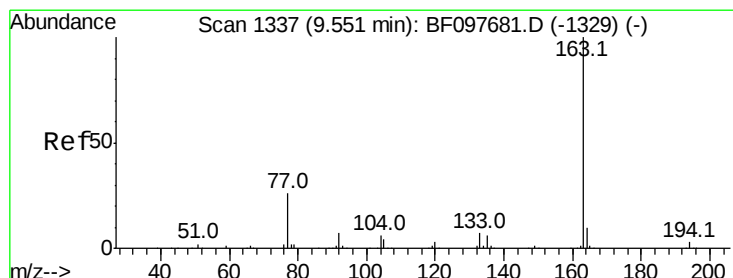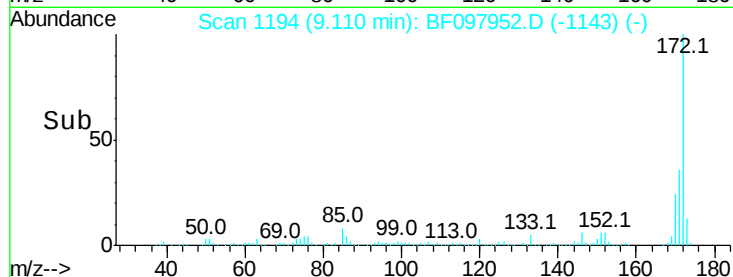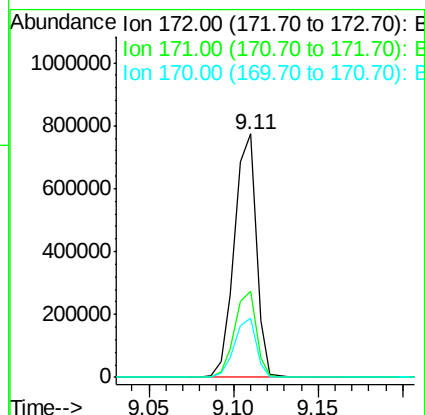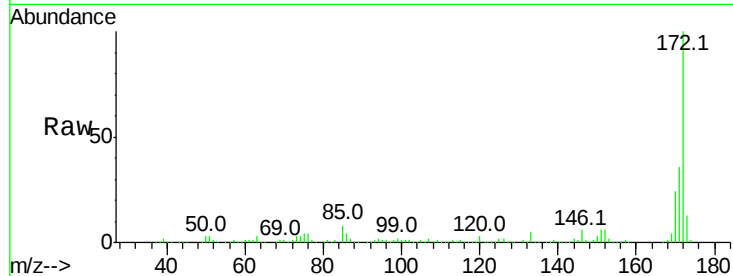

#49
 Dimethylphthalate
 Concen: 11.535 ng
 RT: 9.50 min Scan# 1260
 Delta R.T. -0.02 min
 Lab File: BF097952.D
 Acq: 22 Aug 2017 13:36

Tgt Ion:163 Resp: 111246
 Ion Ratio Lower Upper
 163 100
 194 3.2 2.6 4.0
 164 10.4 8.4 12.6

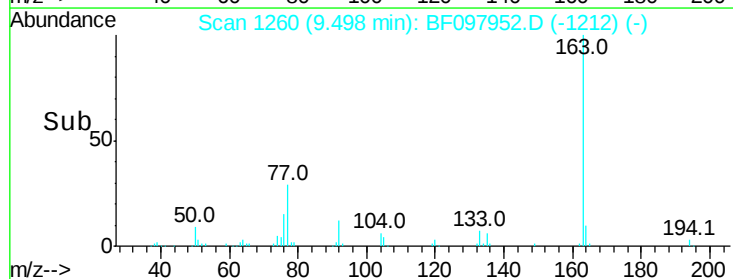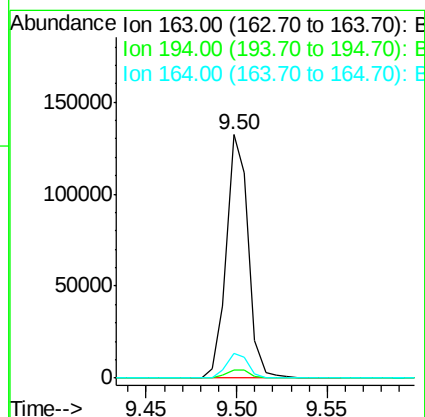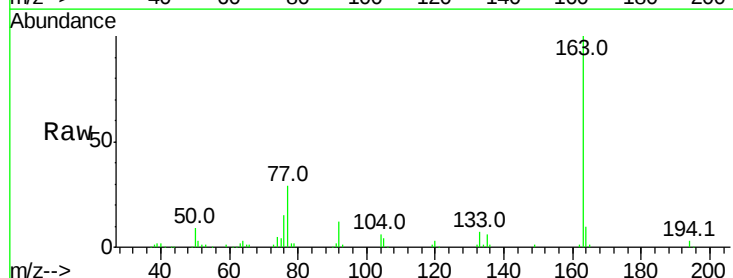


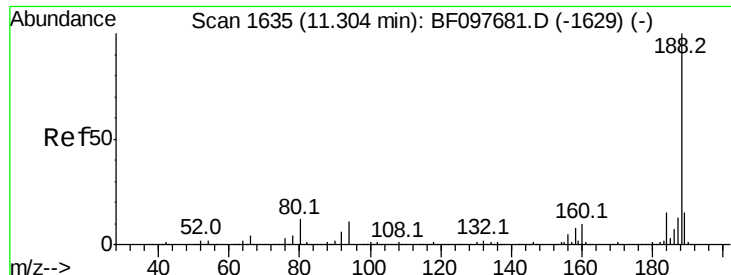




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.26 min Scan# 1560
Delta R.T. 0.00 min
Lab File: BF097952.D
Acq: 22 Aug 2017 13:36

Instrument :
BNA_F
ClientSampleId :
220-1-CONCRETE

Tot Ion	Ratio	Lower	Upper
188	100		
94	11.3	9.4	14.2
80	11.6	10.2	15.2

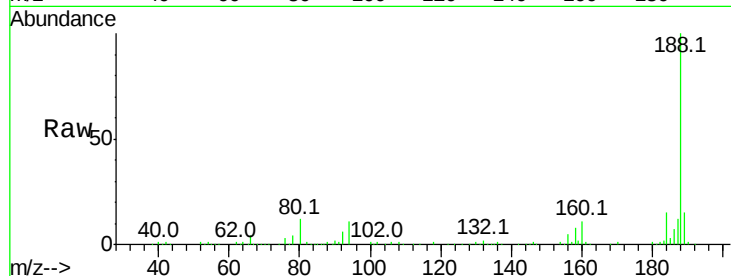


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

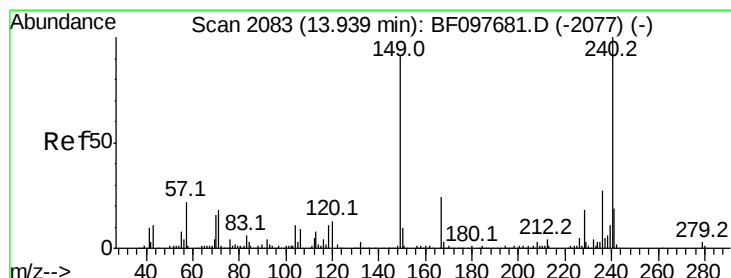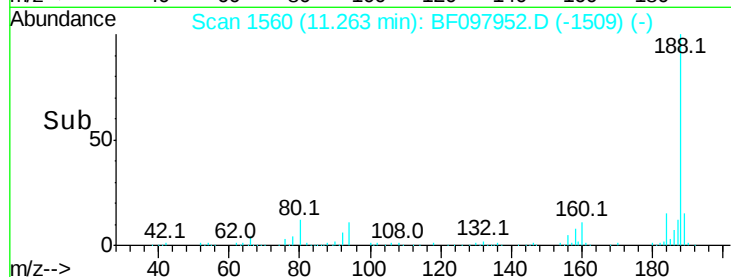
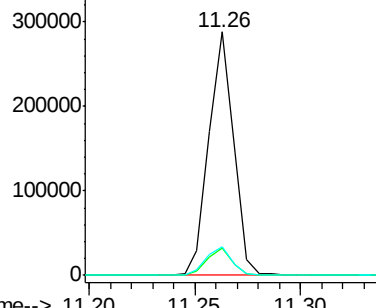



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.89 min Scan# 2007
Delta R.T. -0.01 min
Lab File: BF097952.D
Acq: 22 Aug 2017 13:36

Tgt Ion	Ratio	Lower	Upper
240	100		
120	14.0	5.8	8.8#
236	25.8	20.5	30.7

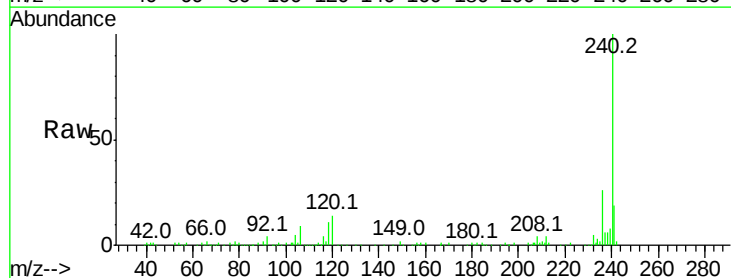

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

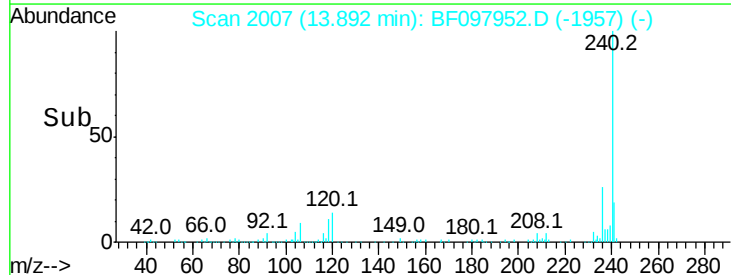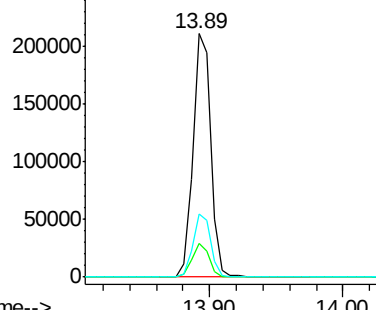

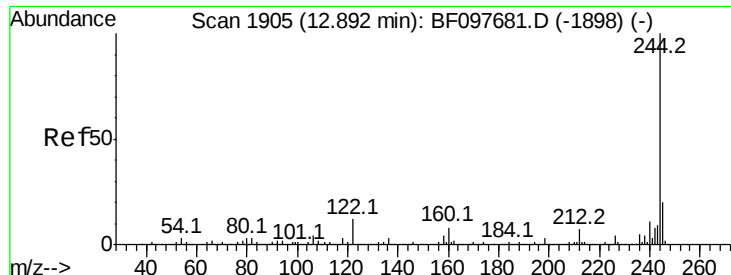

#78

Terphenyl-d14

Concen: 57.202 ng

RT: 12.85 min Scan# 1830

Delta R.T. 0.00 min

Lab File: BF097952.D

Acq: 22 Aug 2017 13:36

Instrument :

BNA_F

ClientSampleId :

220-1-CONCRETE


Tot Ion:244 Resp: 548858

Ion Ratio Lower Upper

244 100

212 7.2 6.0 9.0




122 12.6 10.3 15.5

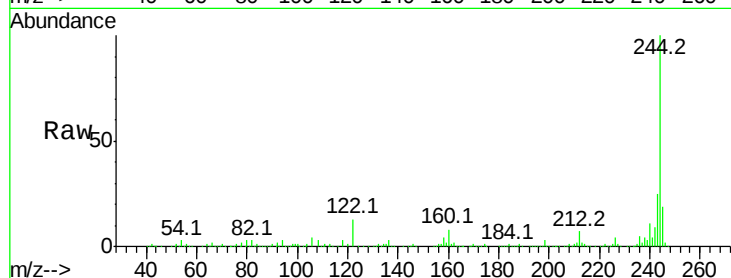

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

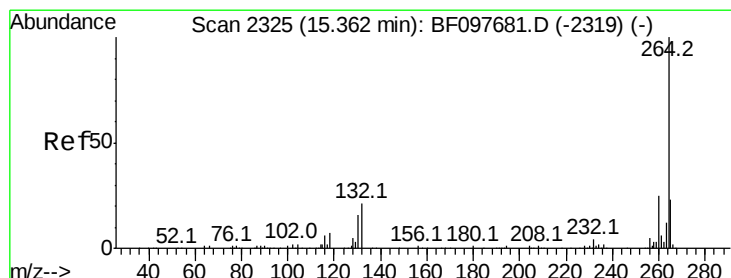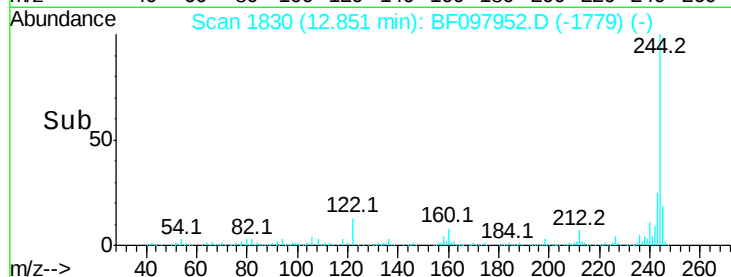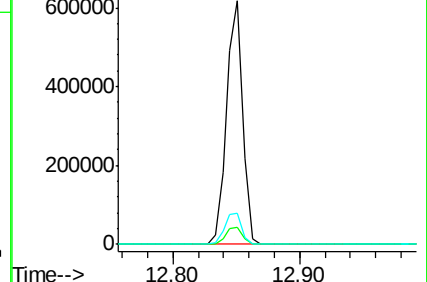

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.32 min Scan# 2249

Delta R.T. 0.01 min

Lab File: BF097952.D

Acq: 22 Aug 2017 13:36


Tgt Ion:264 Resp: 128438

Ion Ratio Lower Upper

264 100

260 24.3 19.5 29.3

265 20.3 17.2 25.8

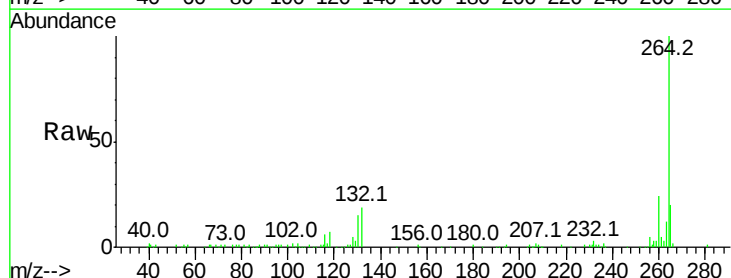

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

