


Data Path : U:\HPCHEM1\BNA F\DATA\BF082117\
 Data File : BF097934.D
 Acq On : 22 Aug 2017 5:09
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

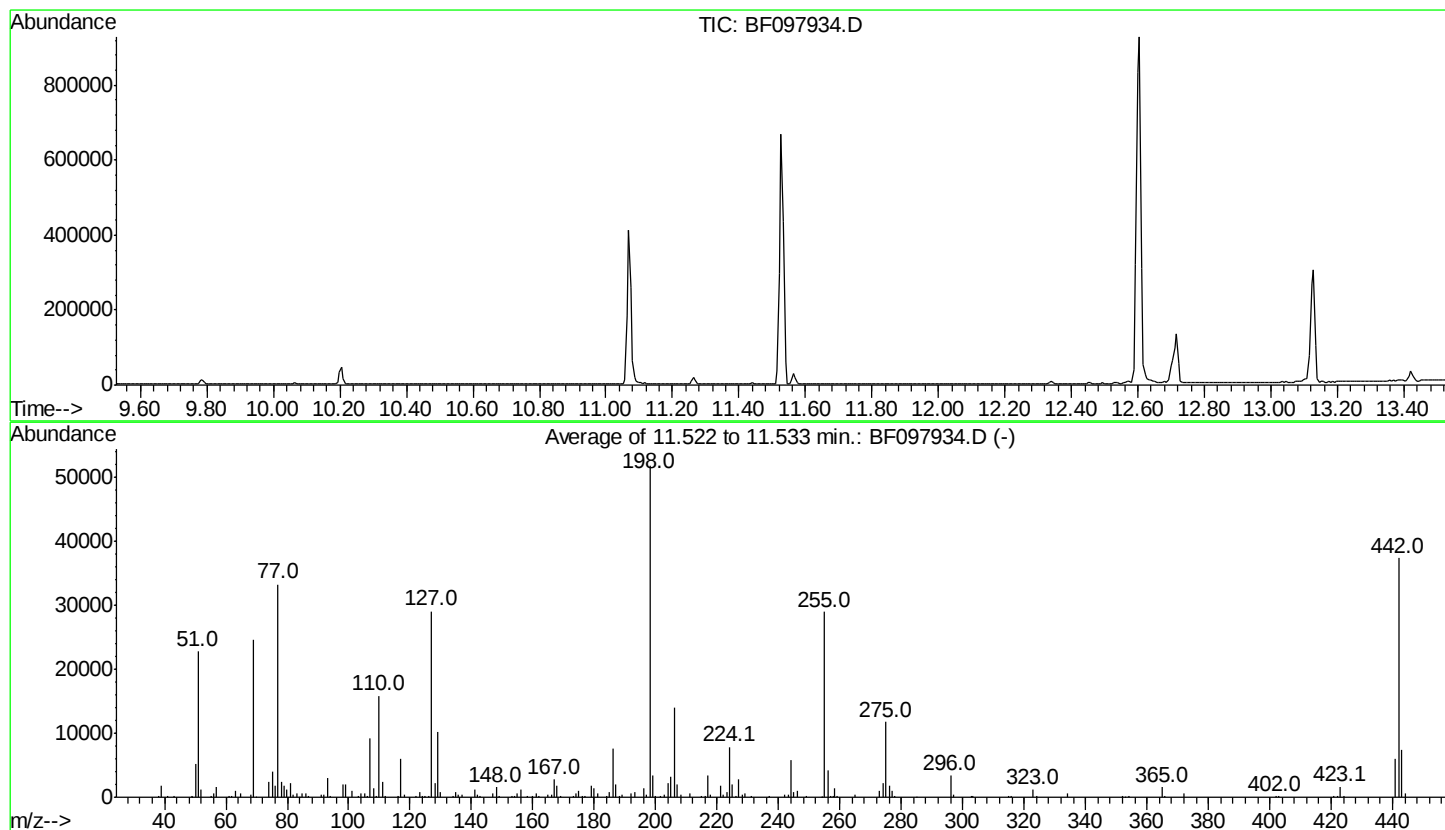

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	22757	PASS
68	69	0.00	2	1.3	330	PASS
69	198	0.00	100	47.7	24728	PASS
70	69	0.00	2	0.4	101	PASS
127	198	10	80	56.2	29133	PASS
197	198	0.00	2	0.9	476	PASS
198	198	100	100	100.0	51880	PASS
199	198	5	9	6.7	3482	PASS
275	198	10	60	22.7	11757	PASS
365	198	1	100	2.9	1530	PASS
441	442	0.01	24	16.3	6086	PASS
442	198	50	100	72.2	37447	PASS
443	442	15	24	20.0	7481	PASS