
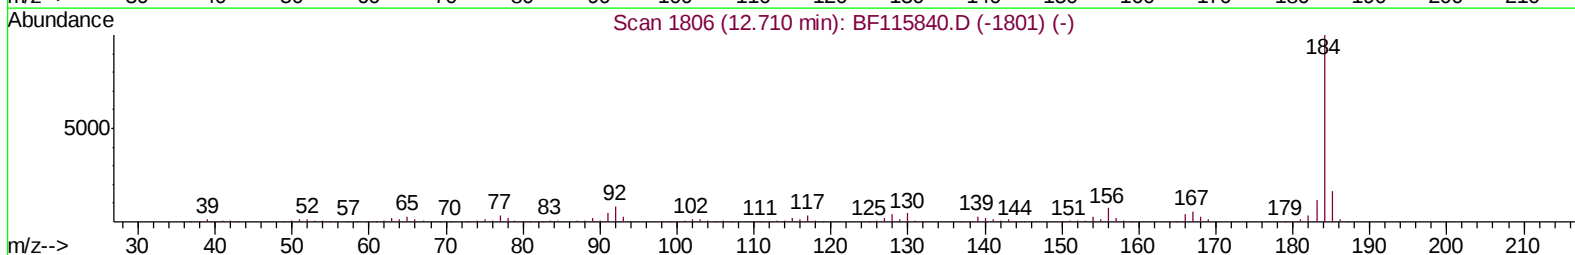
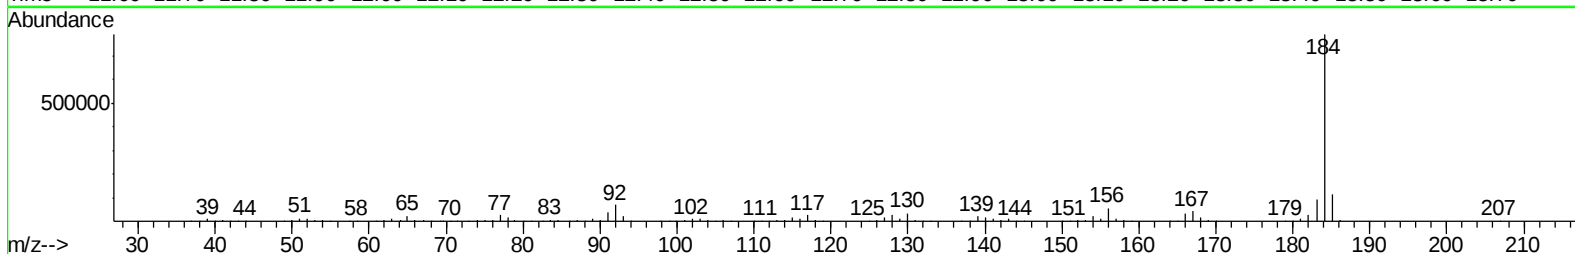


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082119\
 Data File : BF116457.D
 Acq On : 21 Aug 2019 11:09
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:17:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 19 06:03:31 2019
 Response via : Initial Calibration

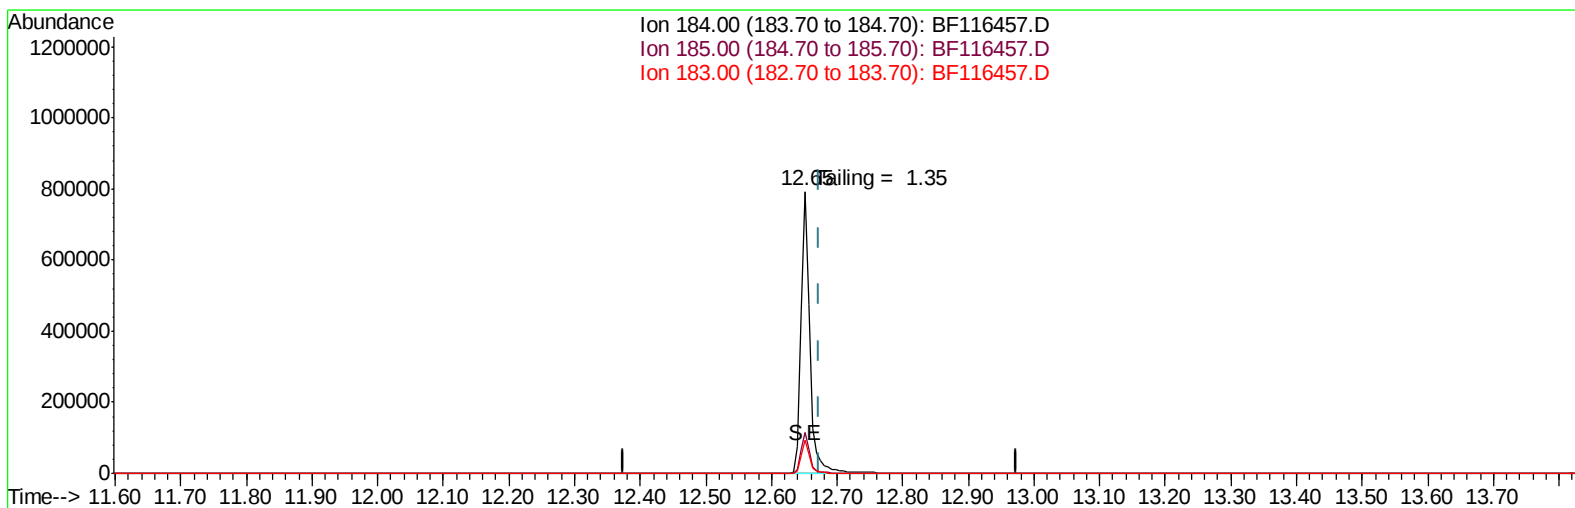

TIC: BF116457.D

(77) Benzidine




12.651min (-0.023) 78682.69ng

response 754938

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	14.61
183.00	11.70	11.66
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082119\
Data File : BF116457.D
Acq On : 21 Aug 2019 11:09
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:17:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 06:03:31 2019
Response via : Initial Calibration

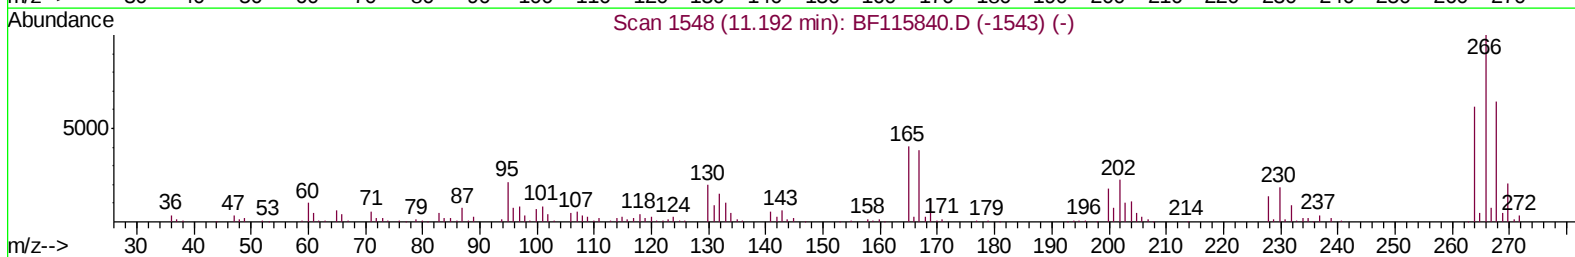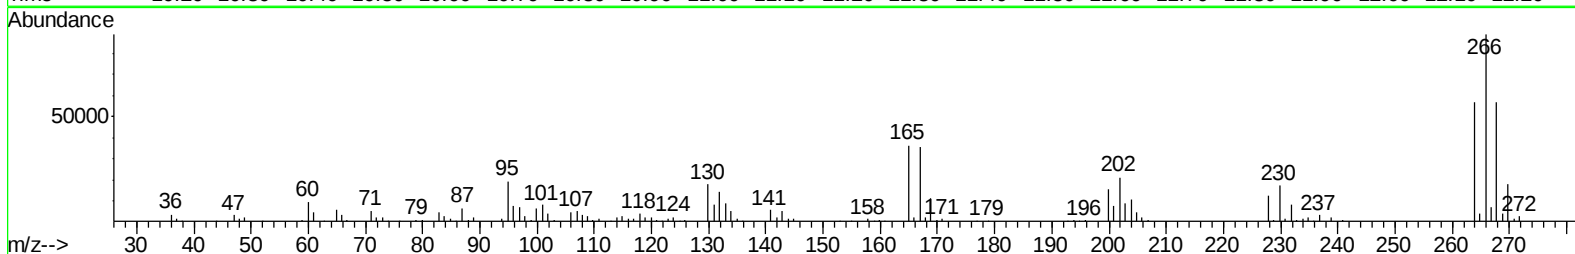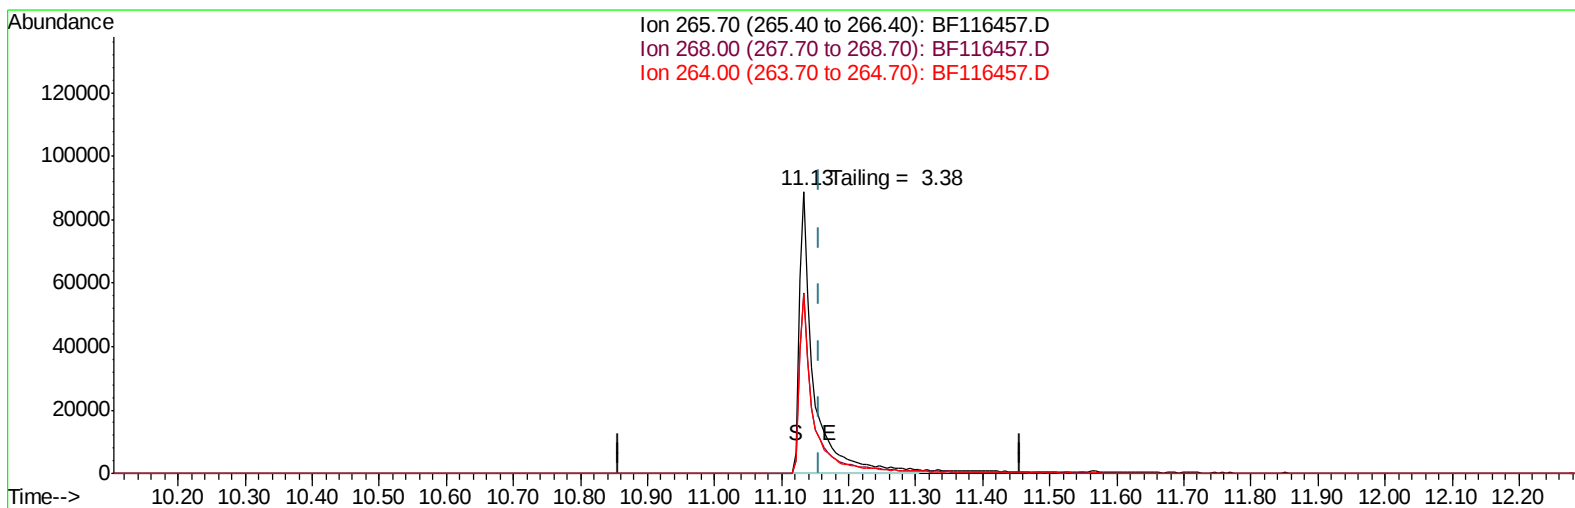

TIC: BF116457.D

(70) Pentachlorophenol (C)

11.133min (-0.023) 60443.82ng

response 131498

Ion	Exp%	Act%
265.70	100	100
268.00	61.00	64.17
264.00	63.30	63.78
0.00	0.00	0.00