


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082119\
 Data File : BF116457.D
 Acq On : 21 Aug 2019 11:09
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 19 06:03:31 2019

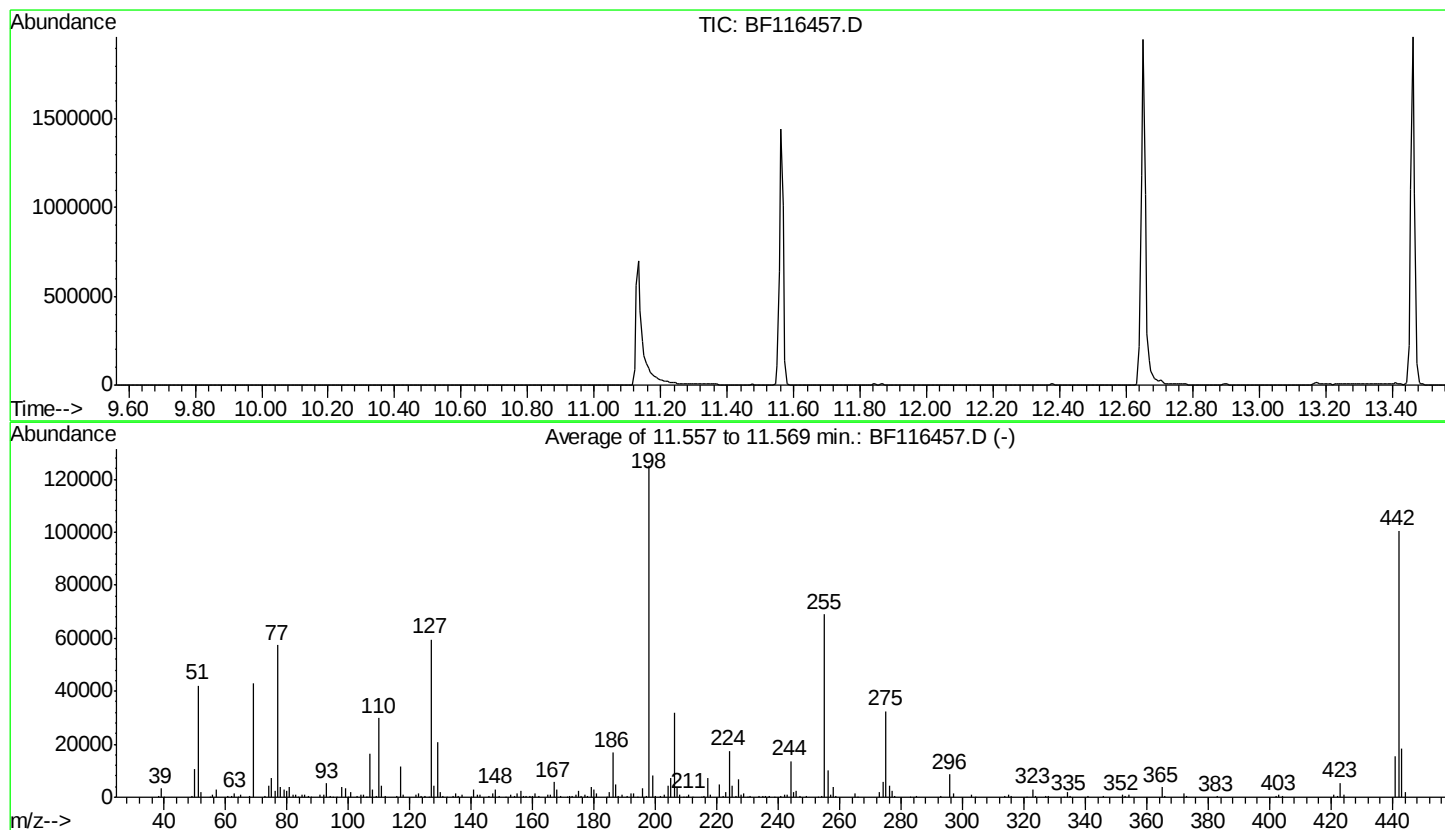

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	42205	PASS
68	69	0.00	2	1.6	670	PASS
69	198	0.00	100	34.5	43109	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	59602	PASS
197	198	0.00	2	0.6	697	PASS
198	198	100	100	100.0	125122	PASS
199	198	5	9	6.6	8270	PASS
275	198	10	60	26.0	32499	PASS
365	198	1	100	3.1	3820	PASS
441	198	0.01	100	12.5	15582	PASS
442	198	50	100	80.4	100576	PASS
443	442	15	24	18.5	18615	PASS