
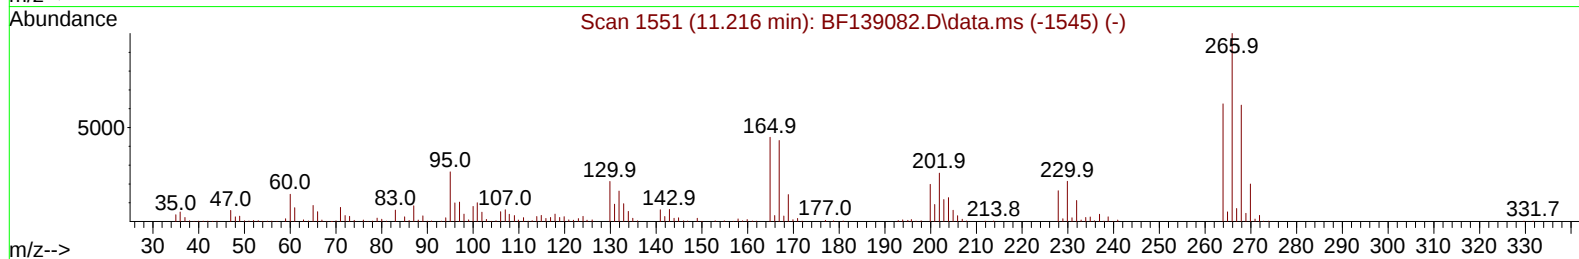
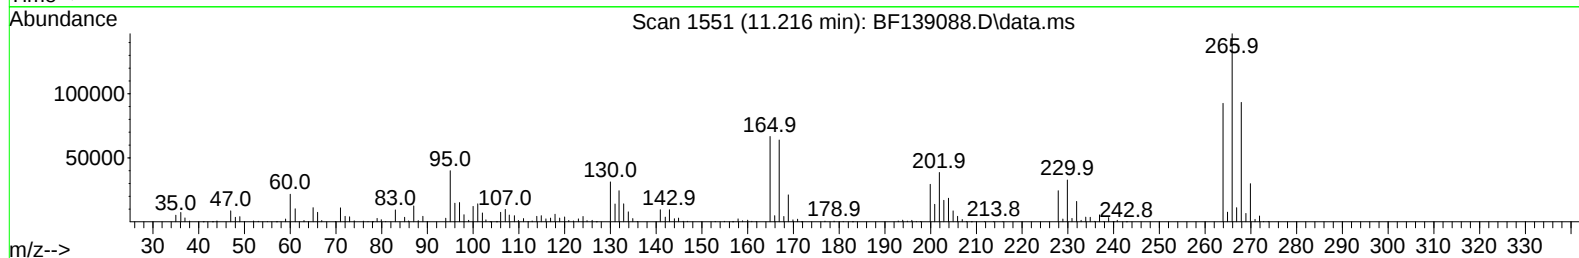


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082124\
Data File : BF139088.D
Acq On : 21 Aug 2024 08:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 10:58:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

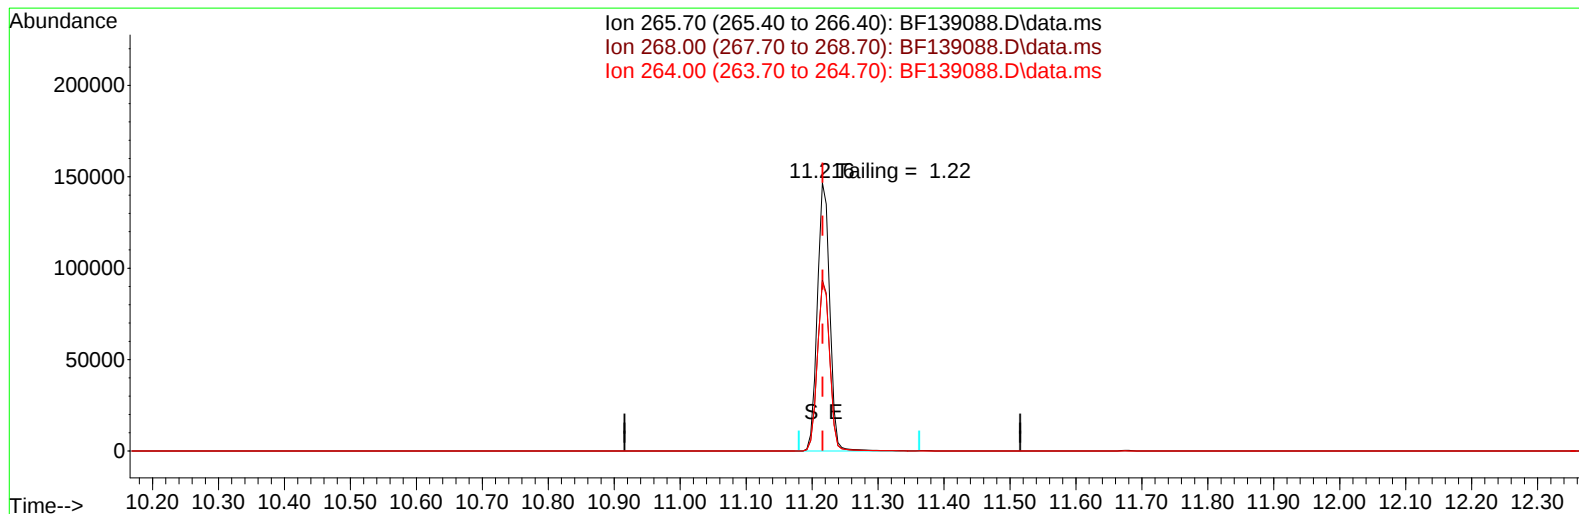

TIC: BF139088.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.000) 37589.26 ng

response 190800

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.56
264.00	62.50	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082124\
Data File : BF139088.D
Acq On : 21 Aug 2024 08:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 10:58:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

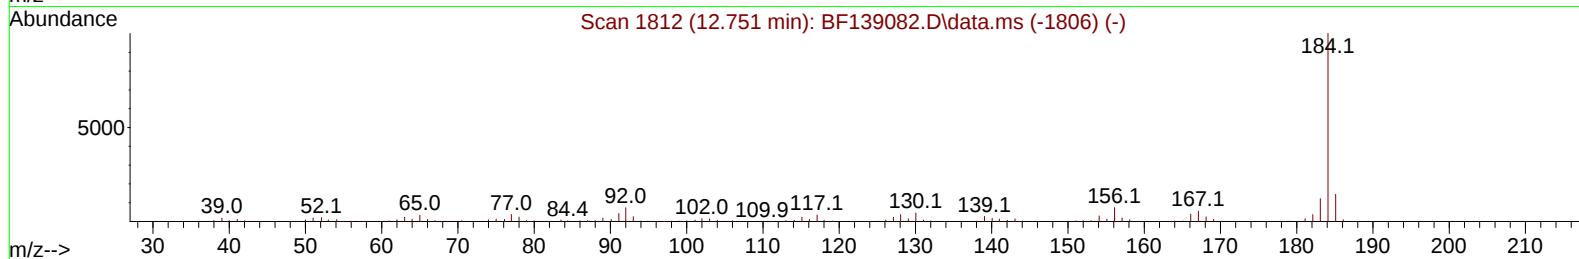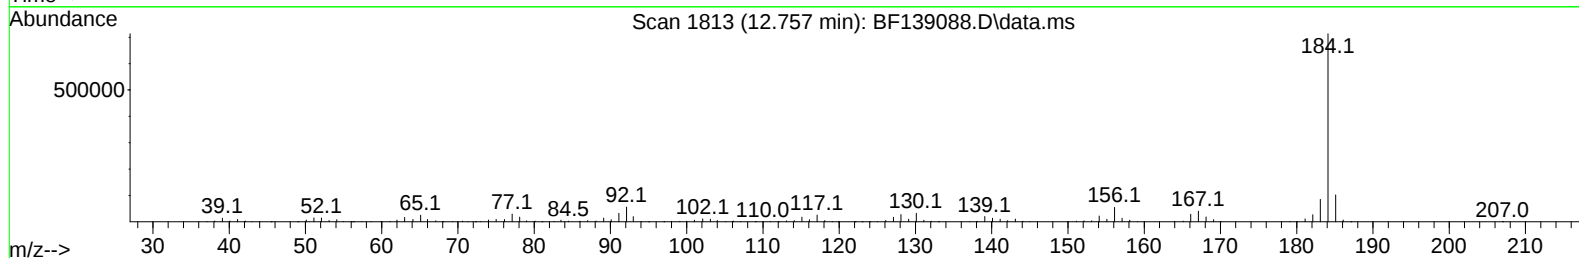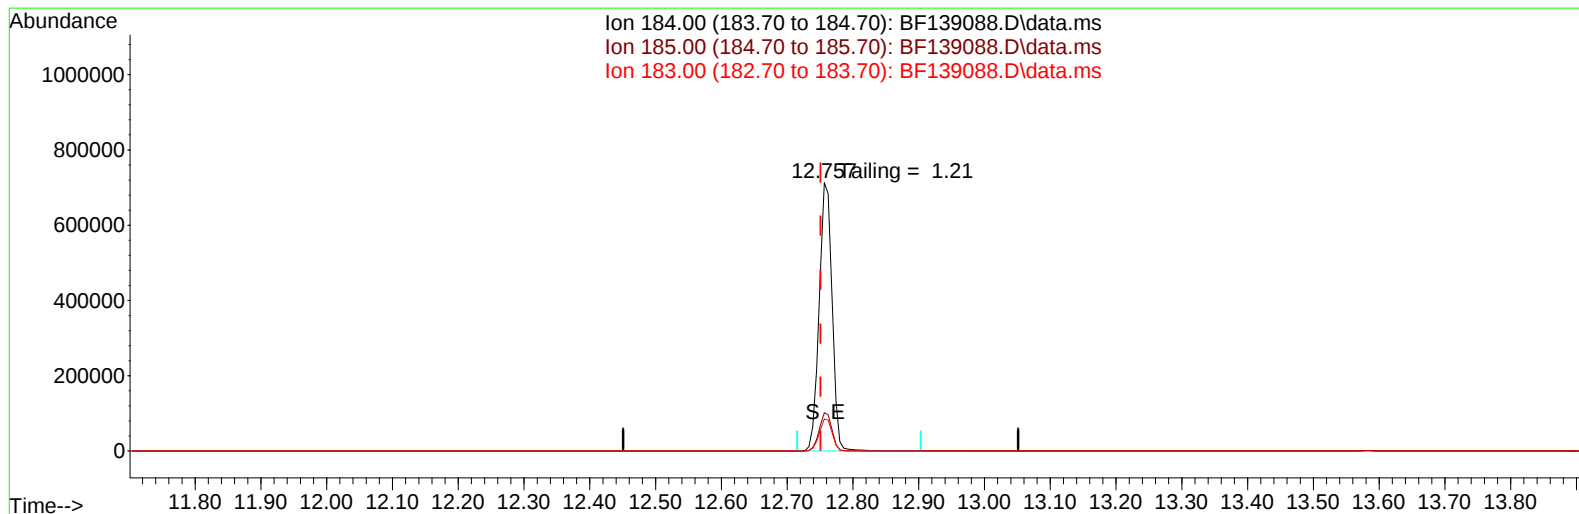

TIC: BF139088.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 977591

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.28
183.00	12.20	11.96
0.00	0.00	0.00