
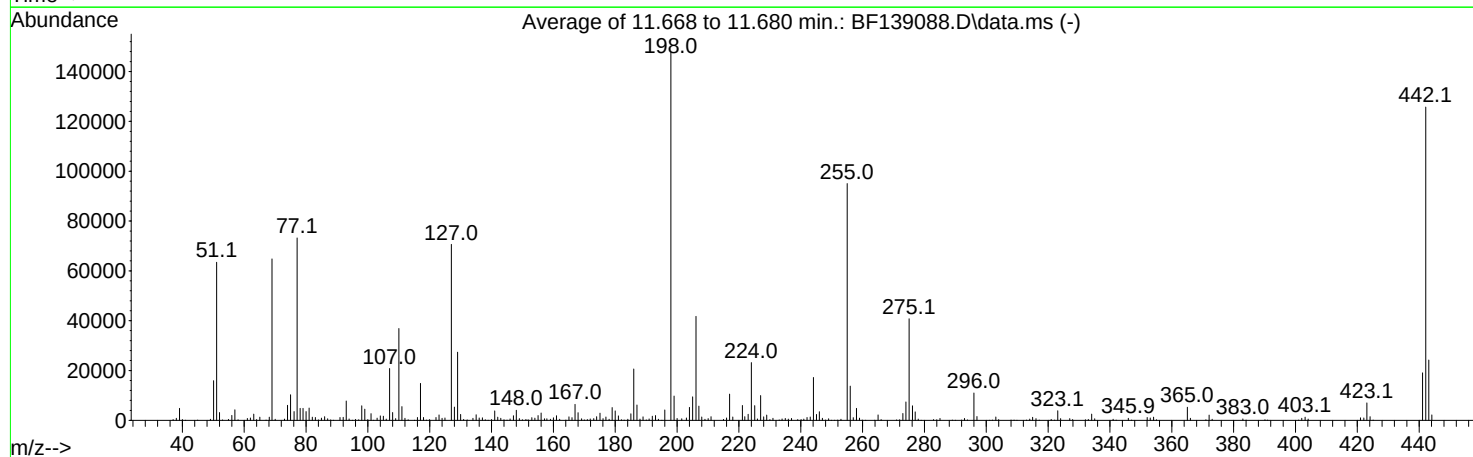


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082124\
Data File : BF139088.D
Acq On : 21 Aug 2024 08:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 21 01:25:05 2024

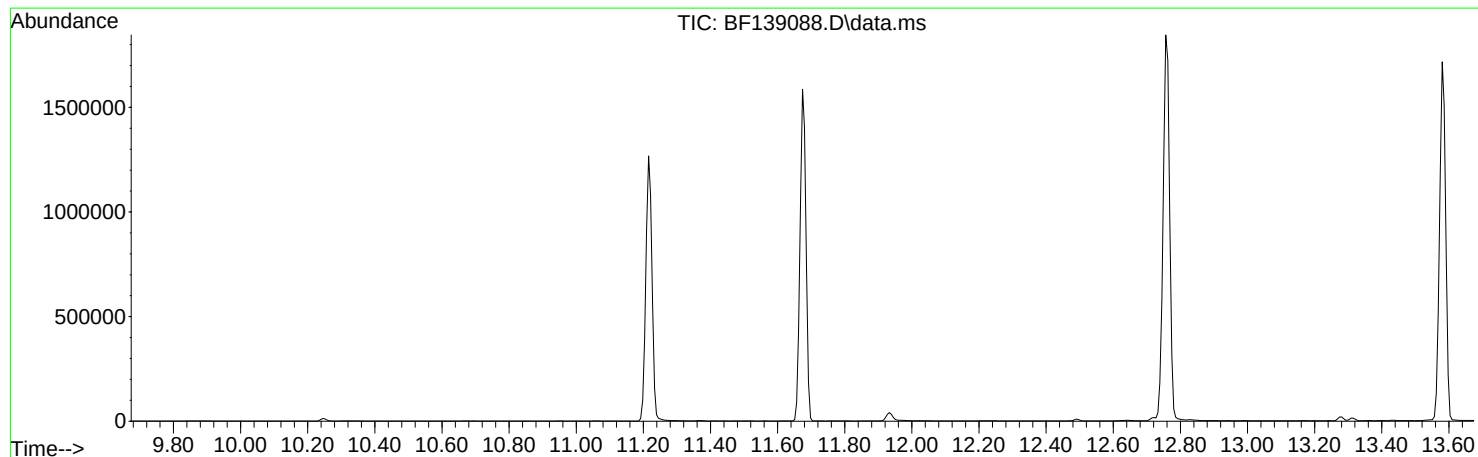

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	63429	PASS
68	69	0.00	2	1.9	1261	PASS
69	198	0.00	100	43.9	64811	PASS
70	69	0.00	2	0.7	430	PASS
127	198	10	80	47.8	70624	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	147637	PASS
199	198	5	9	6.6	9776	PASS
275	198	10	60	27.6	40776	PASS
365	198	1	100	3.6	5276	PASS
441	198	0.01	100	12.9	19087	PASS
442	442	50	100	100.0	125725	PASS
443	442	15	24	19.2	24185	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/21/2024	BNA_F	<u>BF139088.D</u>
Compound Name	Response	Retention Time
DDT	401905	13.58
DDD	8368	13.28
DDE	0	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8368	410273	2.04

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082124\
Data File : BF139088.D
Acq On : 21 Aug 2024 08:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 21 10:58:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

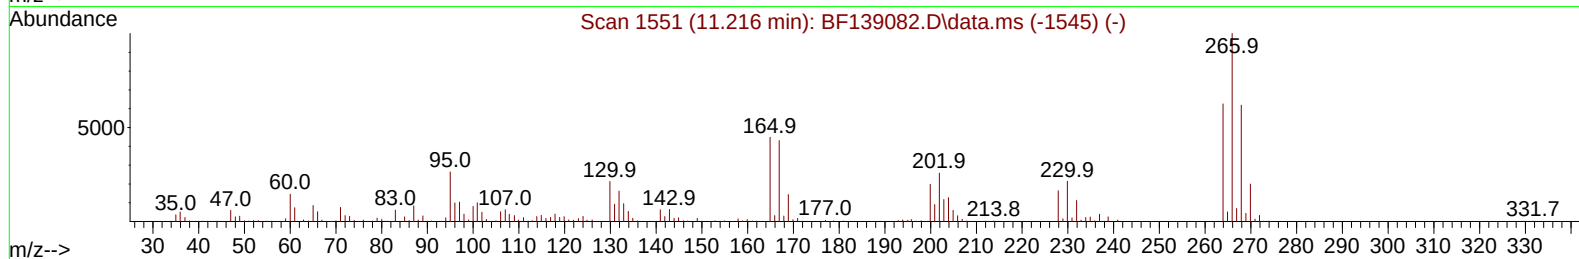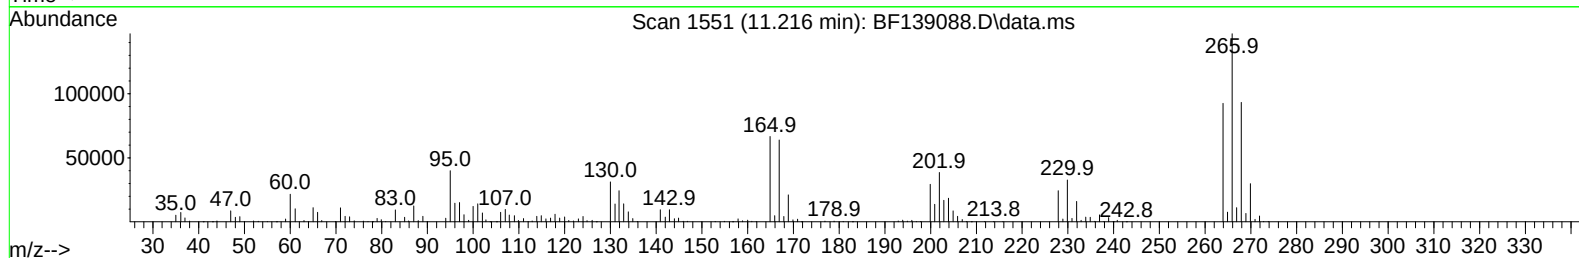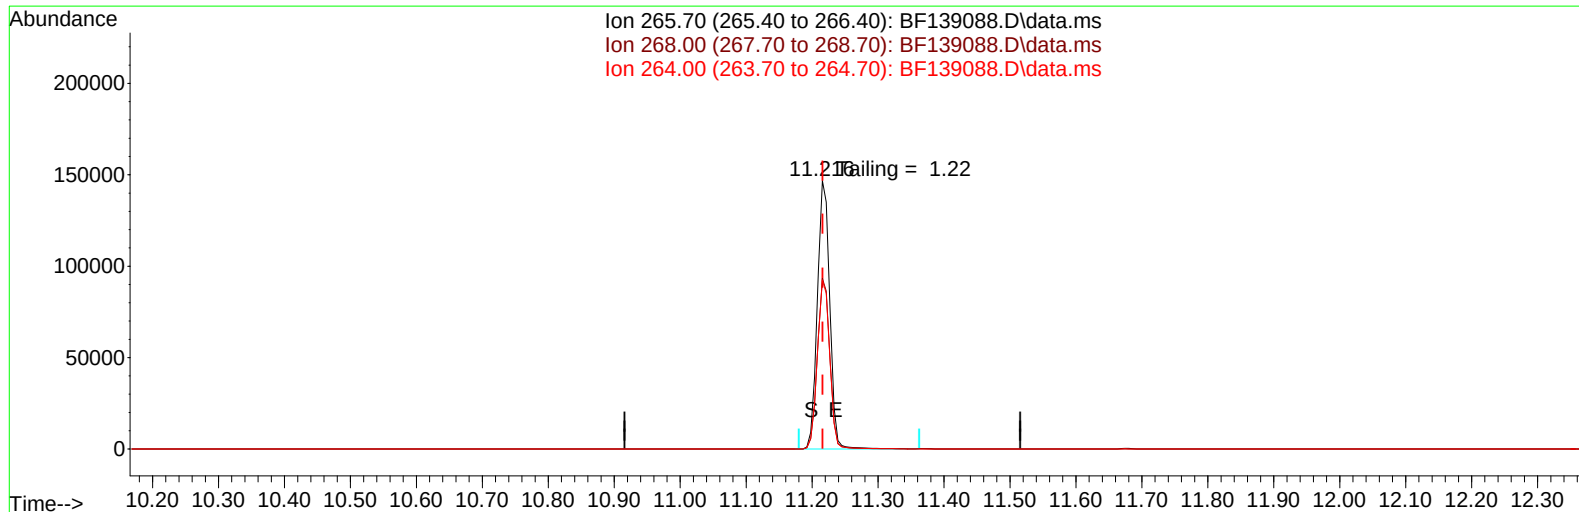

TIC: BF139088.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.000) 37589.26 ng




response 190800

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.56
264.00	62.50	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082124\
Data File : BF139088.D
Acq On : 21 Aug 2024 08:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 21 10:58:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

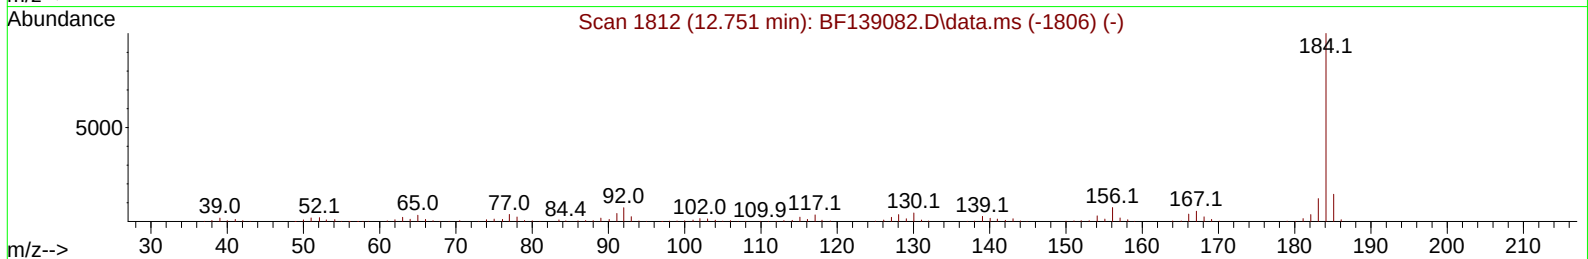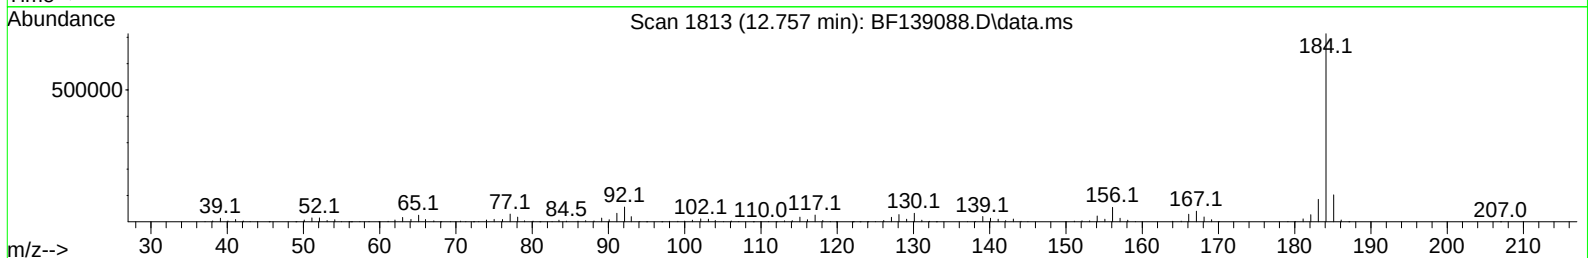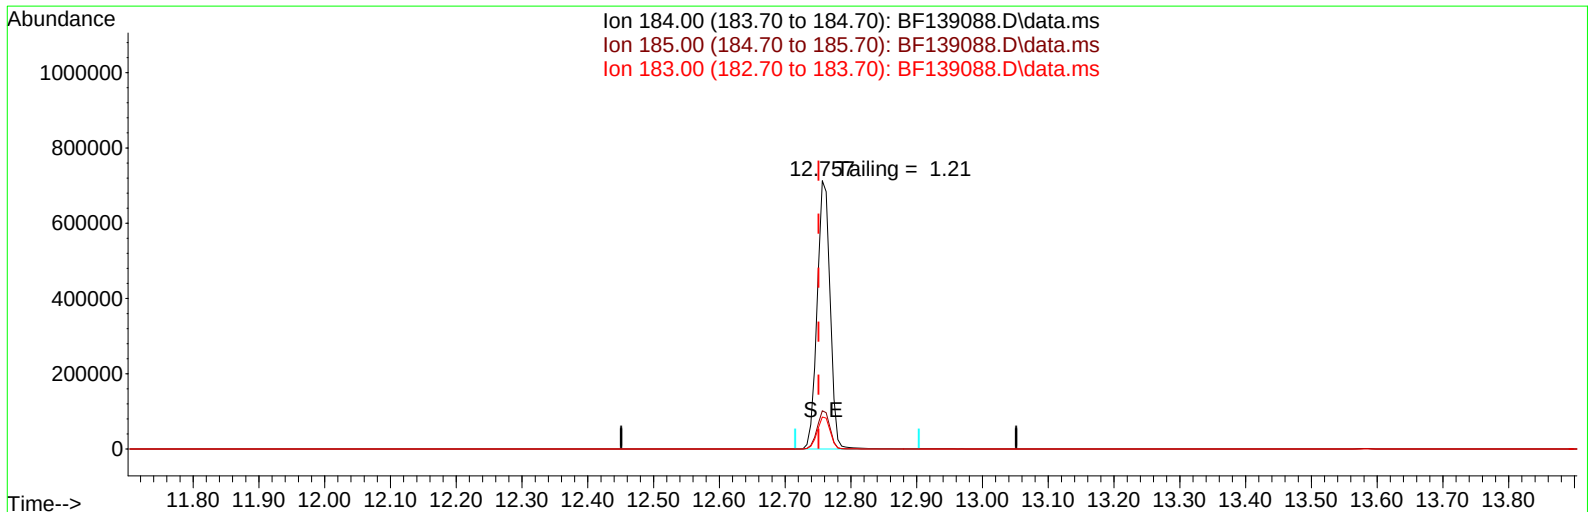

TIC: BF139088.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 977591

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.28
183.00	12.20	11.96
0.00	0.00	0.00