
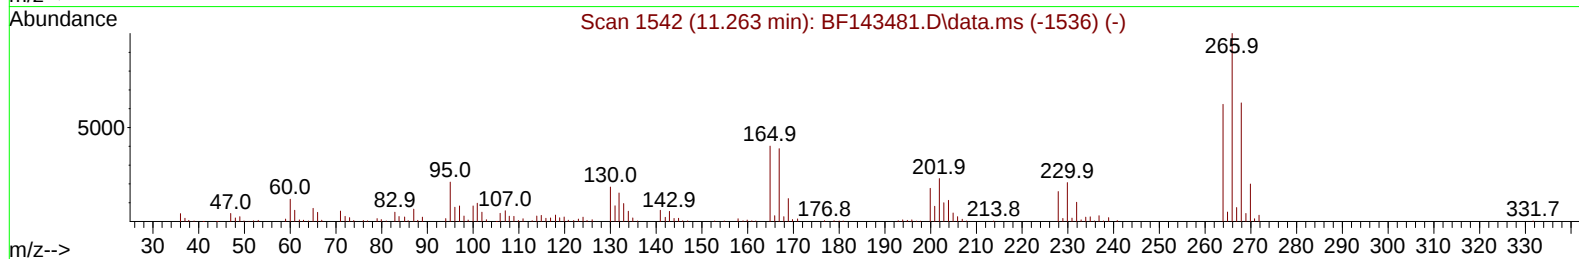
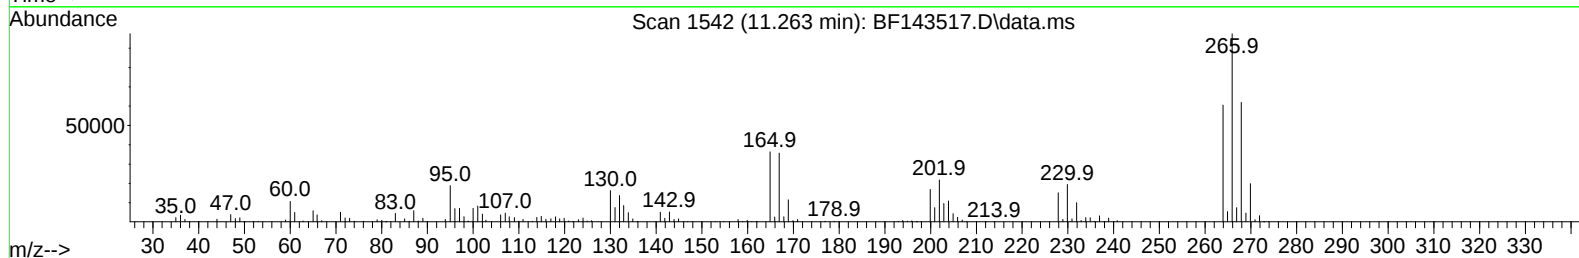


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\
Data File : BF143517.D
Acq On : 21 Aug 2025 08:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 08:42:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration

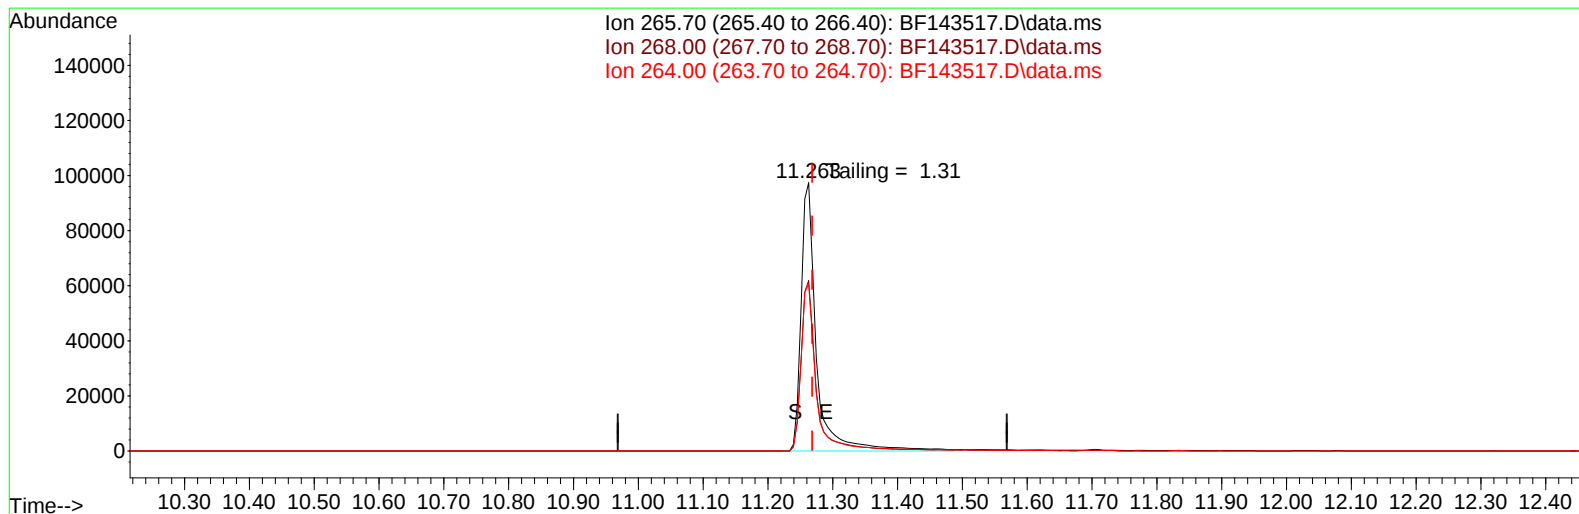

TIC: BF143517.D\data.ms

(70) Pentachlorophenol (C)




11.263min (-0.006) 27043.48 ng

response 160887

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.52
264.00	62.30	62.15
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\  
Data File : BF143517.D  
Acq On    : 21 Aug 2025  08:20  
Operator   : RC/JU  
Sample     : DFTPP  
Misc       :  
ALS Vial   : 1    Sample Multiplier: 1
```

Quant Time: Aug 21 08:42:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration

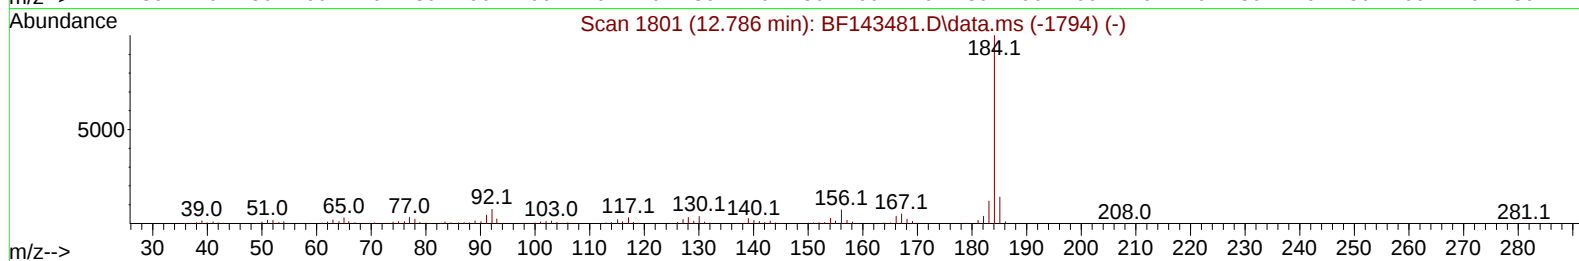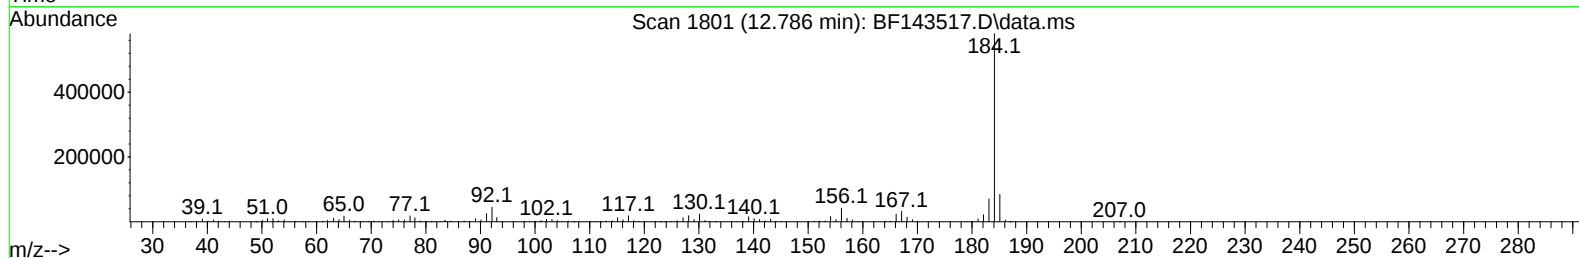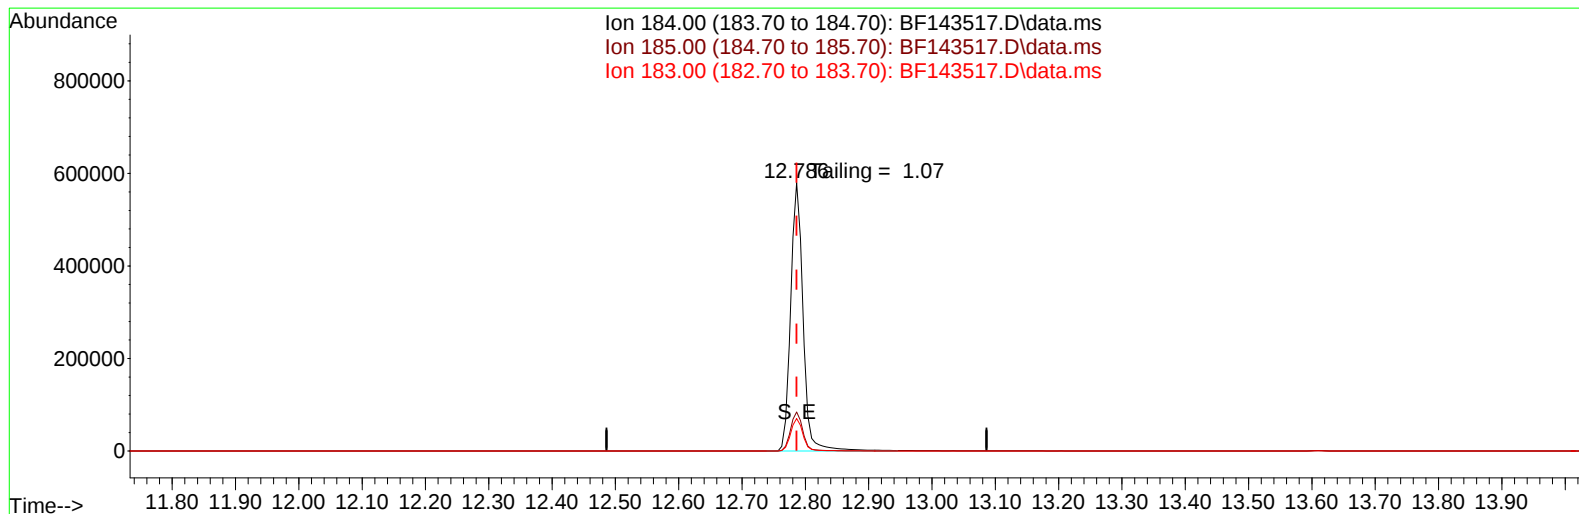

TIC: BF143517.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 116738.94 ng

response **796205**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.10	14.54
--------	-------	-------

183.00	11.90	12.13
--------	-------	-------

0.00 0.00 0.00