

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\
 Data File : BF143521.D
 Acq On : 21 Aug 2025 10:49
 Operator : RC/JU
 Sample : Q2820-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 10PC-S

Quant Time: Aug 21 11:46:16 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 21 06:12:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.928	152	116094	20.000	ng	0.00
21) Naphthalene-d8	8.204	136	448316	20.000	ng	0.00
39) Acenaphthene-d10	9.963	164	237829	20.000	ng	0.00
64) Phenanthrene-d10	11.451	188	358470	20.000	ng	0.00
76) Chrysene-d12	14.092	240	210726	20.000	ng	-0.01
86) Perylene-d12	15.592	264	255976	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.563	112	561340	84.431	ng	0.00
7) Phenol-d6	6.557	99	713706	86.960	ng	-0.02
23) Nitrobenzene-d5	7.481	82	467135	60.804	ng	-0.02
42) 2,4,6-Tribromophenol	10.751	330	193431	87.374	ng	-0.01
45) 2-Fluorobiphenyl	9.281	172	911361	63.330	ng	0.00
79) Terphenyl-d14	13.033	244	743481	61.568	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\
Data File : BF143521.D
Acq On : 21 Aug 2025 10:49
Operator : RC/JU
Sample : Q2820-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
10PC-S

Quant Time: Aug 21 11:46:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration




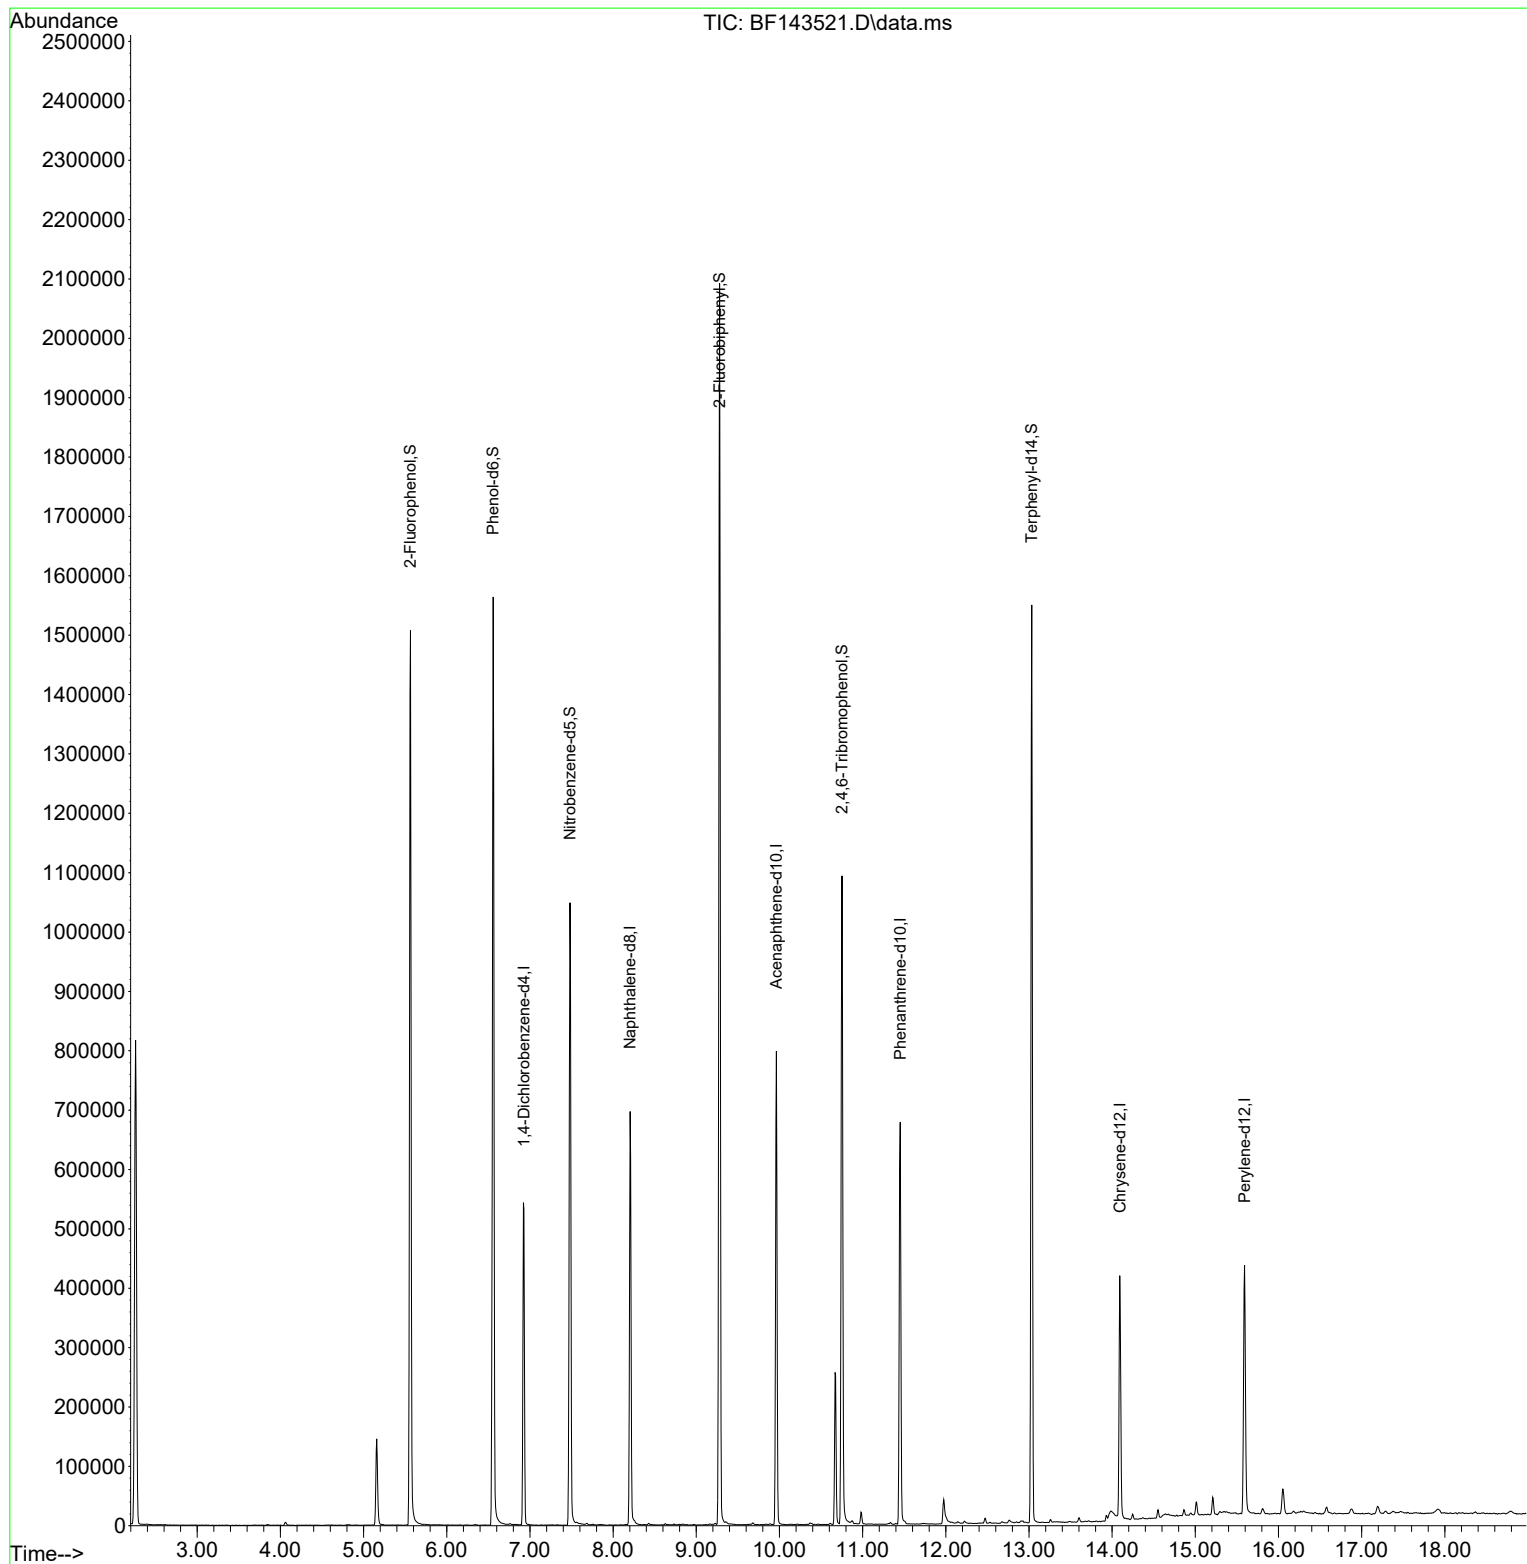


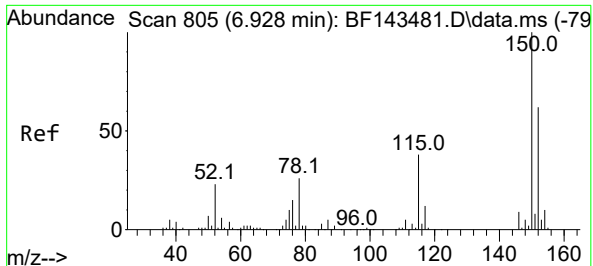

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.928 min Scan# 805
Delta R.T. -0.000 min
Lab File: BF143521.D
Acq: 21 Aug 2025 10:49




Instrument :
BNA_F
ClientSampleId :
10PC-S

Tgt Ion:152 Resp: 116094
Ion Ratio Lower Upper
152 100
150 158.1 128.9 193.3
115 60.3 49.2 73.8

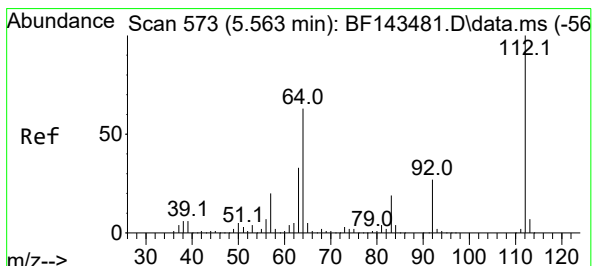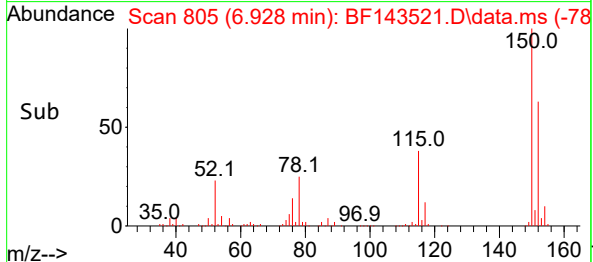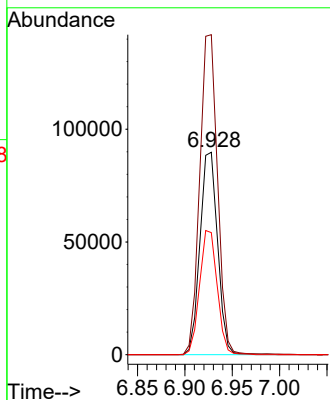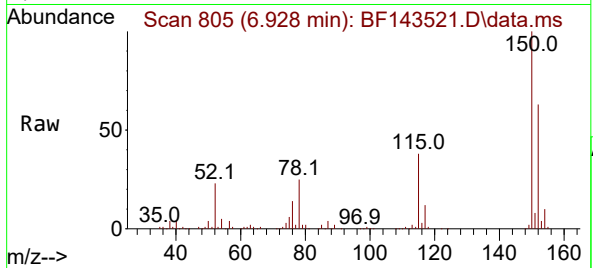

#5
2-Fluorophenol
Concen: 84.431 ng
RT: 5.563 min Scan# 573
Delta R.T. 0.000 min
Lab File: BF143521.D
Acq: 21 Aug 2025 10:49

Tgt Ion:112 Resp: 561340
Ion Ratio Lower Upper
112 100
64 63.3 50.4 75.6
63 32.8 26.4 39.6

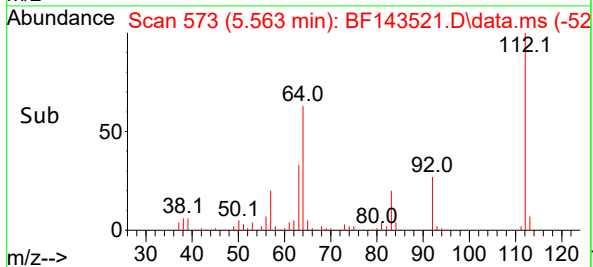
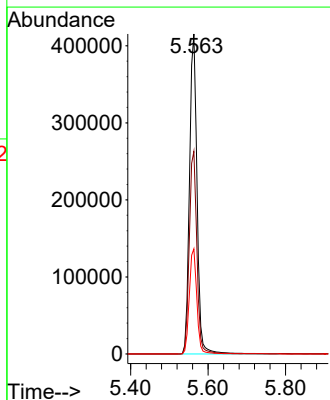
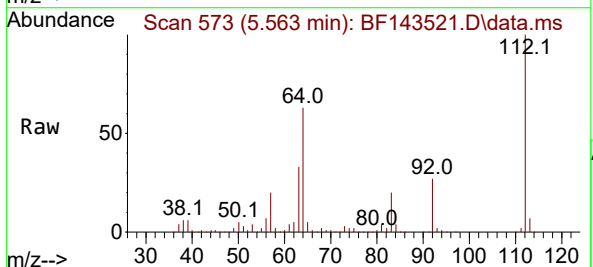




#7
Phenol-d6
Concen: 86.960 ng
RT: 6.557 min Scan# 743
Delta R.T. -0.018 min
Lab File: BF143521.D
Acq: 21 Aug 2025 10:49




Instrument :
BNA_F
ClientSampleId :
10PC-S


Tgt Ion: 99 Resp: 713706
Ion Ratio Lower Upper
99 100
42 20.0 16.3 24.5
71 36.2 28.2 42.2

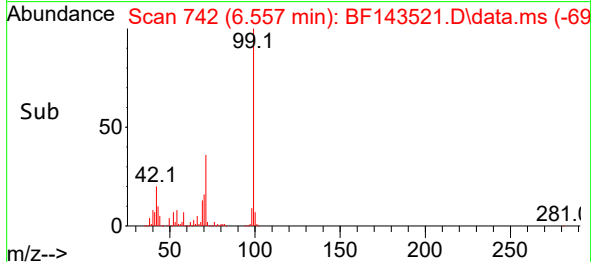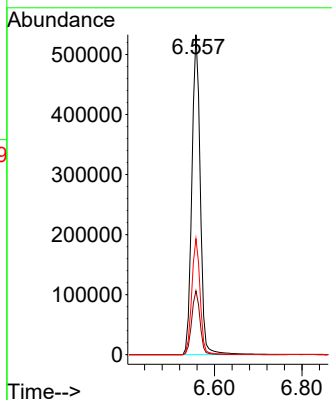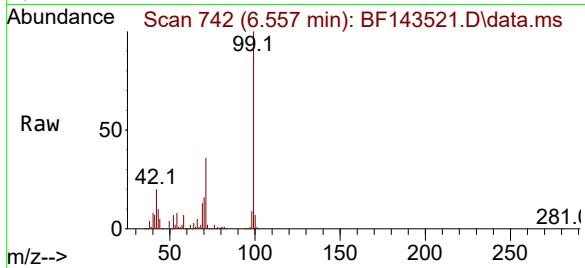

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.204 min Scan# 1022
Delta R.T. -0.006 min
Lab File: BF143521.D
Acq: 21 Aug 2025 10:49

Tgt Ion: 136 Resp: 448316
Ion Ratio Lower Upper
136 100
137 11.3 9.0 13.4
54 9.4 7.4 11.2
68 6.0 5.0 7.4

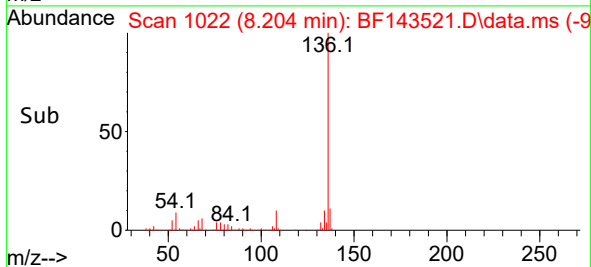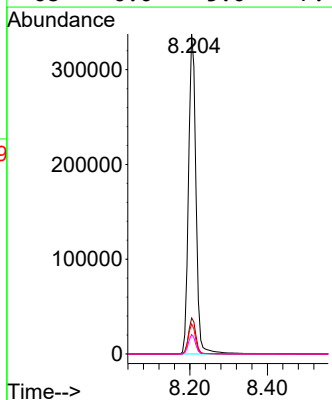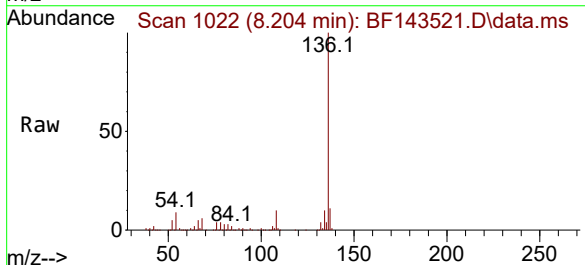

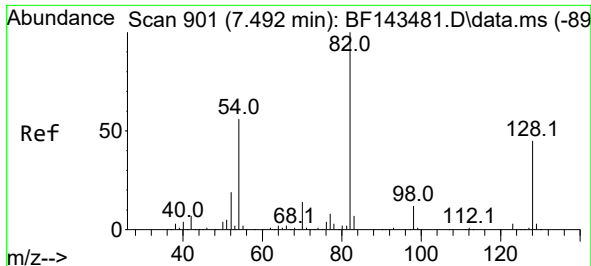

#23

Nitrobenzene-d5

Concen: 60.804 ng

RT: 7.481 min Scan# 899

Delta R.T. -0.018 min

Lab File: BF143521.D

Acq: 21 Aug 2025 10:49

Instrument :

BNA_F

ClientSampleId :

10PC-S





Tgt Ion: 82 Resp: 467135

Ion Ratio Lower Upper

82 100

128 42.8 35.5 53.3

54 56.8 44.3 66.5

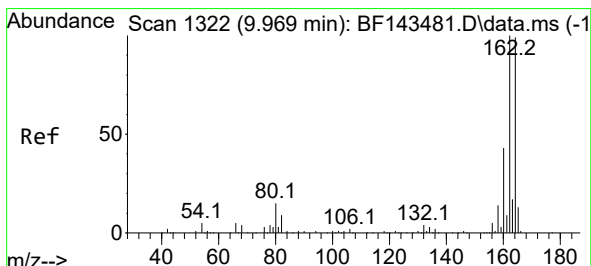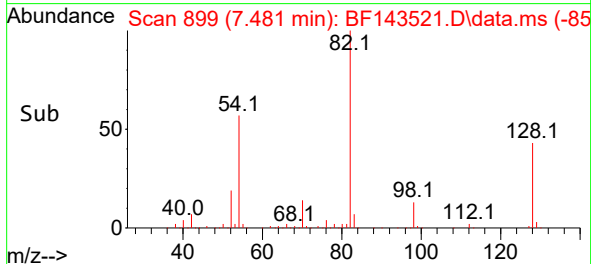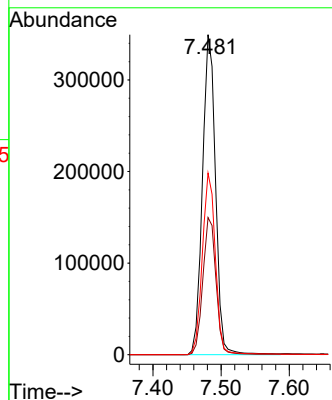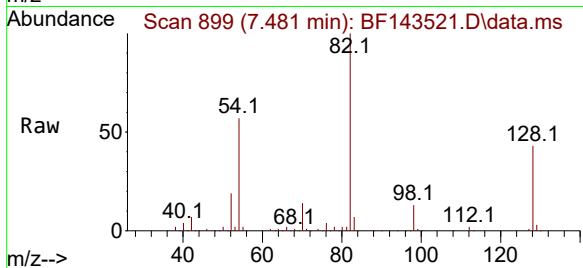

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.963 min Scan# 1321

Delta R.T. -0.006 min

Lab File: BF143521.D

Acq: 21 Aug 2025 10:49




Tgt Ion:164 Resp: 237829


Ion Ratio Lower Upper

164 100

162 101.0 80.5 120.7

160 42.8 34.3 51.5


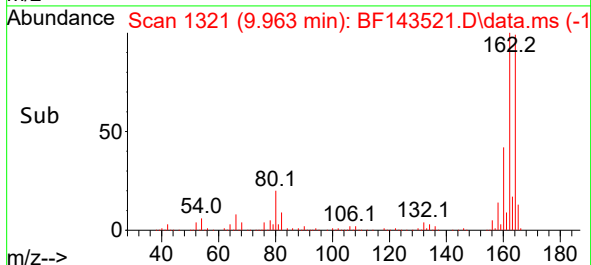
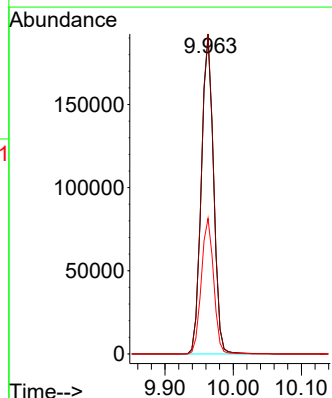
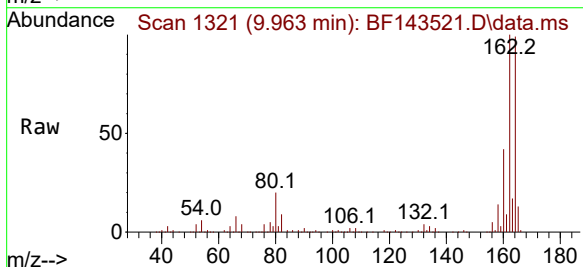


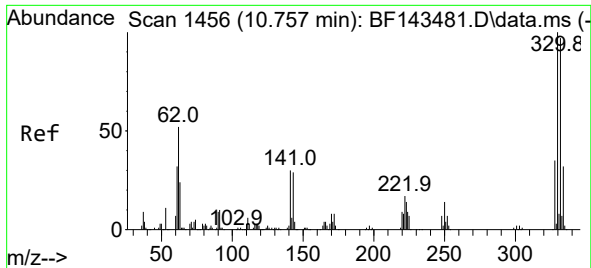

#42
2,4,6-Tribromophenol
Concen: 87.374 ng
RT: 10.751 min Scan# 1456
Delta R.T. -0.012 min
Lab File: BF143521.D
Acq: 21 Aug 2025 10:49




Instrument :
BNA_F
ClientSampleId :
10PC-S


Tgt Ion:330 Resp: 193431
Ion Ratio Lower Upper
330 100
332 97.6 78.0 117.0
141 30.3 23.7 35.5

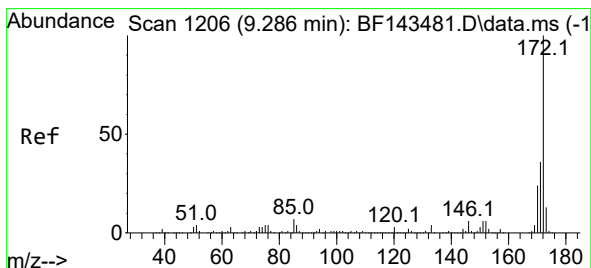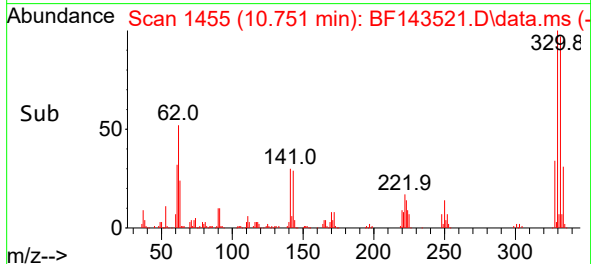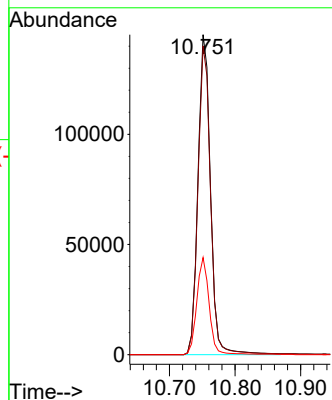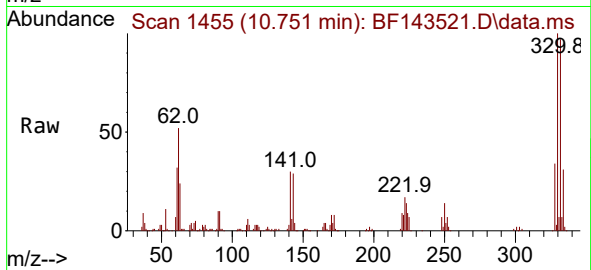

#45
2-Fluorobiphenyl
Concen: 63.330 ng
RT: 9.281 min Scan# 1205
Delta R.T. -0.006 min
Lab File: BF143521.D
Acq: 21 Aug 2025 10:49

Tgt Ion:172 Resp: 911361
Ion Ratio Lower Upper
172 100
171 35.8 28.8 43.2
170 23.6 18.8 28.2


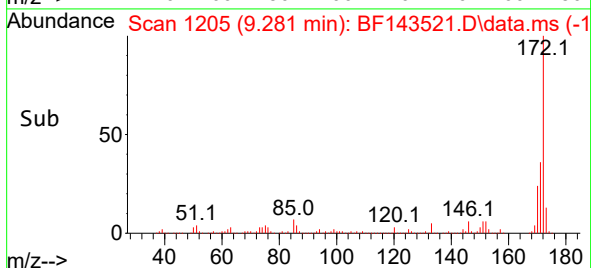
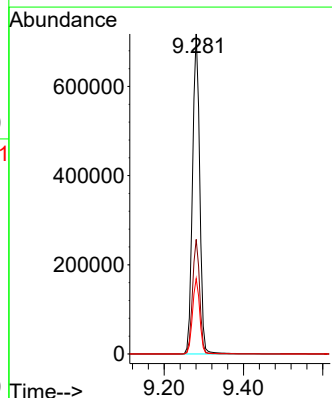
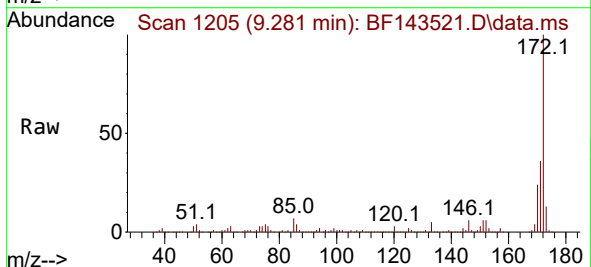


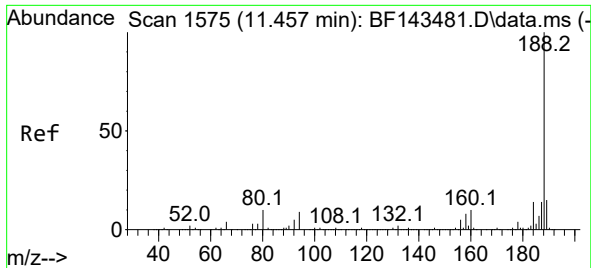

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF143521.D
Acq: 21 Aug 2025 10:49




Instrument :
BNA_F
ClientSampleId :
10PC-S


Tgt Ion:188 Resp: 358470
Ion Ratio Lower Upper
188 100
94 9.3 7.4 11.2
80 10.3 8.2 12.4

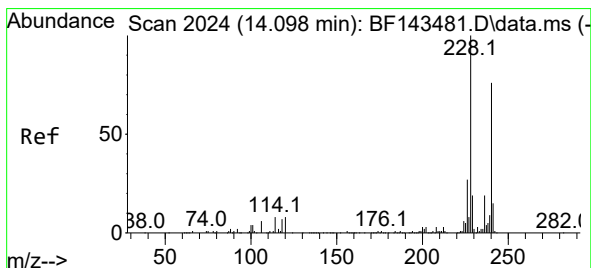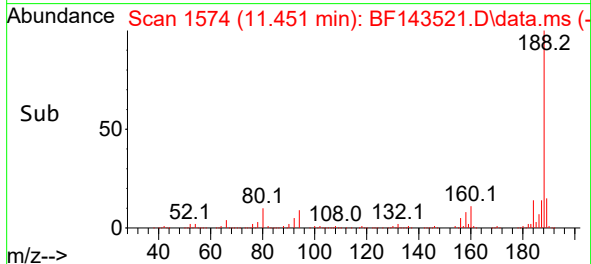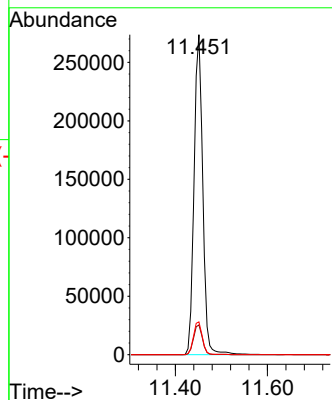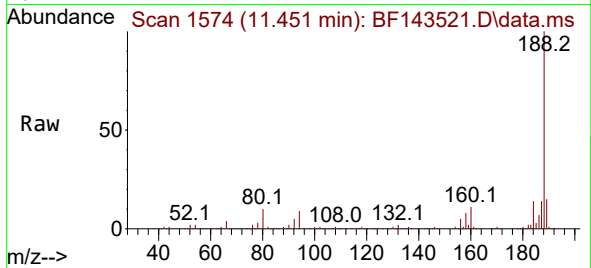

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.092 min Scan# 2023
Delta R.T. -0.012 min
Lab File: BF143521.D
Acq: 21 Aug 2025 10:49

Tgt Ion:240 Resp: 210726
Ion Ratio Lower Upper
240 100
120 10.4 8.6 12.8
236 24.5 20.4 30.6


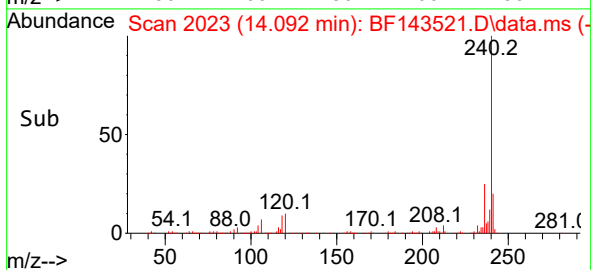
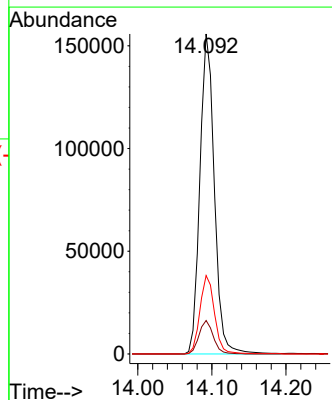
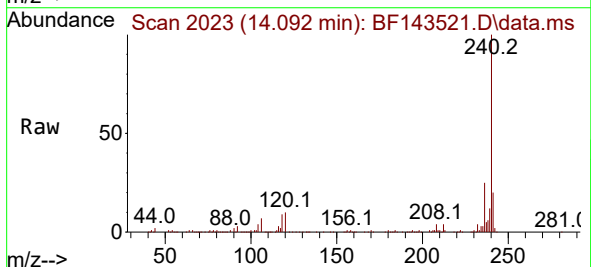


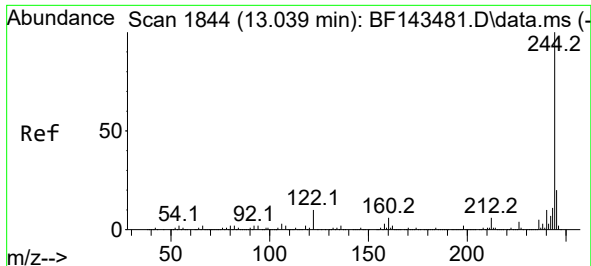

#79
 Terphenyl-d14
 Concen: 61.568 ng
 RT: 13.033 min Scan# 1844
 Delta R.T. -0.006 min
 Lab File: BF143521.D
 Acq: 21 Aug 2025 10:49

Instrument :
 BNA_F
 ClientSampleId :
 10PC-S

Tgt Ion:244 Resp: 743481
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.2 7.8
 122 10.0 7.9 11.9

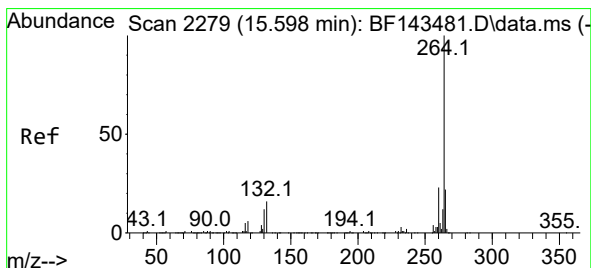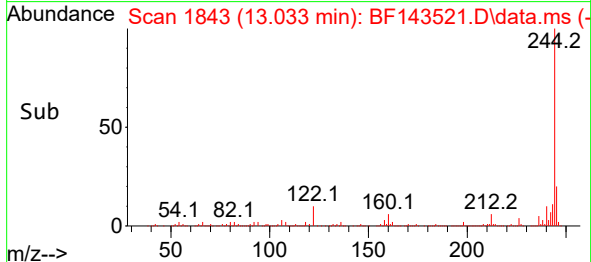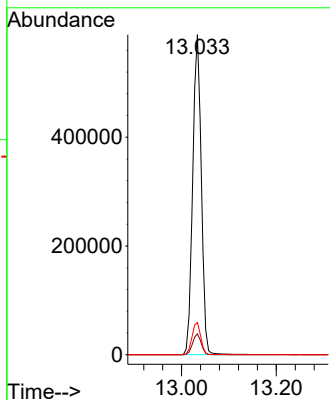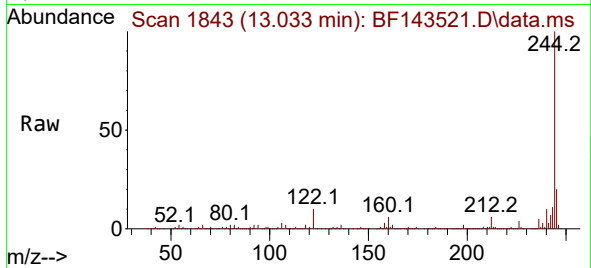

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.592 min Scan# 2278
 Delta R.T. -0.006 min
 Lab File: BF143521.D
 Acq: 21 Aug 2025 10:49

Tgt Ion:264 Resp: 255976
 Ion Ratio Lower Upper
 264 100
 260 23.5 18.7 28.1
 265 21.6 17.6 26.4

