
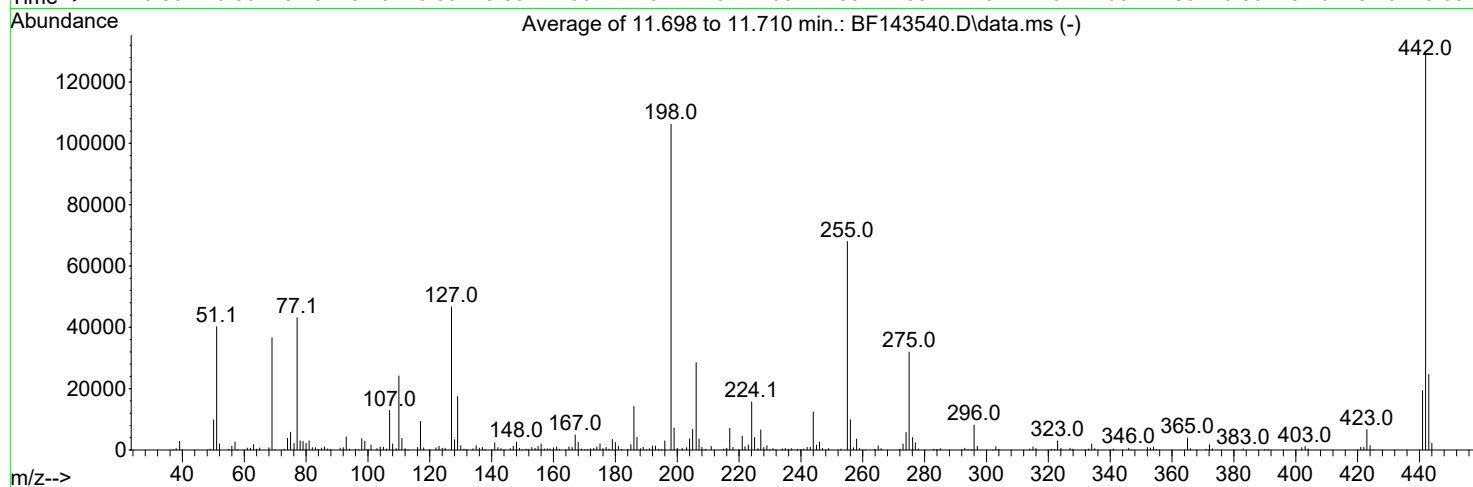


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\
Data File : BF143540.D
Acq On : 21 Aug 2025 20:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 21 06:12:21 2025

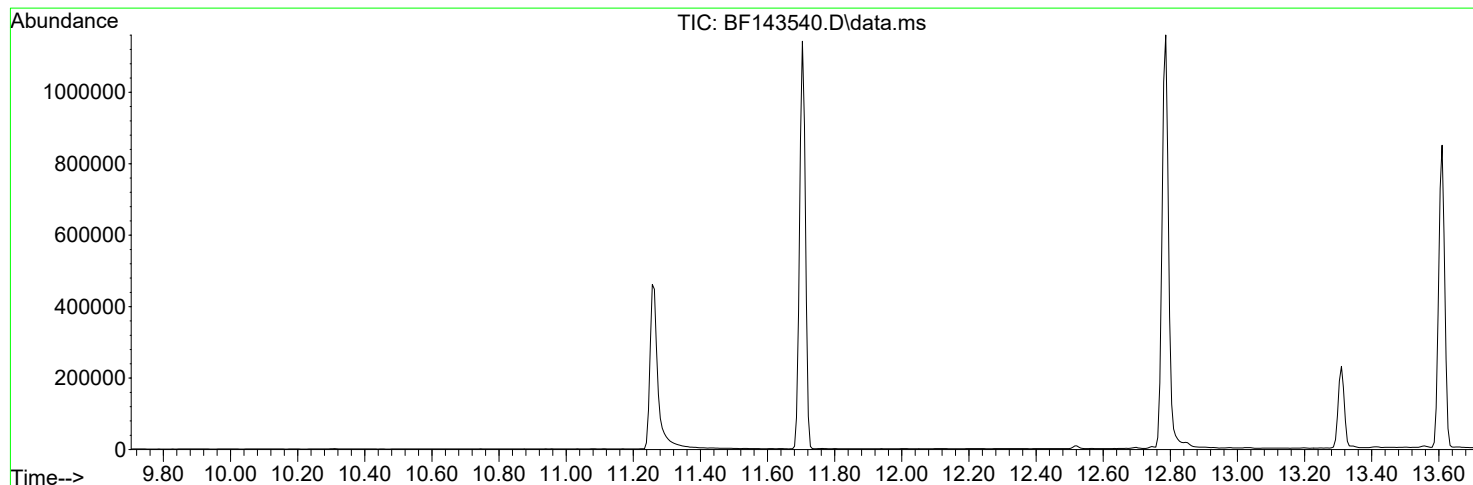

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	724	PASS
69	69	100	100	100.0	36616	PASS
70	69	0.00	2	0.4	144	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106203	PASS
199	198	5	9	6.7	7166	PASS
365	198	1	100	3.7	3899	PASS
441	443	0.01	150	78.9	19432	PASS
442	442	100	100	100.0	128741	PASS
443	442	15	24	19.1	24627	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/21/2025	BNA_F	<u>BF143540.D</u>
Compound Name	Response	Retention Time
DDT	210961	13.61
DDD		13.31
DDE	530	12.974
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
530	211491	0.25

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\
Data File : BF143540.D
Acq On : 21 Aug 2025 20:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 22 01:26:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration

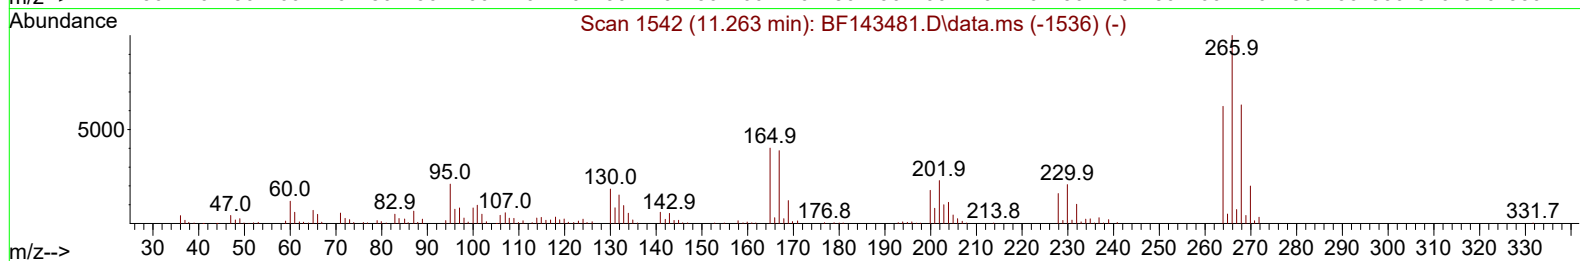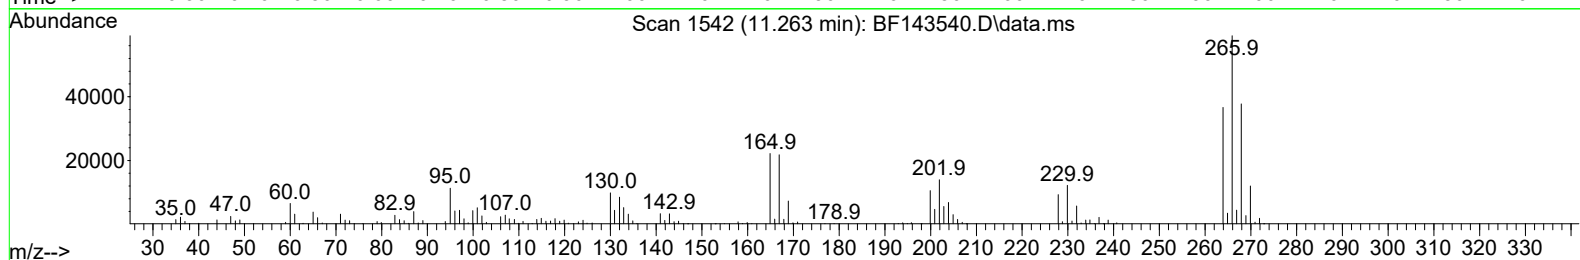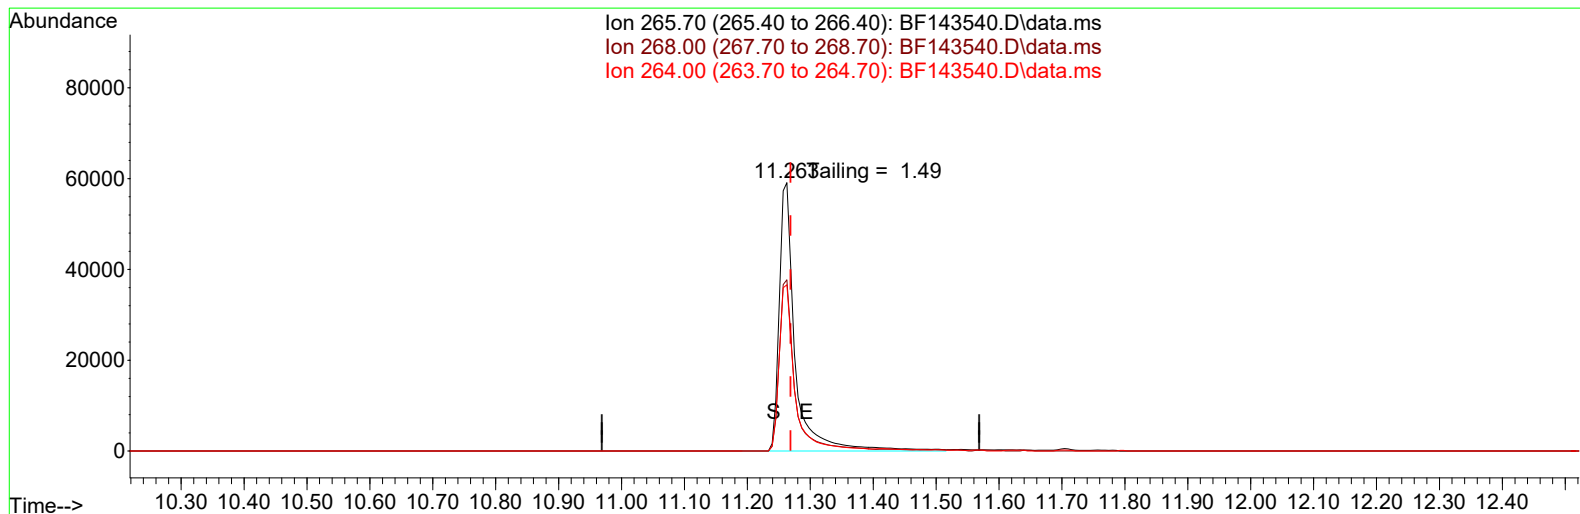

TIC: BF143540.D\data.ms

(70) Pentachlorophenol (C)

11.263min (-0.006) 34019.73 ng




response 104802

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.80
264.00	62.30	61.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\
Data File : BF143540.D
Acq On : 21 Aug 2025 20:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 22 01:26:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration

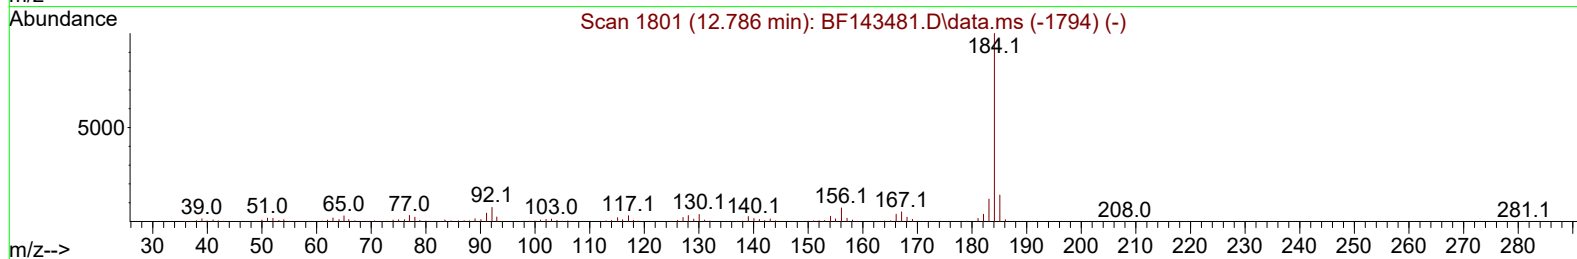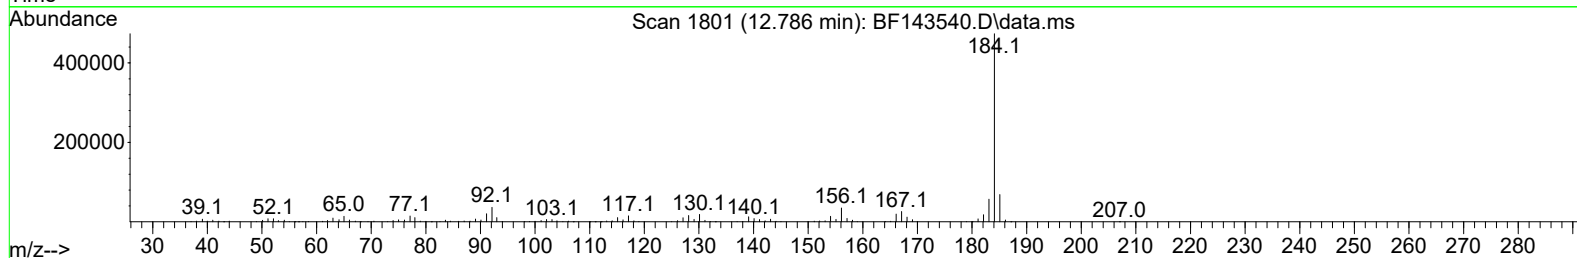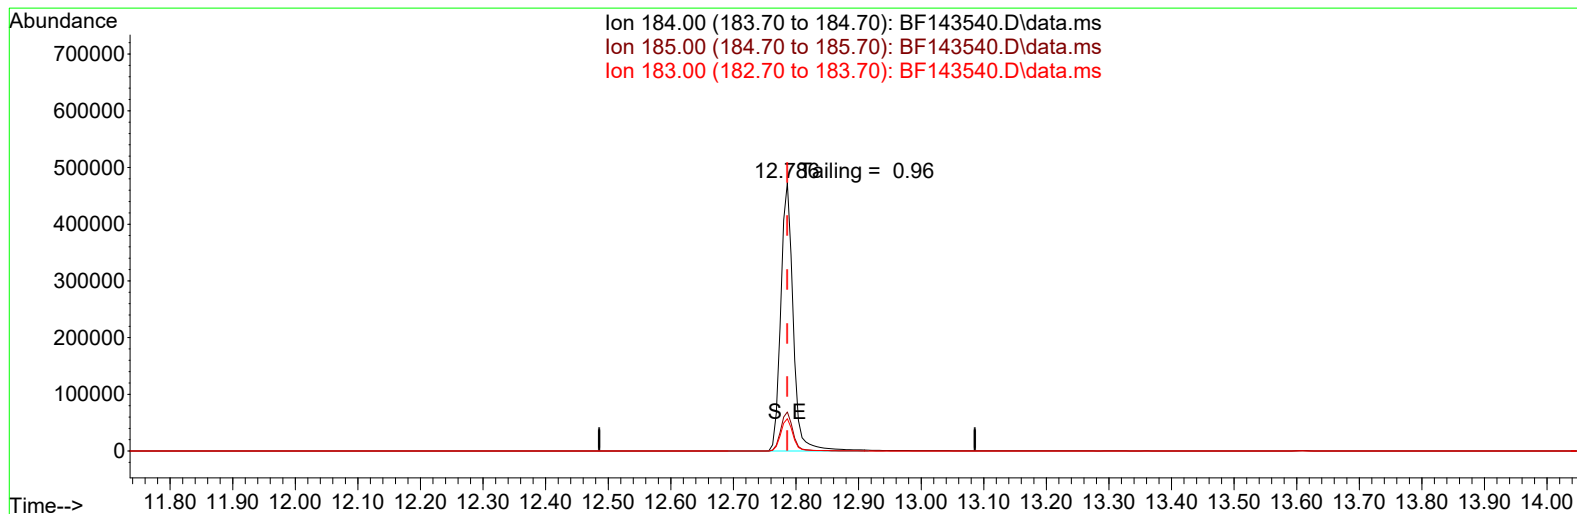

TIC: BF143540.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 0.00 ng

response 658976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.54
183.00	11.90	12.04
0.00	0.00	0.00