
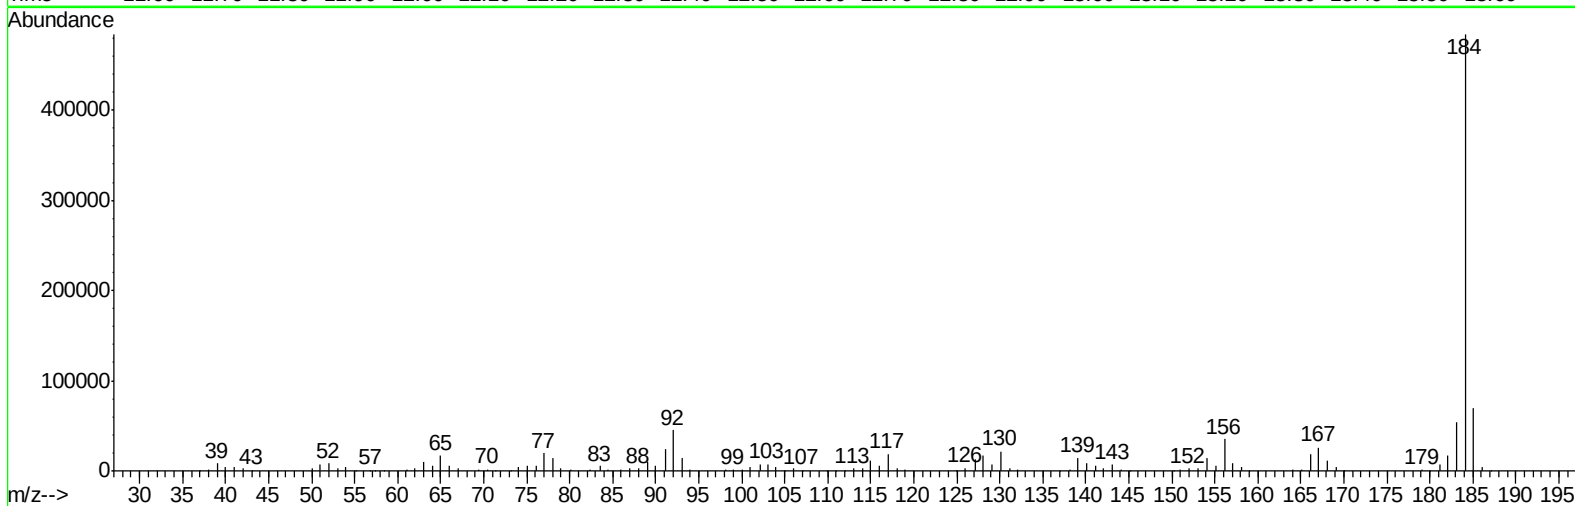


Data Path : Z:\HPCHEM1\BNA F\Data\BF082217\
Data File : BF097957.D
Acq On : 22 Aug 2017 16:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 04:48:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

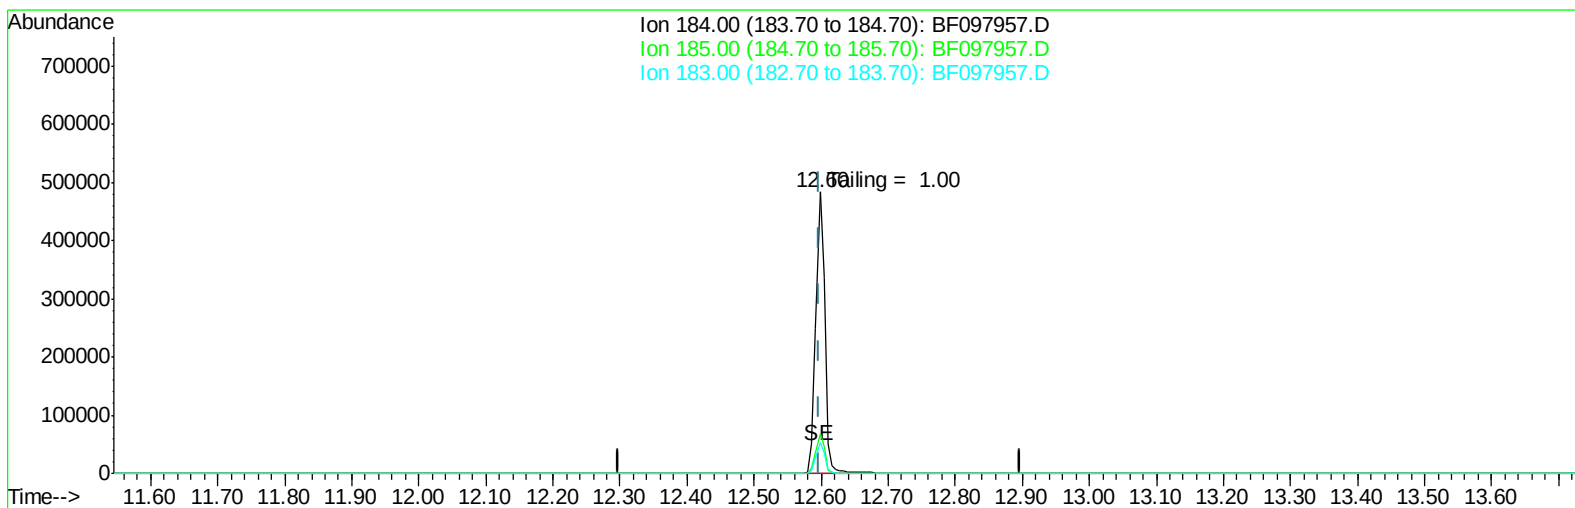

TIC: BF097957.D

(76) Benzidine



12.598min (-0.000) 2018.98ng

response 431478

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.28#
183.00	12.20	11.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF082217\
Data File : BF097957.D
Acq On : 22 Aug 2017 16:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 04:48:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

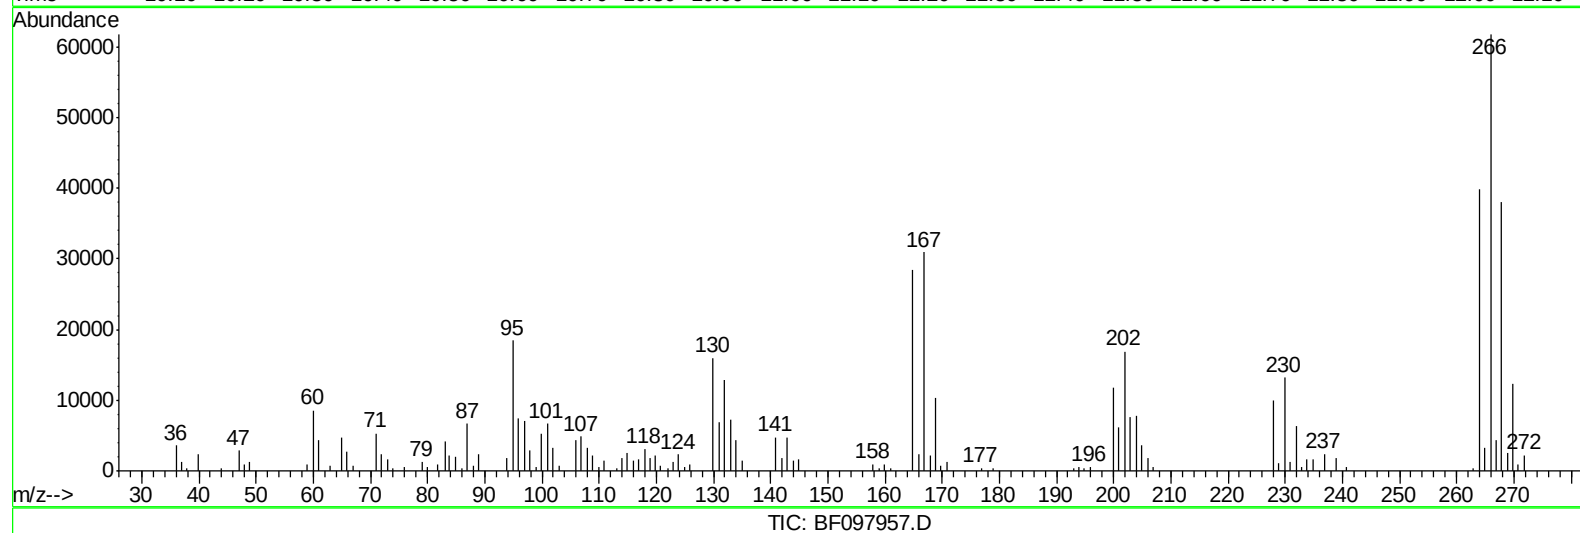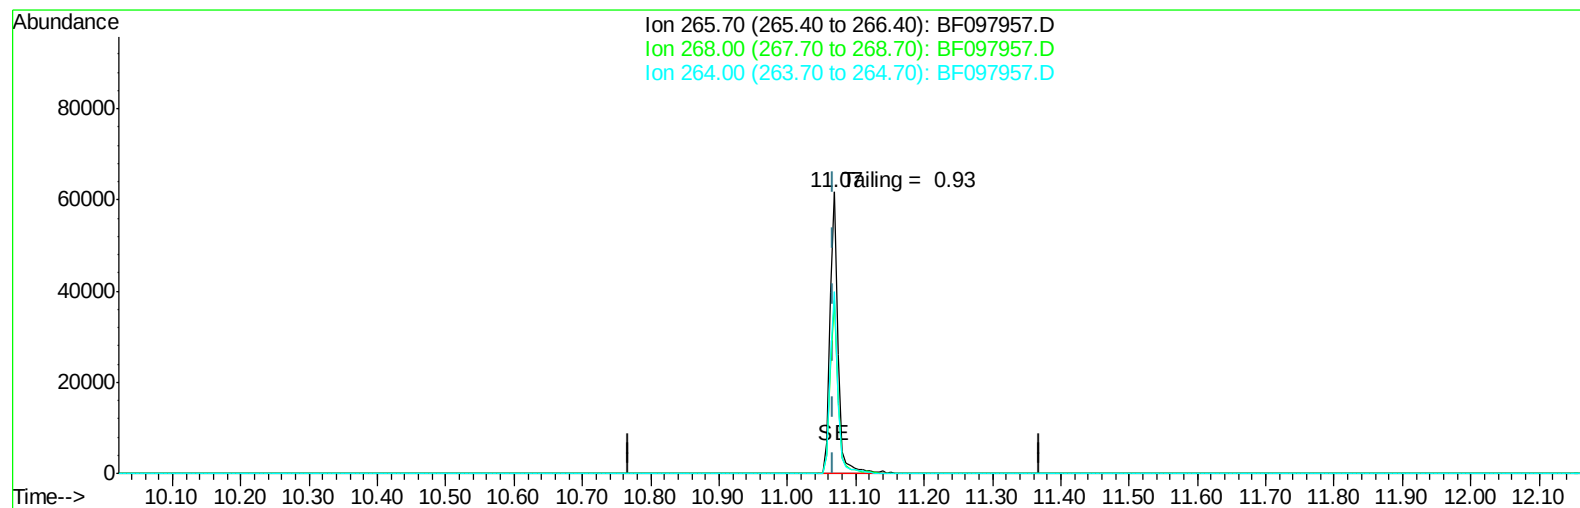

(69) Pentachlorophenol (C)

11.069min (-0.000) 6867.33ng

response 52255

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.54
264.00	64.60	64.59
0.00	0.00	0.00