
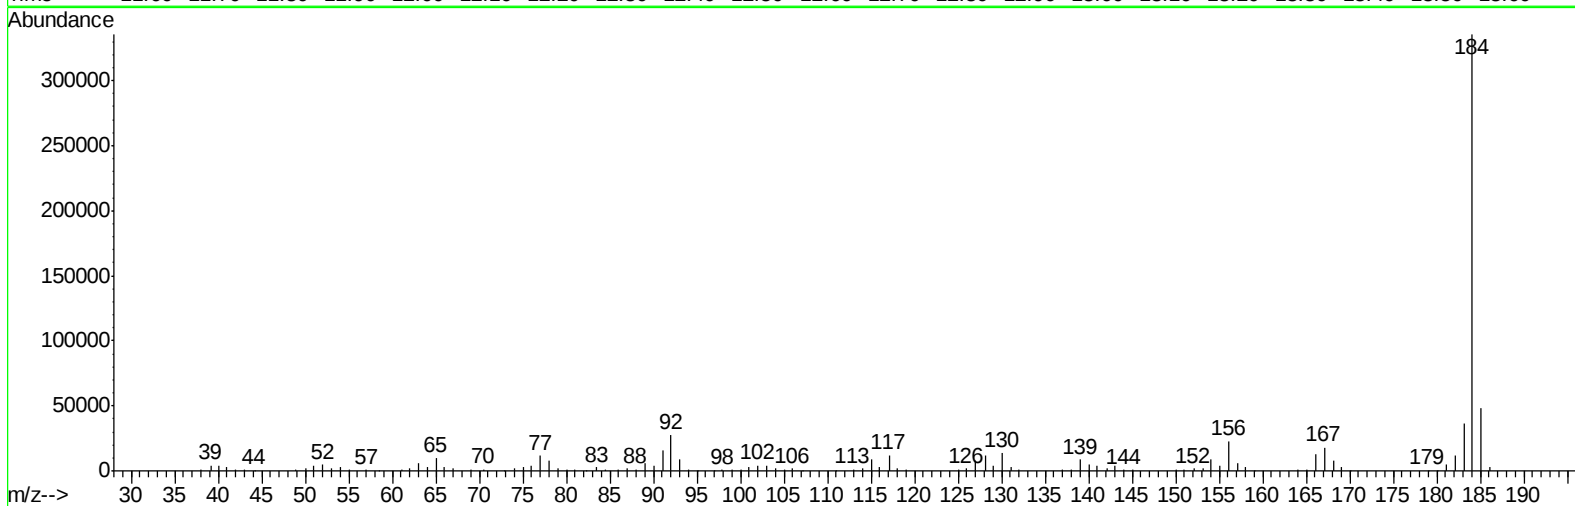


Data Path : Z:\HPCHEM1\BNA F\DATA\BF082217\
 Data File : BF097983.D
 Acq On : 23 Aug 2017 5:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 07:49:08 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 21 15:59:04 2017
 Response via : Initial Calibration

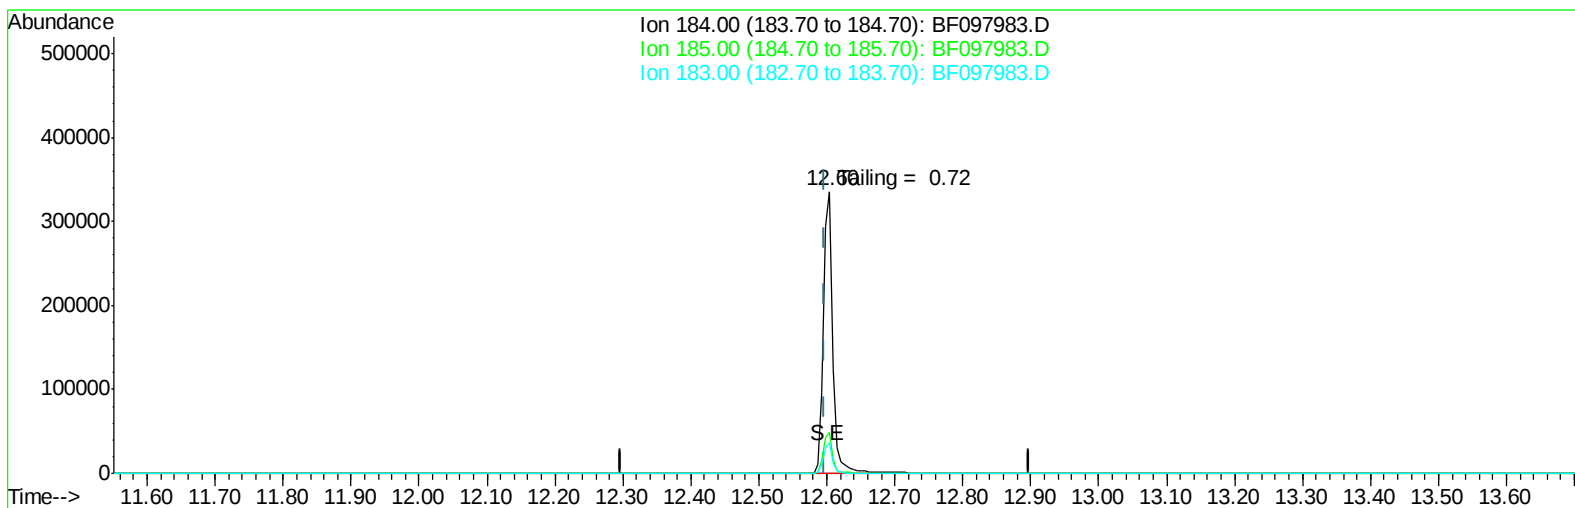

TIC: BF097983.D

(76) Benzidine



12.604min (+0.006) 6404.85ng

response 333271

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.50#
183.00	12.20	10.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082217\
Data File : BF097983.D
Acq On : 23 Aug 2017 5:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 07:49:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

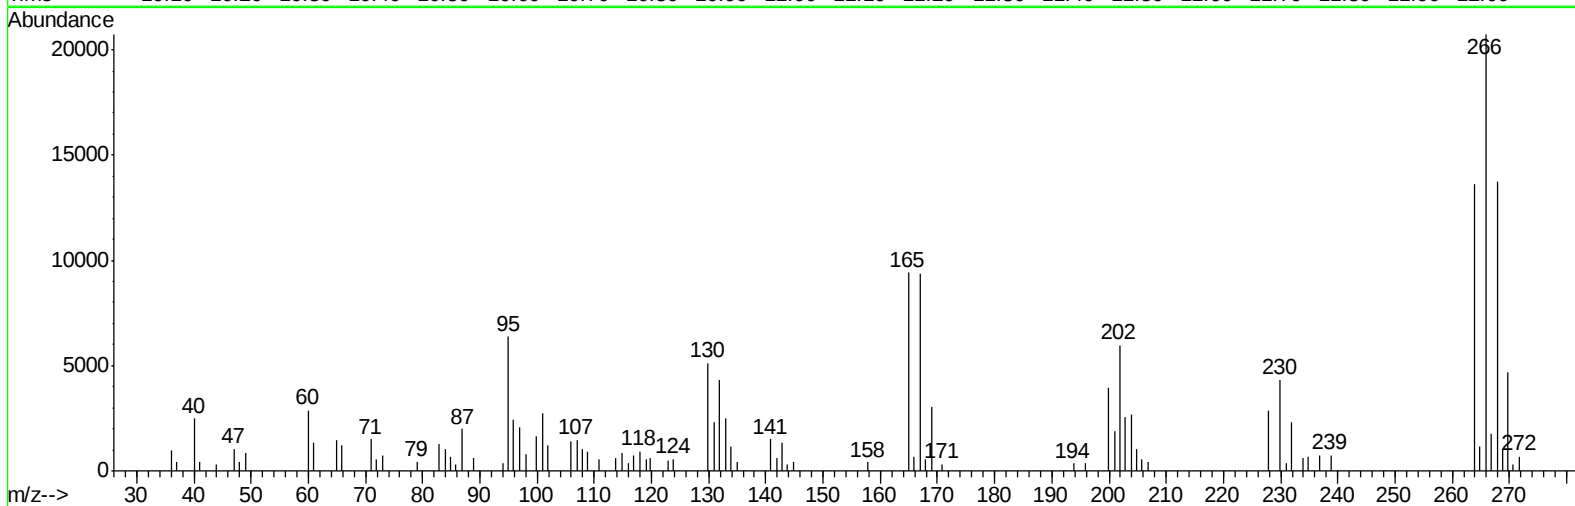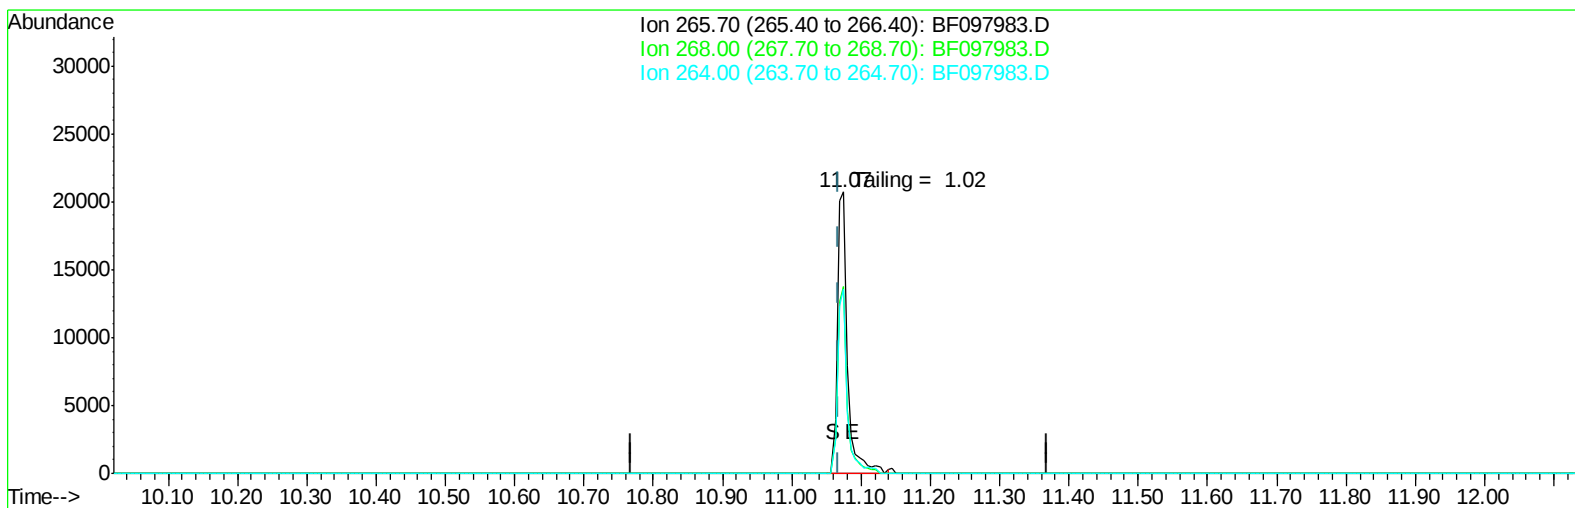

TIC: BF097983.D

(69) Pentachlorophenol (C)

11.074min (+0.006) 7969.20ng

response 21541

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.19
264.00	64.60	65.62
0.00	0.00	0.00