


Data Path : U:\HPCHEM1\BNA F\Data\BF082217\
 Data File : BF097957.D
 Acq On : 22 Aug 2017 16:45
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

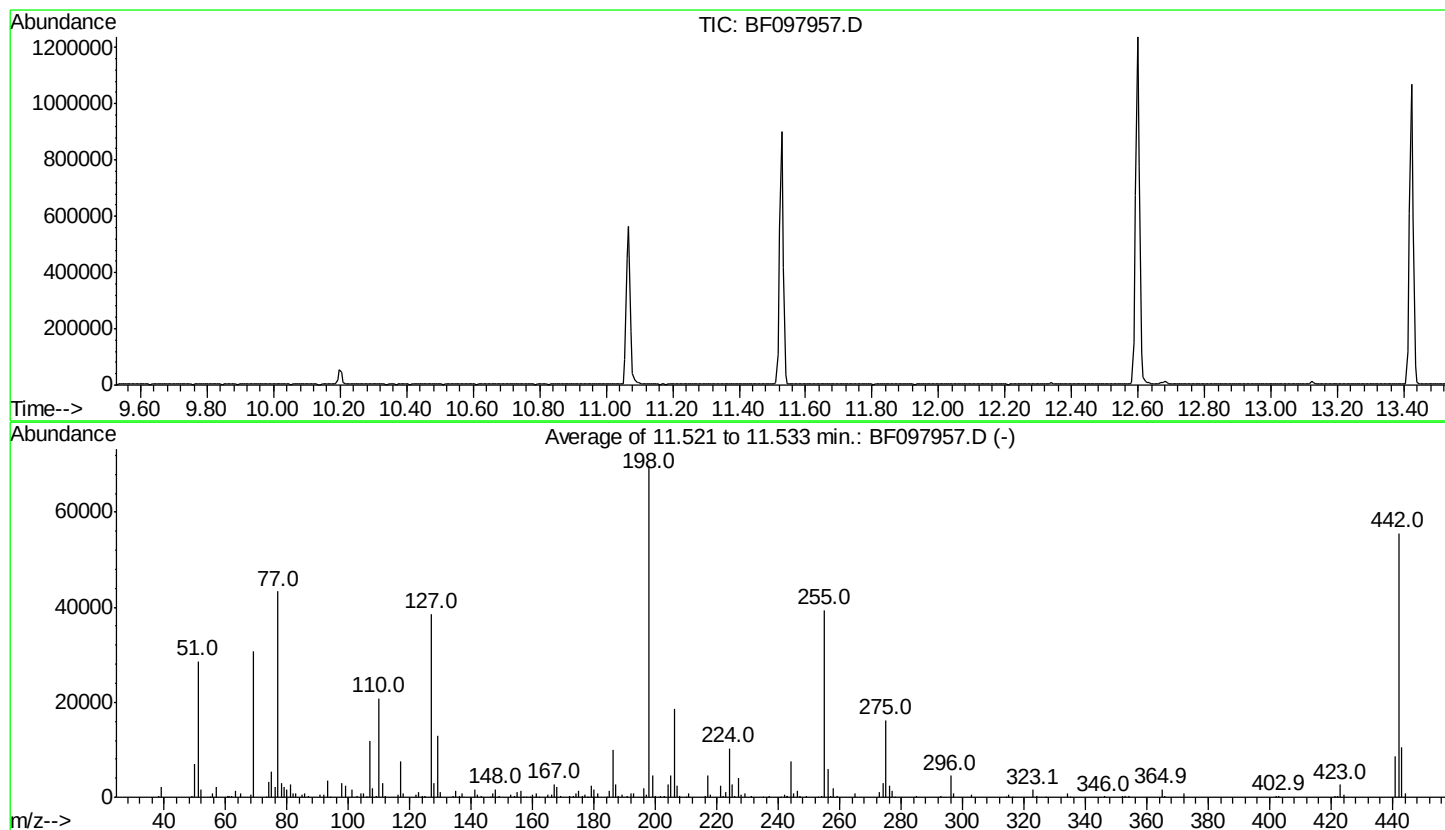

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	28686	PASS
68	69	0.00	2	1.5	475	PASS
69	198	0.00	100	44.2	30855	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.4	38672	PASS
197	198	0.00	2	1.0	677	PASS
198	198	100	100	100.0	69824	PASS
199	198	5	9	6.7	4691	PASS
275	198	10	60	23.3	16256	PASS
365	198	1	100	2.3	1623	PASS
441	442	0.01	24	15.4	8542	PASS
442	198	50	100	79.7	55645	PASS
443	442	15	24	18.7	10409	PASS