


Data Path : U:\HPCHEM1\BNA F\Data\BF082217\
 Data File : BF097983.D
 Acq On : 23 Aug 2017 5:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

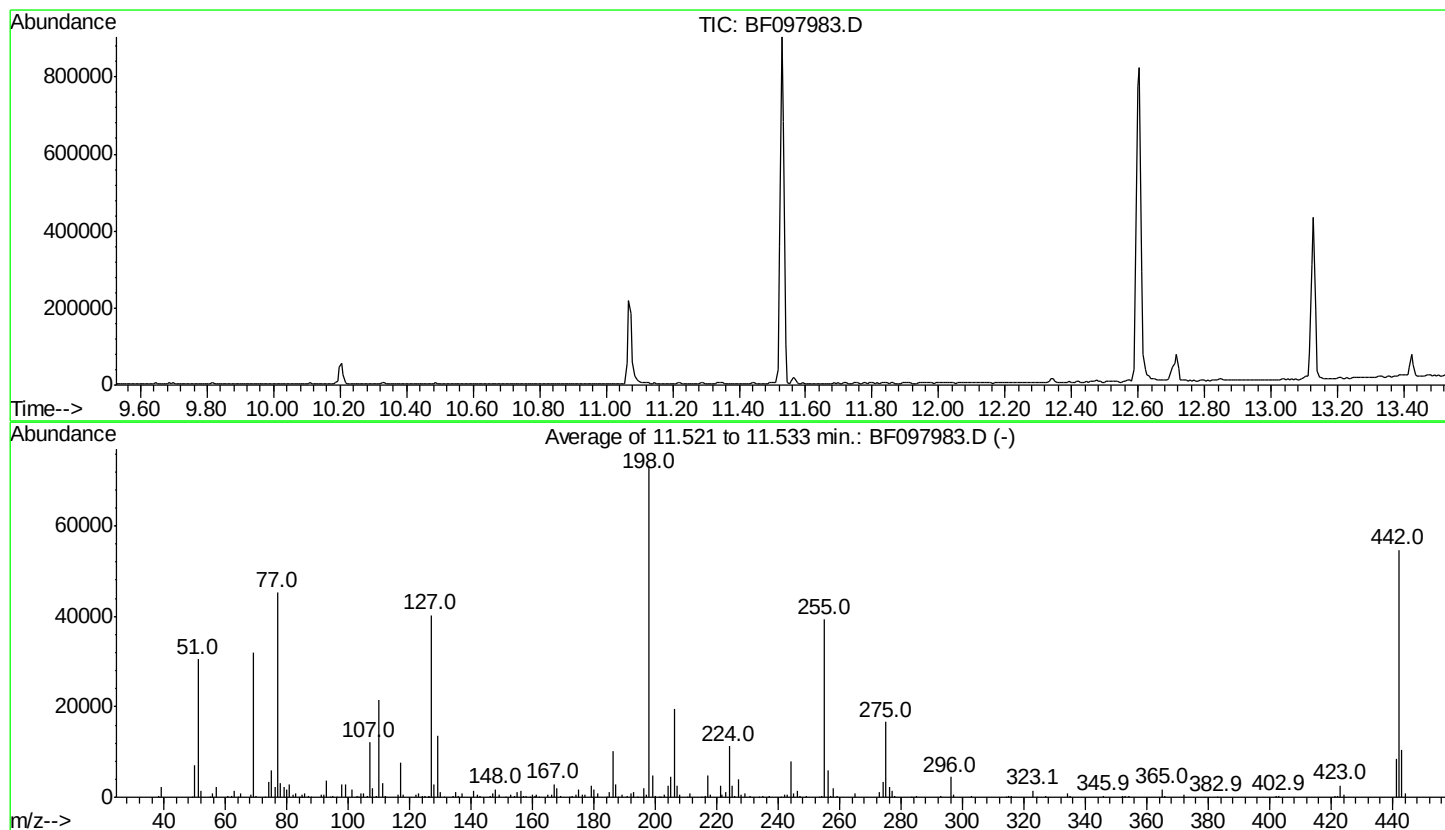

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	30464	PASS
68	69	0.00	2	1.7	557	PASS
69	198	0.00	100	43.8	32082	PASS
70	69	0.00	2	0.7	210	PASS
127	198	10	80	54.8	40216	PASS
197	198	0.00	2	0.8	603	PASS
198	198	100	100	100.0	73322	PASS
199	198	5	9	6.4	4699	PASS
275	198	10	60	22.7	16647	PASS
365	198	1	100	2.5	1815	PASS
441	442	0.01	24	15.6	8511	PASS
442	198	50	100	74.6	54679	PASS
443	442	15	24	19.2	10509	PASS