
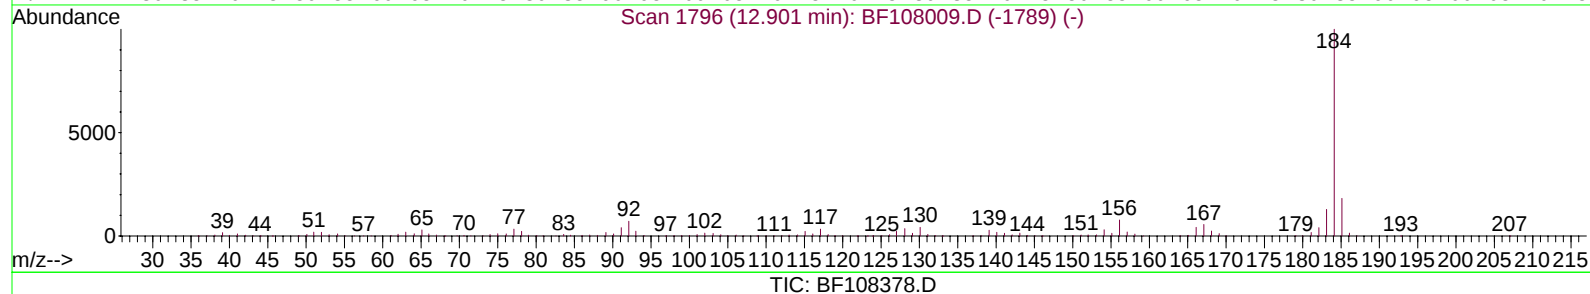
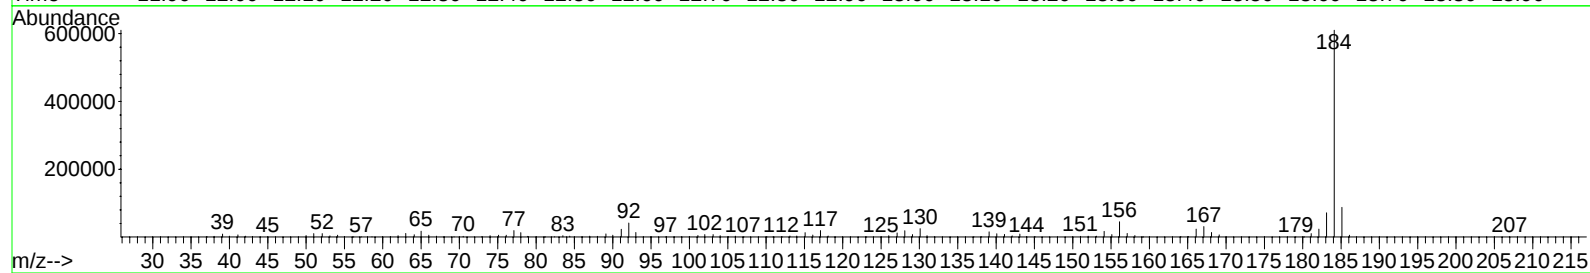


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF082218\
 Data File : BF108378.D
 Acq On : 22 Aug 2018 12:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 18:35:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 22 11:01:45 2018
 Response via : Initial Calibration

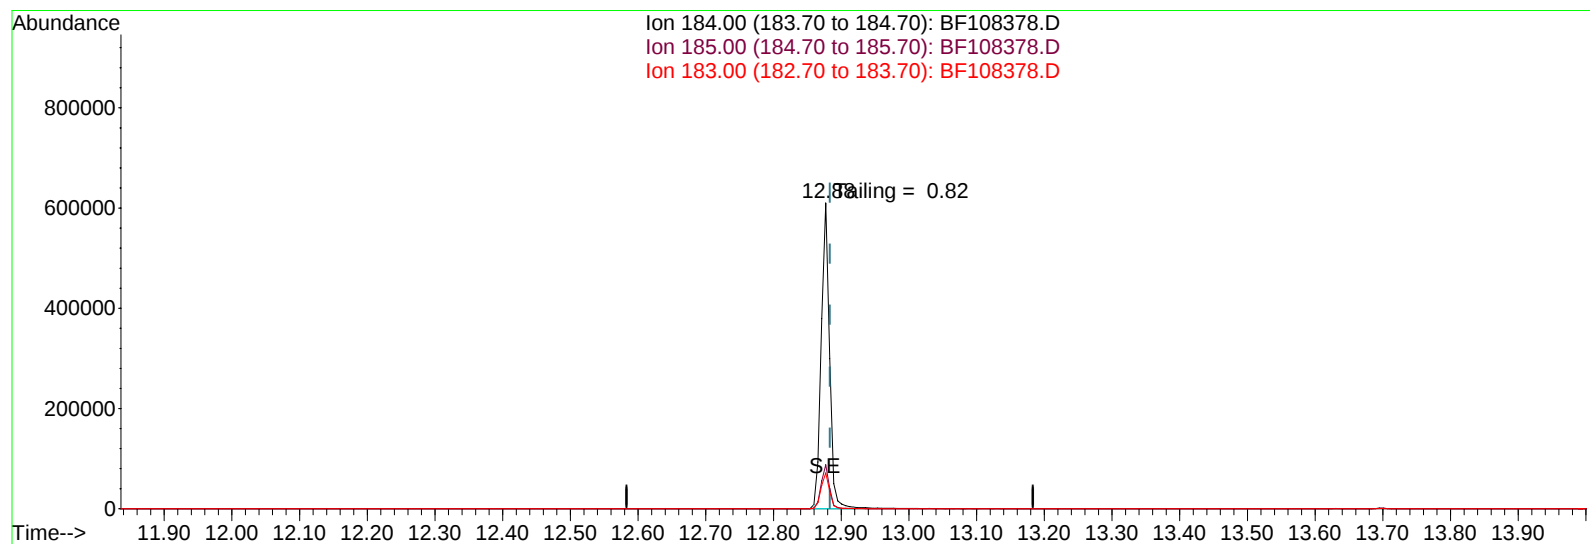

(76) Benzidine




12.877min (-0.006) 5754.54ng

response 527619

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.38
183.00	11.60	11.74
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF082218\  
Data File   : BF108378.D  
Acq On      : 22 Aug 2018   12:22  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Aug 22 18:35:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

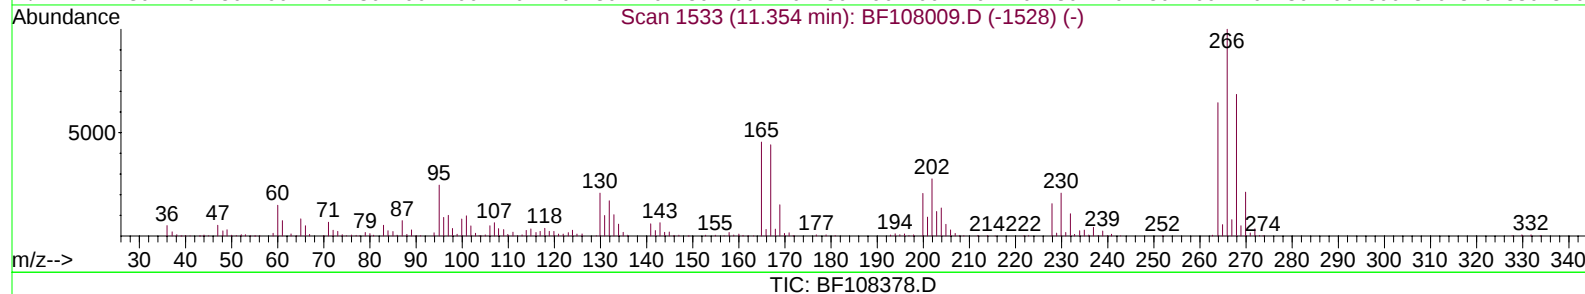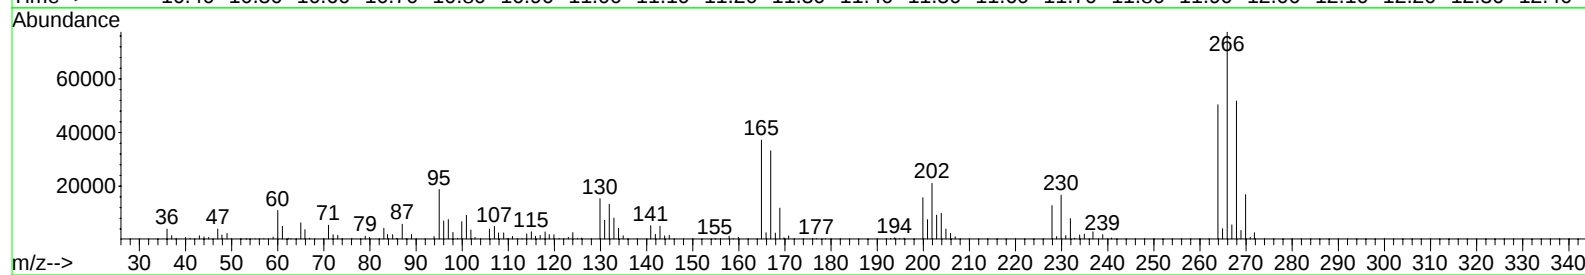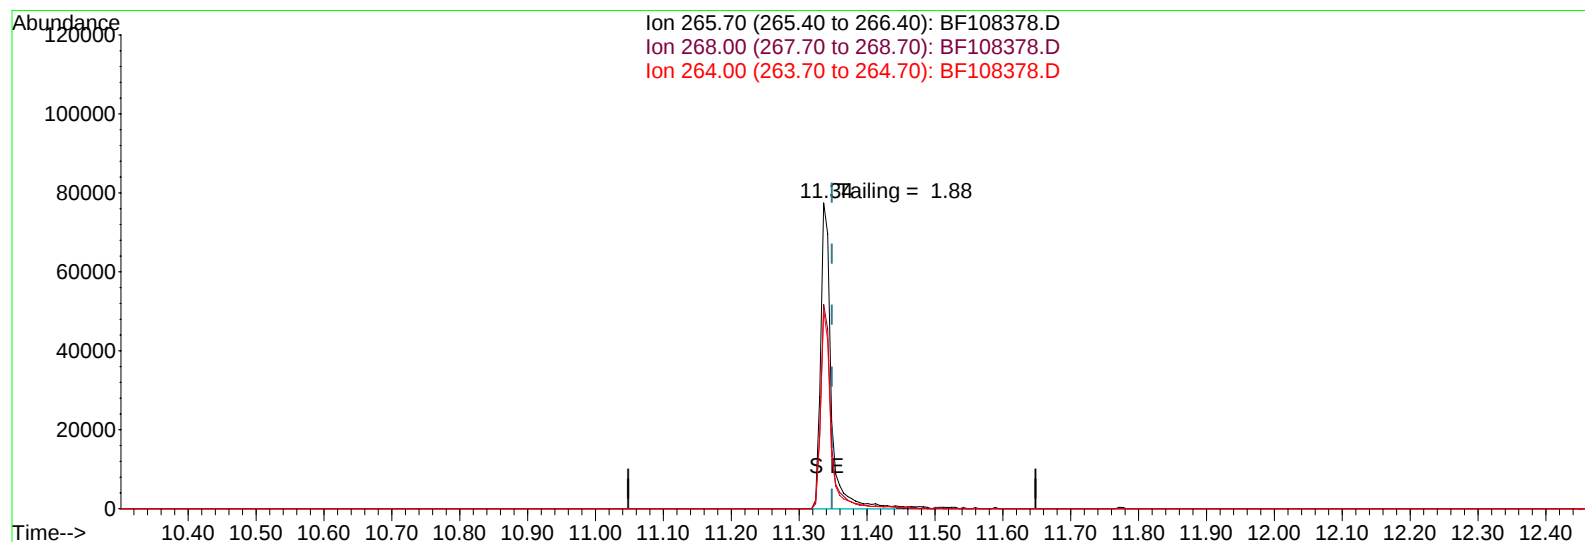

(69) Pentachlorophenol (C)

11.336min (-0.012) 28472.97ng

response 83836

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.82
264.00	61.90	65.08
0.00	0.00	0.00