

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
 Data File : BF108385.D
 Acq On : 22 Aug 2018 16:12
 Operator : JU/SJ
 Sample : TEST01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TEST01

Quant Time: Aug 22 17:20:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 22 11:01:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.00	152	147937	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	558435	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	294938	20.00	ng	-0.01
63) Phenanthrene-d10	11.54	188	625386	20.00	ng	0.00
75) Chrysene-d12	14.19	240	523121	20.00	ng	0.00
86) Perylene-d12	15.75	264	351120	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	1145026	140.13	ng	0.00
7) Phenol-d6	6.62	99	1527197	140.65	ng	0.00
23) Nitrobenzene-d5	7.57	82	1025017	102.42	ng	0.00
41) 2,4,6-Tribromophenol	10.84	330	500873	170.25	ng	0.00
44) 2-Fluorobiphenyl	9.36	172	1949152	106.10	ng	0.00
78) Terphenyl-d14	13.14	244	2326408	113.07	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
Data File : BF108385.D
Acq On : 22 Aug 2018 16:12
Operator : JU/SJ
Sample : TEST01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST01

Quant Time: Aug 22 17:20:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

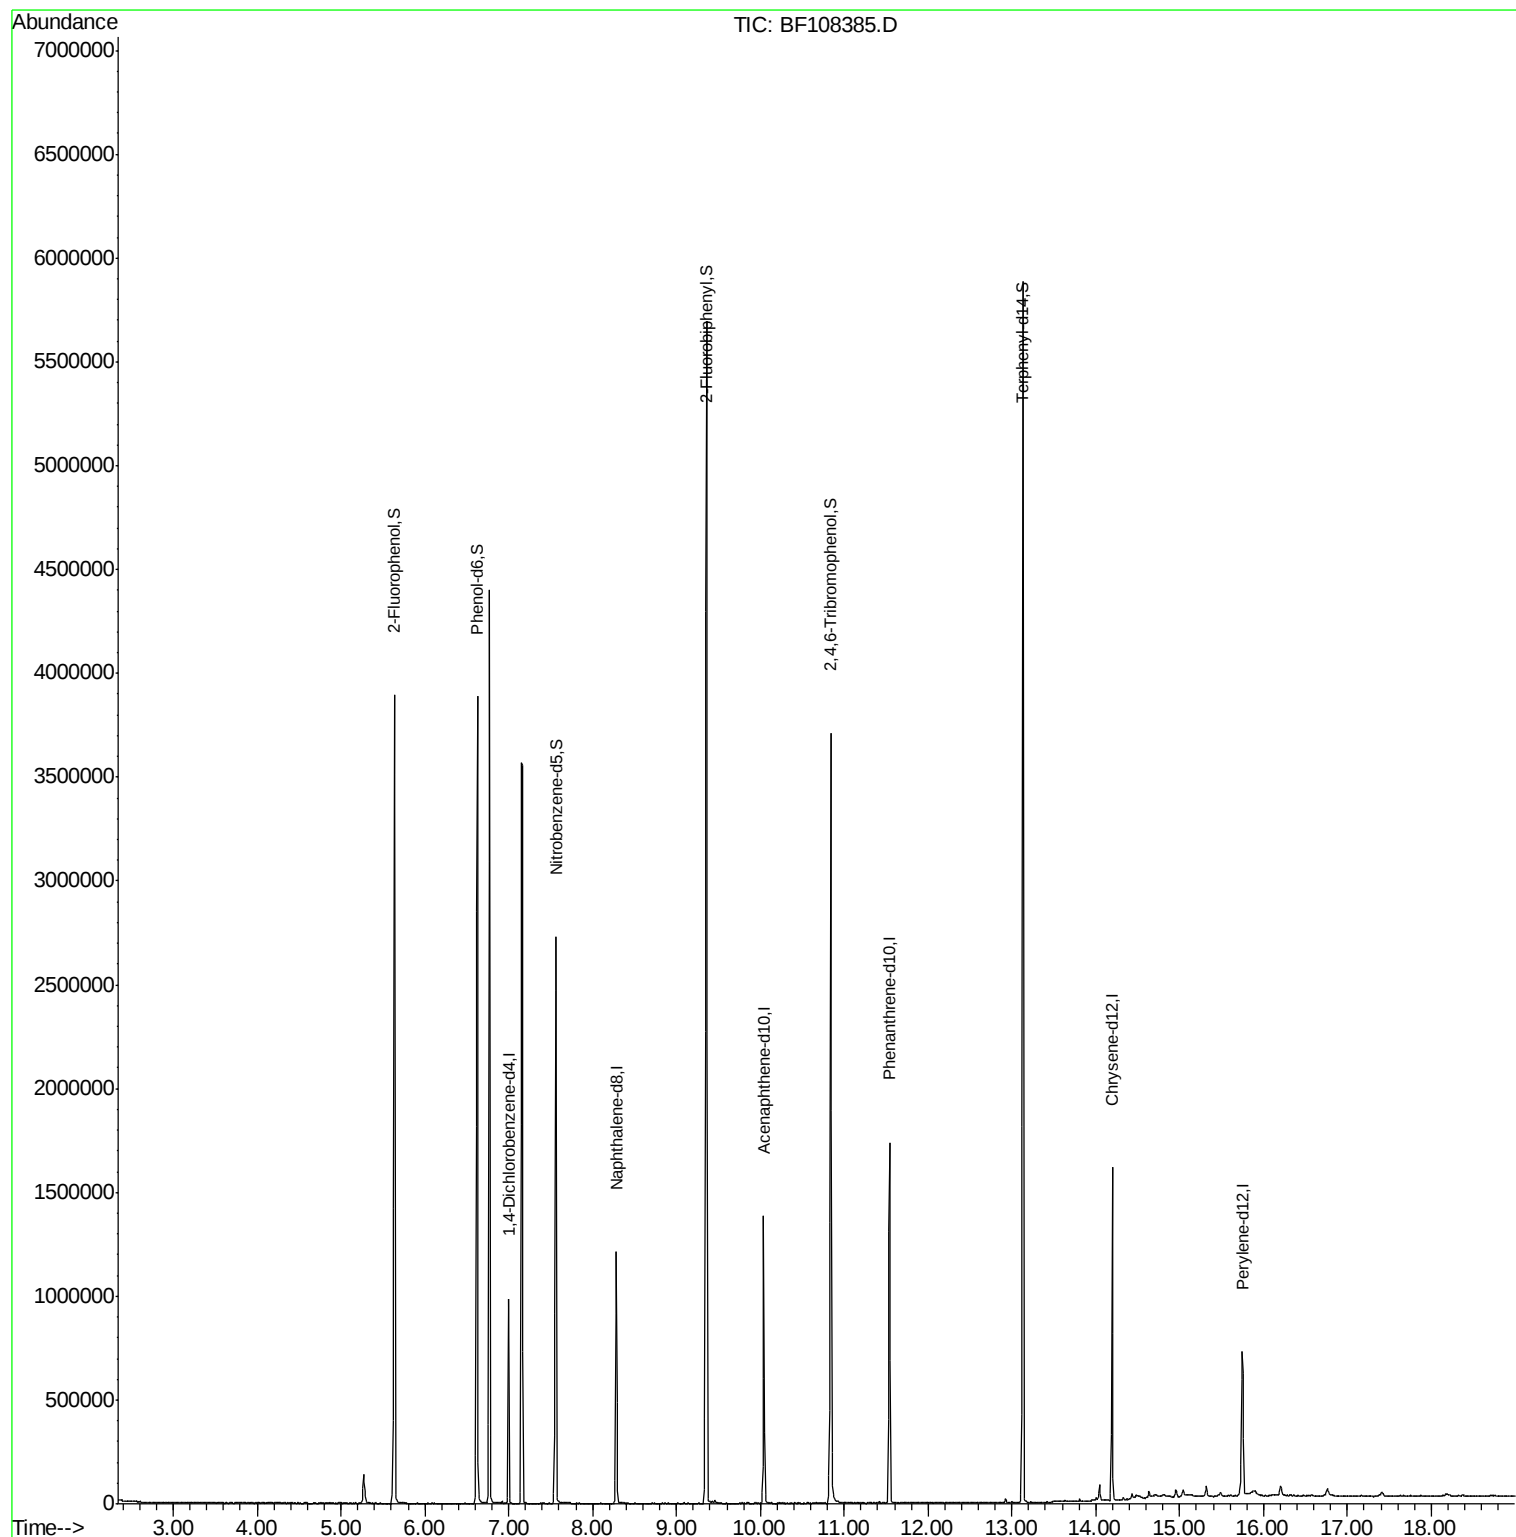

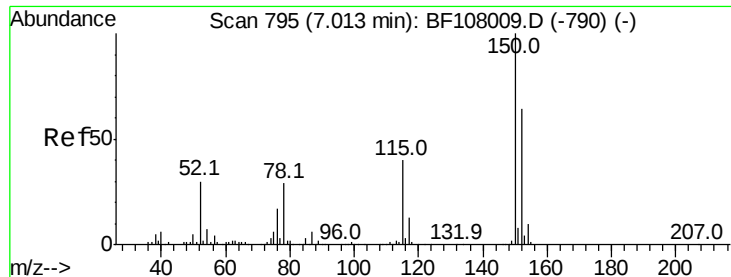


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.00 min Scan# 793
Delta R.T. -0.01 min
Lab File: BF108385.D
Acq: 22 Aug 2018 16:12

Instrument :
BNA_F
ClientSampleId :
TEST01

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.7	124.6	186.8
115	56.2	50.1	75.1



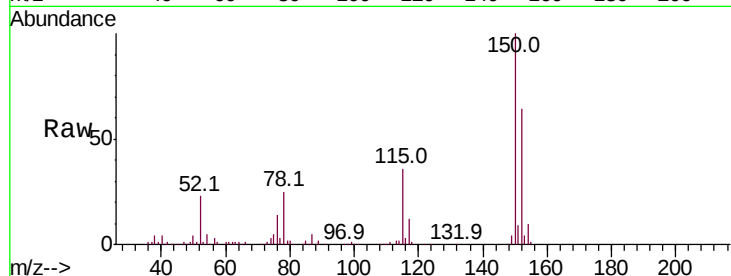


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

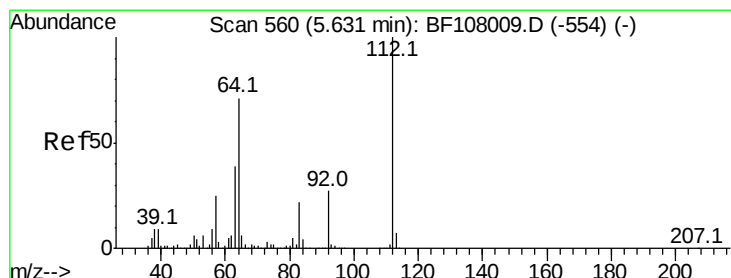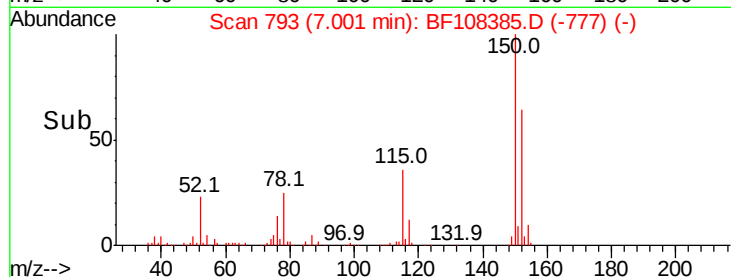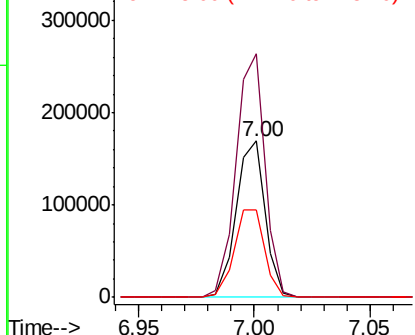

#5

2-Fluorophenol
Concen: 140.128 ng
RT: 5.64 min Scan# 561
Delta R.T. 0.01 min
Lab File: BF108385.D
Acq: 22 Aug 2018 16:12

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.0	47.9	71.9
63	37.4	23.7	35.5


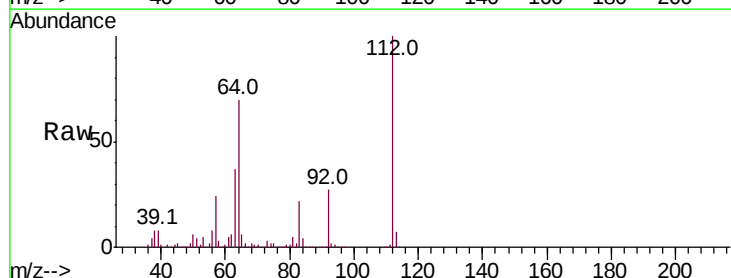



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

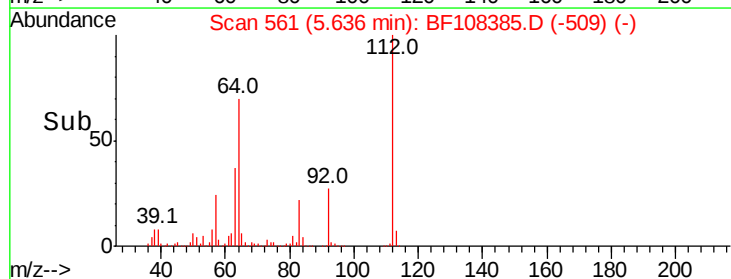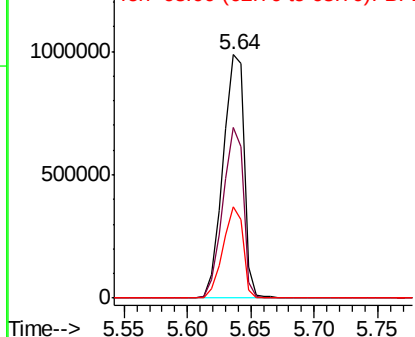

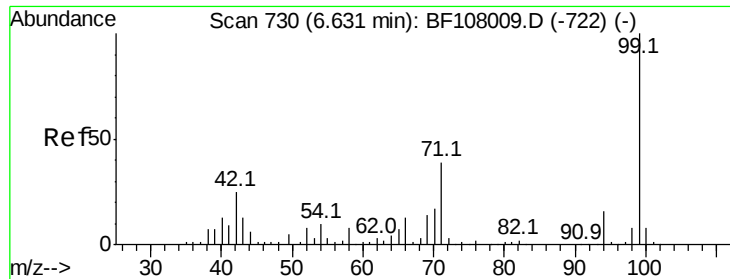

#7

Phenol-d6

Concen: 140.645 ng

RT: 6.62 min Scan# 729

Delta R.T. -0.01 min

Lab File: BF108385.D

Acq: 22 Aug 2018 16:12

Instrument :


BNA_F

ClientSampleId :




TEST01

Tot Ion: 99 Resp: 1527197

Ion	Ratio	Lower	Upper
99	100		
42	23.1	14.5	21.7#
71	38.2	25.4	38.0#

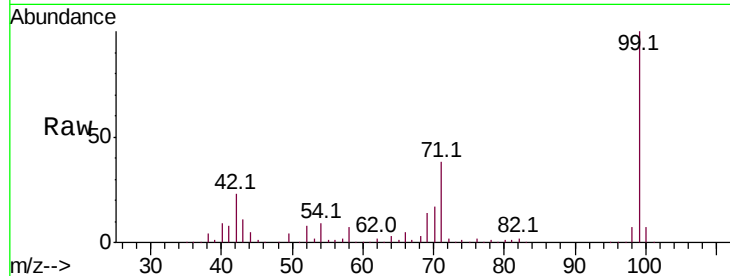

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

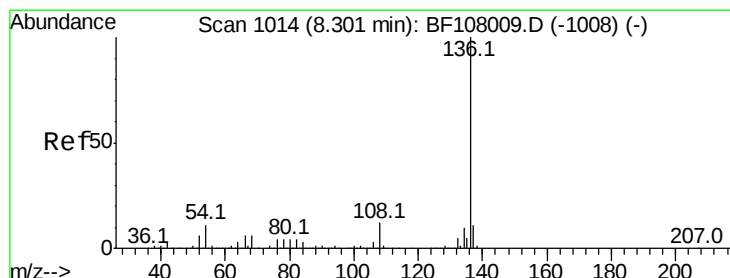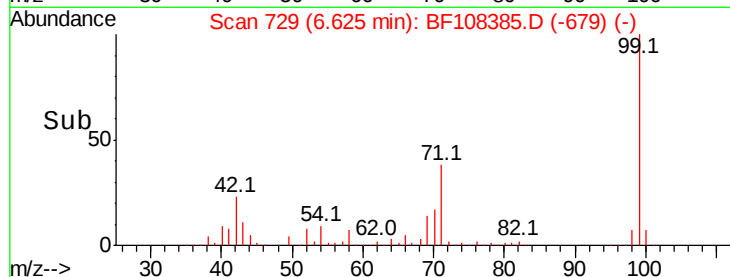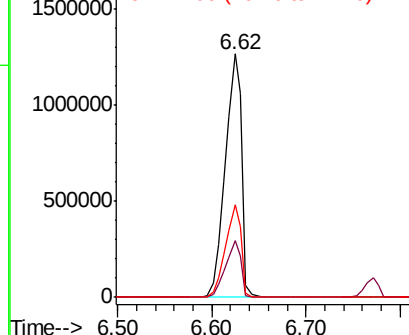

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.28 min Scan# 1011


Delta R.T. -0.01 min

Lab File: BF108385.D



Acq: 22 Aug 2018 16:12


Tgt Ion: 136 Resp: 558435

Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.9	13.3
54	8.9	6.6	9.8
68	5.6	5.0	7.4

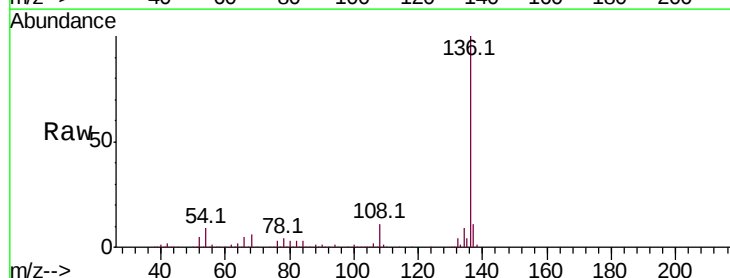

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



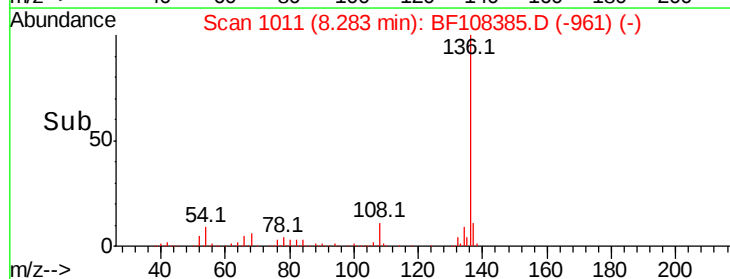
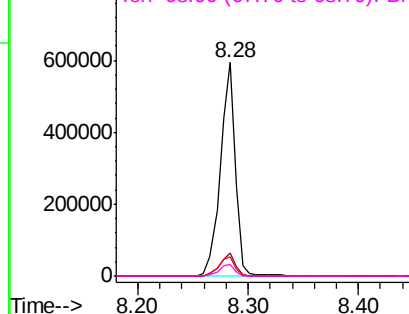


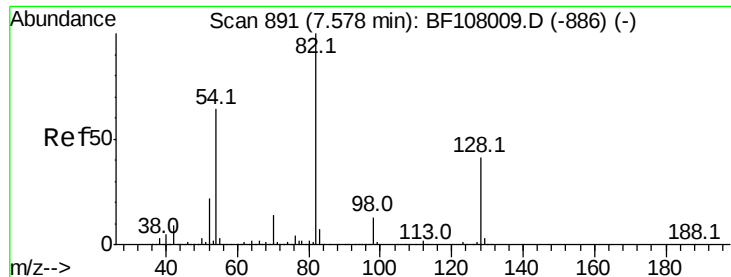

#23
 Nitrobenzene-d5
 Concen: 102.425 ng
 RT: 7.57 min Scan# 889
 Delta R.T. -0.01 min
 Lab File: BF108385.D
 Acq: 22 Aug 2018 16:12




Instrument :
 BNA_F
 ClientSampleId :
 TEST01


Tot Ion: 82 Resp: 1025017
 Ion Ratio Lower Upper
 82 100
 128 43.9 36.1 54.1
 54 55.9 41.4 62.2

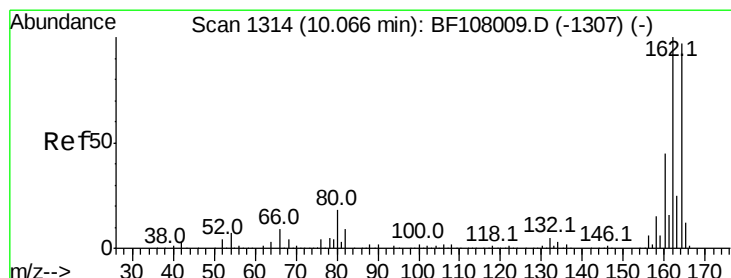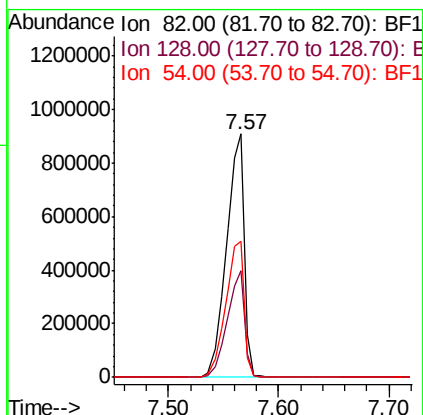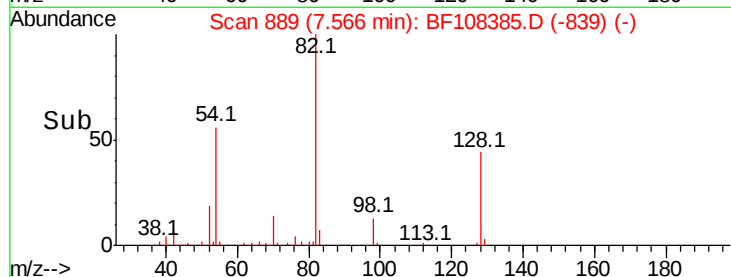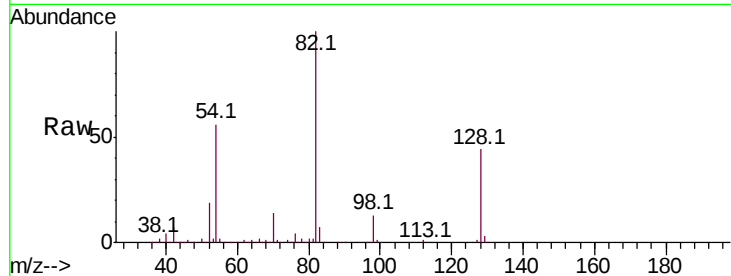

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.04 min Scan# 1310
 Delta R.T. -0.01 min
 Lab File: BF108385.D
 Acq: 22 Aug 2018 16:12

Tgt Ion: 164 Resp: 294938
 Ion Ratio Lower Upper
 164 100
 162 102.3 86.1 129.1
 160 46.7 38.3 57.5

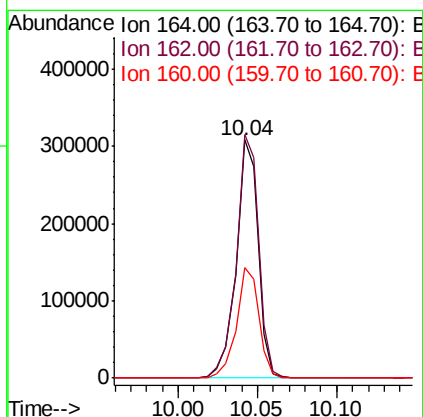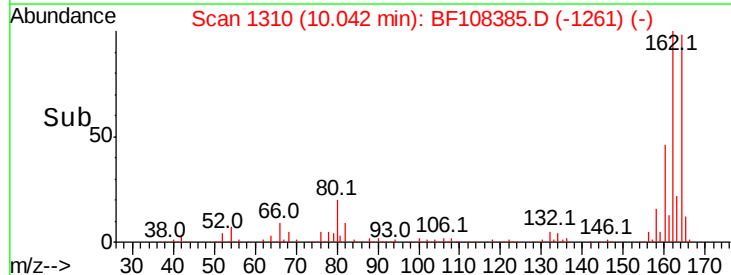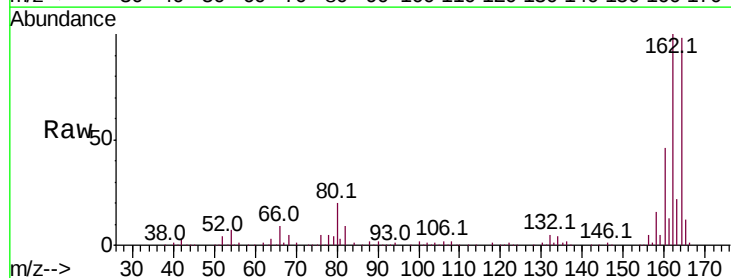


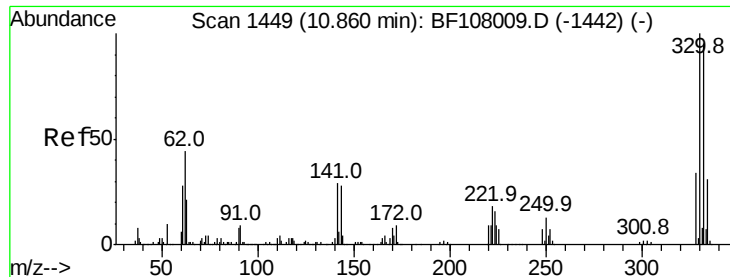




#41
 2,4,6-Tribromophenol
 Concen: 170.253 ng
 RT: 10.84 min Scan# 1446
 Delta R.T. -0.01 min
 Lab File: BF108385.D
 Acq: 22 Aug 2018 16:12

Instrument :
 BNA_F
 ClientSampleId :
 TEST01

Tot Ion:330 Resp: 500873
 Ion Ratio Lower Upper
 330 100
 332 96.3 77.0 115.6
 141 31.5 29.9 44.9

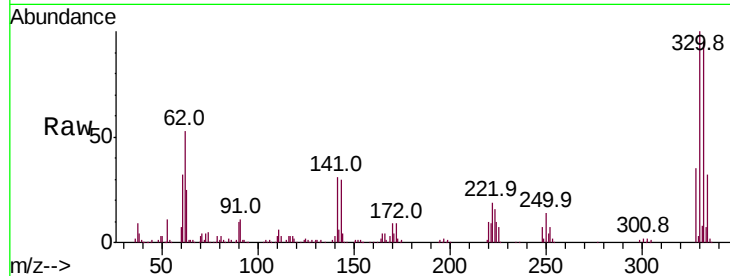


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

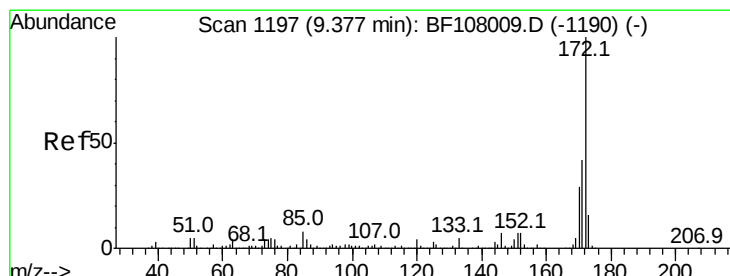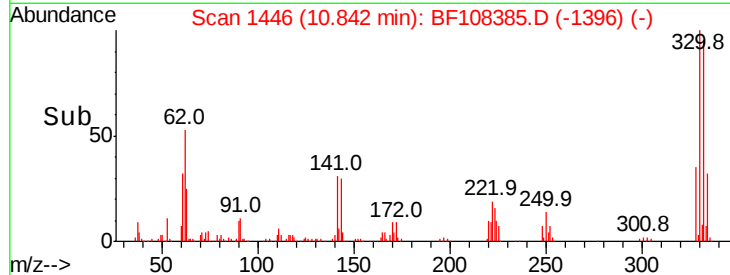
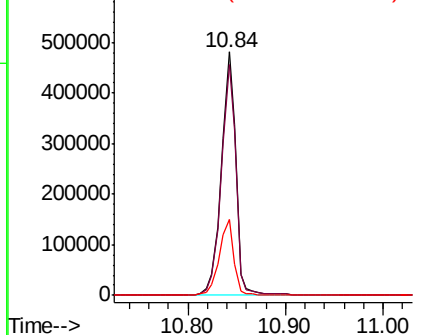



#44
 2-Fluorobiphenyl
 Concen: 106.100 ng
 RT: 9.36 min Scan# 1194
 Delta R.T. -0.01 min
 Lab File: BF108385.D
 Acq: 22 Aug 2018 16:12

Tgt Ion:172 Resp: 1949152
 Ion Ratio Lower Upper
 172 100
 171 37.6 29.7 44.5
 170 25.0 19.6 29.4

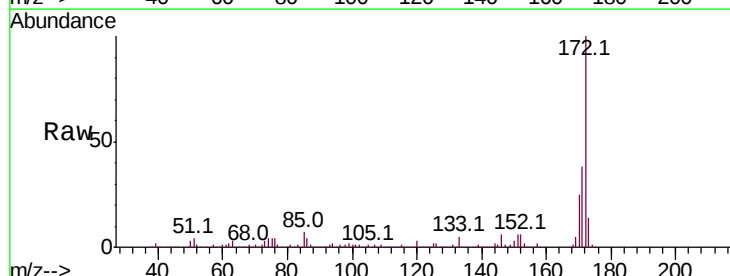

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

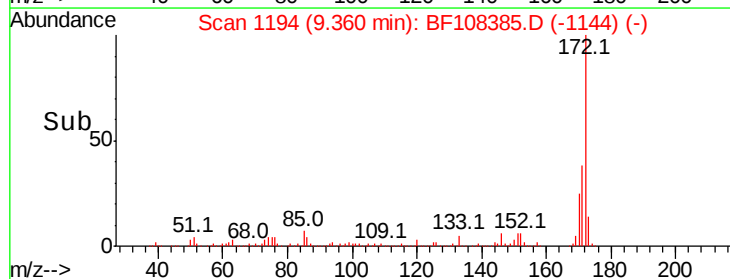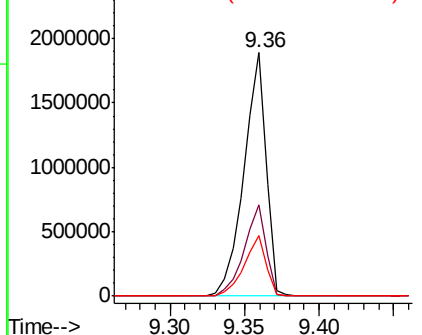


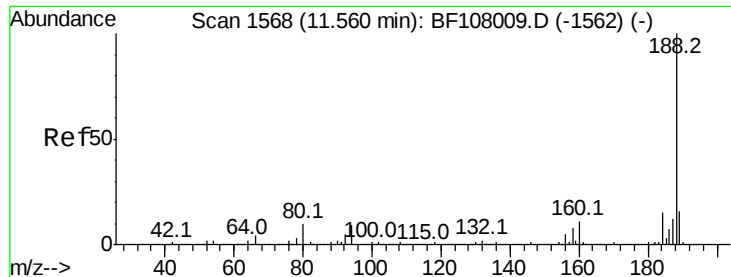




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.54 min Scan# 1565
Delta R.T. -0.01 min
Lab File: BF108385.D
Acq: 22 Aug 2018 16:12

Instrument :
BNA_F
ClientSampleId :
TEST01

Tot Ion	Ratio	Lower	Upper
188	100		
94	8.2	8.5	12.7#
80	9.2	9.2	13.8

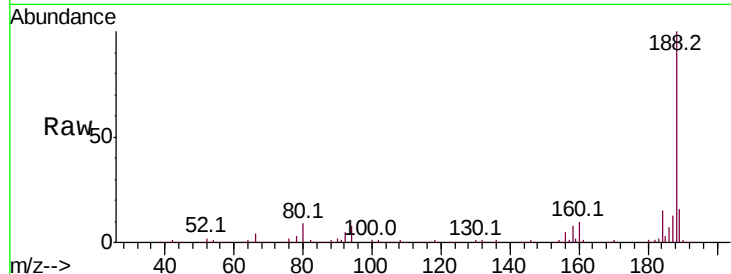


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

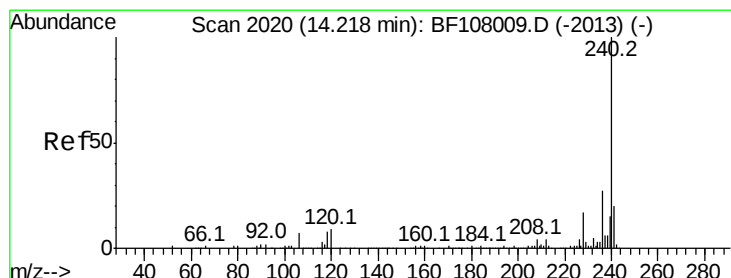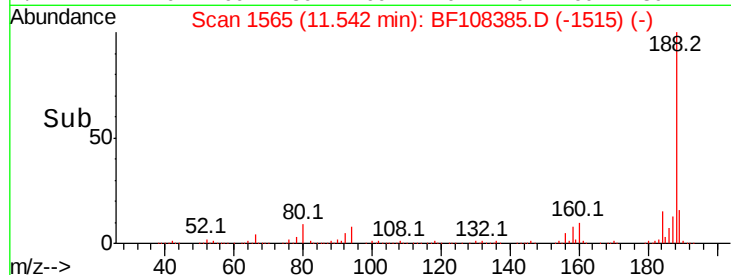
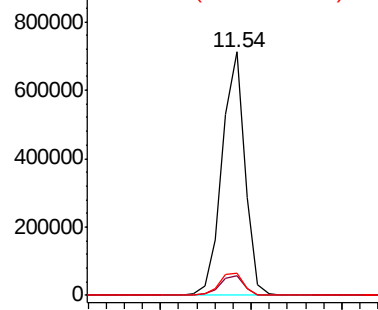



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.19 min Scan# 2016
Delta R.T. -0.01 min
Lab File: BF108385.D
Acq: 22 Aug 2018 16:12

Tgt Ion	Ratio	Lower	Upper
240	100		
120	9.5	9.5	14.3
236	26.0	20.7	31.1

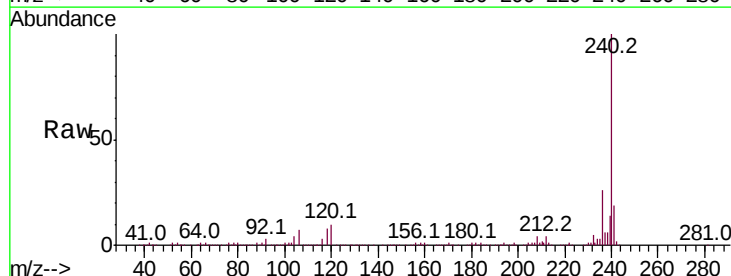

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

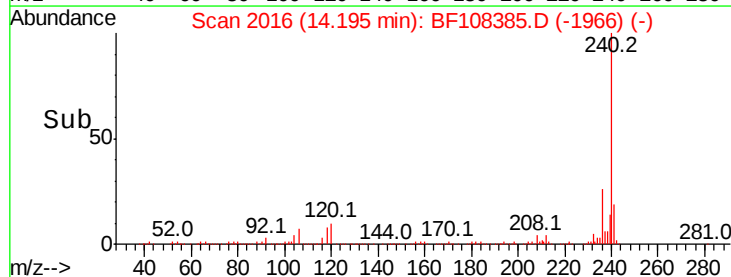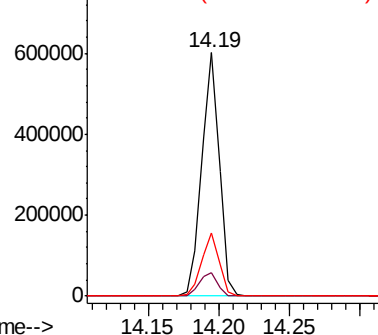


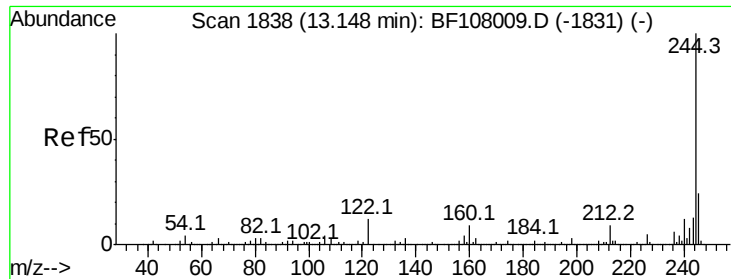




#78
 Terphenyl-d14
 Concen: 113.072 ng
 RT: 13.14 min Scan# 1836
 Delta R.T. 0.01 min
 Lab File: BF108385.D
 Acq: 22 Aug 2018 16:12

Instrument :
 BNA_F
 ClientSampleId :
 TEST01

Tot Ion:244 Resp: 2326408
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.4 8.0
 122 9.0 11.0 16.4#

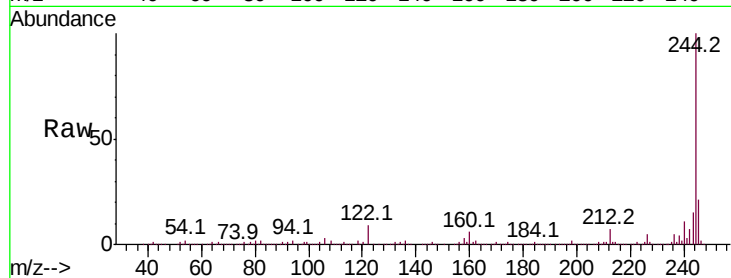


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

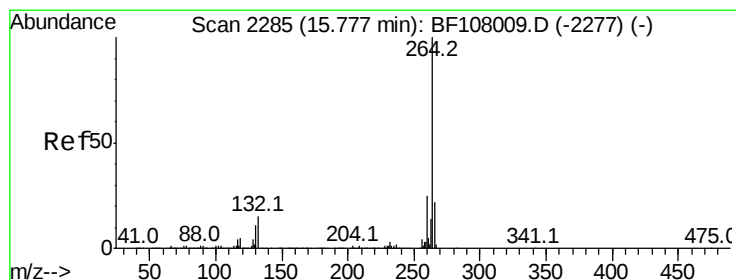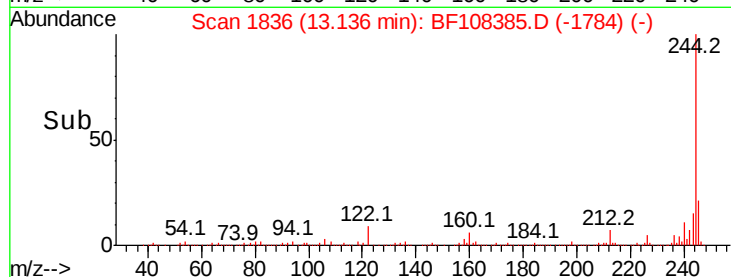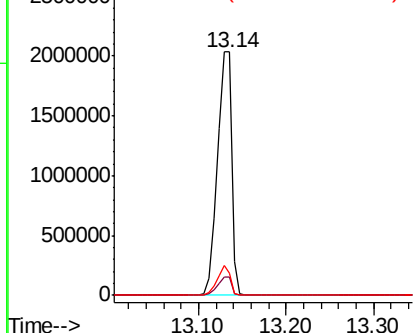

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.75 min Scan# 2280
 Delta R.T. -0.01 min
 Lab File: BF108385.D
 Acq: 22 Aug 2018 16:12

Tgt Ion:264 Resp: 351120
 Ion Ratio Lower Upper
 264 100
 260 24.5 19.2 28.8
 265 21.7 17.5 26.3

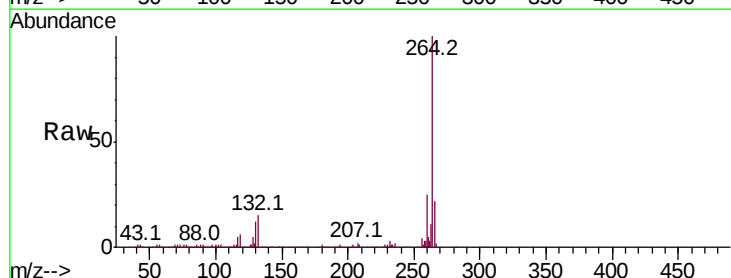

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

