

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
 Data File : BF108387.D
 Acq On : 22 Aug 2018 17:06
 Operator : JU/SJ
 Sample : J4566-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NUTLEY-DRUM

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.613	554	557	572	rBV	250755	245415	14.74%	2.006%
2	6.607	723	726	737	rBV	156745	161937	9.73%	1.324%
3	6.766	749	753	764	rBV	555231	486148	29.20%	3.974%
4	7.001	788	793	796	rBV	1183949	1055044	63.38%	8.625%
5	7.154	815	819	823	rBV	516008	433547	26.04%	3.544%
6	7.554	883	887	893	rBV	404223	382032	22.95%	3.123%
7	8.283	1006	1011	1015	rBV	1665260	1403217	84.29%	11.471%
8	9.354	1188	1193	1203	rBV	976041	772499	46.40%	6.315%
9	9.748	1255	1260	1263	rBV	31734	27585	1.66%	0.226%
10	9.848	1274	1277	1280	rBV	128784	88212	5.30%	0.721%
11	10.048	1303	1311	1314	rBV	1859490	1649021	99.06%	13.481%
12	10.836	1441	1445	1453	rBV	474835	457273	27.47%	3.738%
13	11.383	1535	1538	1541	rVB	67453	49566	2.98%	0.405%
14	11.542	1561	1565	1568	rBV	2048945	1664738	100.00%	13.609%
15	11.895	1617	1625	1627	rBV5	14744	28080	1.69%	0.230%
16	13.124	1830	1834	1837	rBV	885936	776770	46.66%	6.350%
17	14.048	1987	1991	1994	rVB	27008	27567	1.66%	0.225%
18	14.195	2012	2016	2019	rBV	1231170	1094516	65.75%	8.948%
19	14.465	2055	2062	2064	rBV7	44361	90643	5.44%	0.741%
20	14.607	2083	2086	2088	rBV2	20889	23986	1.44%	0.196%
21	14.630	2088	2090	2093	rVB2	23163	23365	1.40%	0.191%
22	14.954	2143	2145	2150	rVB	31842	36798	2.21%	0.301%
23	15.042	2157	2160	2164	rVB	43268	44832	2.69%	0.367%
24	15.318	2204	2207	2211	rVB	38259	46062	2.77%	0.377%
25	15.748	2273	2280	2287	rBV	714775	1012031	60.79%	8.273%
26	16.206	2354	2358	2364	rVB2	43514	73424	4.41%	0.600%
27	16.753	2447	2451	2461	rVB4	35995	77974	4.68%	0.637%


Sum of corrected areas: 12232282

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
Data File : BF108387.D
Acq On : 22 Aug 2018 17:06
Operator : JU/SJ
Sample : J4566-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NUTLEY-DRUM

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

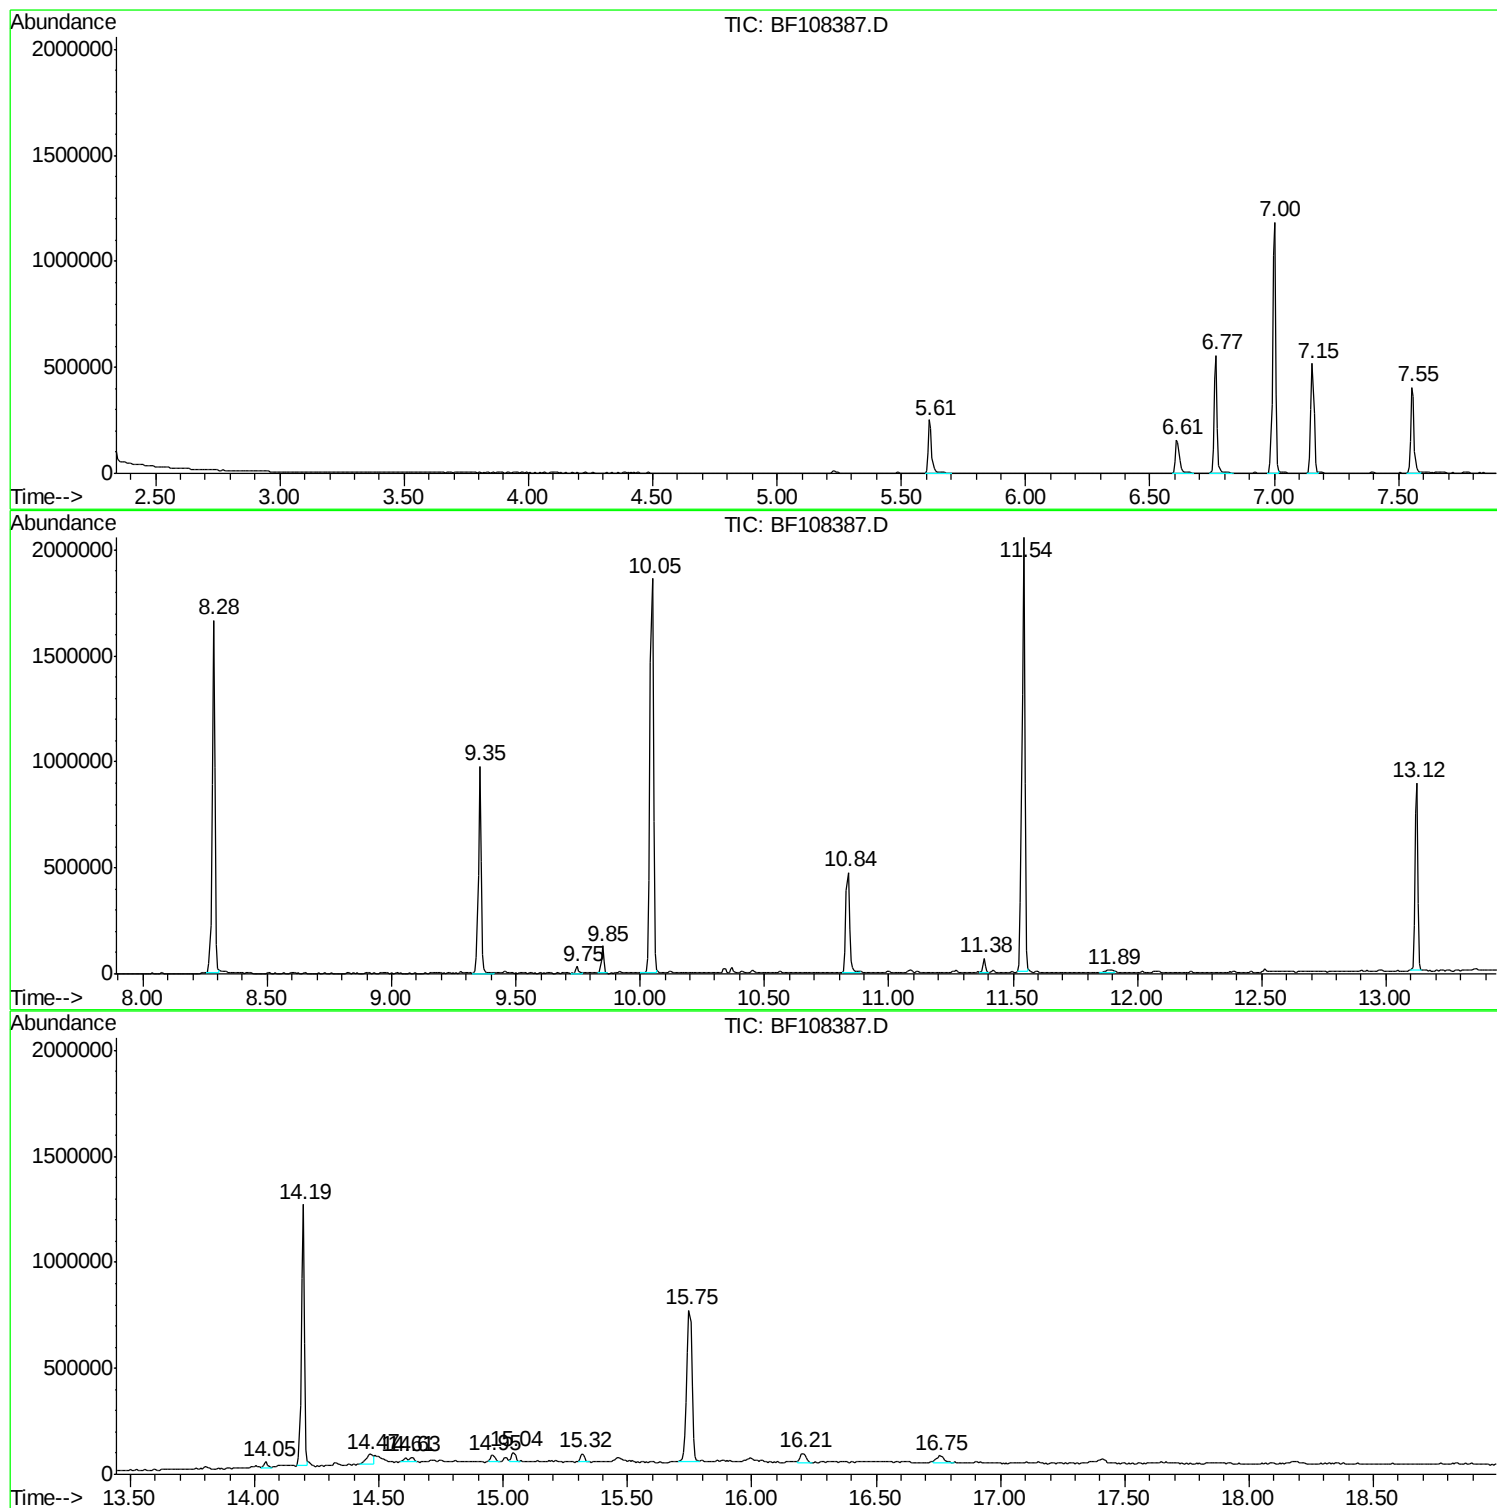

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
Data File : BF108387.D
Acq On : 22 Aug 2018 17:06
Operator : JU/SJ
Sample : J4566-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NUTLEY-DRUM










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	9.22 ng	486148	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Tranlylcypropromine-propionyl	189	C12H15NO	1000123-86-3	10
2		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
3		5-Aminoindole	132	C8H8N2	005192-03-0	9
4		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9

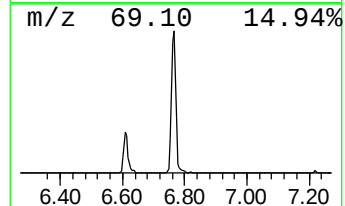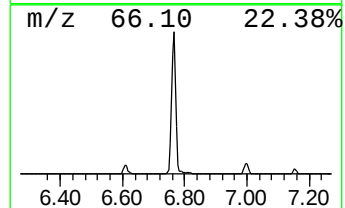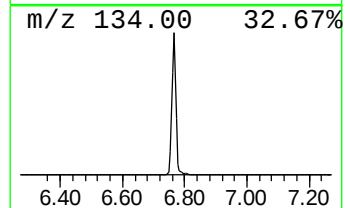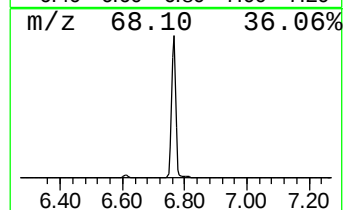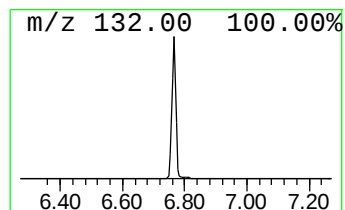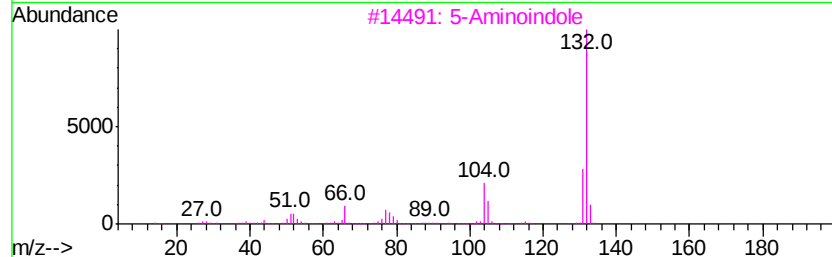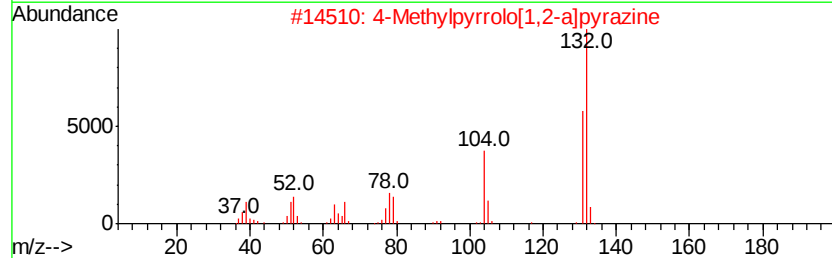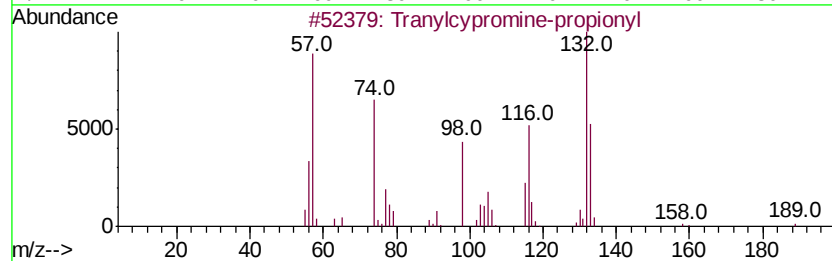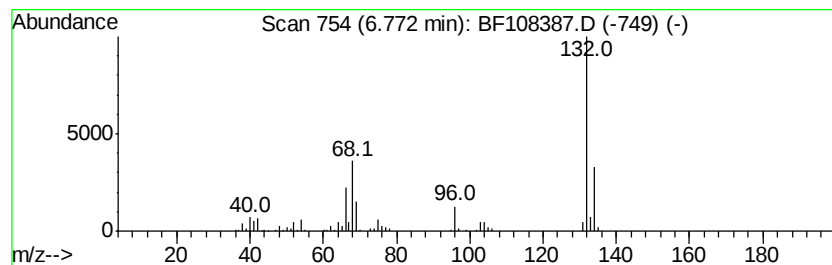

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082218\
Data File : BF108387.D
Acq On : 22 Aug 2018 17:06
Operator : JU/SJ
Sample : J4566-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NUTLEY-DRUM

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.77	6.77	9.2	ng	486148	1	7.00	1055040	20.0