

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082218\
 Data File : BF108409.D
 Acq On : 23 Aug 2018 4:53
 Operator : JU/SJ
 Sample : J4525-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 081518-SIDI-F-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.360	3	4	18	rVB	1382087	1351027	26.77%	4.806%
2	5.237	490	493	502	rBV	67746	79501	1.58%	0.283%
3	5.625	555	559	562	rBV	1651419	1381255	27.37%	4.913%
4	6.613	723	727	731	rBV	1093873	963379	19.09%	3.427%
5	6.642	731	732	739	rVB	101317	71134	1.41%	0.253%
6	6.772	749	754	757	rBV	2716963	2476206	49.07%	8.808%
7	7.001	789	793	796	rBV	1106488	909070	18.02%	3.234%
8	7.160	815	820	823	rBV	3799092	3371156	66.81%	11.992%
9	7.566	883	889	892	rBV	2761681	2817280	55.83%	10.022%
10	8.283	1007	1011	1025	rBV	1354977	1117791	22.15%	3.976%
11	9.360	1189	1194	1197	rBV	5604163	5046089	100.00%	17.950%
12	9.748	1256	1260	1266	rBV	154779	137929	2.73%	0.491%
13	10.048	1307	1311	1322	rVB	1266642	1196272	23.71%	4.255%
14	10.701	1419	1422	1426	rBV	122801	92982	1.84%	0.331%
15	10.836	1441	1445	1458	rBV	1561735	1388320	27.51%	4.939%
16	11.542	1561	1565	1568	rBV	1180373	1019652	20.21%	3.627%
17	13.124	1830	1834	1838	rBV	3258253	3271172	64.83%	11.636%
18	14.195	2012	2016	2020	rBV	800051	764568	15.15%	2.720%
19	15.748	2274	2280	2285	rBV	476483	657176	13.02%	2.338%


Sum of corrected areas: 28111959

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
Data File : BF108409.D
Acq On : 23 Aug 2018 4:53
Operator : JU/SJ
Sample : J4525-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081518-SIDI-F-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

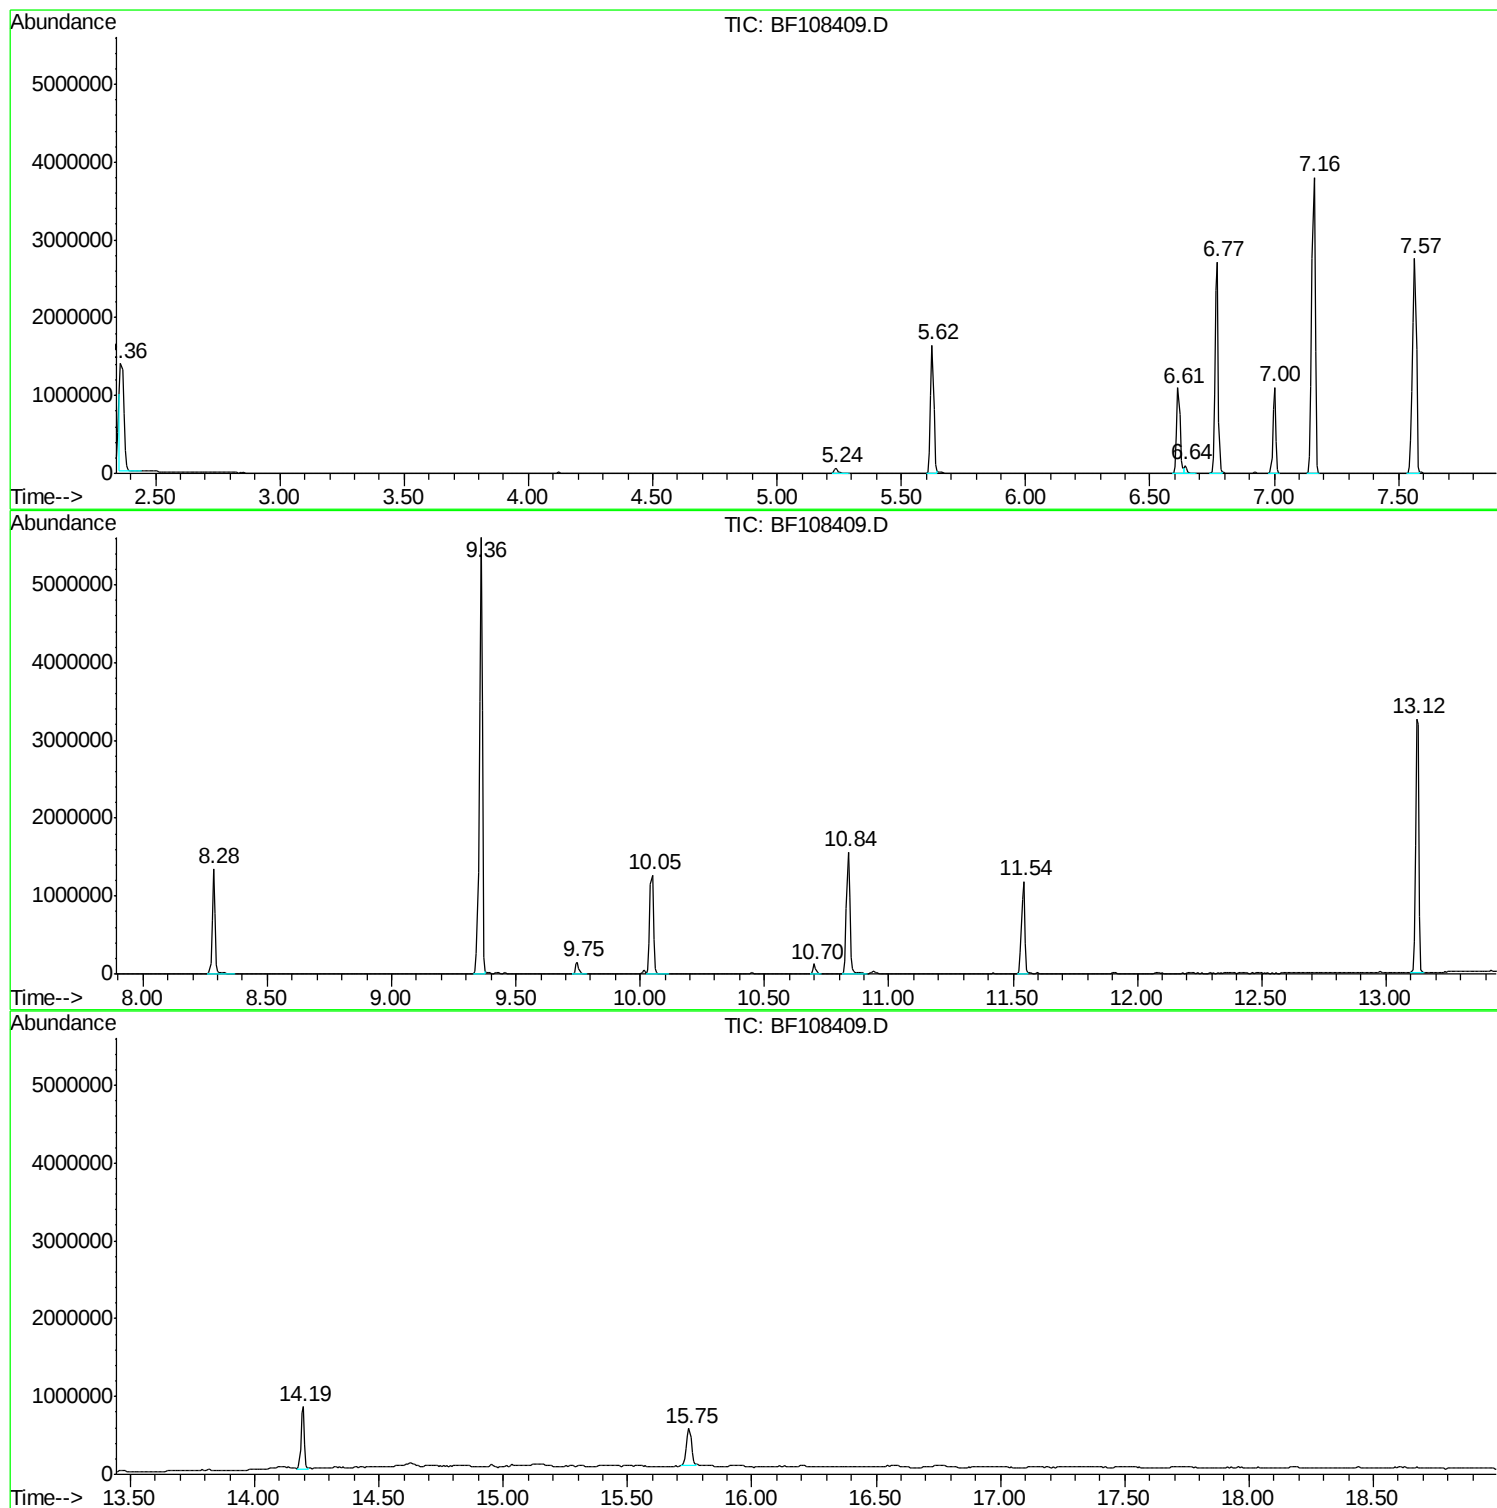

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
Data File : BF108409.D
Acq On : 23 Aug 2018 4:53
Operator : JU/SJ
Sample : J4525-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081518-SIDI-F-D-M










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.36	29.72 ng	1351030	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
3		Silane, tetramethyl-	88	C4H12Si	000075-76-3	38
4		1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	32
5		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

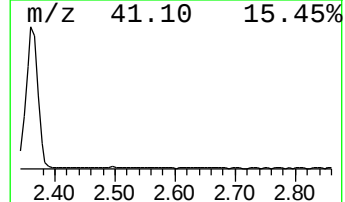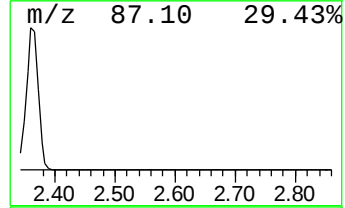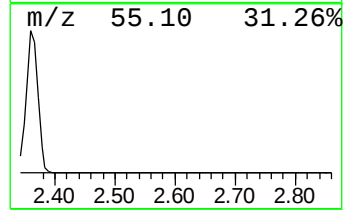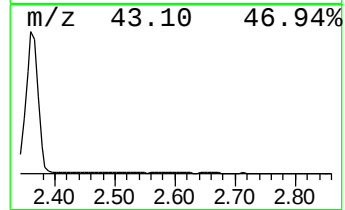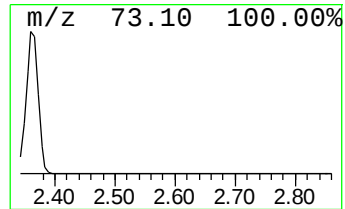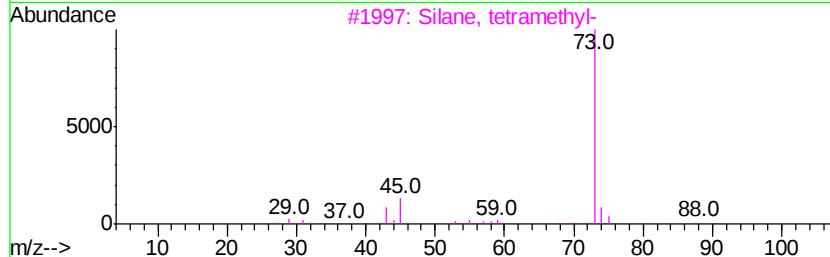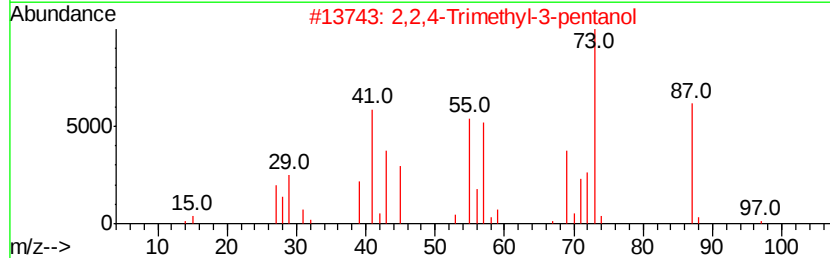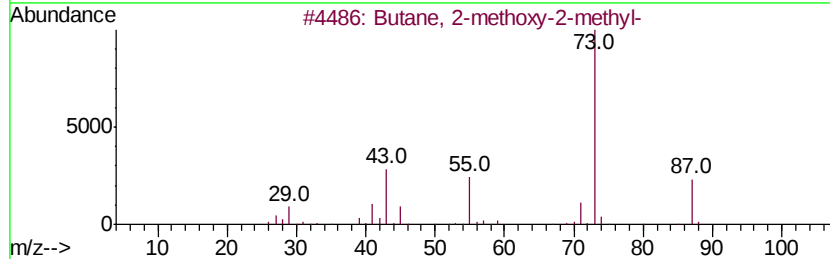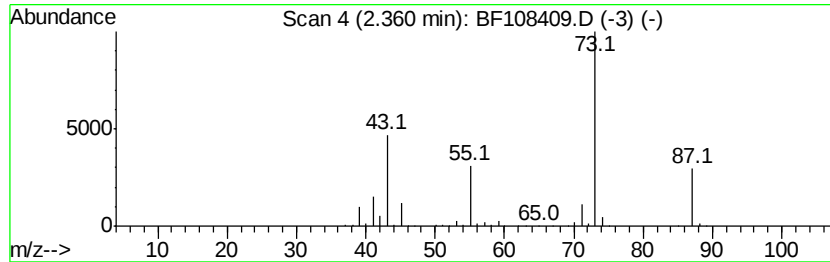

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
Data File : BF108409.D
Acq On : 23 Aug 2018 4:53
Operator : JU/SJ
Sample : J4525-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081518-SIDI-F-D-M







Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.77 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	54.48 ng	2476210	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27	
2	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27	
3	Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10	
4	1,2,4-Trifluorobenzene	132	C6H3F3	000367-23-7	9	
5	1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9	

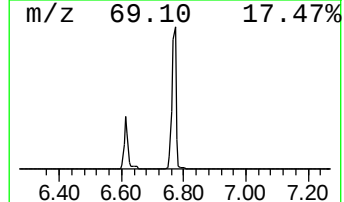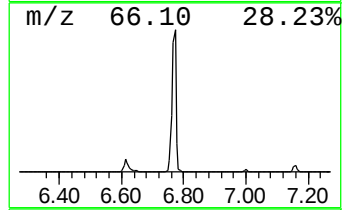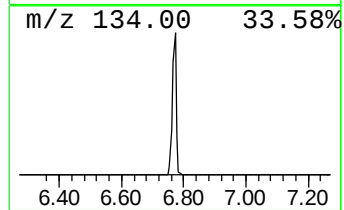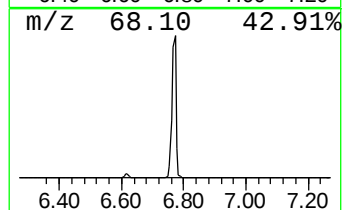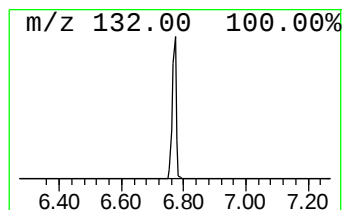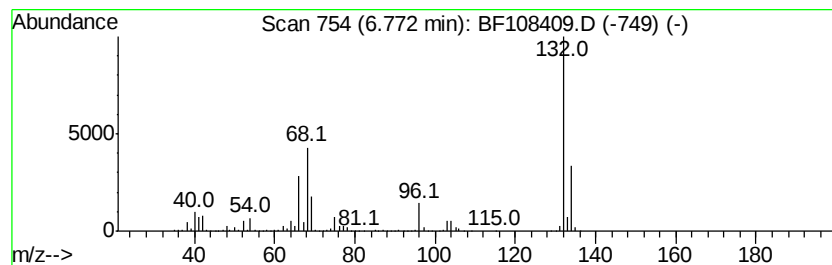

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082218\
Data File : BF108409.D
Acq On : 23 Aug 2018 4:53
Operator : JU/SJ
Sample : J4525-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081518-SIDI-F-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.36	29.7	ng	1351030	1	7.00	909070	20.0
unknown6.77	6.77	54.5	ng	2476210	1	7.00	909070	20.0