

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082218\
 Data File : BF108412.D
 Acq On : 23 Aug 2018 6:14
 Operator : JU/SJ
 Sample : J4525-13
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 081518-SIDI-F-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.237	489	493	502	rBV	62091	72335	1.42%	0.271%
2	5.625	555	559	568	rBV	1324273	1253590	24.62%	4.698%
3	6.613	723	727	730	rBV	984582	823835	16.18%	3.087%
4	6.642	730	732	736	rVB	96762	83186	1.63%	0.312%
5	6.766	749	753	757	rBV	2428750	2384302	46.83%	8.936%
6	7.001	789	793	796	rBV	1071685	920466	18.08%	3.450%
7	7.160	815	820	823	rBV	3808453	3420467	67.18%	12.819%
8	7.566	883	889	892	rBV	2875232	2848321	55.94%	10.675%
9	8.283	1007	1011	1015	rBV	1349260	1112844	21.86%	4.171%
10	9.360	1188	1194	1197	rBV	5636786	5091623	100.00%	19.082%
11	9.748	1256	1260	1265	rBV	130295	117333	2.30%	0.440%
12	10.042	1307	1310	1318	rVB	1260441	1206174	23.69%	4.520%
13	10.701	1419	1422	1425	rBV	102391	76782	1.51%	0.288%
14	10.836	1441	1445	1458	rBV	1560524	1407171	27.64%	5.274%
15	11.542	1561	1565	1568	rBV	1132903	1053028	20.68%	3.946%
16	13.124	1830	1834	1838	rBV	3517248	3330859	65.42%	12.483%
17	14.189	2012	2015	2022	rVB	877690	808087	15.87%	3.028%
18	15.742	2273	2279	2288	rVB	469530	672647	13.21%	2.521%


Sum of corrected areas: 26683050

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
Data File : BF108412.D
Acq On : 23 Aug 2018 6:14
Operator : JU/SJ
Sample : J4525-13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081518-SIDI-F-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

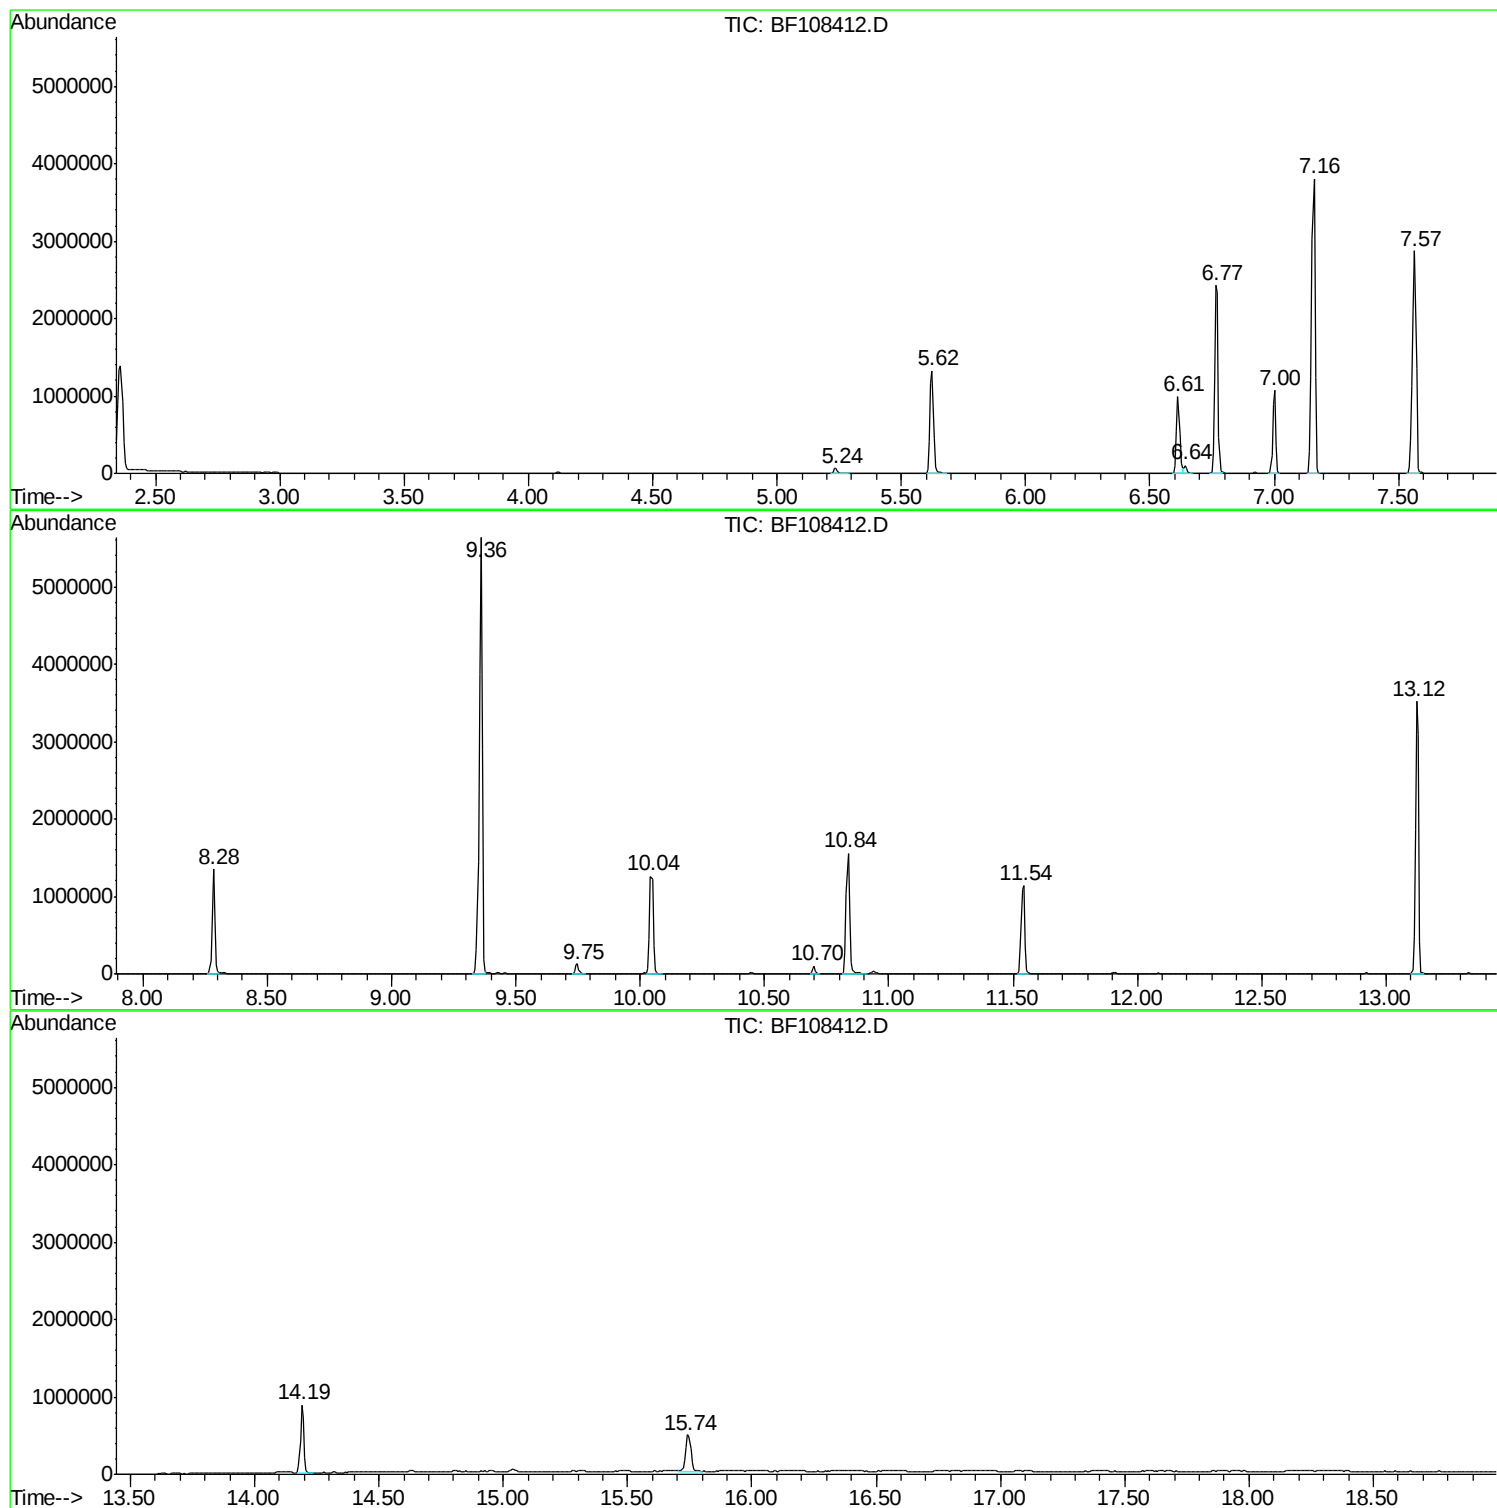

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
Data File : BF108412.D
Acq On : 23 Aug 2018 6:14
Operator : JU/SJ
Sample : J4525-13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081518-SIDI-F-U-M










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	51.81 ng	2384300	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
2		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
3		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
4		Xenon	132	Xe	007440-63-3	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

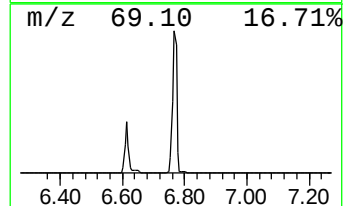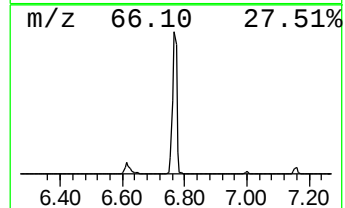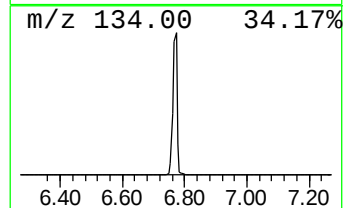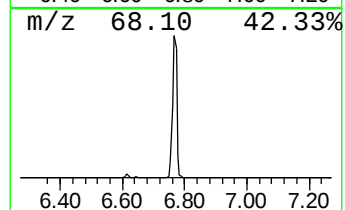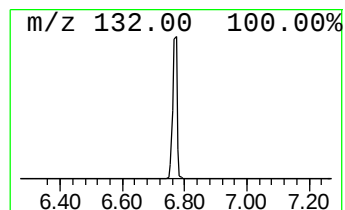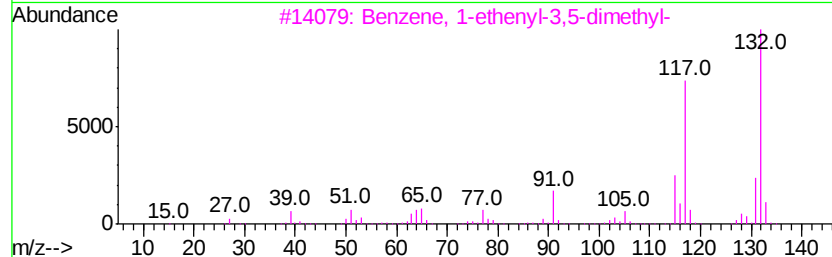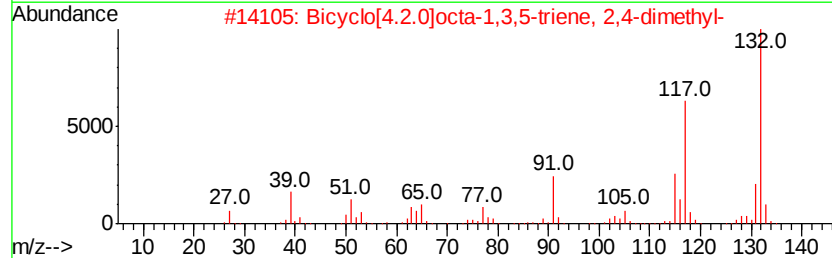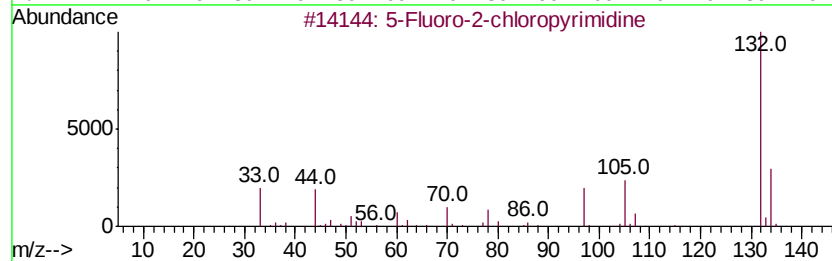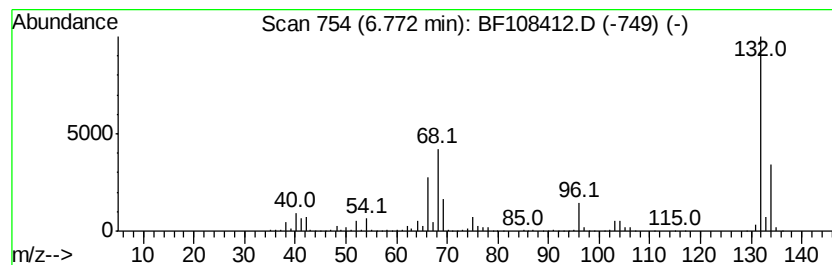

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082218\
Data File : BF108412.D
Acq On : 23 Aug 2018 6:14
Operator : JU/SJ
Sample : J4525-13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081518-SIDI-F-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.77	6.77	51.8	ng	2384300	1	7.00	920466	20.0