

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082218\
 Data File : BF108413.D
 Acq On : 23 Aug 2018 6:41
 Operator : JU/SJ
 Sample : J4525-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 081518-SIDI-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.237	489	493	502	rBV	66349	72061	1.33%	0.251%
2	5.625	555	559	562	rBV	1679137	1493050	27.53%	5.203%
3	6.613	723	727	730	rBV	1199307	1024351	18.89%	3.570%
4	6.642	730	732	741	rVB	106926	94833	1.75%	0.330%
5	6.772	749	754	757	rBV	2679793	2691529	49.63%	9.379%
6	7.001	789	793	796	rBV	1086784	946938	17.46%	3.300%
7	7.160	815	820	823	rBV	4046793	3642942	67.18%	12.695%
8	7.566	883	889	892	rBV	2880526	3082833	56.85%	10.743%
9	8.284	1007	1011	1014	rBV	1394177	1132425	20.88%	3.946%
10	9.360	1188	1194	1197	rBV	5790226	5422870	100.00%	18.897%
11	9.748	1256	1260	1265	rBV	206404	190946	3.52%	0.665%
12	10.042	1307	1310	1318	rVB	1260101	1229117	22.67%	4.283%
13	10.701	1419	1422	1430	rVB	108939	83107	1.53%	0.290%
14	10.836	1441	1445	1458	rBV	1729062	1549522	28.57%	5.400%
15	11.542	1561	1565	1568	rBV	1143659	1044172	19.25%	3.639%
16	13.124	1830	1834	1838	rBV	3668081	3462256	63.85%	12.065%
17	14.113	1993	2002	2005	rBV7	26273	71217	1.31%	0.248%
18	14.189	2011	2015	2019	rBV	851817	793576	14.63%	2.765%
19	15.748	2273	2280	2289	rVB	461412	668898	12.33%	2.331%


Sum of corrected areas: 28696643

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
Data File : BF108413.D
Acq On : 23 Aug 2018 6:41
Operator : JU/SJ
Sample : J4525-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081518-SIDI-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

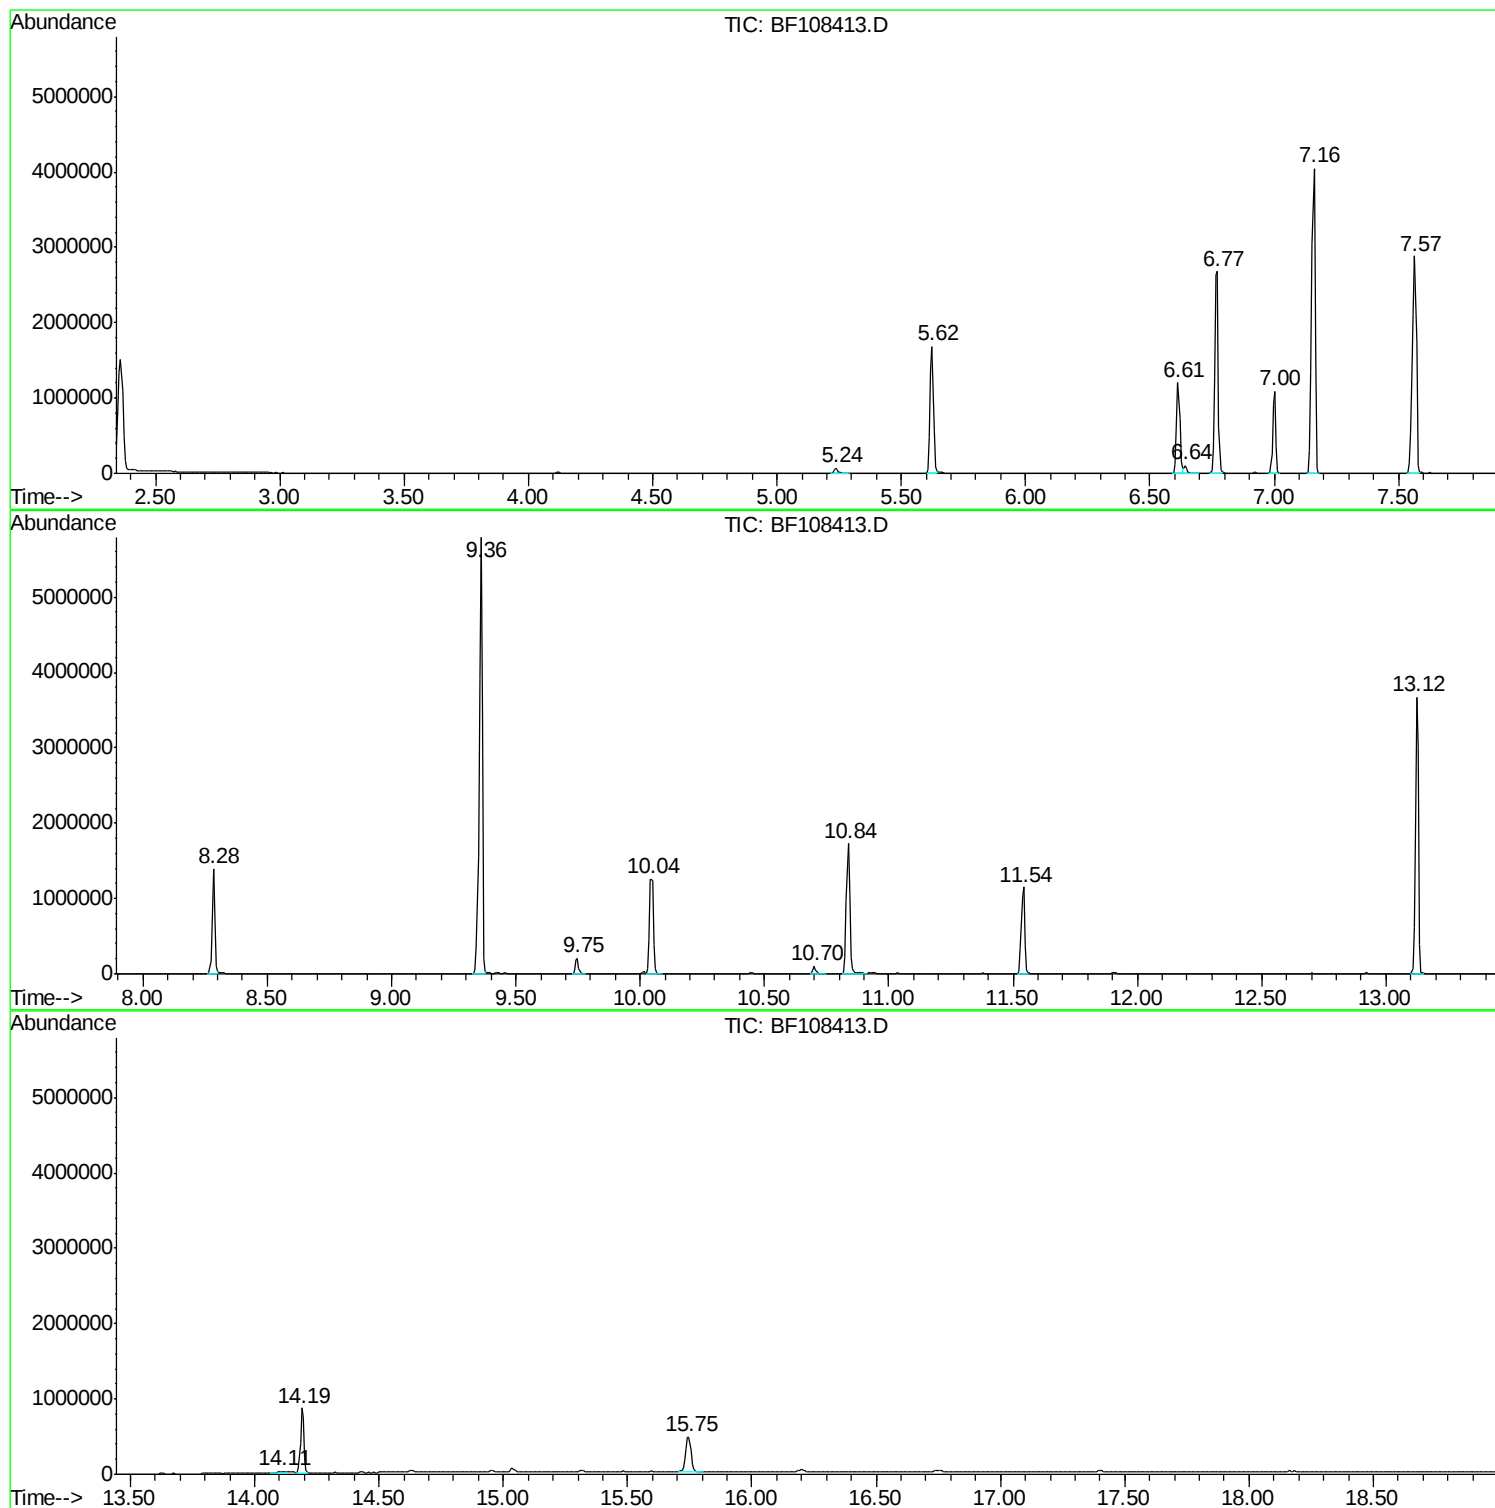

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082218\
Data File : BF108413.D
Acq On : 23 Aug 2018 6:41
Operator : JU/SJ
Sample : J4525-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081518-SIDI-F-U-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	56.85 ng	2691530	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

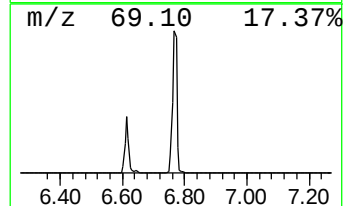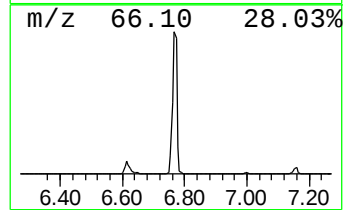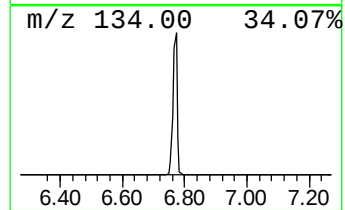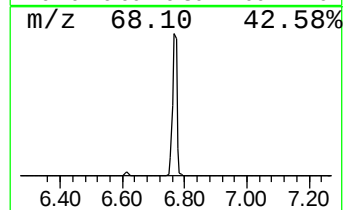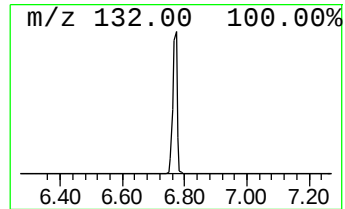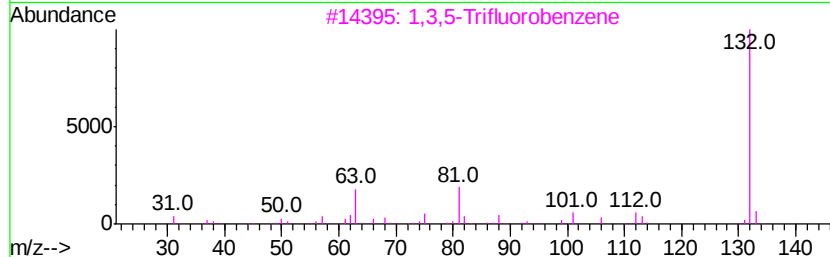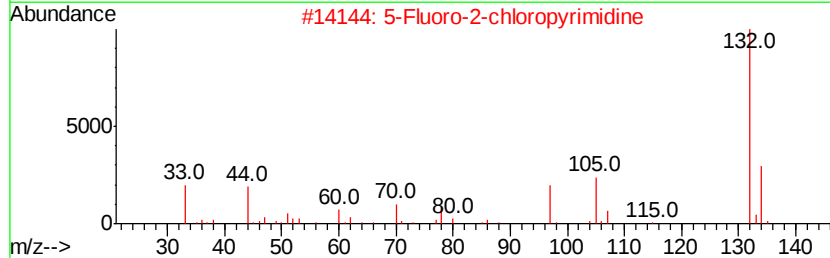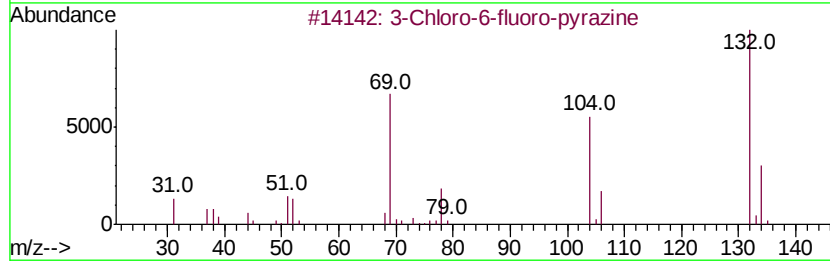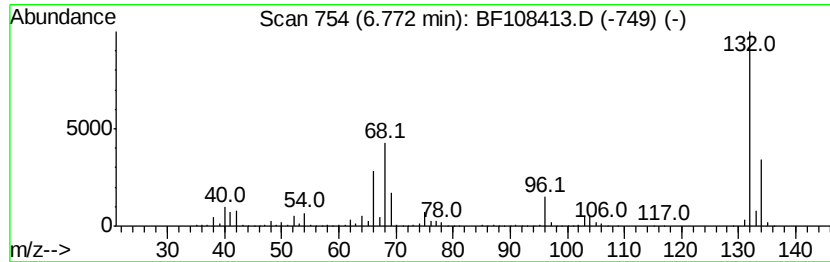

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082218\
Data File : BF108413.D
Acq On : 23 Aug 2018 6:41
Operator : JU/SJ
Sample : J4525-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
081518-SIDI-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.77	6.77	56.9	ng	2691530	1	7.00	946938	20.0