


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082218\
 Data File : BF108378.D
 Acq On : 22 Aug 2018 12:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 11:01:45 2018

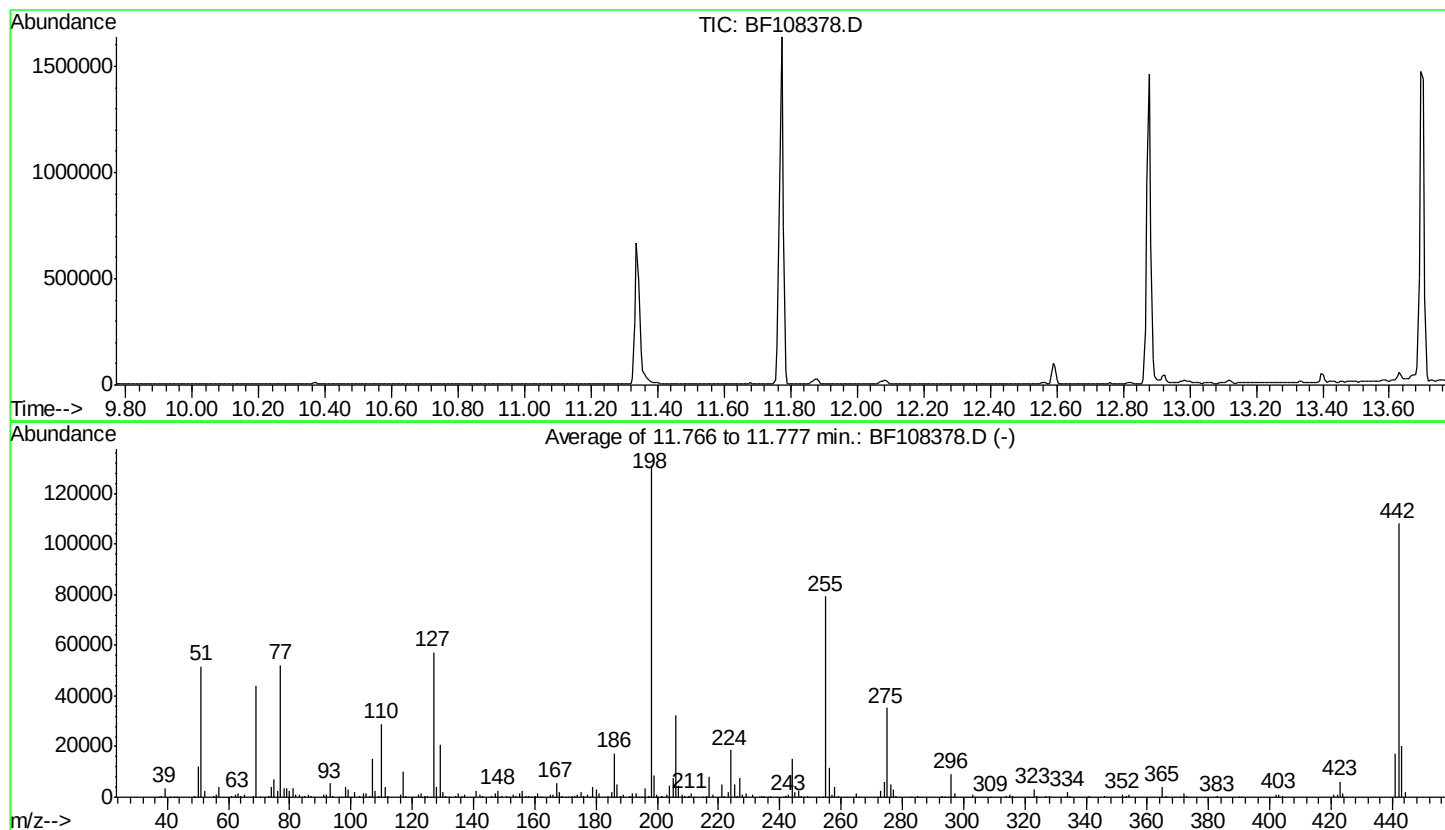

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	51608	PASS
68	69	0.00	2	1.6	727	PASS
69	198	0.00	100	33.7	44197	PASS
70	69	0.00	2	0.6	271	PASS
127	198	10	80	43.8	57328	PASS
197	198	0.00	2	0.5	720	PASS
198	198	100	100	100.0	131029	PASS
199	198	5	9	6.7	8759	PASS
275	198	10	60	27.0	35381	PASS
365	198	1	100	3.2	4246	PASS
441	198	0.01	100	13.2	17339	PASS
442	198	50	100	82.5	108050	PASS
443	442	15	24	18.5	20034	PASS