


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082218\
 Data File : BF108404.D
 Acq On : 23 Aug 2018 1:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 11:01:45 2018

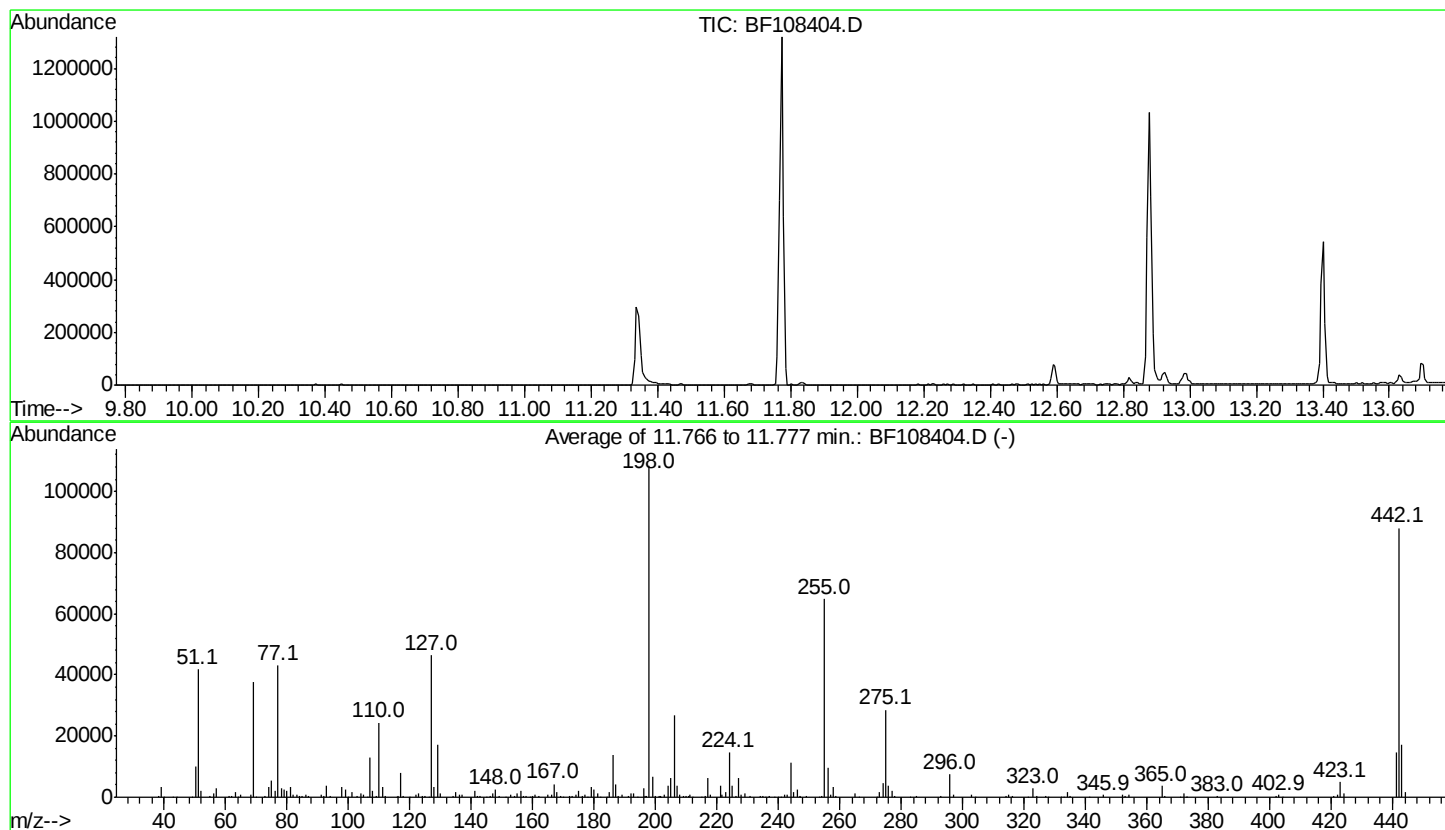

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	41720	PASS
68	69	0.00	2	2.0	736	PASS
69	198	0.00	100	34.6	37509	PASS
70	69	0.00	2	0.3	106	PASS
127	198	10	80	42.8	46450	PASS
197	198	0.00	2	0.4	430	PASS
198	198	100	100	100.0	108408	PASS
199	198	5	9	6.3	6786	PASS
275	198	10	60	26.3	28466	PASS
365	198	1	100	3.4	3697	PASS
441	198	0.01	100	13.6	14746	PASS
442	198	50	100	81.2	88058	PASS
443	442	15	24	19.5	17150	PASS