
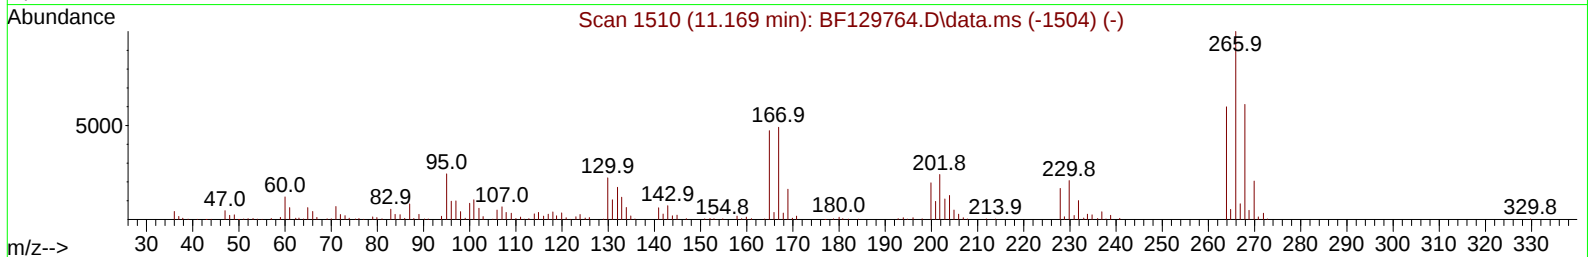
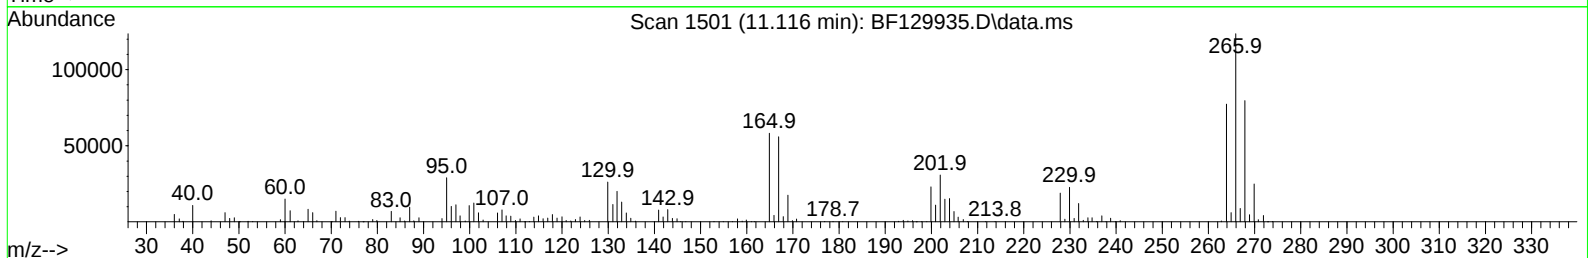


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082222\
Data File : BF129935.D
Acq On : 22 Aug 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 05:51:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 04:41:40 2022
Response via : Initial Calibration

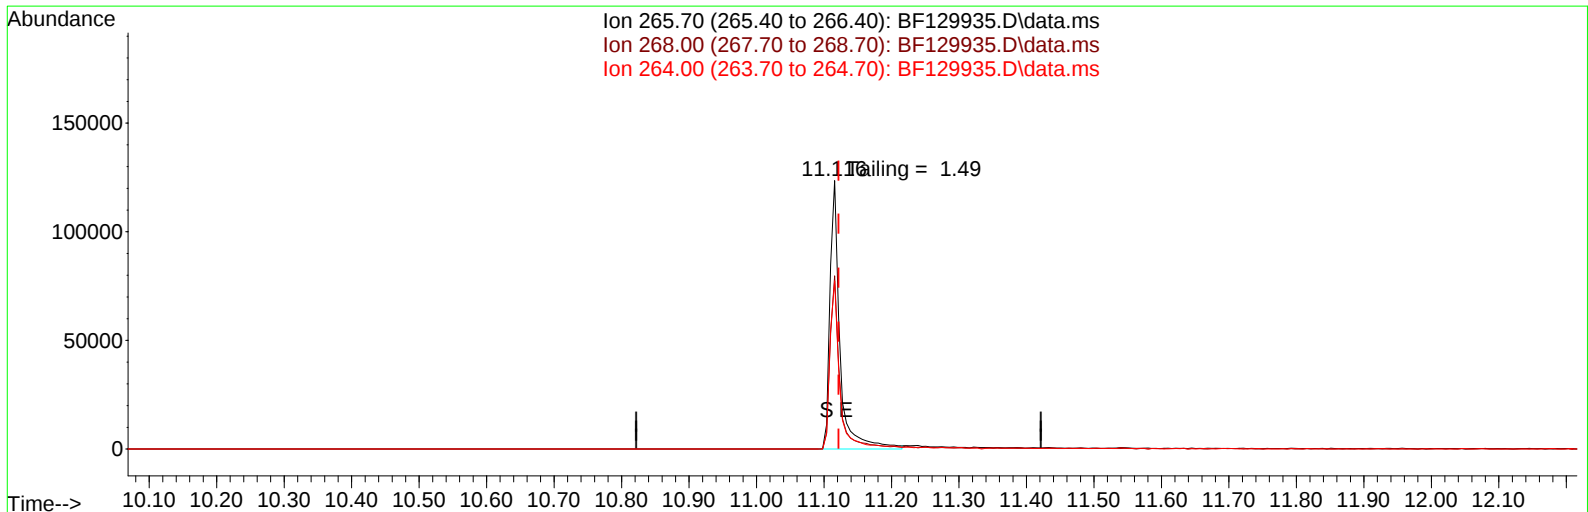

TIC: BF129935.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.006) 424021.03 ng

response 127595

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.50
264.00	59.90	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082222\
Data File : BF129935.D
Acq On : 22 Aug 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 05:51:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 04:41:40 2022
Response via : Initial Calibration

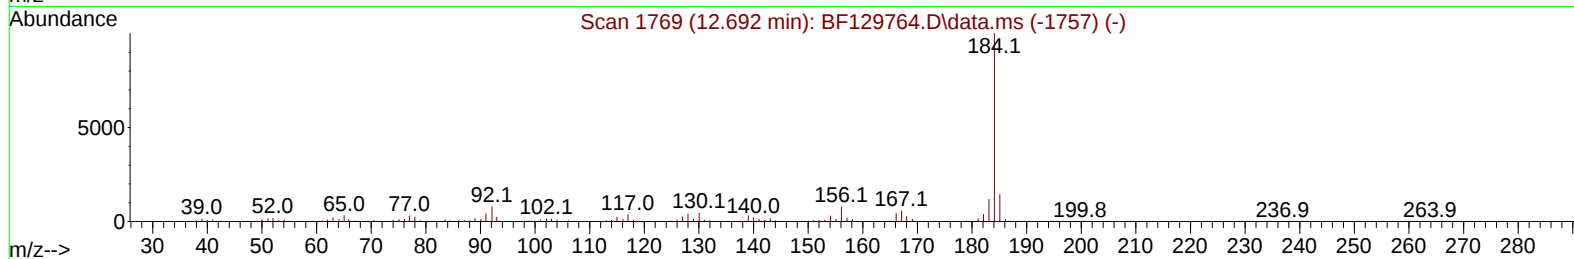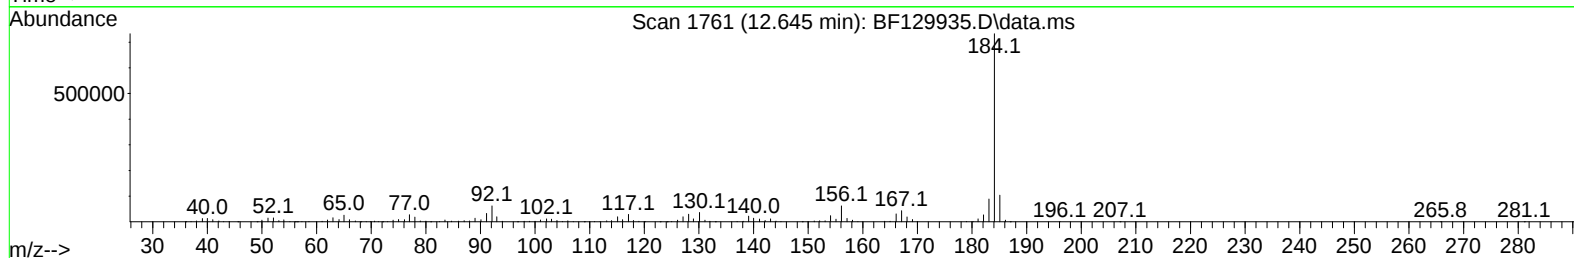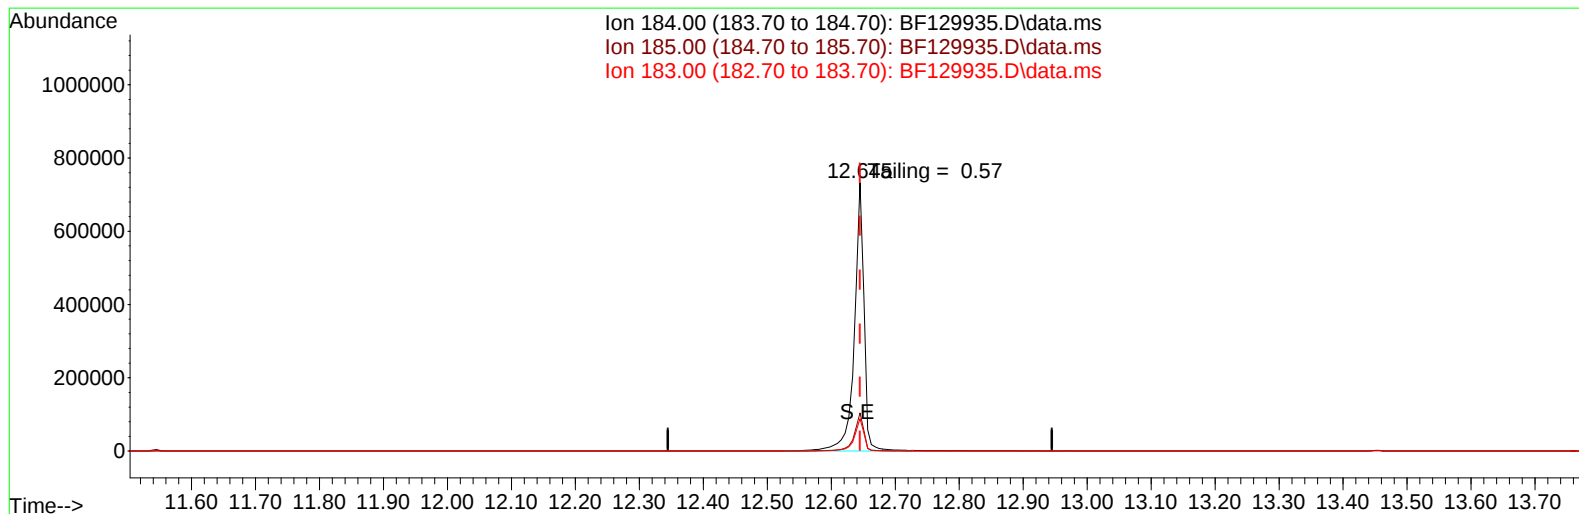

TIC: BF129935.D\data.ms

(77) Benzidine

12.645min (0.000) 75500.03 ng

response 777534

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.18
183.00	11.80	12.07
0.00	0.00	0.00