

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082222\
 Data File : BF129938.D
 Acq On : 22 Aug 2022 13:23
 Operator : CG\JU
 Sample : PB147058BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147058BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	529	533	556	rBV	3938424	3664775	68.16%	12.240%
2	6.434	700	705	724	rBV	3831820	3713669	69.07%	12.403%
3	6.775	759	763	772	rBV	950129	798968	14.86%	2.668%
4	7.345	855	860	863	rBV	2474455	2404015	44.71%	8.029%
5	8.057	976	981	992	rBV	1163585	1077742	20.04%	3.599%
6	9.134	1158	1164	1167	rBV	4643648	4646993	86.43%	15.520%
7	9.810	1273	1279	1282	rBV	1516269	1270155	23.62%	4.242%
8	10.610	1409	1415	1418	rBV	3281314	2989130	55.59%	9.983%
9	11.298	1528	1532	1536	rBV	1589104	1337725	24.88%	4.468%
10	12.886	1797	1802	1805	rBV	5535922	5376618	100.00%	17.957%
11	13.945	1978	1982	1989	rBV	1399258	1230461	22.89%	4.109%
12	15.398	2220	2229	2240	rBV	846831	1118271	20.80%	3.735%
13	15.786	2291	2295	2303	rVB	54063	77019	1.43%	0.257%
14	16.268	2372	2377	2385	rVB	49390	87031	1.62%	0.291%
15	16.833	2468	2473	2480	rVB4	38441	72897	1.36%	0.243%
16	17.498	2580	2586	2594	rVB3	31679	76419	1.42%	0.255%




Sum of corrected areas: 29941888

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082222\
Data File : BF129938.D
Acq On : 22 Aug 2022 13:23
Operator : CG\JU
Sample : PB147058BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147058BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

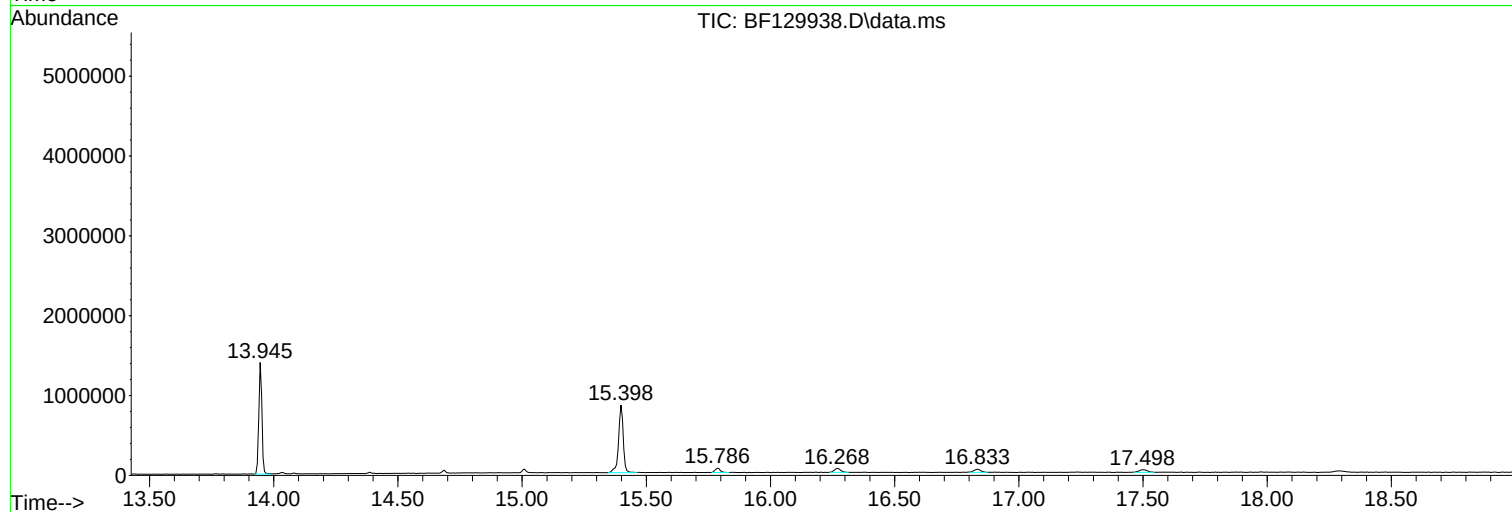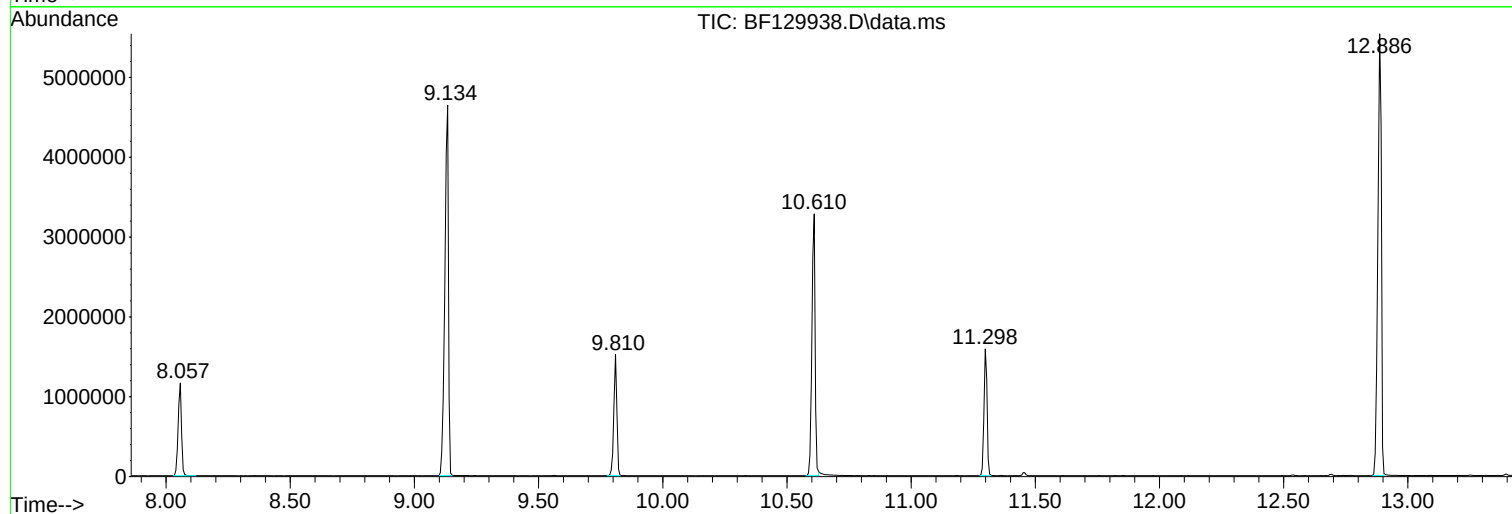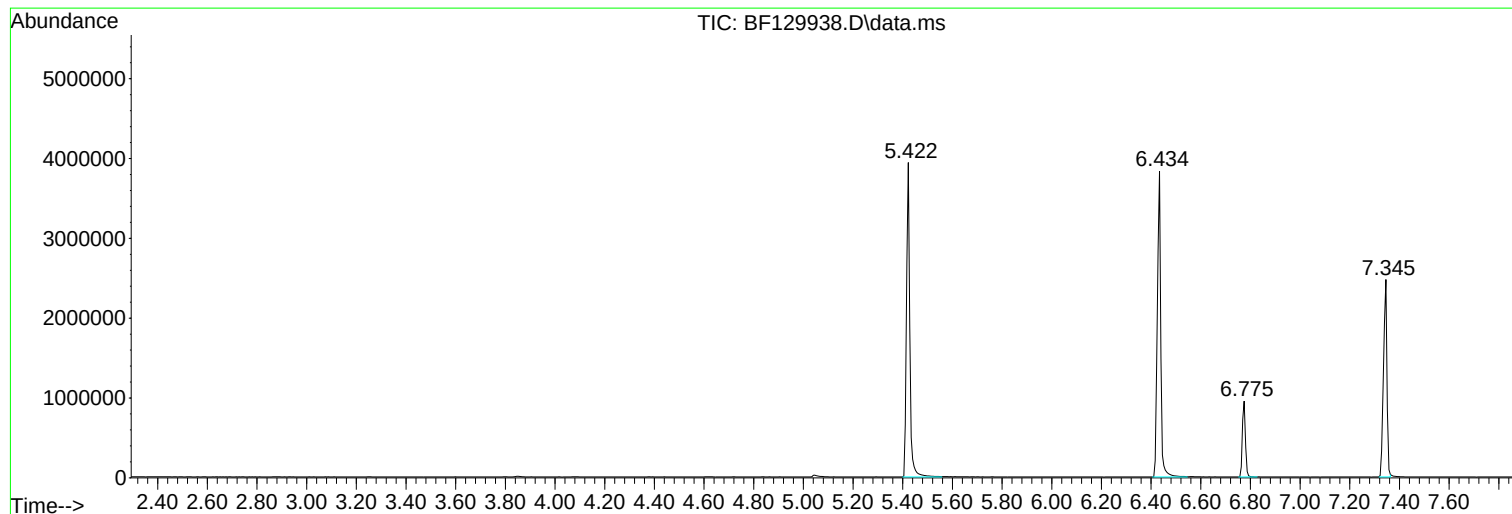

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082222\
Data File : BF129938.D
Acq On : 22 Aug 2022 13:23
Operator : CG\JU
Sample : PB147058BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147058BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082222\
Data File : BF129938.D
Acq On : 22 Aug 2022 13:23
Operator : CG\JU
Sample : PB147058BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147058BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------