


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082222\
 Data File : BF129935.D
 Acq On : 22 Aug 2022 11:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 23 04:41:40 2022

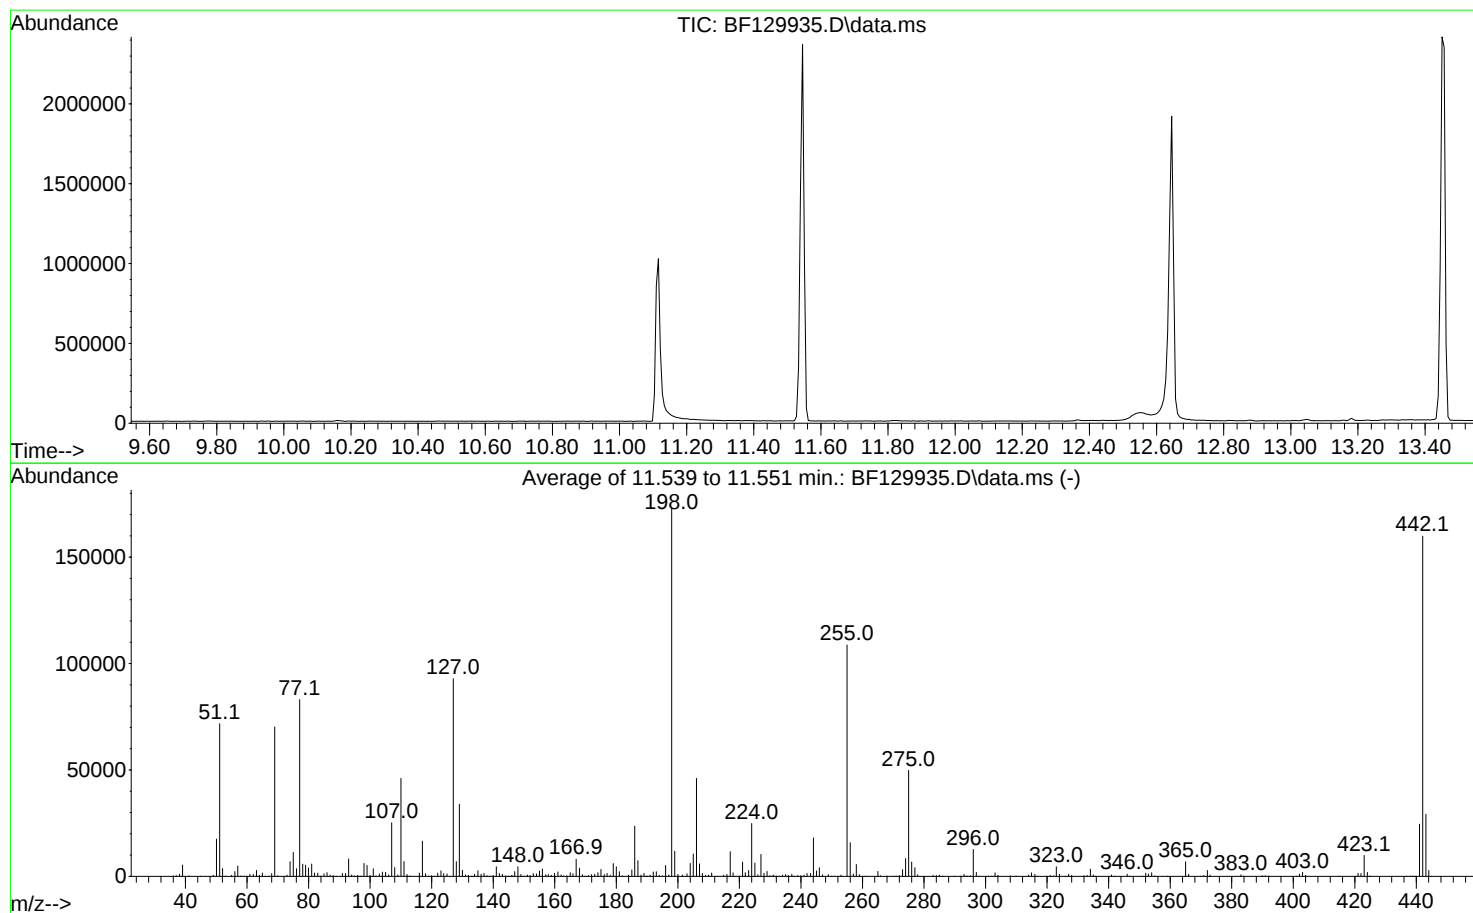

AutoFind: Scans 1573, 1574, 1575; Background Corrected with Scan 1568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	71701	PASS
68	69	0.00	2	1.9	1313	PASS
69	198	0.00	100	40.6	70245	PASS
70	69	0.00	2	0.4	316	PASS
127	198	10	80	53.7	92845	PASS
197	198	0.00	2	0.4	650	PASS
198	198	100	100	100.0	172835	PASS
199	198	5	9	6.8	11790	PASS
275	198	10	60	28.8	49736	PASS
365	198	1	100	4.0	6859	PASS
441	198	0.01	100	14.2	24512	PASS
442	442	50	100	100.0	159824	PASS
443	442	15	24	18.3	29171	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/22/2022	BNA_F	<u>BF129935.D</u>
Compound Name	Response	Retention Time
DDT	419554	13.457
DDD	3862	13.18
DDE	824	12.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4686	424240	1.10

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082222\
Data File : BF129935.D
Acq On : 22 Aug 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 23 05:51:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 04:41:40 2022
Response via : Initial Calibration

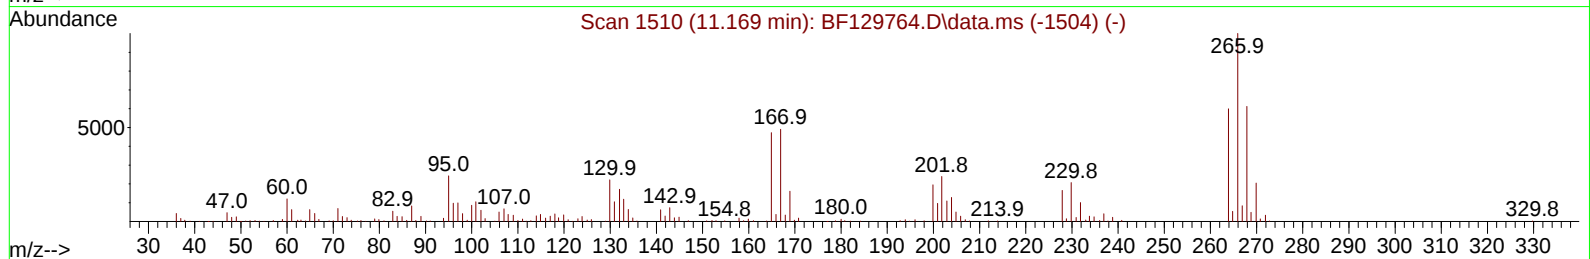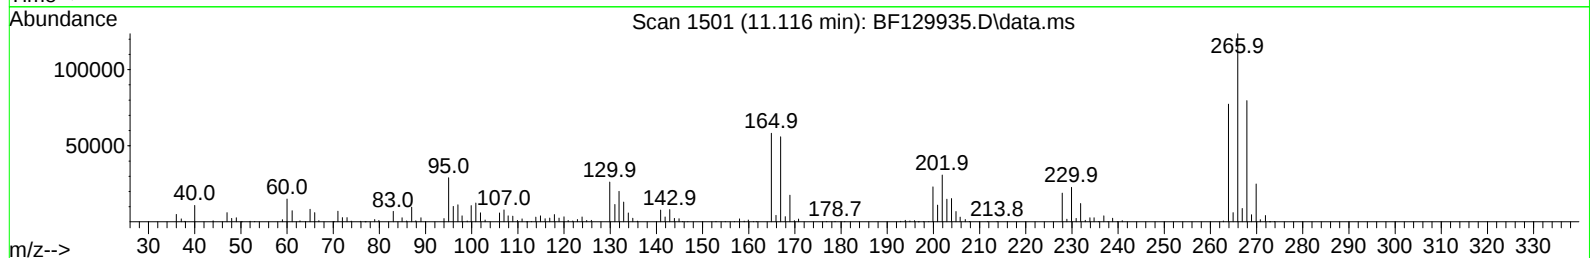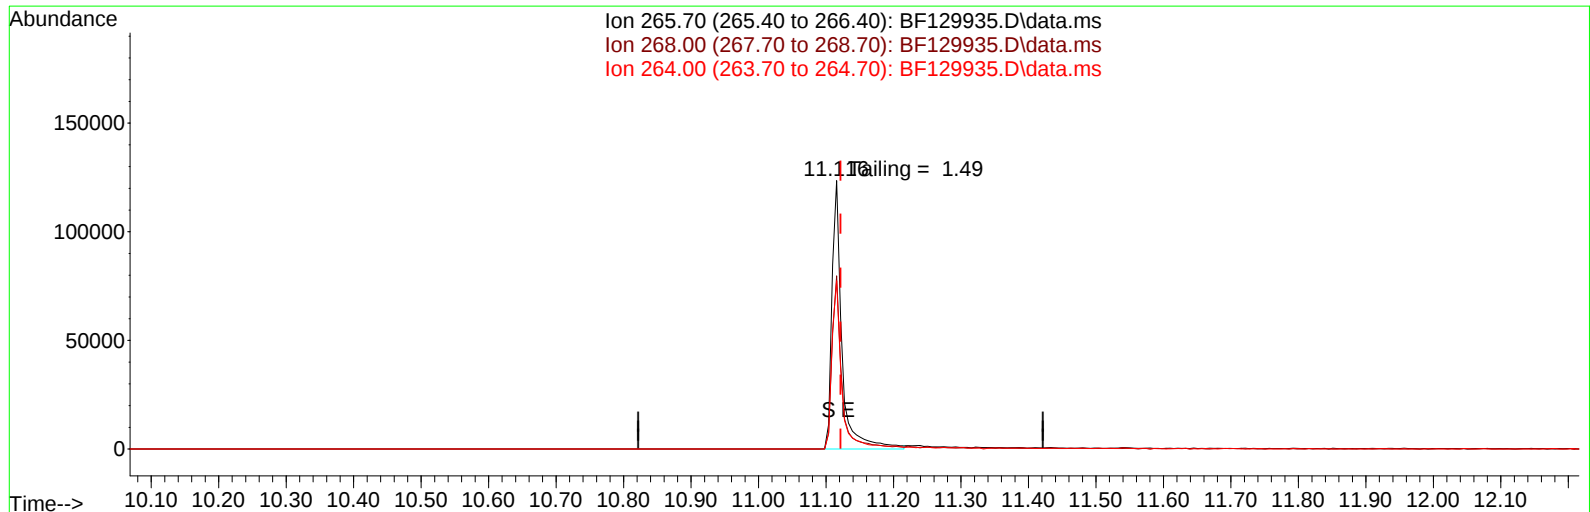

TIC: BF129935.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.006) 424021.03 ng




response 127595

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.50
264.00	59.90	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082222\
Data File : BF129935.D
Acq On : 22 Aug 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 23 05:51:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 04:41:40 2022
Response via : Initial Calibration

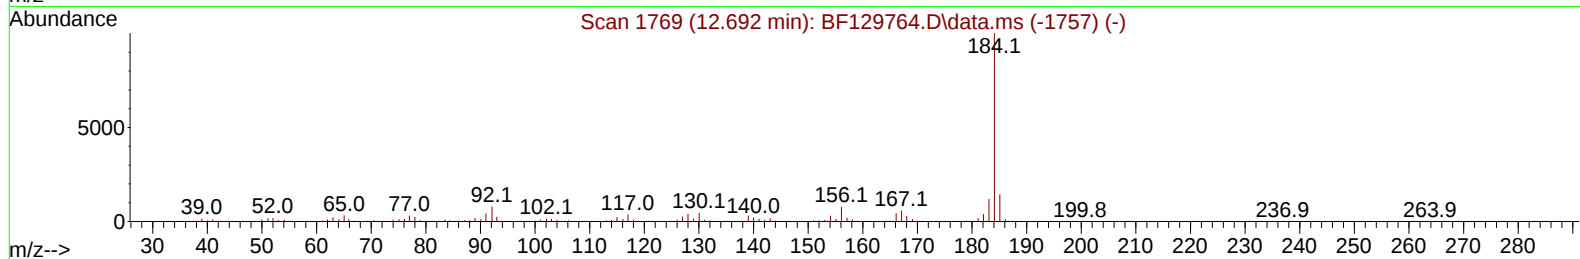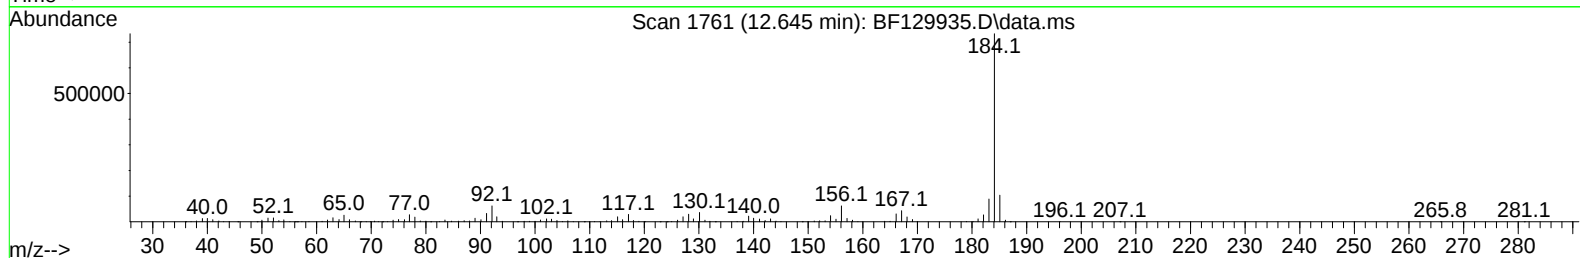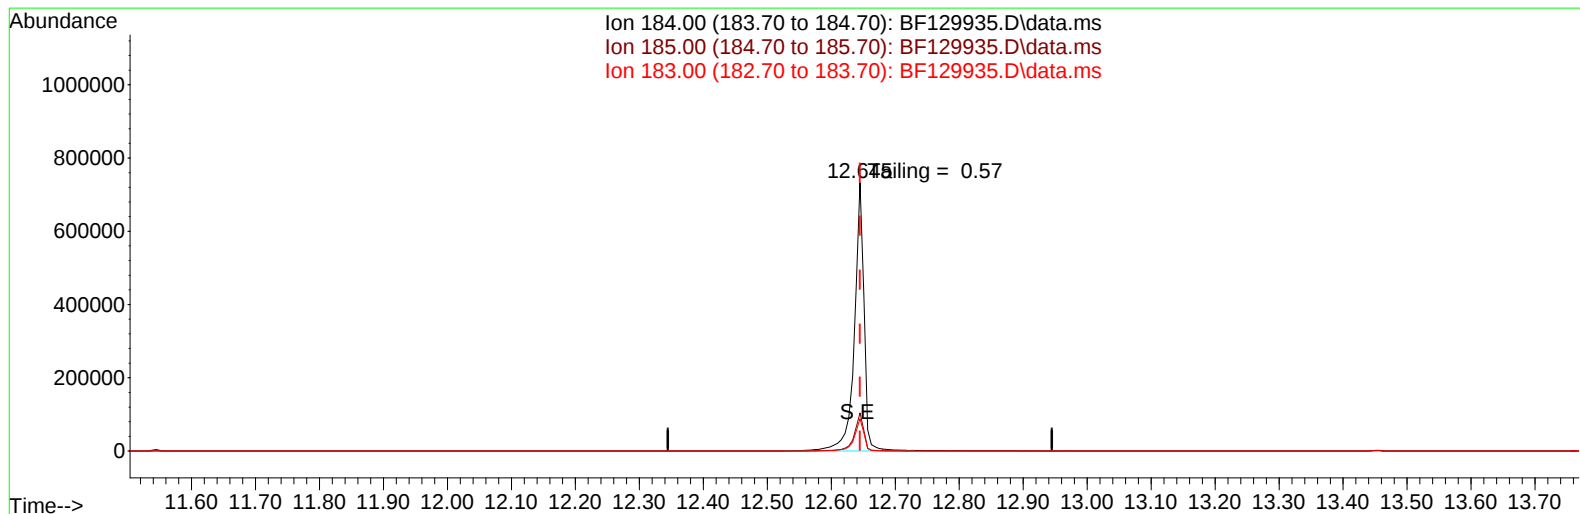

TIC: BF129935.D\data.ms

(77) Benzidine

12.645min (0.000) 75500.03 ng

response 777534

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.18
183.00	11.80	12.07
0.00	0.00	0.00