
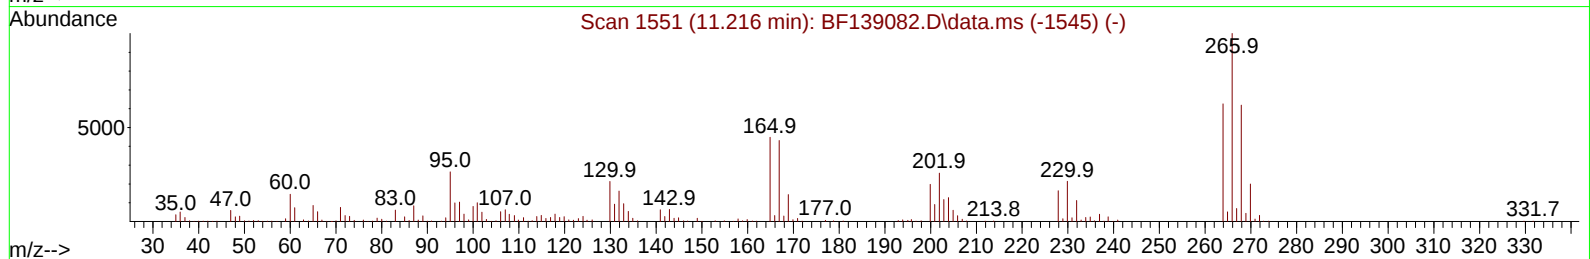
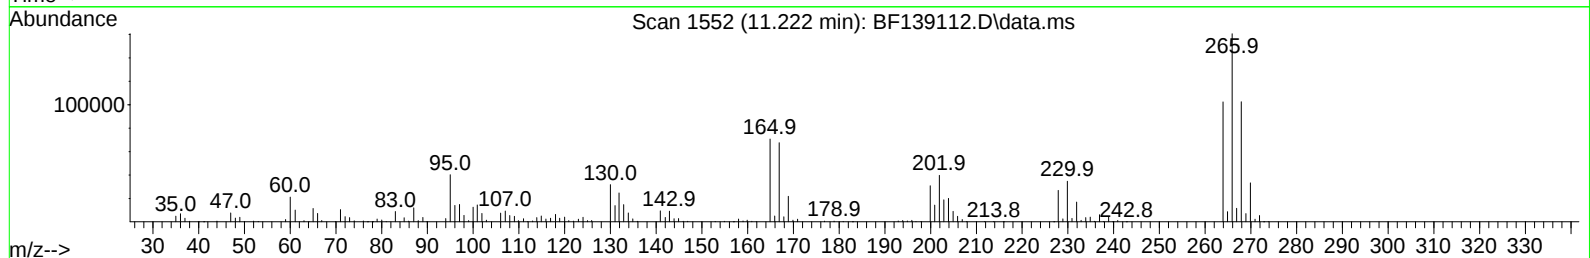


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082224\
Data File : BF139112.D
Acq On : 22 Aug 2024 09:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 10:59:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

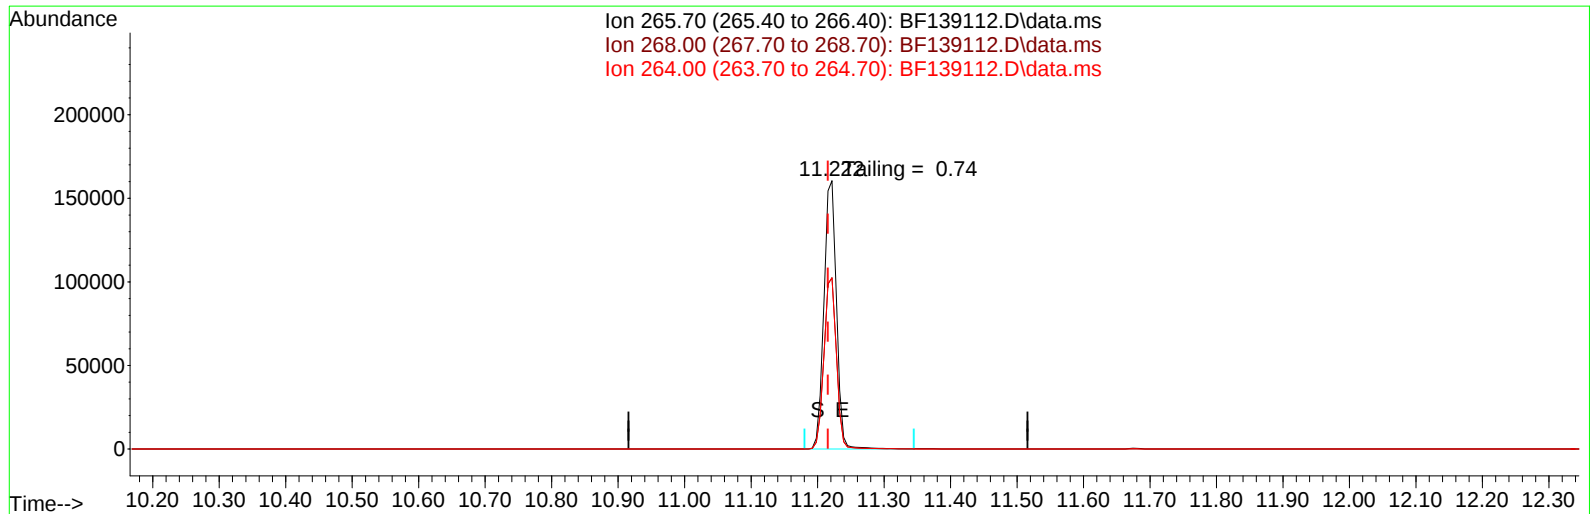

TIC: BF139112.D\data.ms

(70) Pentachlorophenol (C)




11.222min (+ 0.006) 34840.56 ng

response 211256

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.87
264.00	62.50	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082224\
Data File : BF139112.D
Acq On : 22 Aug 2024 09:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 10:59:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

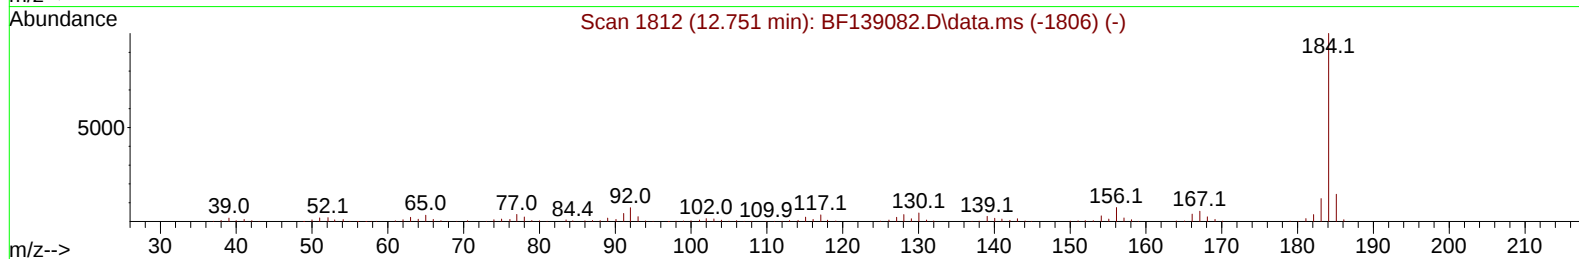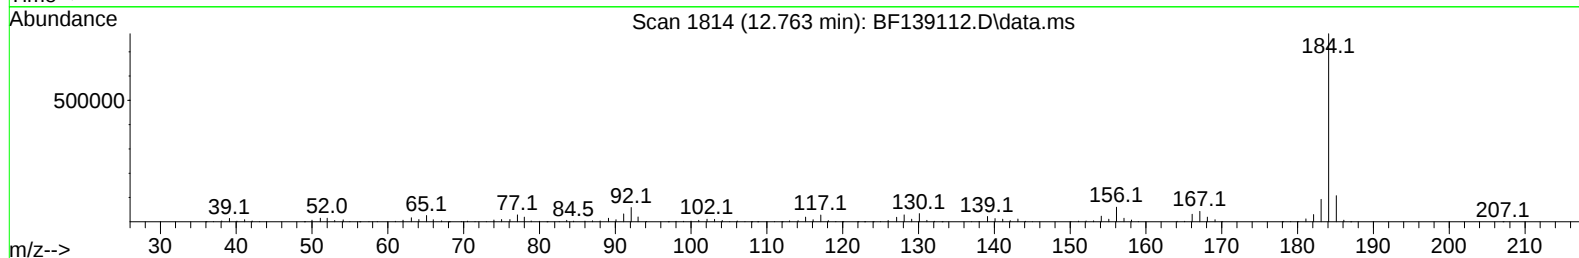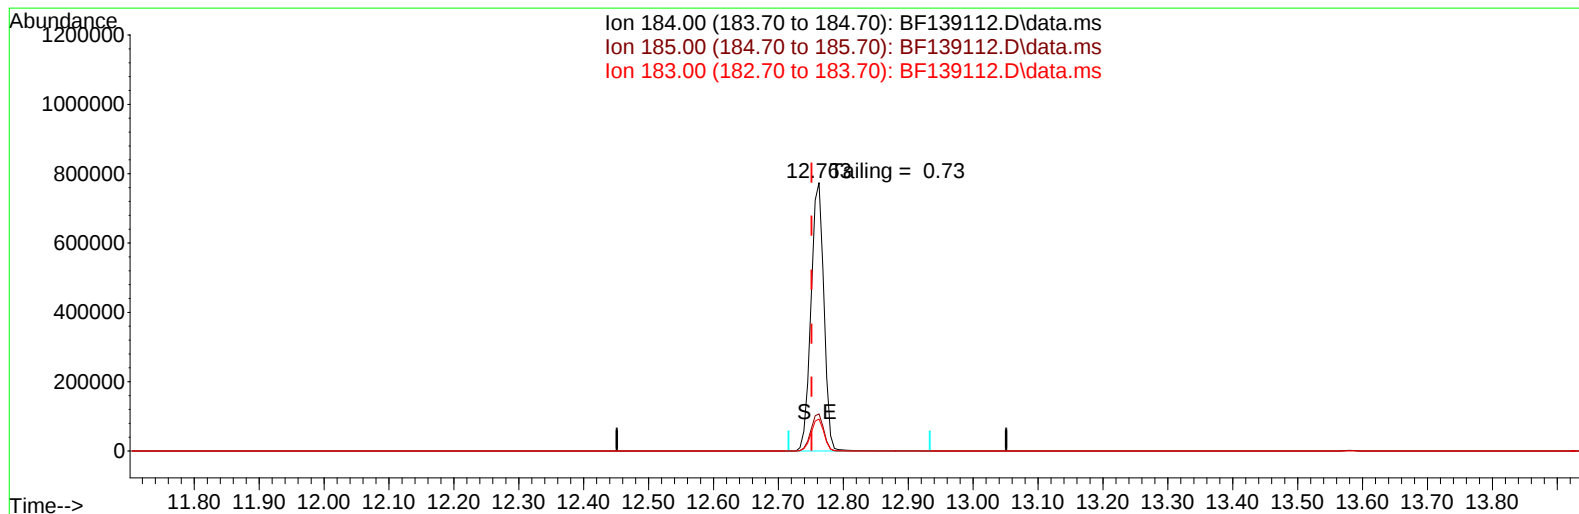

TIC: BF139112.D\data.ms

(77) Benzidine

12.763min (+ 0.012) 0.00 ng

response 1070049

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.87
183.00	12.20	11.96
0.00	0.00	0.00