
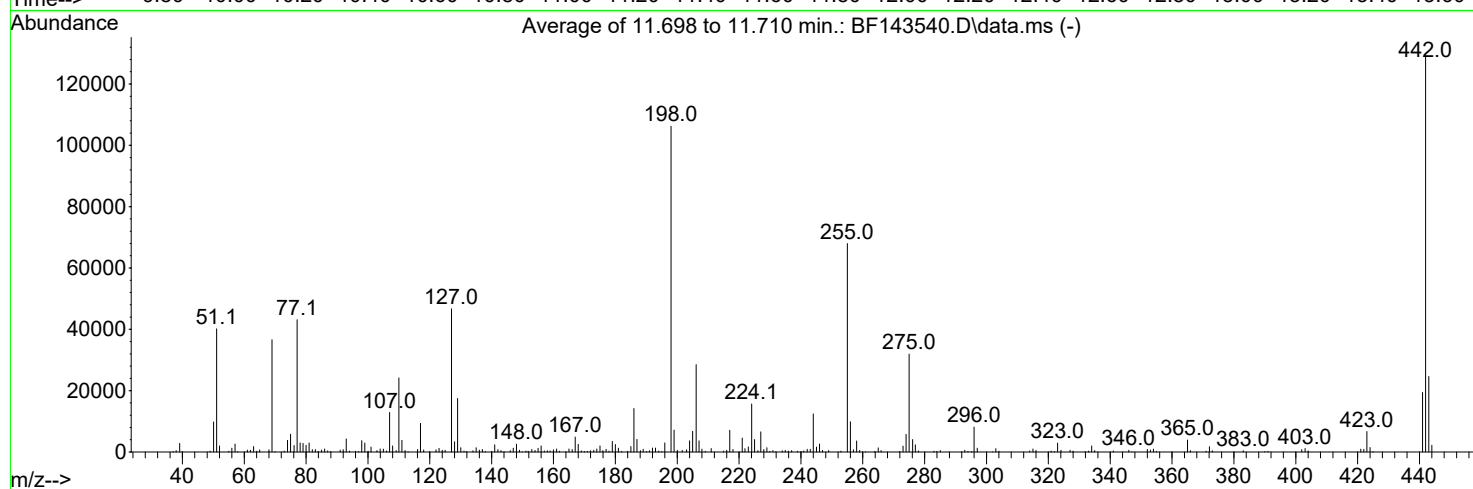


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\
Data File : BF143540.D
Acq On : 21 Aug 2025 20:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 21 06:12:21 2025

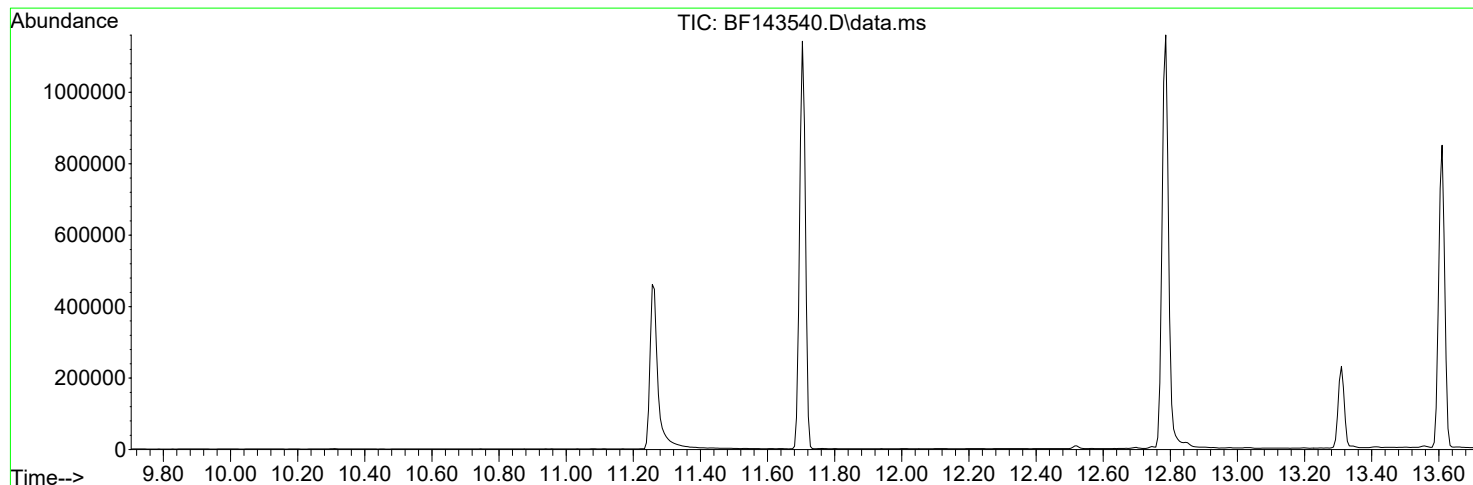

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	724	PASS
69	69	100	100	100.0	36616	PASS
70	69	0.00	2	0.4	144	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106203	PASS
199	198	5	9	6.7	7166	PASS
365	198	1	100	3.7	3899	PASS
441	443	0.01	150	78.9	19432	PASS
442	442	100	100	100.0	128741	PASS
443	442	15	24	19.1	24627	PASS