
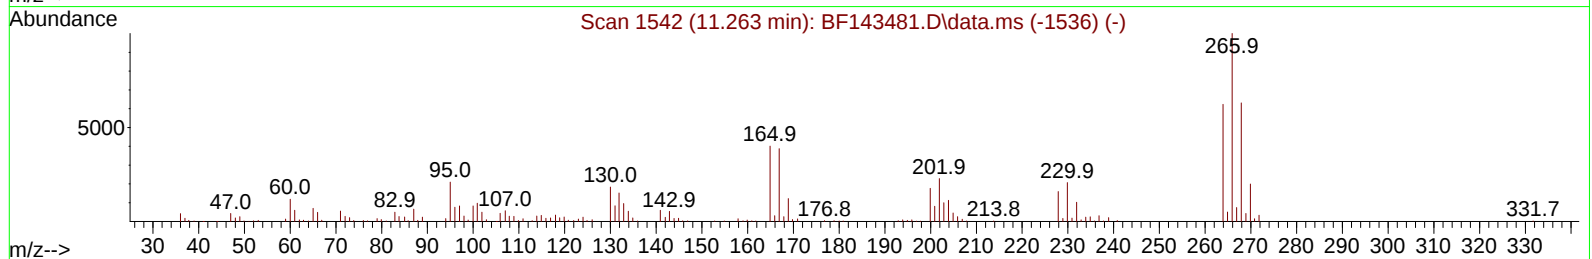
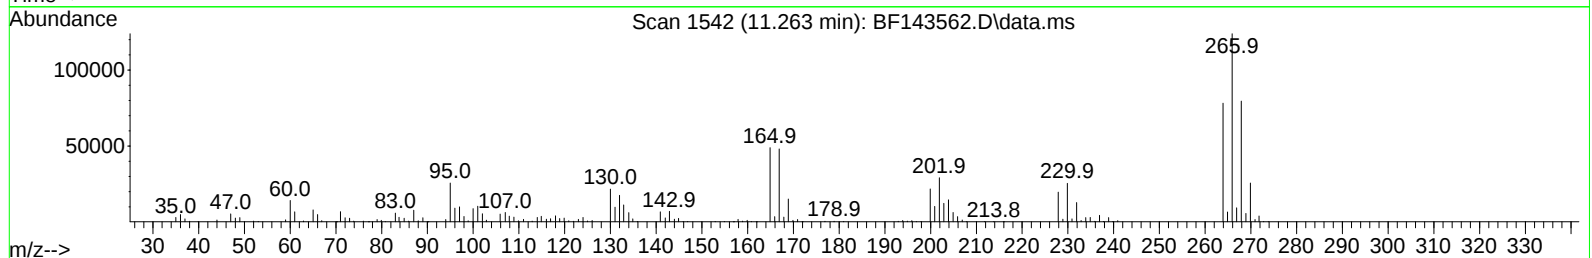


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082225\
Data File : BF143562.D
Acq On : 22 Aug 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 09:53:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration

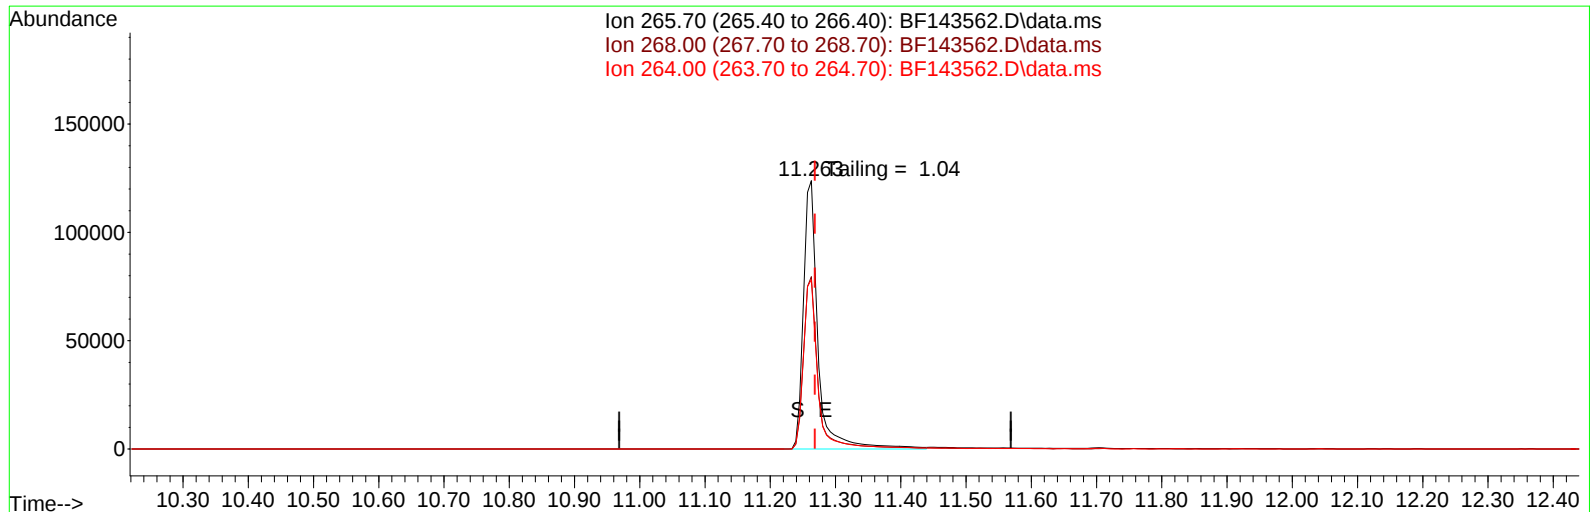

TIC: BF143562.D\data.ms

(70) Pentachlorophenol (C)




11.263min (-0.006) 106263.89 ng

response 193411

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.25
264.00	62.30	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082225\
Data File : BF143562.D
Acq On : 22 Aug 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 09:53:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration

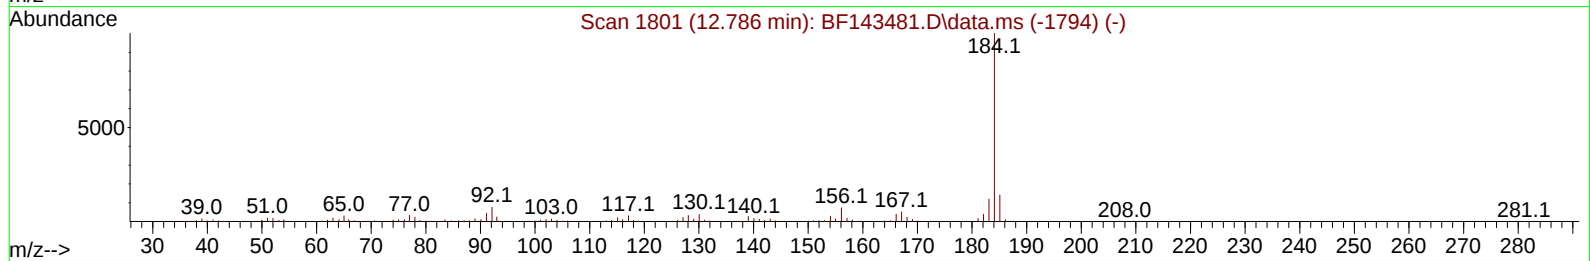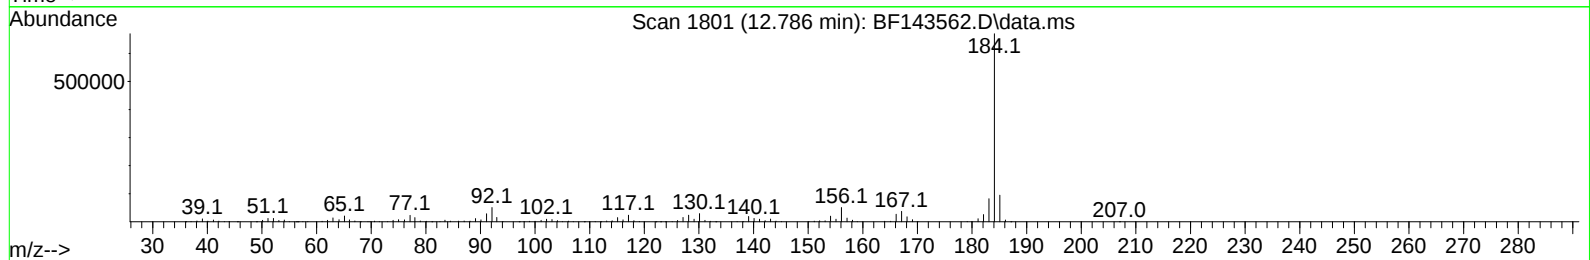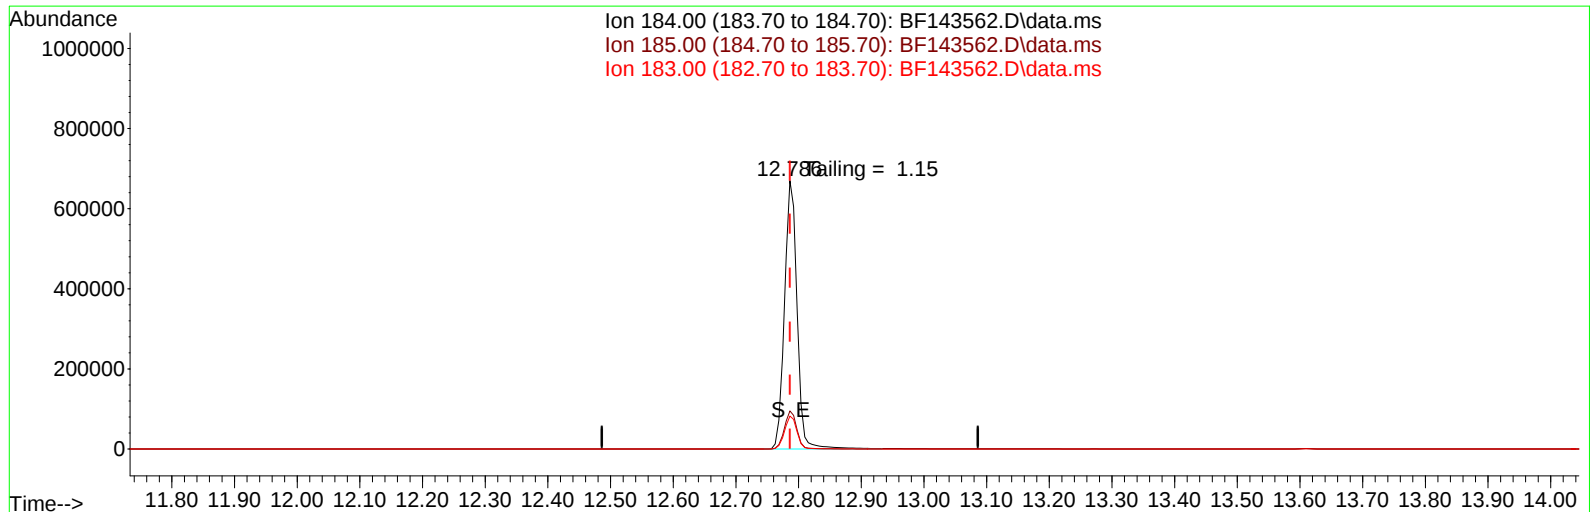

TIC: BF143562.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 666495.20 ng

response 941621

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.18
183.00	11.90	12.27
0.00	0.00	0.00