

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082316\
 Data File : BF089834.D
 Acq On : 23 Aug 2016 14:59
 Operator : UM/SJ
 Sample : H4547-11
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 D-8(2.5-3)

Quant Time: Aug 25 13:44:31 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 19 14:02:57 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.66	152	458976	20.00	ng	-0.02
21) Naphthalene-d8	7.95	136	1938448	20.00	ng	-0.02
38) Acenaphthene-d10	9.70	164	886842	20.00	ng	-0.01
63) Phenanthrene-d10	11.18	188	1622478	20.00	ng	-0.01
75) Chrysene-d12	13.84	240	1477138	20.00	ng	-0.03
86) Perylene-d12	15.31	264	1209775	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.24	112	2871848	107.30	ng	-0.01
7) Phenol-d6	6.31	99	3737091	113.75	ng	-0.01
23) Nitrobenzene-d5	7.23	82	2147881	68.84	ng	-0.02
41) 2,4,6-Tribromophenol	10.49	330	825052	97.89	ng	-0.01
44) 2-Fluorobiphenyl	9.04	172	3943268	78.15	ng	-0.01
78) Terphenyl-d14	12.78	244	3454768	52.91	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.43	163	1076906	17.25	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082316\
Data File : BF089834.D
Acq On : 23 Aug 2016 14:59
Operator : UM/SJ
Sample : H4547-11
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
D-8(2.5-3)

Quant Time: Aug 25 13:44:31 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 19 14:02:57 2016
Response via : Initial Calibration




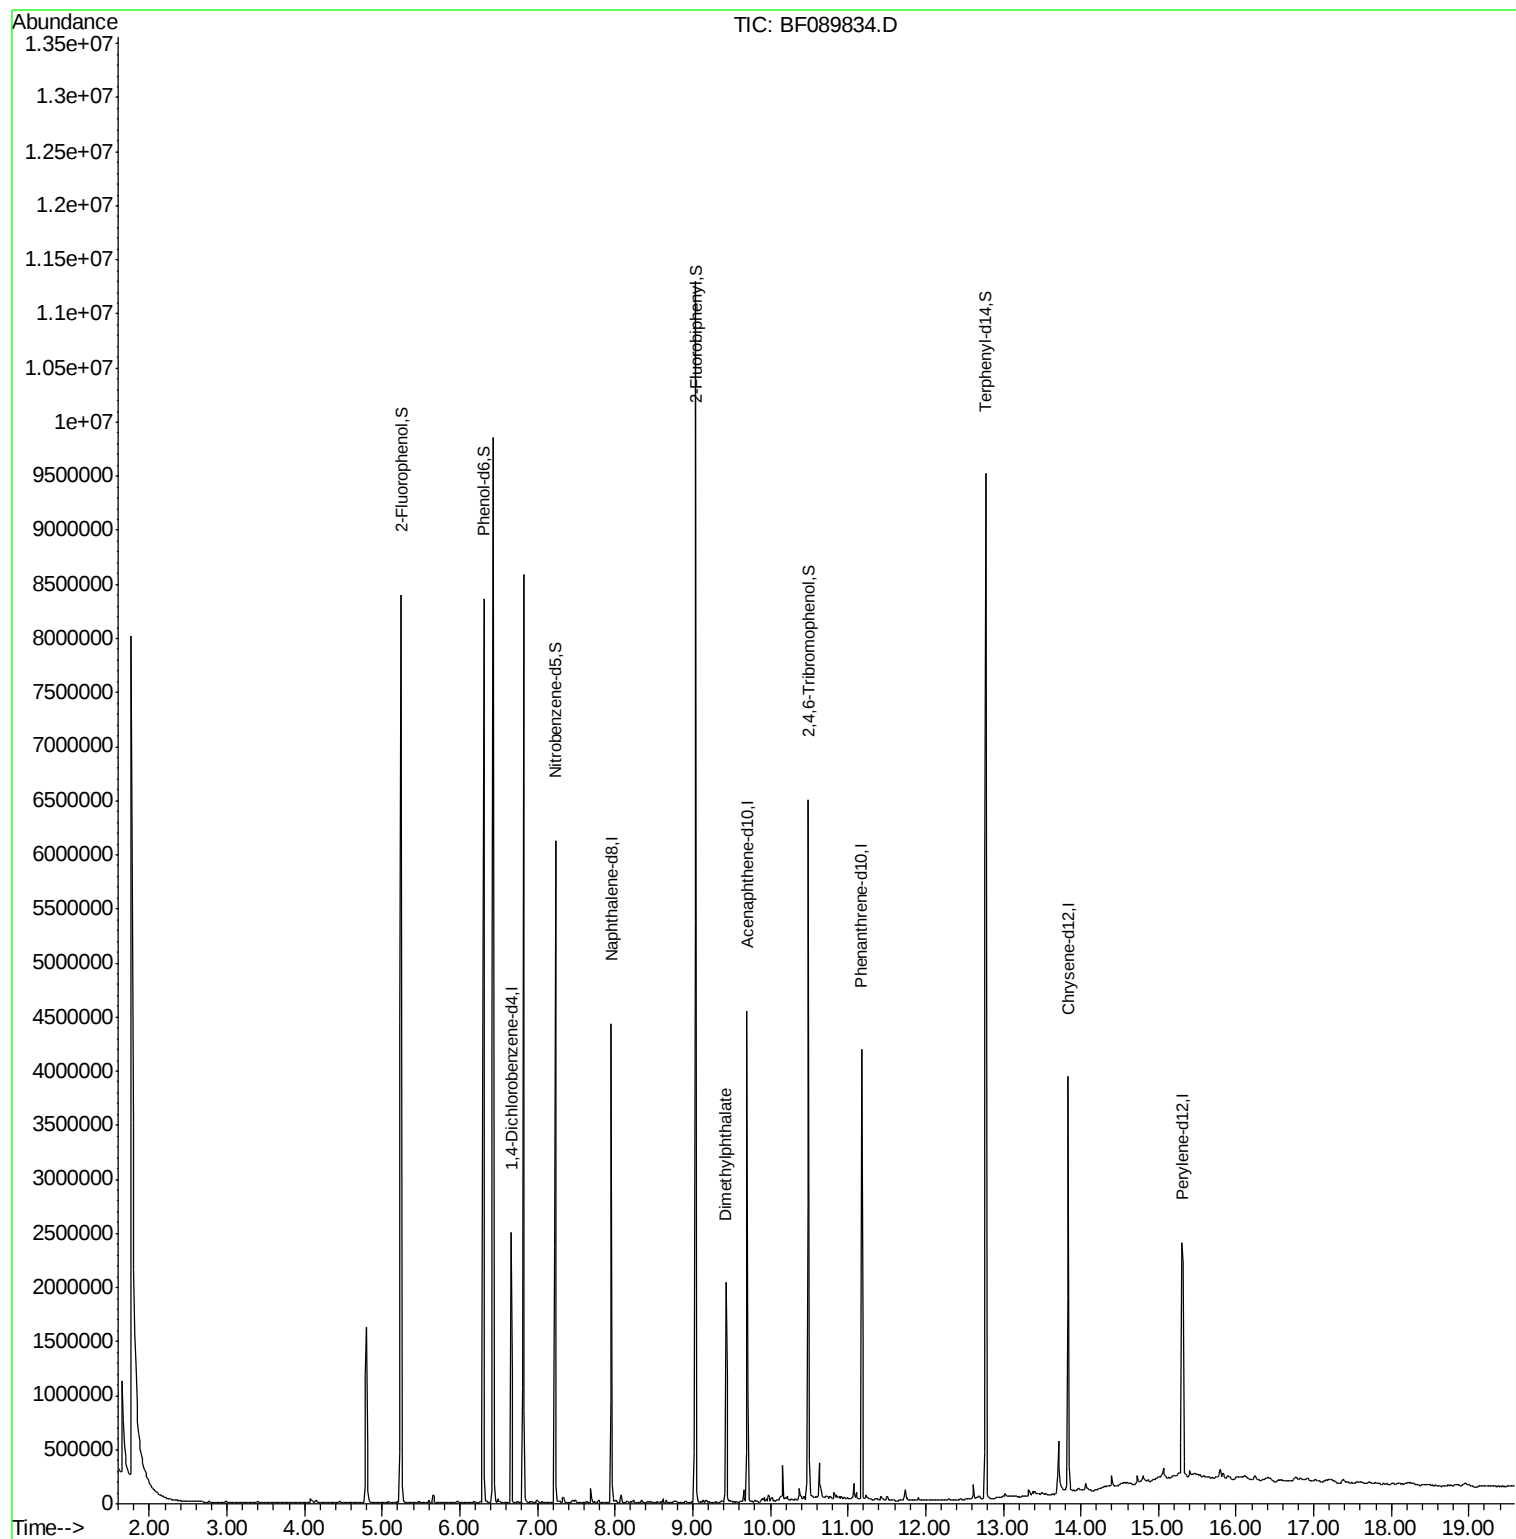


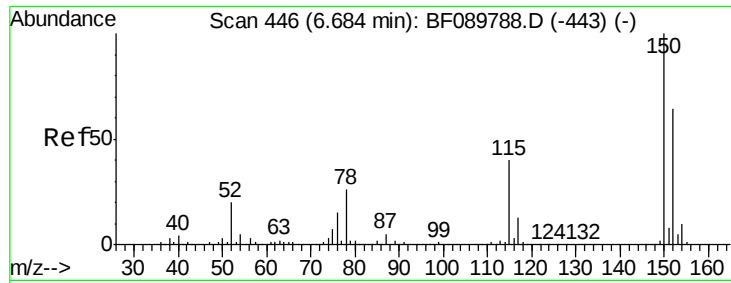

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.66 min Scan# 444
 Delta R.T. -0.02 min
 Lab File: BF089834.D
 Acq: 23 Aug 2016 14:59




Instrument :
 BNA_F
 ClientSampleId :
 D-8(2.5-3)


Tgt Ion:152 Resp: 458976
 Ion Ratio Lower Upper
 152 100
 150 157.3 125.3 187.9
 115 66.2 40.9 61.3#

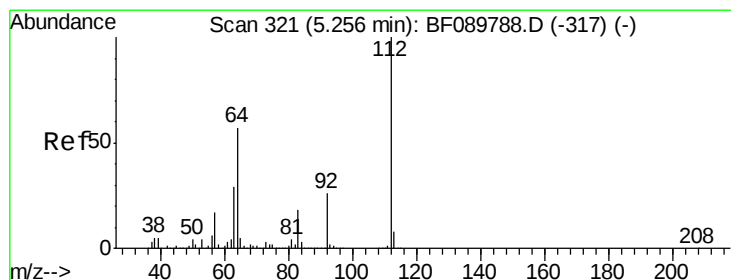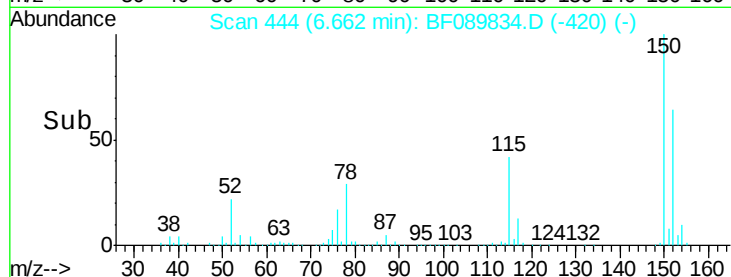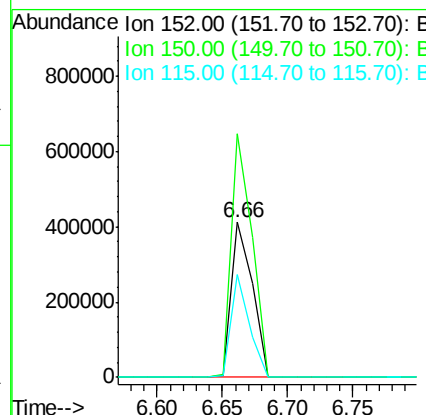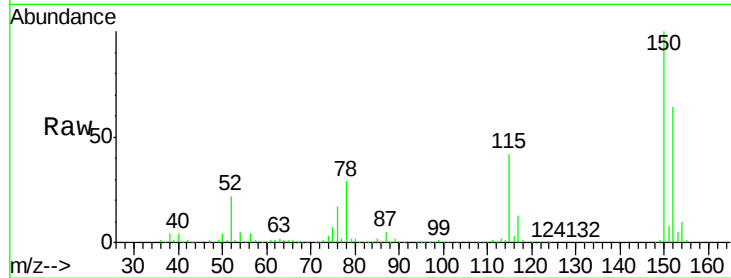

#5
 2-Fluorophenol
 Concen: 107.30 ng
 RT: 5.24 min Scan# 320
 Delta R.T. -0.01 min
 Lab File: BF089834.D
 Acq: 23 Aug 2016 14:59

Tgt Ion:112 Resp: 2871848
 Ion Ratio Lower Upper
 112 100
 64 52.7 45.0 67.4
 63 26.3 23.1 34.7

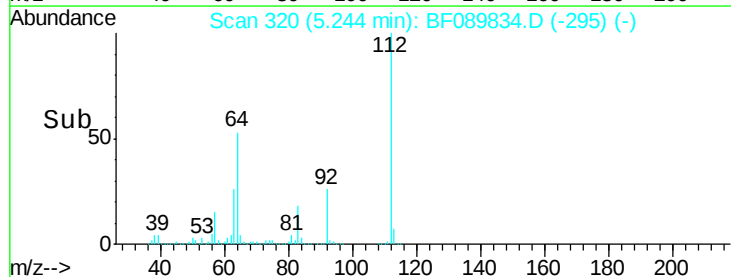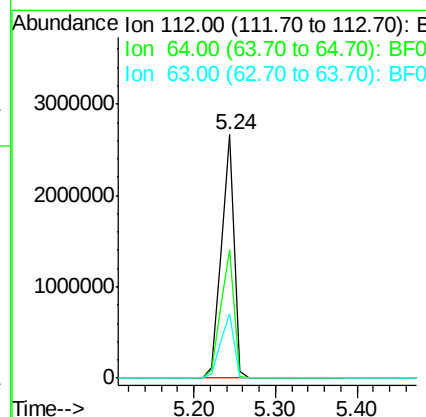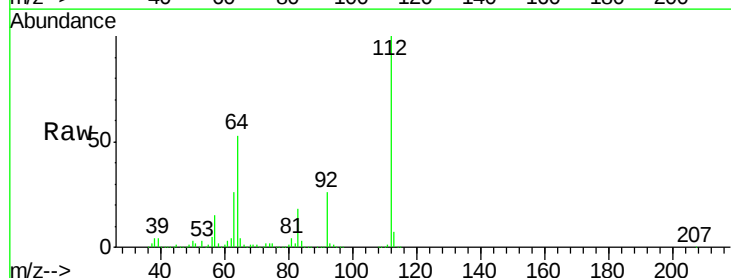

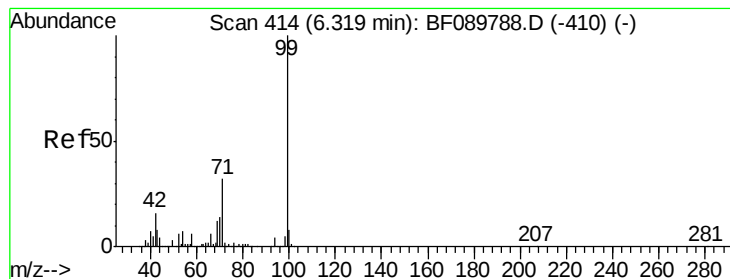

#7

Phenol-d6

Concen: 113.75 ng

RT: 6.31 min Scan# 413

Delta R.T. -0.01 min

Lab File: BF089834.D

Acq: 23 Aug 2016 14:59

Instrument :

BNA_F

ClientSampleId :

D-8(2.5-3)


Tgt Ion: 99 Resp: 3737091

Ion Ratio Lower Upper

99 100

42 13.3 12.2 18.4




71 30.3 23.8 35.8

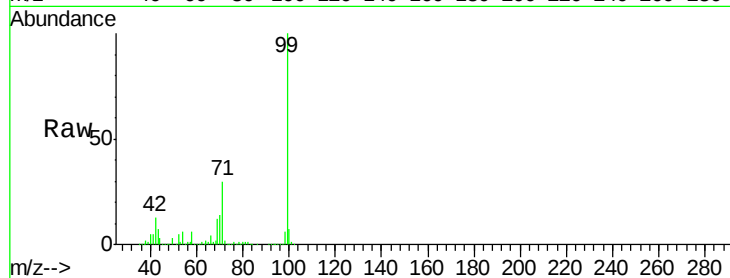

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

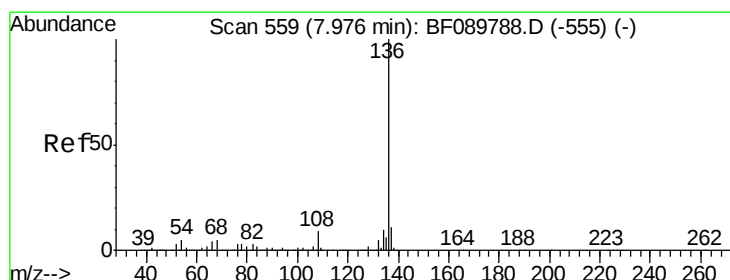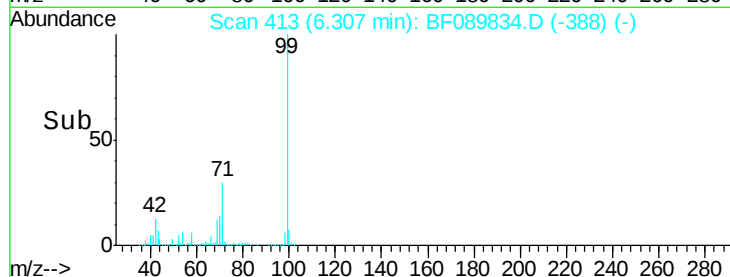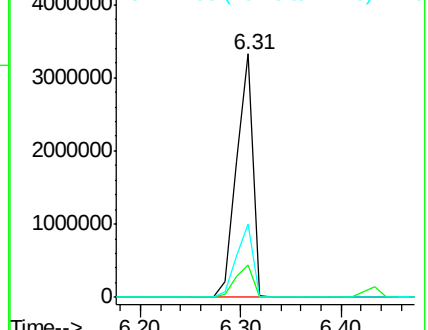

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.95 min Scan# 557

Delta R.T. -0.02 min

Lab File: BF089834.D

Acq: 23 Aug 2016 14:59

Tgt Ion: 136 Resp: 1938448


Ion Ratio Lower Upper

136 100

137 11.6 9.2 13.8

54 6.1 7.2 10.8#

68 5.7 5.8 8.8#


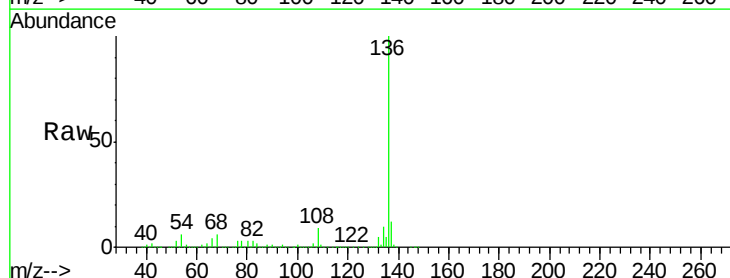



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



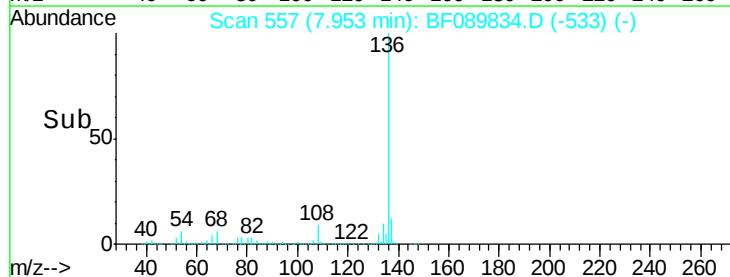
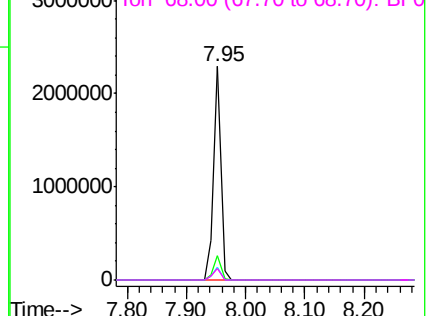


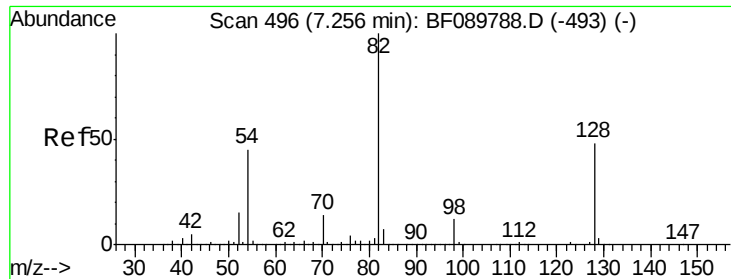

#23
 Nitrobenzene-d5
 Concen: 68.84 ng
 RT: 7.23 min Scan# 494
 Delta R.T. -0.02 min
 Lab File: BF089834.D
 Acq: 23 Aug 2016 14:59




Instrument :
 BNA_F
 ClientSampleId :
 D-8(2.5-3)


Tgt Ion: 82 Resp: 2147881
 Ion Ratio Lower Upper
 82 100
 128 48.5 34.4 51.6
 54 43.7 40.3 60.5

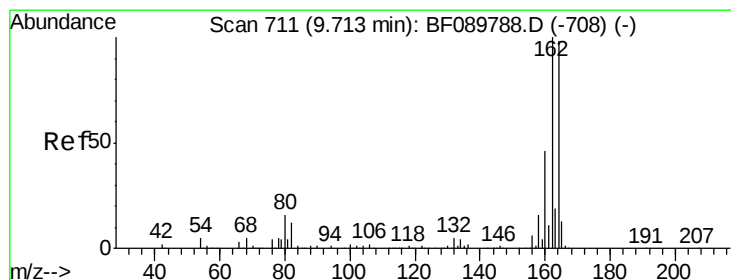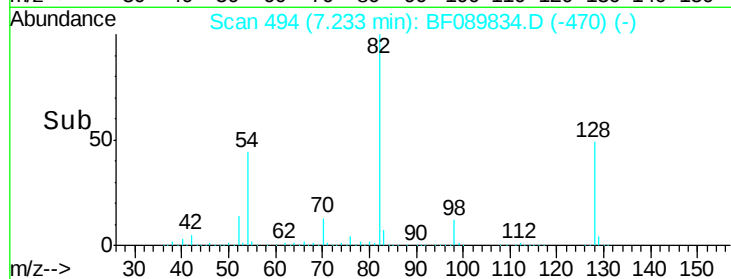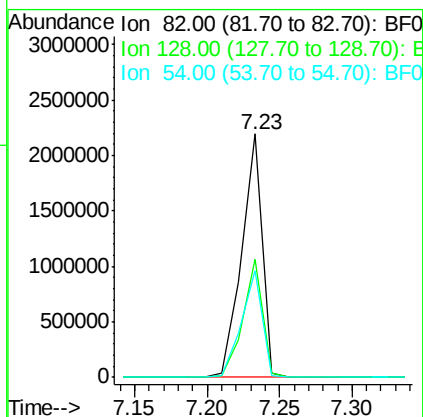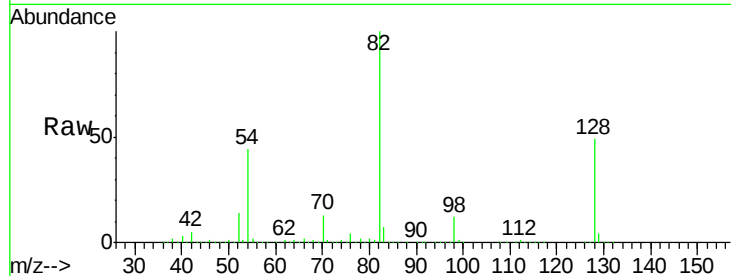

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.70 min Scan# 710
 Delta R.T. -0.01 min
 Lab File: BF089834.D
 Acq: 23 Aug 2016 14:59

Tgt Ion: 164 Resp: 886842
 Ion Ratio Lower Upper
 164 100
 162 100.9 81.4 122.2
 160 47.2 37.8 56.6

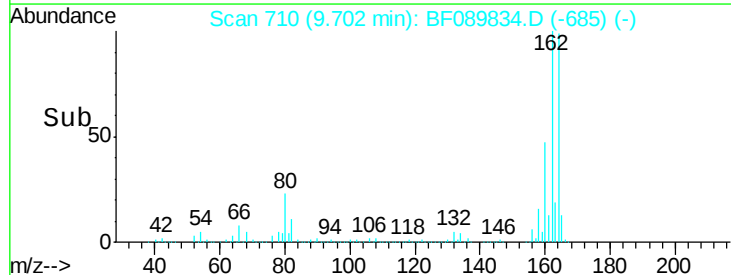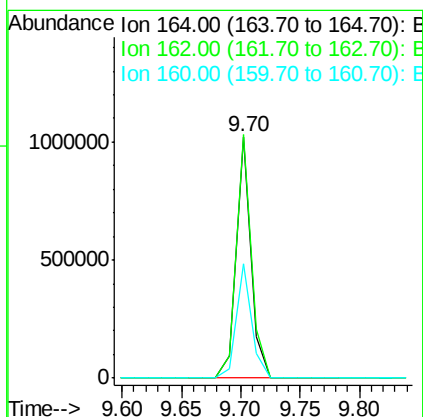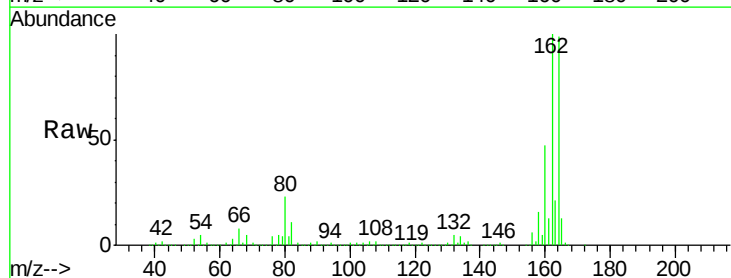


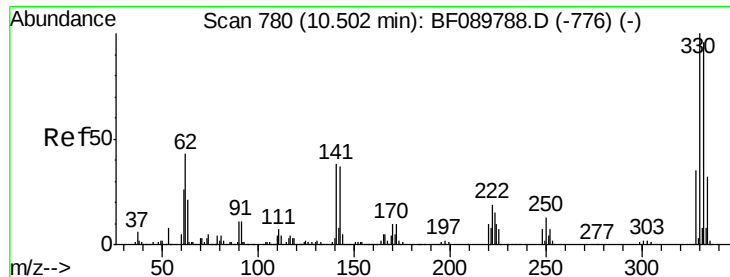




#41
 2,4,6-Tribromophenol
 Concen: 97.89 ng
 RT: 10.49 min Scan# 779
 Delta R.T. -0.01 min
 Lab File: BF089834.D
 Acq: 23 Aug 2016 14:59

Instrument :
 BNA_F
 ClientSampleId :
 D-8(2.5-3)

Tgt Ion:330 Resp: 825052
 Ion Ratio Lower Upper
 330 100
 332 96.6 76.7 115.1
 141 41.4 30.2 45.2

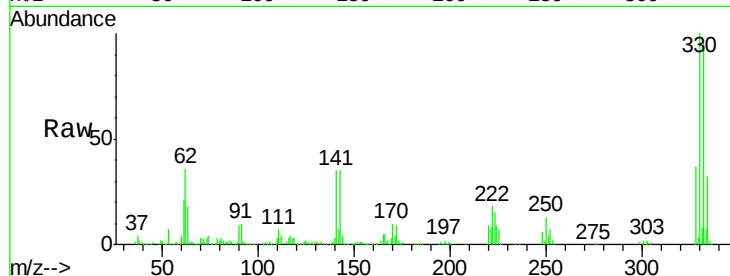


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

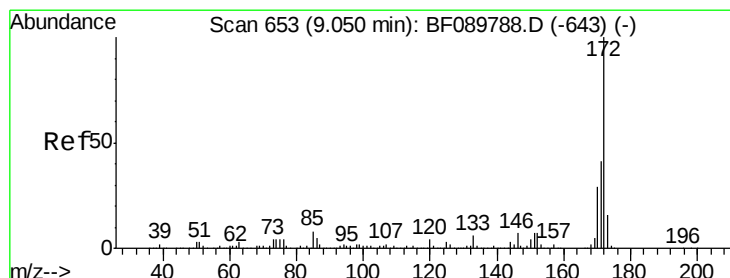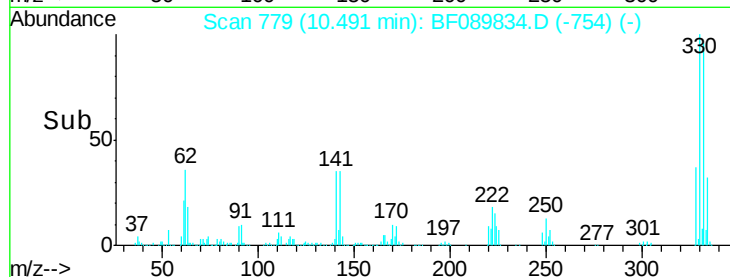
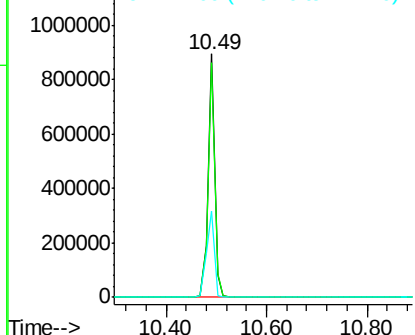



#44
 2-Fluorobiphenyl
 Concen: 78.15 ng
 RT: 9.04 min Scan# 652
 Delta R.T. -0.01 min
 Lab File: BF089834.D
 Acq: 23 Aug 2016 14:59

Tgt Ion:172 Resp: 3943268
 Ion Ratio Lower Upper
 172 100
 171 39.2 30.5 45.7
 170 27.3 20.6 31.0

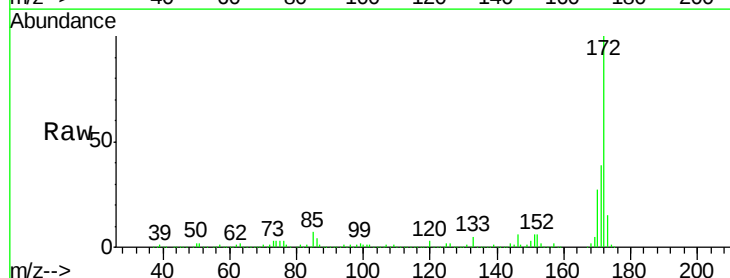

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

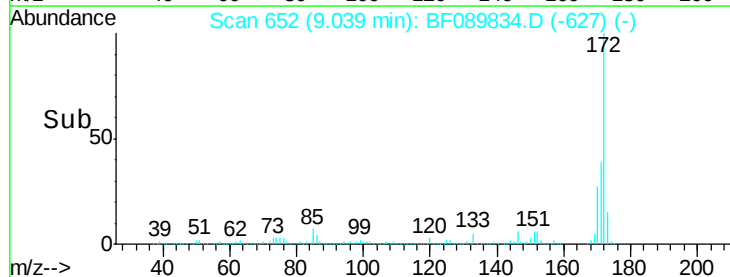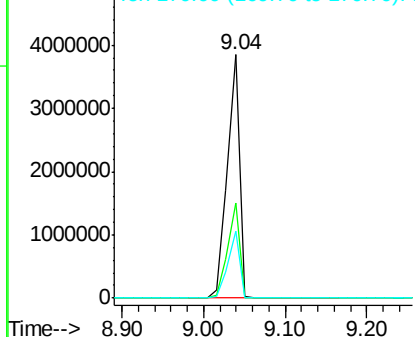

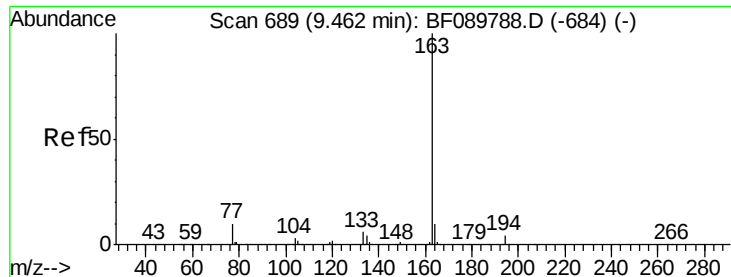

#49

Dimethylphthalate

Concen: 17.25 ng

RT: 9.43 min Scan# 686

Delta R.T. -0.03 min

Lab File: BF089834.D

Acq: 23 Aug 2016 14:59

Instrument :

BNA_F

ClientSampleId :

D-8(2.5-3)


Tgt Ion:163 Resp: 1076906

Ion Ratio Lower Upper

163 100

194 2.7 2.6 3.8




164 11.1 8.6 12.8

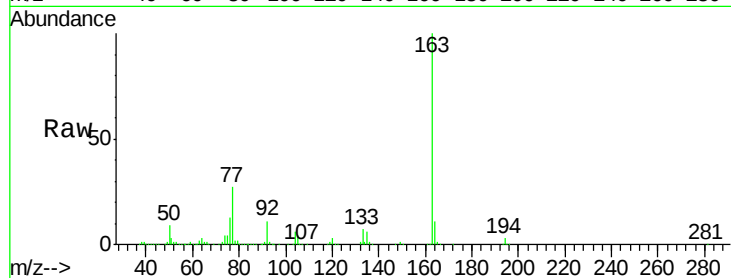

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

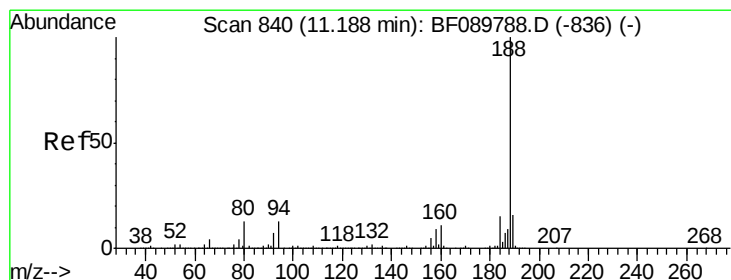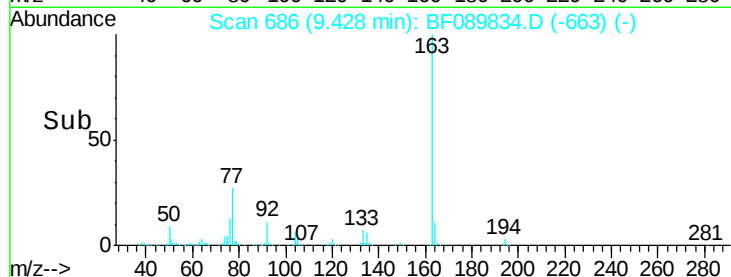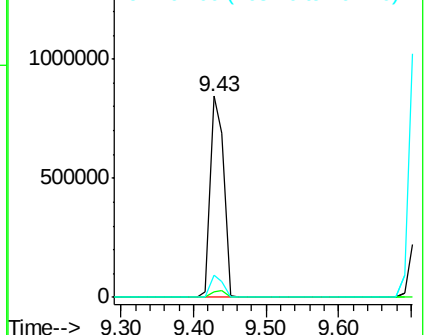

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.18 min Scan# 839

Delta R.T. -0.01 min

Lab File: BF089834.D

Acq: 23 Aug 2016 14:59


Tgt Ion:188 Resp: 1622478

Ion Ratio Lower Upper

188 100

94 12.8 10.2 15.2



80 13.4 10.9 16.3

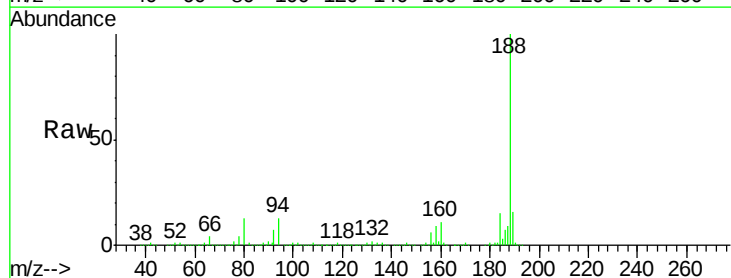


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

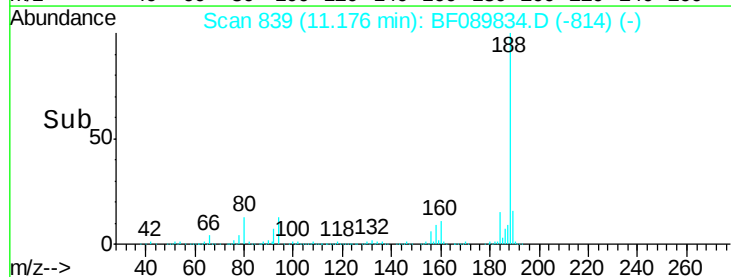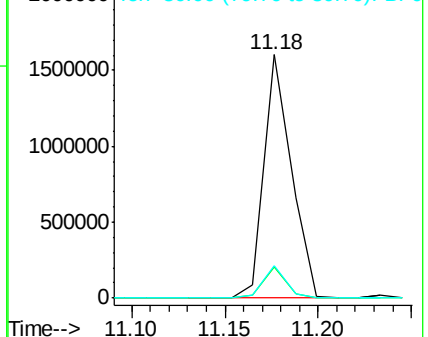

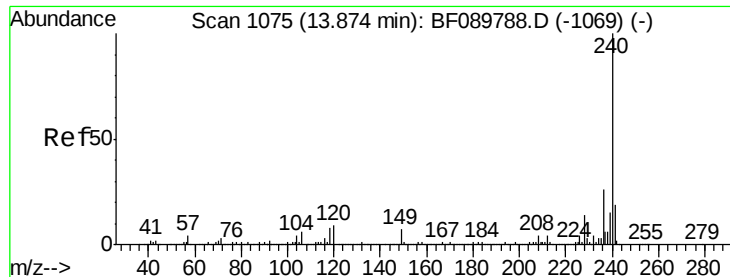

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.84 min Scan# 1072

Delta R.T. -0.03 min

Lab File: BF089834.D

Acq: 23 Aug 2016 14:59

Instrument :

BNA_F

ClientSampleId :

D-8(2.5-3)


Tgt Ion:240 Resp: 1477138

Ion Ratio Lower Upper

240 100

120 10.4 8.3 12.5




236 26.7 21.3 31.9

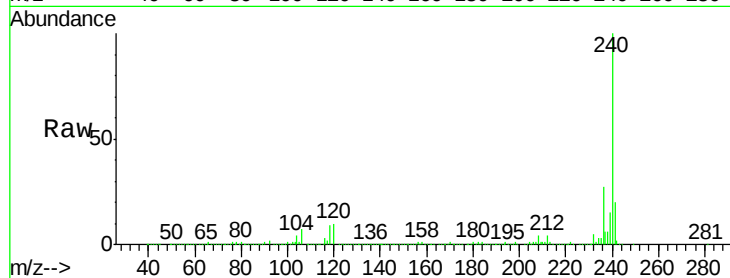

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

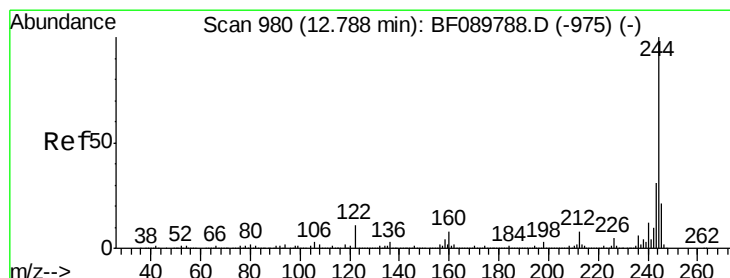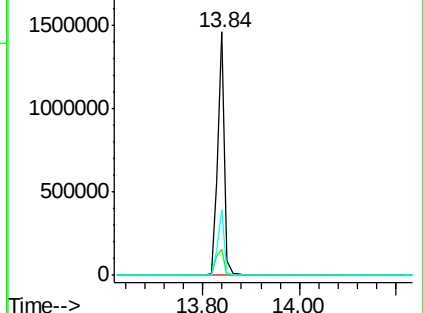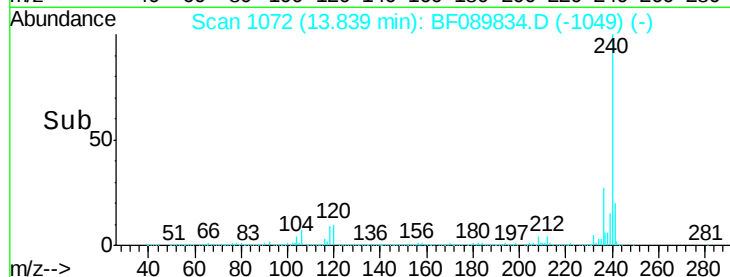

#78

Terphenyl-d14

Concen: 52.91 ng

RT: 12.78 min Scan# 979

Delta R.T. -0.01 min

Lab File: BF089834.D

Acq: 23 Aug 2016 14:59


Tgt Ion:244 Resp: 3454768

Ion Ratio Lower Upper

244 100

212 8.2 6.3 9.5



122 12.3 12.0 18.0

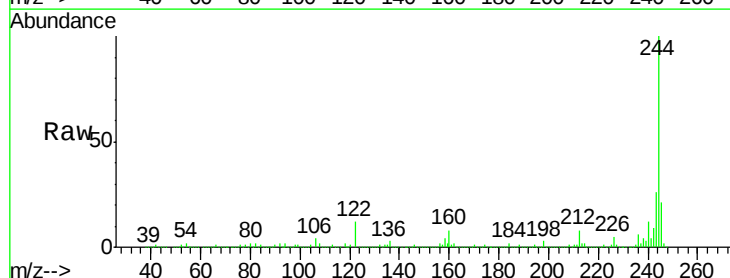


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

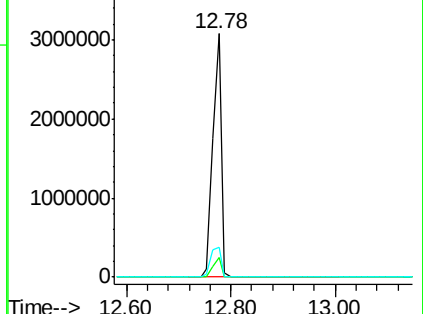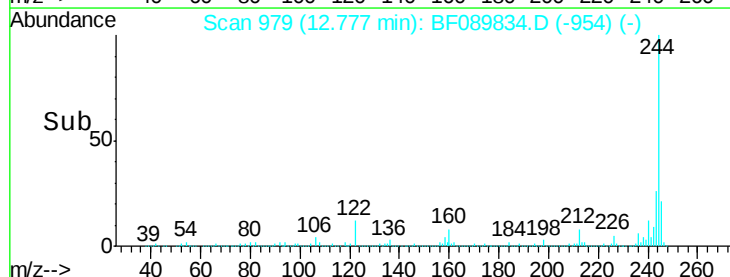

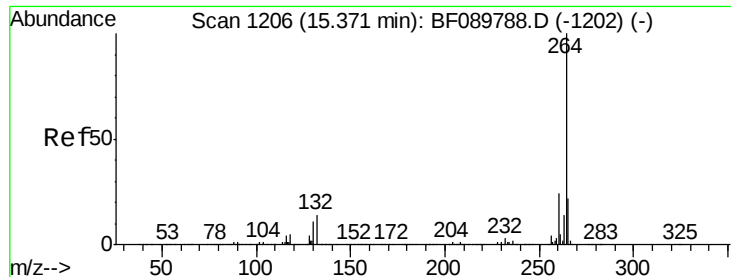

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.31 min Scan# 1201
Delta R.T. -0.06 min
Lab File: BF089834.D
Acq: 23 Aug 2016 14:59

Instrument :
BNA_F
ClientSampleId :
D-8(2.5-3)

Tgt Ion: 264 Resp: 1209775

Ion	Ratio	Lower	Upper
264	100		
260	23.4	20.2	30.2
265	21.7	17.4	26.2

